

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
 Data File : VX047926.D
 Acq On : 01 Oct 2025 09:14
 Operator : JC/MD
 Sample : VX1001MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1001MBL01

Quant Time: Oct 03 01:15:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.531	168	126415	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.745	114	260581	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	262910	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	128303	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.934	65	99175	49.287	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.580%
35) Dibromofluoromethane	5.367	113	82968	47.475	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.960%
50) Toluene-d8	8.628	98	285418	47.200	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.400%
62) 4-Bromofluorobenzene	11.061	95	119715	52.164	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	104.320%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
Data File : VX047926.D
Acq On : 01 Oct 2025 09:14
Operator : JC/MD
Sample : VX1001MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1001MBL01

Quant Time: Oct 03 01:15:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration



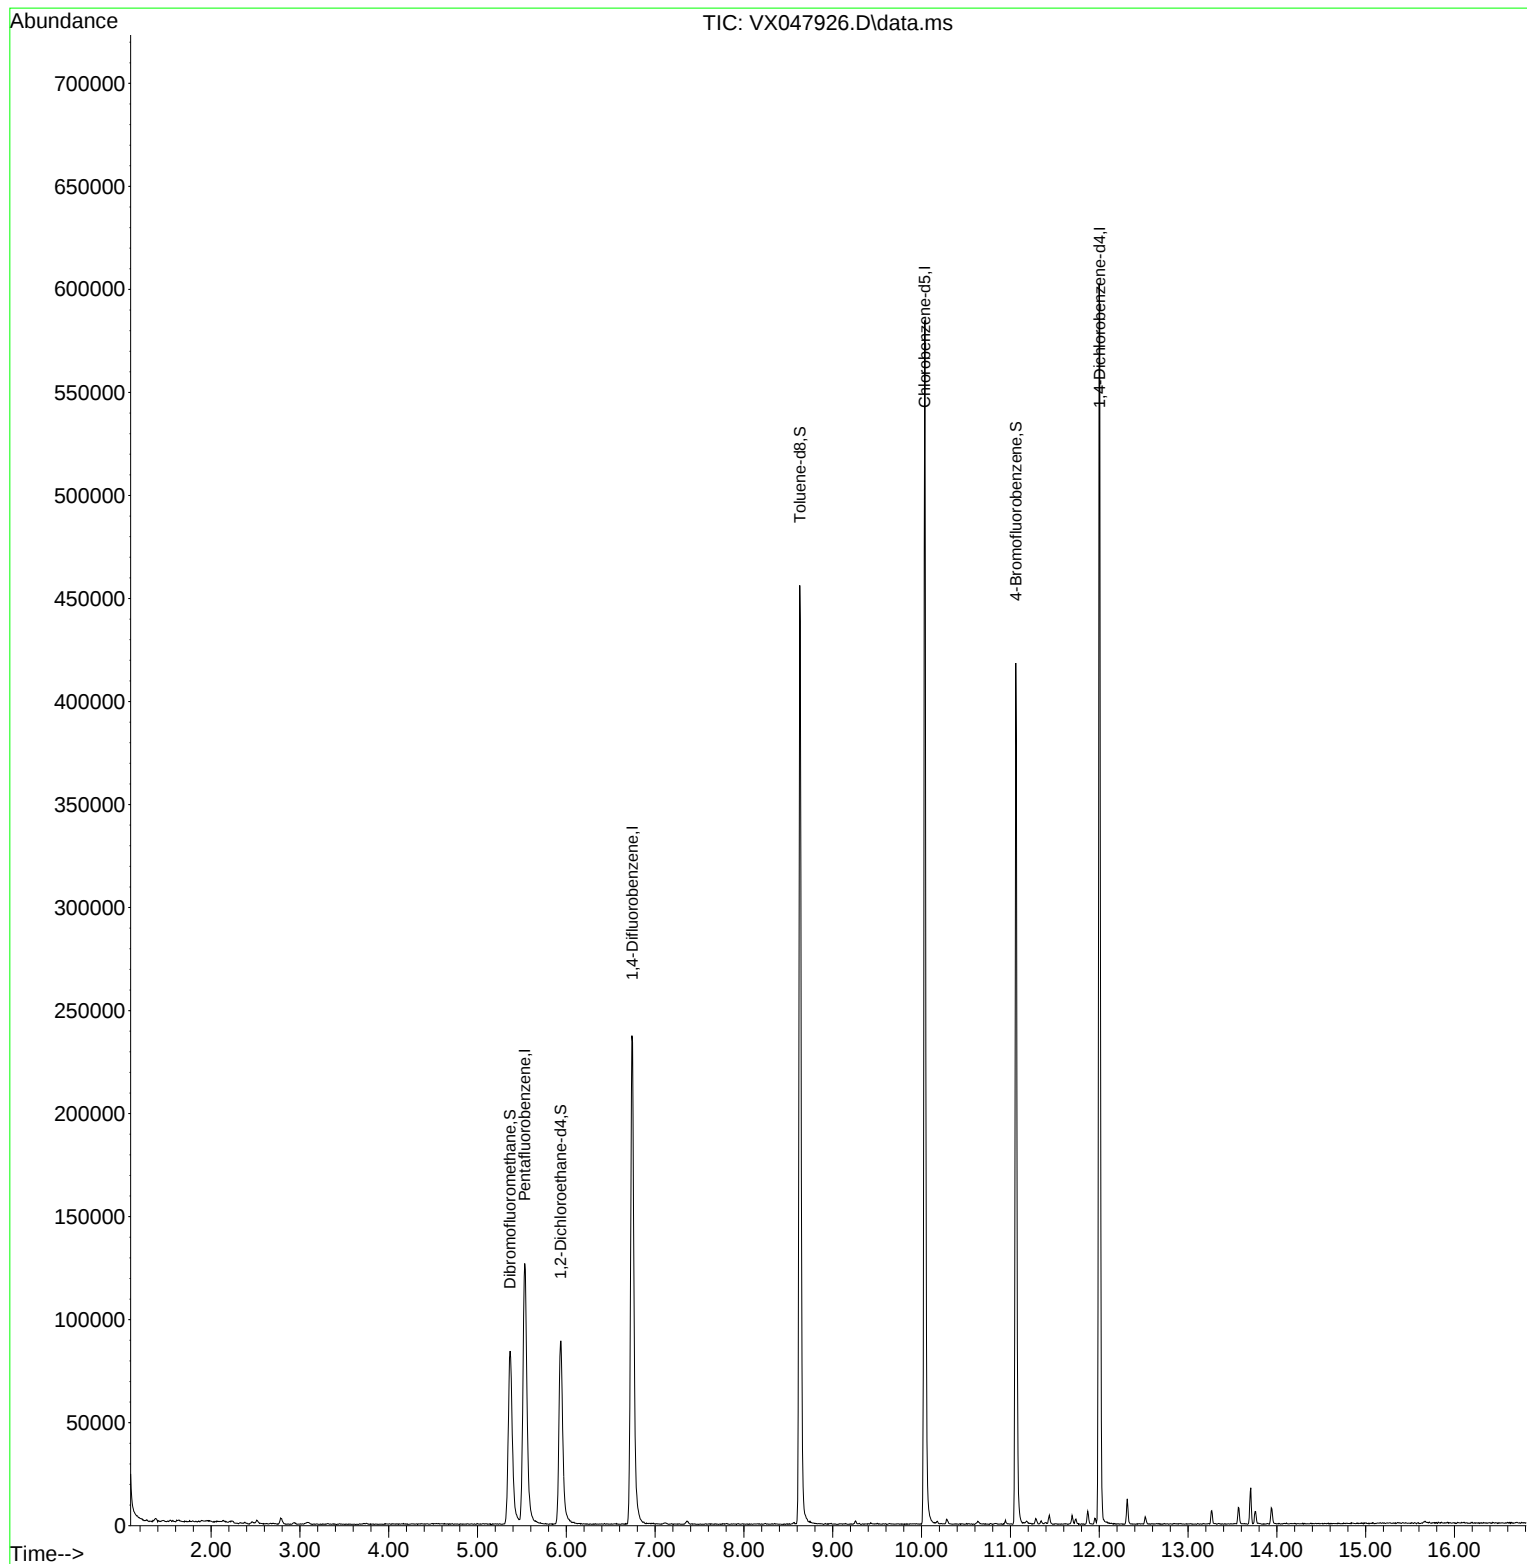




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.531 min Scan# 71
Delta R.T. -0.013 min
Lab File: VX047926.D
Acq: 01 Oct 2025 09:14




Instrument :
MSVOA_X
ClientSampleId :
VX1001MBL01


Tgt Ion:168 Resp: 126415
Ion Ratio Lower Upper
168 100
99 63.6 48.8 73.2

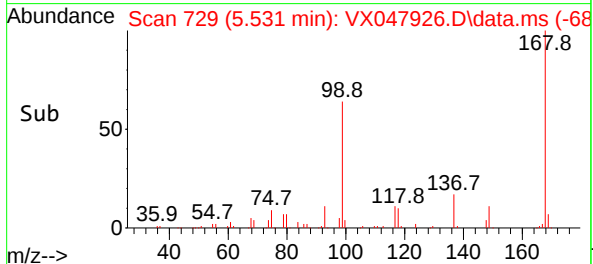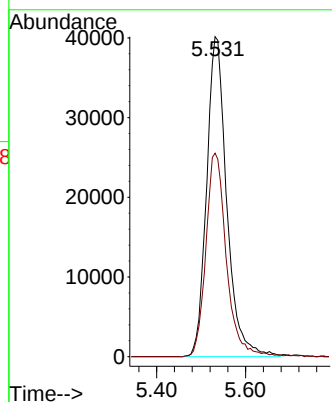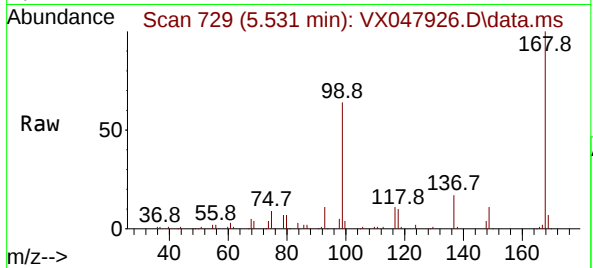

#33
1,2-Dichloroethane-d4
Concen: 49.287 ug/l
RT: 5.934 min Scan# 795
Delta R.T. -0.006 min
Lab File: VX047926.D
Acq: 01 Oct 2025 09:14

Tgt Ion: 65 Resp: 99175
Ion Ratio Lower Upper
65 100
67 51.2 0.0 103.0

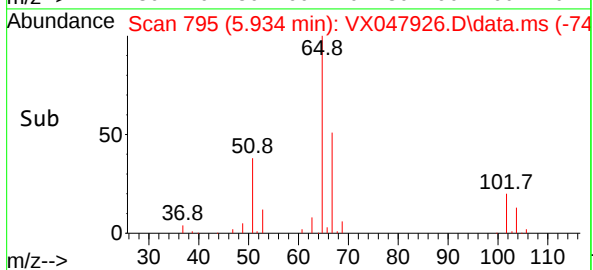
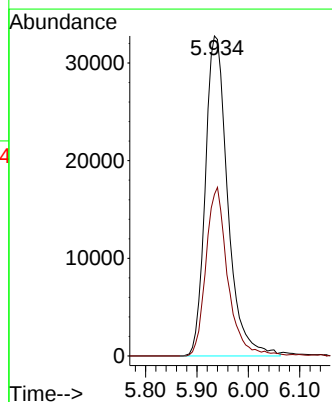
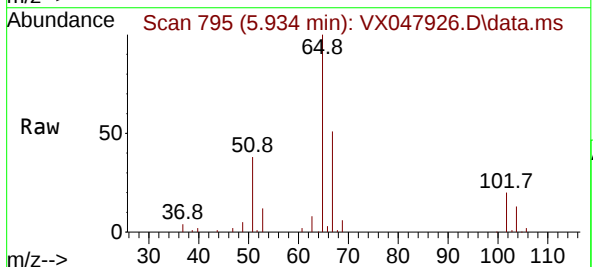


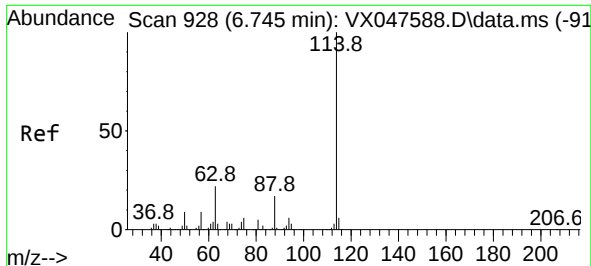

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX047926.D
Acq: 01 Oct 2025 09:14




Instrument :
MSVOA_X
ClientSampleId :
VX1001MBL01

Tgt Ion:114 Resp: 260581
Ion Ratio Lower Upper
114 100
63 21.8 0.0 44.0
88 16.0 0.0 34.2

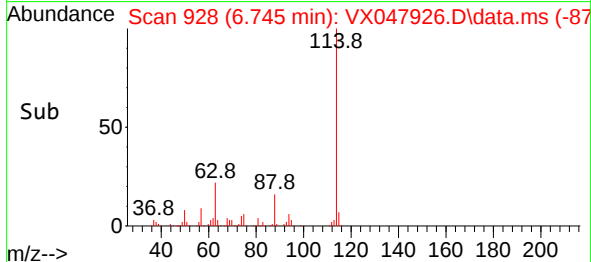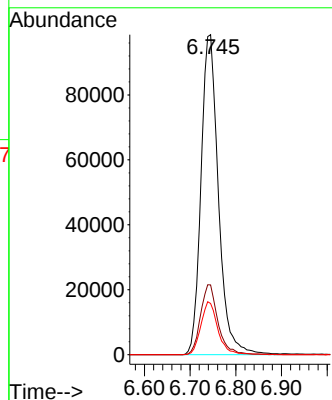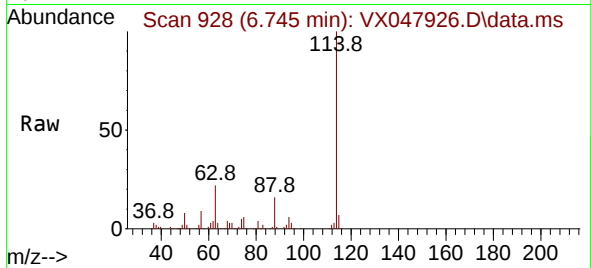

#35
Dibromofluoromethane
Concen: 47.475 ug/l
RT: 5.367 min Scan# 702
Delta R.T. -0.006 min
Lab File: VX047926.D
Acq: 01 Oct 2025 09:14

Tgt Ion:113 Resp: 82968
Ion Ratio Lower Upper
113 100
111 103.5 80.9 121.3
192 18.6 14.2 21.4

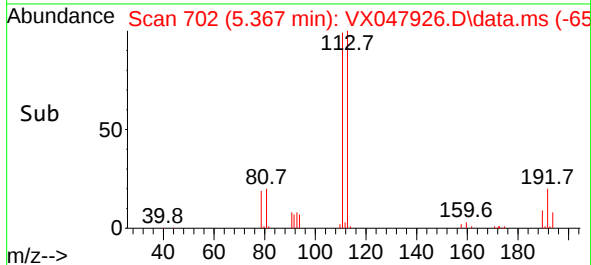
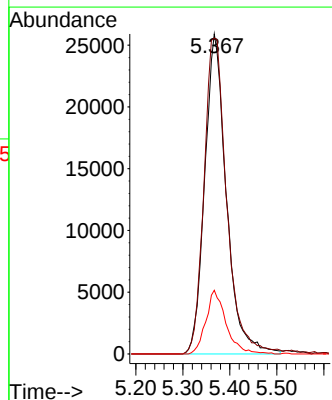
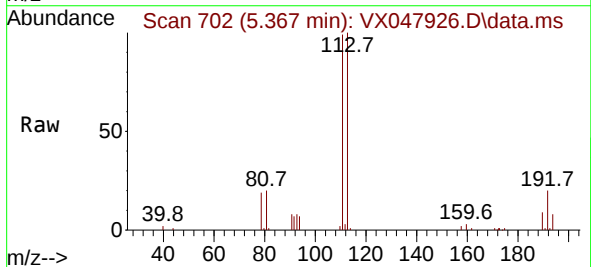




#50
Toluene-d8
Concen: 47.200 ug/l
RT: 8.628 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX047926.D
Acq: 01 Oct 2025 09:14




Instrument :
MSVOA_X
ClientSampleId :
VX1001MBL01


Tgt Ion: 98 Resp: 285418
Ion Ratio Lower Upper
98 100
100 66.3 53.0 79.4

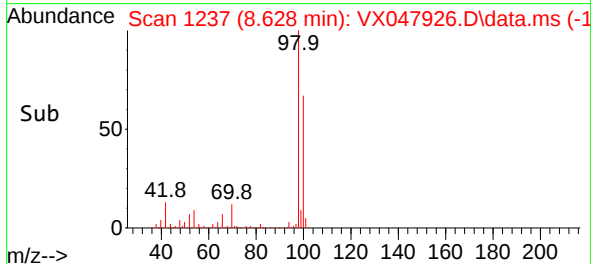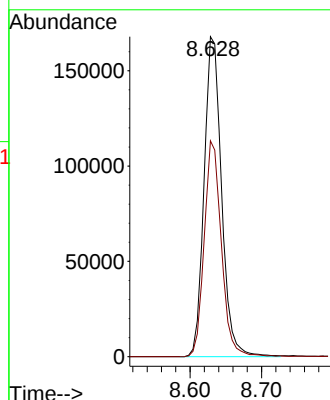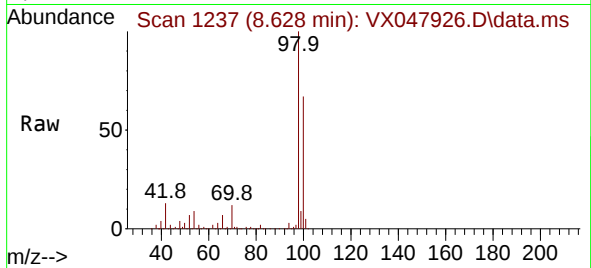

#62
4-Bromofluorobenzene
Concen: 52.164 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX047926.D
Acq: 01 Oct 2025 09:14

Tgt Ion: 95 Resp: 119715
Ion Ratio Lower Upper
95 100
174 71.4 0.0 141.6
176 69.4 0.0 138.4

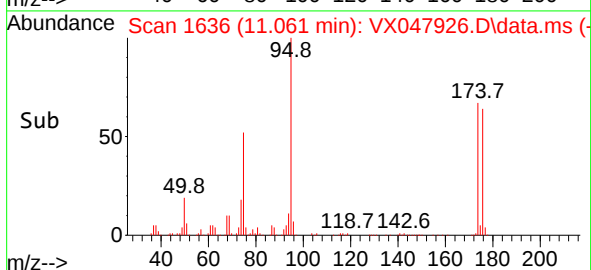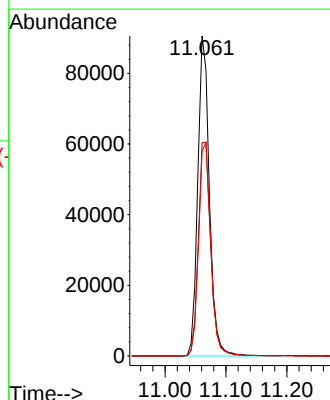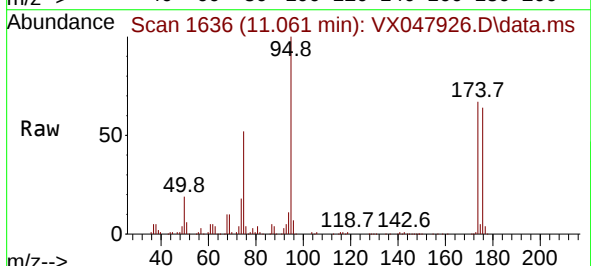

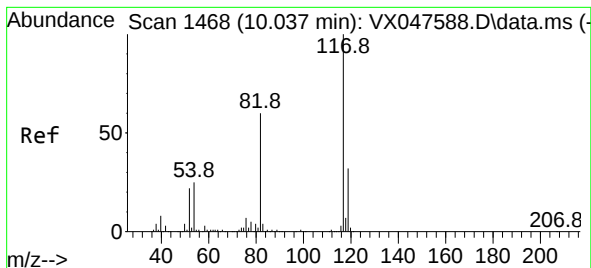

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.037 min Scan# 1468

Delta R.T. -0.000 min

Lab File: VX047926.D

Acq: 01 Oct 2025 09:14

Instrument :

MSVOA_X

ClientSampleId :

VX1001MBL01





Tgt Ion:117 Resp: 262910

Ion Ratio Lower Upper

117 100

82 55.9 47.8 71.6

119 32.7 25.2 37.8

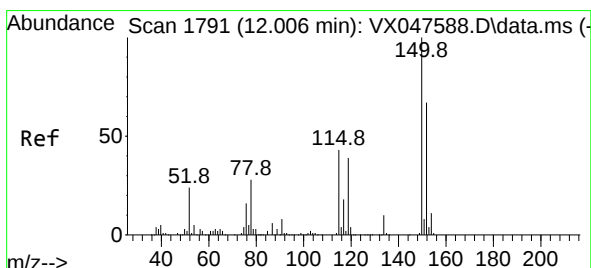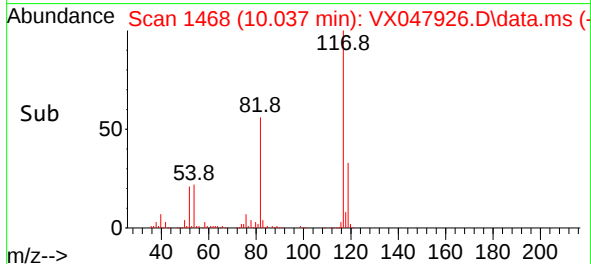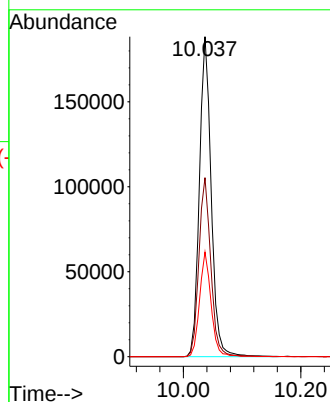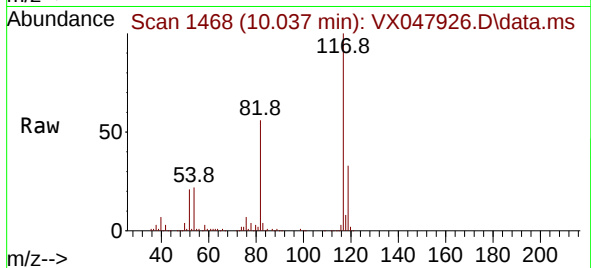

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX047926.D

Acq: 01 Oct 2025 09:14

Tgt Ion:152 Resp: 128303

Ion Ratio Lower Upper

152 100

115 61.9 44.9 134.5

150 158.6 0.0 352.0

