

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
 Data File : VX047941.D
 Acq On : 01 Oct 2025 15:30
 Operator : JC/MD
 Sample : Q3193-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW203D-20250923

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M

Title : SW846 8260

Signal : TIC: VX047941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.489	548	558	566	rBV3	6488	20718	2.17%	0.377%
2	5.373	692	703	720	rBV	100816	329769	34.58%	6.006%
3	5.538	720	730	757	rVB2	139571	448604	47.04%	8.171%
4	5.946	787	797	823	rBV	111978	332262	34.84%	6.052%
5	6.745	918	928	950	rBV	270050	707674	74.21%	12.889%
6	7.110	979	988	1003	rBV3	61013	145297	15.24%	2.646%
7	8.635	1231	1238	1255	rBV	548444	905710	94.98%	16.496%
8	9.263	1336	1341	1348	rBV2	9327	15684	1.64%	0.286%
9	10.037	1462	1468	1487	rBV	665974	953572	100.00%	17.368%
10	11.067	1631	1637	1651	rBV	512680	683324	71.66%	12.446%
11	12.006	1785	1791	1803	rBV	724361	947904	99.41%	17.264%




Sum of corrected areas: 5490518

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
Data File : VX047941.D
Acq On : 01 Oct 2025 15:30
Operator : JC/MD
Sample : Q3193-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW203D-20250923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

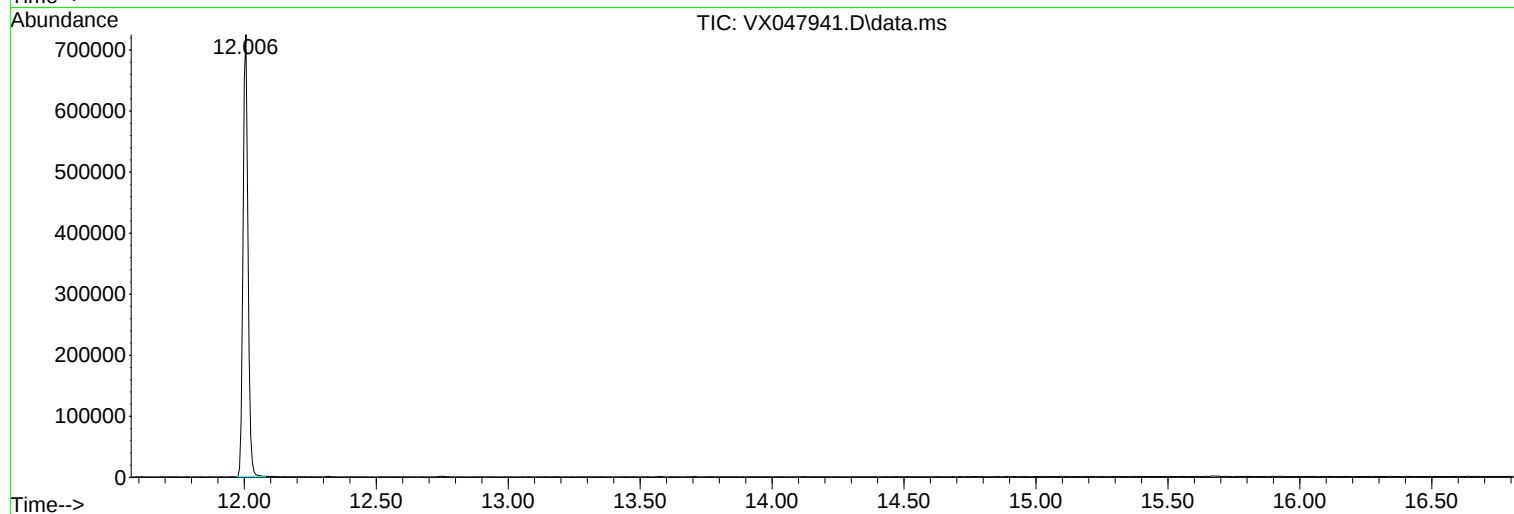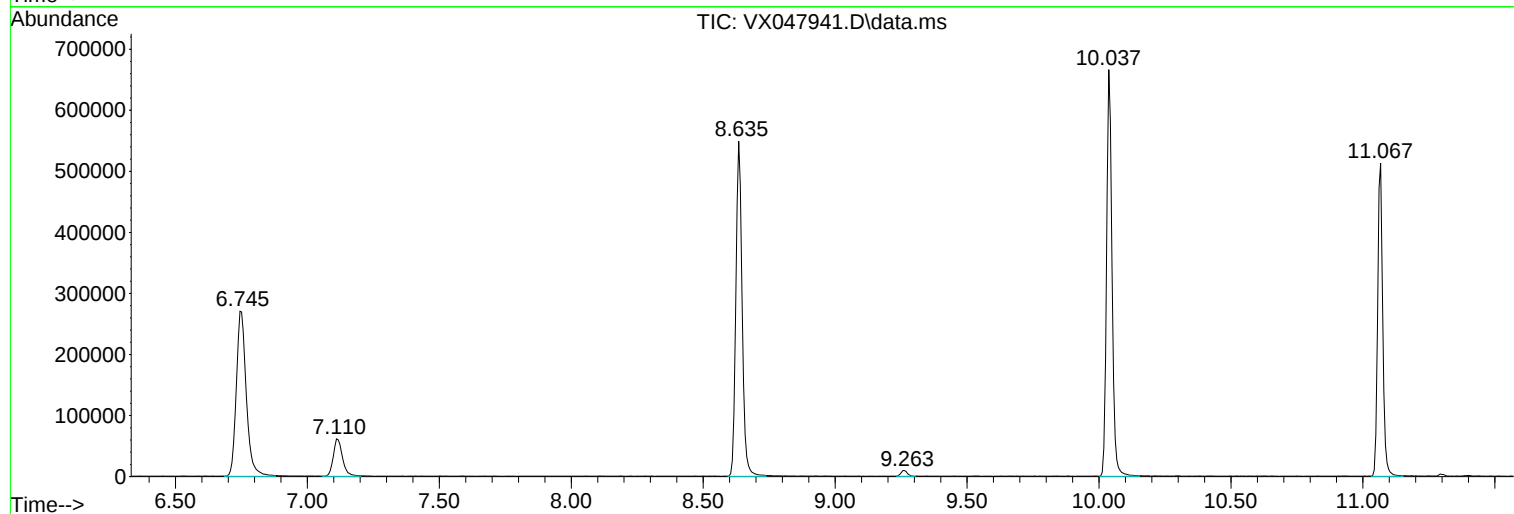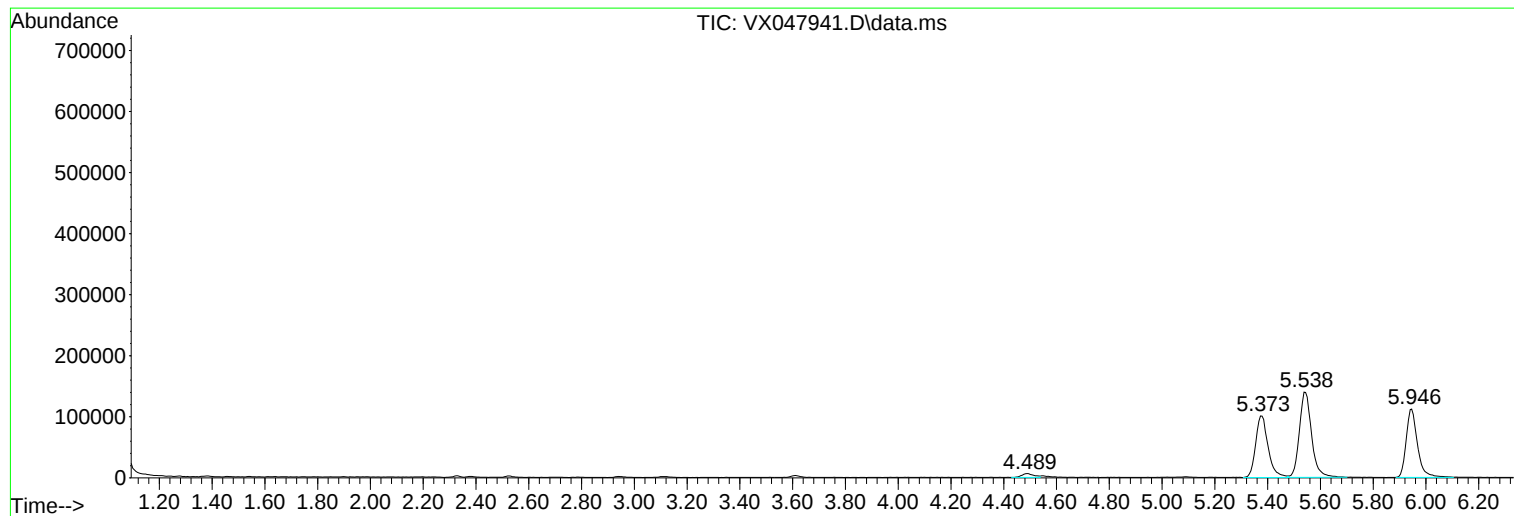

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
Data File : VX047941.D
Acq On : 01 Oct 2025 15:30
Operator : JC/MD
Sample : Q3193-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW203D-20250923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100125\
Data File : VX047941.D
Acq On : 01 Oct 2025 15:30
Operator : JC/MD
Sample : Q3193-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW203D-20250923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
