


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100218\
 Data File : VX004909.D
 Acq On : 02 Oct 2018 09:22
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X100218W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Oct 03 04:49:12 2018

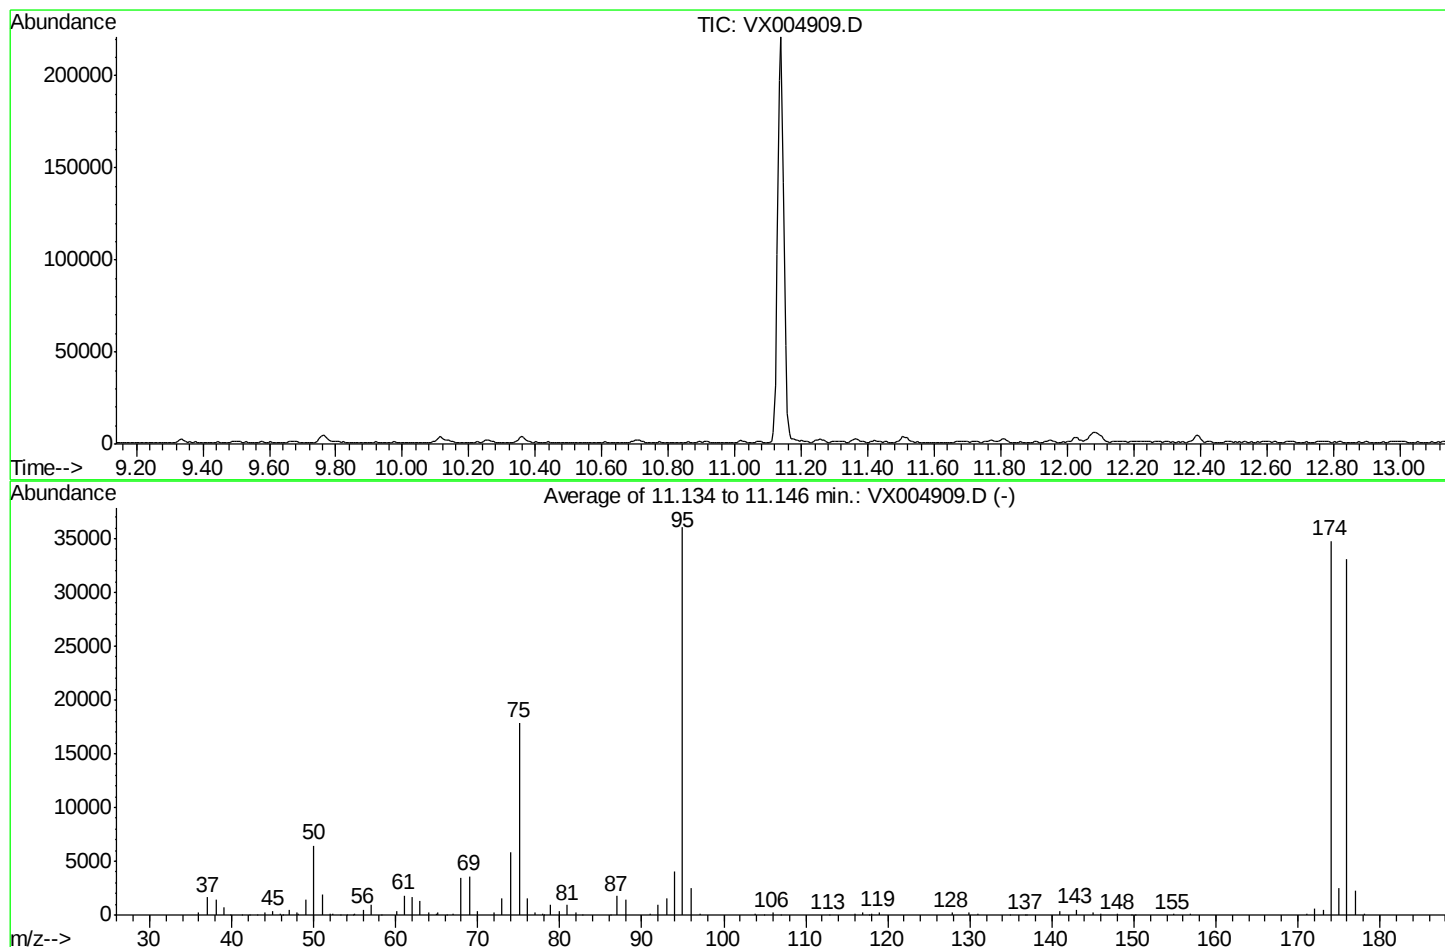

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	6430	PASS
75	95	30	60	49.6	17880	PASS
95	95	100	100	100.0	36050	PASS
96	95	5	9	7.0	2533	PASS
173	174	0.00	2	1.4	482	PASS
174	95	50	100	96.5	34802	PASS
175	174	5	9	7.2	2501	PASS
176	174	95	101	95.0	33069	PASS
177	176	5	9	6.7	2228	PASS