

Data Path : C:\Users\seuser\Desktop\USHA\VN081419\
Data File : VN057277.D
Acq On : 14 Aug 2019 10:49
Operator : JC/SP
Sample : VN0814WBL01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 3 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: RTEINT.P

Peak Number 2 p-Bromofluorobenzene Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.35	50.00 ug/l	2049570	1,4-Dichlorobenzene-d4	13.35
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		p-Bromofluorobenzene	174 C6H4BrF	000460-00-4 97
2		Benzene, 1-bromo-3-fluoro-	174 C6H4BrF	001073-06-9 95
3		Benzene, 1-bromo-2-fluoro-	174 C6H4BrF	001072-85-1 94
4		Pyrazole, 3-(2-bromoethyl)-	174 C5H7BrN2	211738-72-6 45
5		4(1H)-Pyrimidinone, 5-bromo-	174 C4H3BrN2O	019808-30-1 37

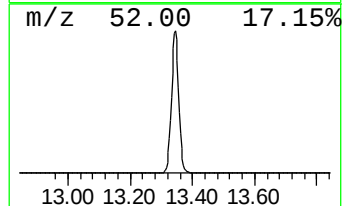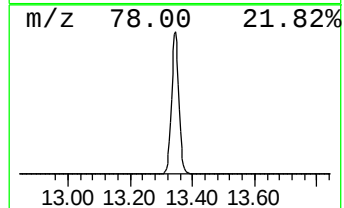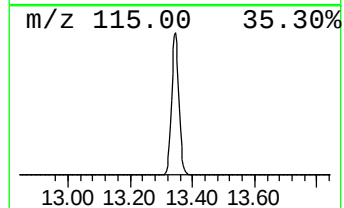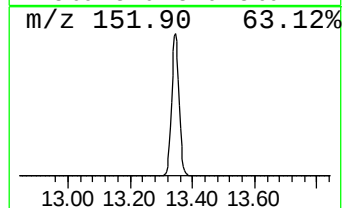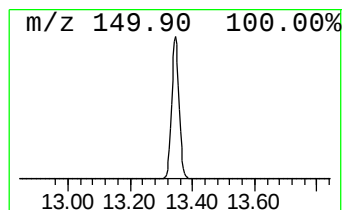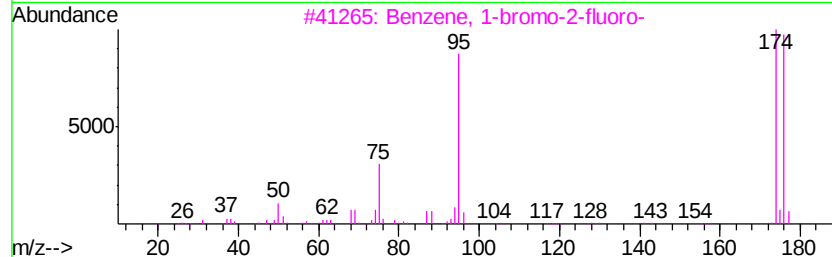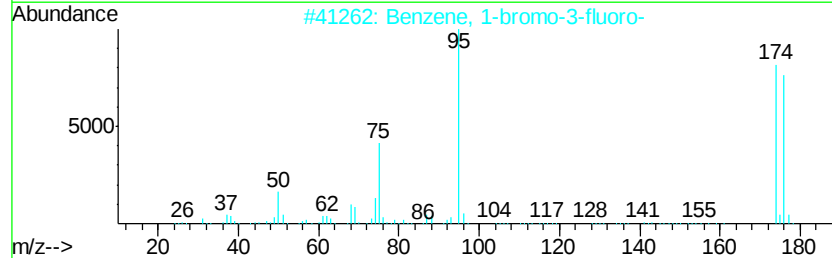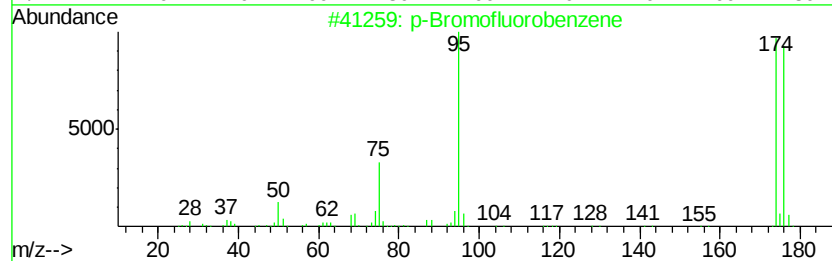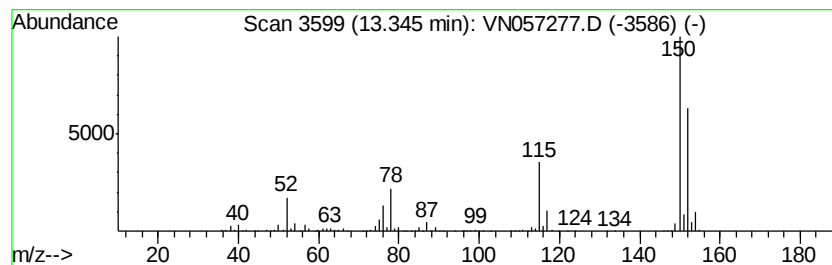

Data Path : C:\Users\euser\Desktop\USHA\VN081419\
Data File : VN057277.D
Acq On : 14 Aug 2019 10:49
Operator : JC/SP
Sample : VN0814WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
p-Bromofluorobenzene	13.35	50.0	ug/l	2049570	4	13.35	2049570	50.0
p-Bromofluorobenzene	13.35	50.0	ug/l	2049570	4	13.35	2049570	50.0