

(QT Reviewed)


```
Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100220\  
Data File : VX018739.D  
Acq On    : 02 Oct 2020   10:55  
Operator  : JC/SP  
Sample    : VSTD00165  
Misc      : 25.0mL/MSVOA_X/WATER  
ALS Vial  : 3      Sample Multiplier: 1
```

Instrument :
MSVOA_X
ClientSampleId :
VSTD00165

Manual Integrations
APPROVED

MMDadoda
10/6/2020 1:25:19 PM

Quant Time: Oct 02 11:57:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 11:50:55 2020
Response via : Initial Calibration

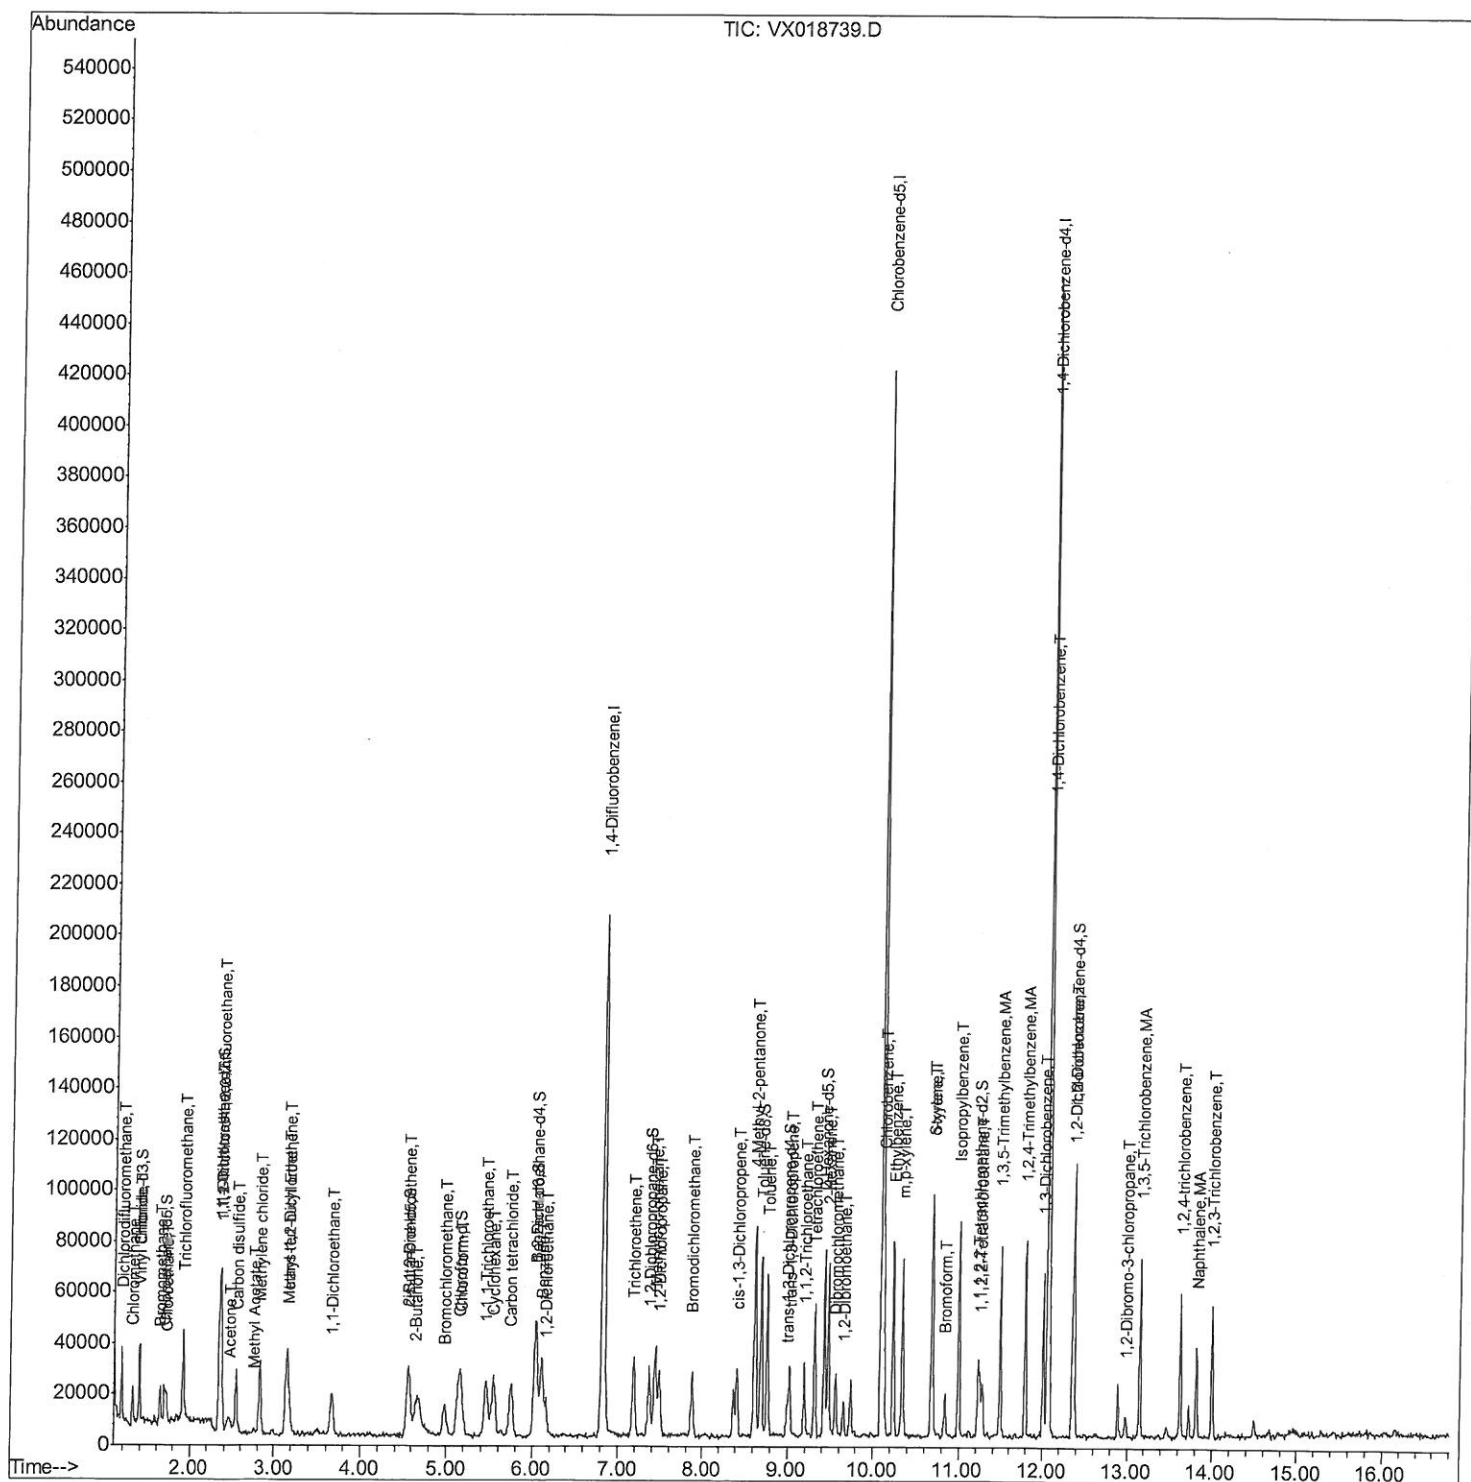

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100220\
Data File : VX018739.D
Acq On : 02 Oct 2020 10:55
Operator : JC/SP
Sample : VSTD00165
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTD00165

Manual Integrations
APPROVED

MMDadoda
10/6/2020 1:25:19 PM

Quant Time: Oct 02 11:53:37 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 11:50:55 2020
Response via : Initial Calibration

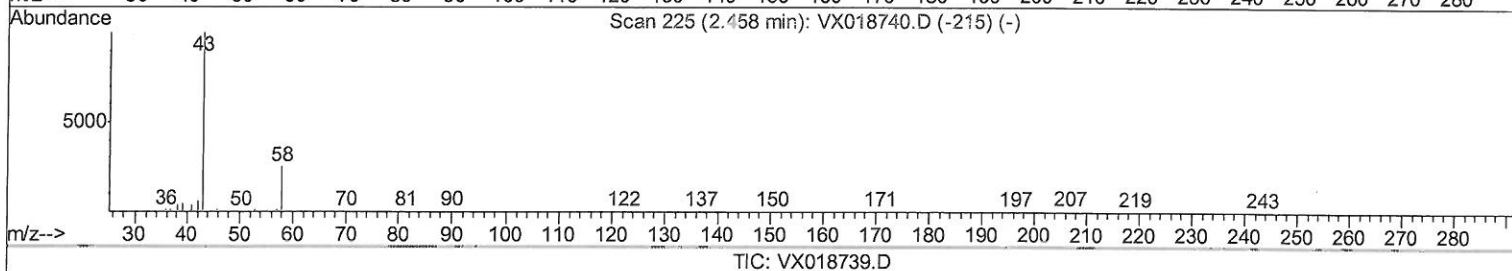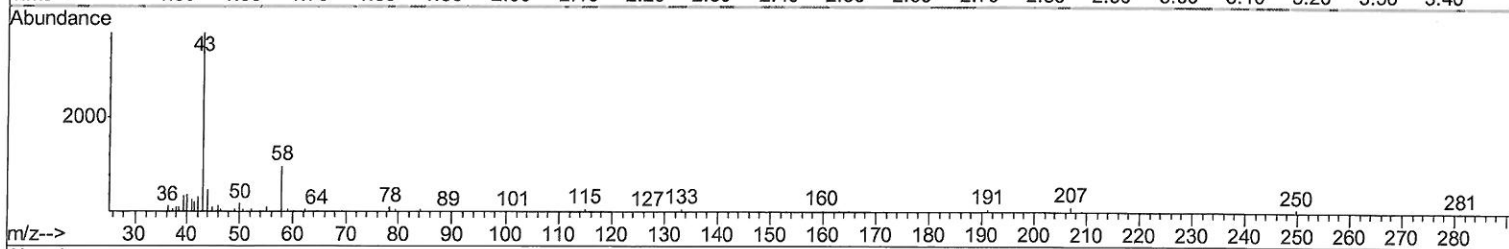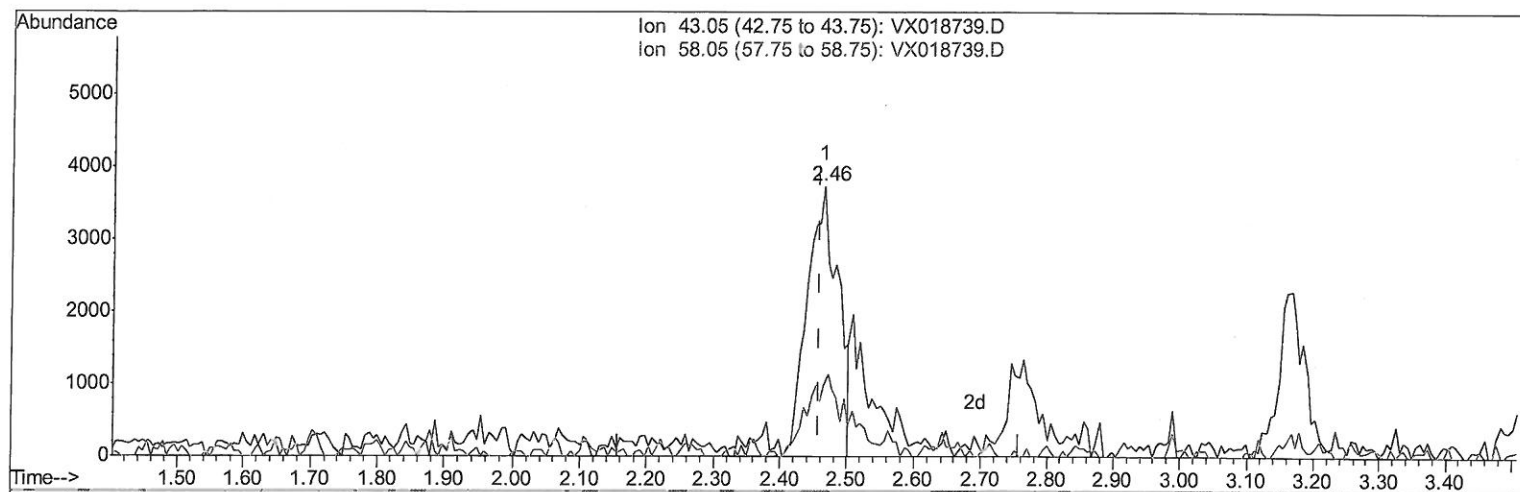

TIC: VX018739.D

(13) Acetone (T)

2.465min (+0.007) 5.03ug/L

response 12028

Ion	Exp%	Act%
43.05	100	100
58.05	28.20	39.61
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100220\
 Data File : VX018739.D
 Acq On : 02 Oct 2020 10:55
 Operator : JC/SP
 Sample : VSTD00165
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD00165

Manual Integrations
 APPROVED

MMDadoda
 10/6/2020 1:25:19 PM

Quant Time: Oct 02 11:53:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 11:50:55 2020
 Response via : Initial Calibration

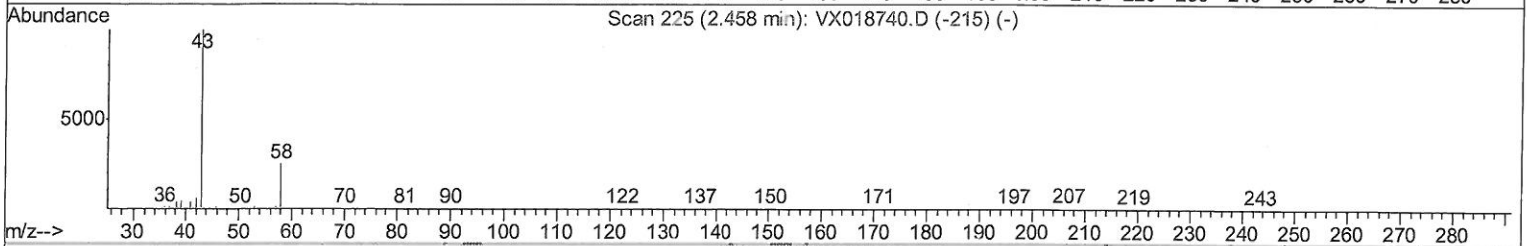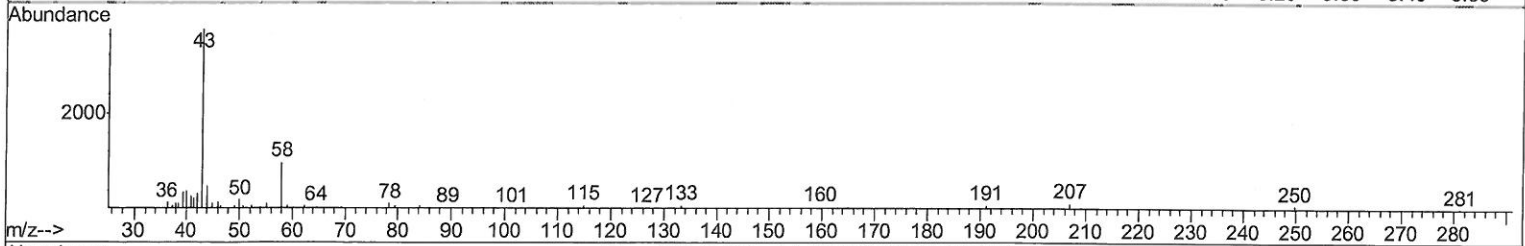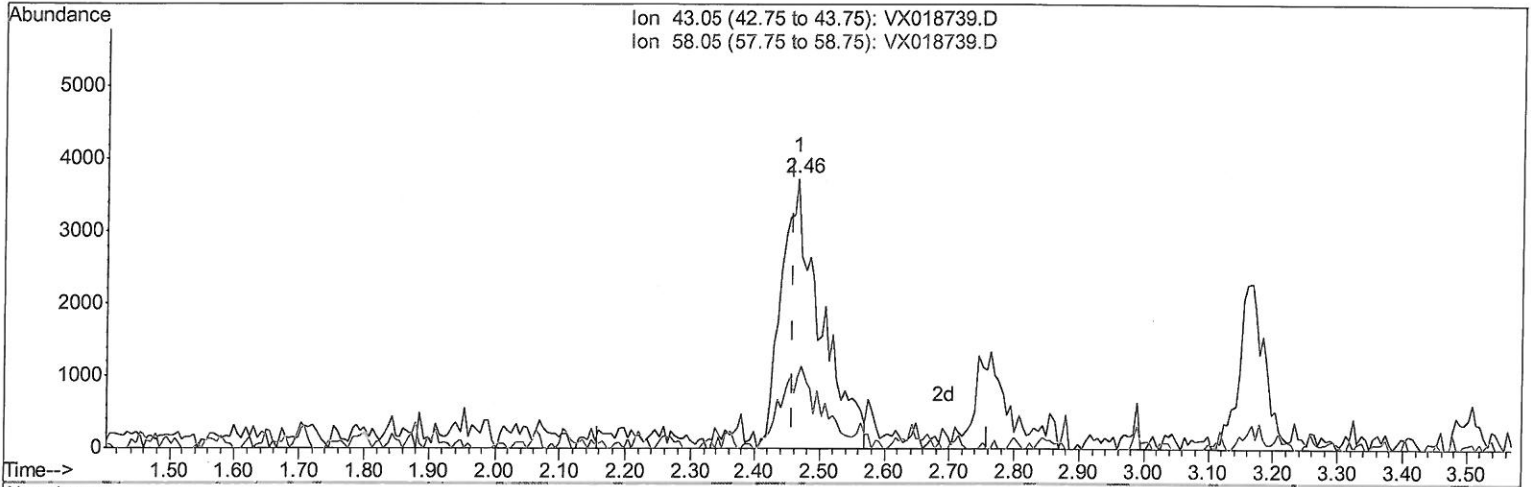

TIC: VX018739.D

(13) Acetone (T)

2.465min (+0.007) 6.56ug/L m

response 15700

Ion	Exp%	Act%
43.05	100	100
58.05	28.20	30.34
0.00	0.00	0.00
0.00	0.00	0.00

Signature
 10/06/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100220\
 Data File : VX018739.D
 Acq On : 02 Oct 2020 10:55
 Operator : JC/SP
 Sample : VSTD00165
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD00165

Manual Integrations
 APPROVED

MMDadoda
 10/6/2020 1:25:19 PM

Quant Time: Oct 02 11:53:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 11:50:55 2020
 Response via : Initial Calibration

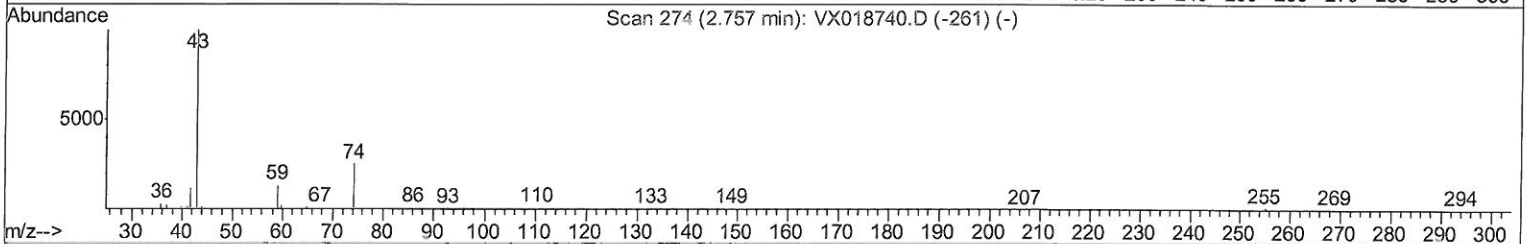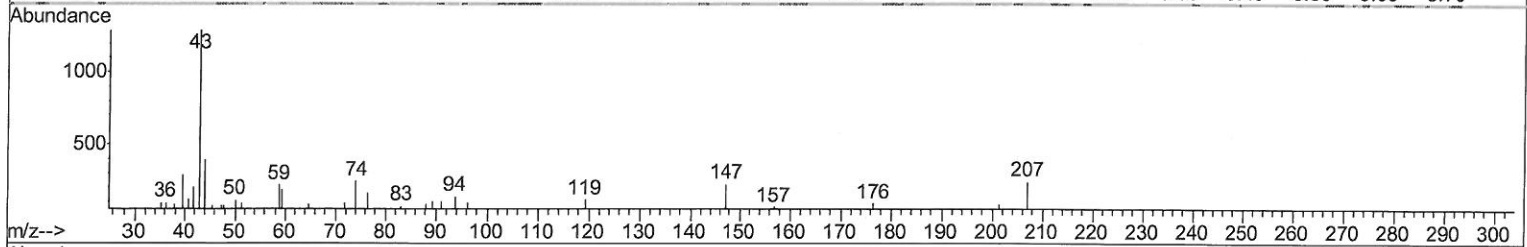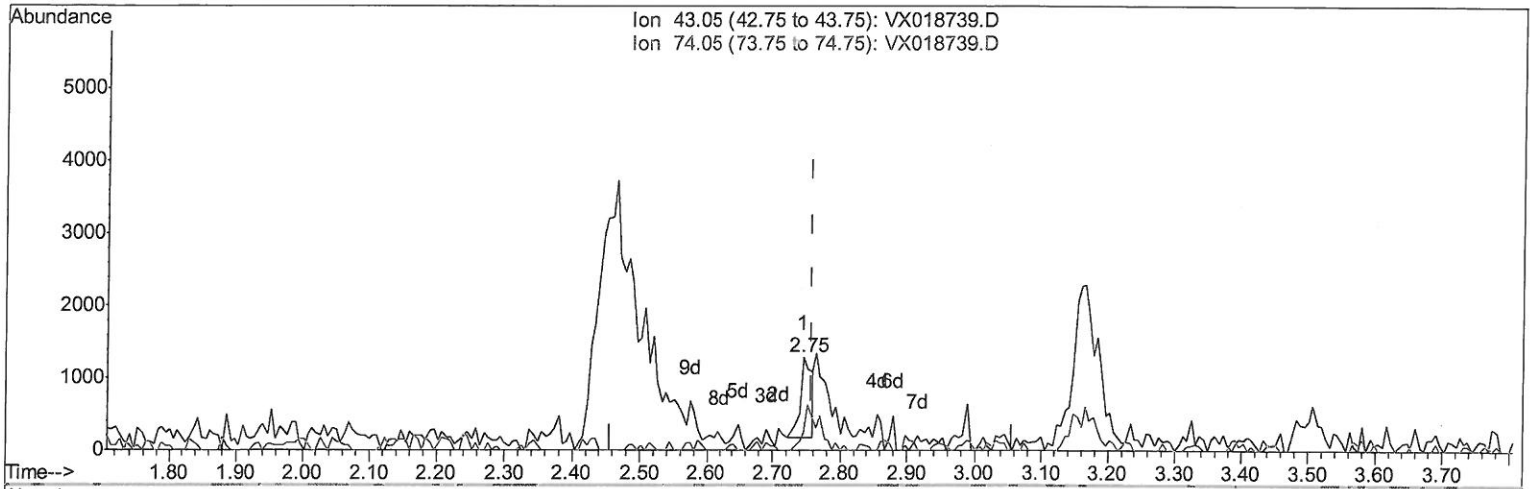

TIC: VX018739.D

(15) Methyl Acetate (T)

2.745min (-0.012) 0.19ug/L

response 1325

Ion	Exp%	Act%
43.05	100	100
74.05	27.40	75.70#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100220\
Data File : VX018739.D
Acq On : 02 Oct 2020 10:55
Operator : JC/SP
Sample : VSTD00165
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
VSTD00165

Manual Integrations
APPROVED

MMDadoda
10/6/2020 1:25:19 PM

Quant Time: Oct 02 11:53:37 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 11:50:55 2020
Response via : Initial Calibration

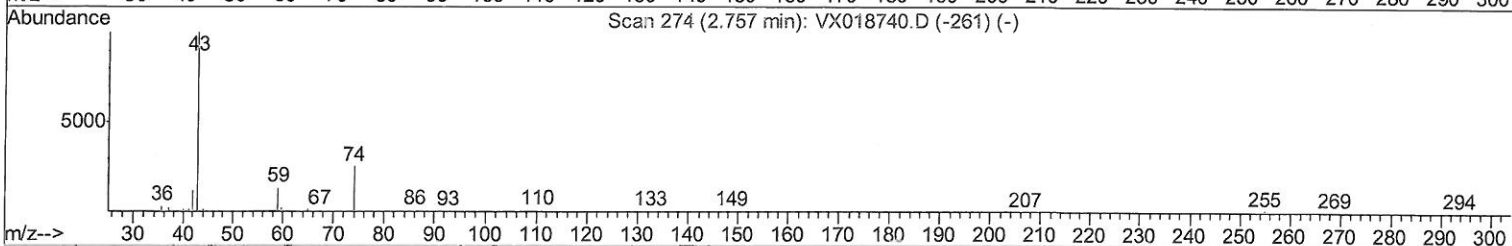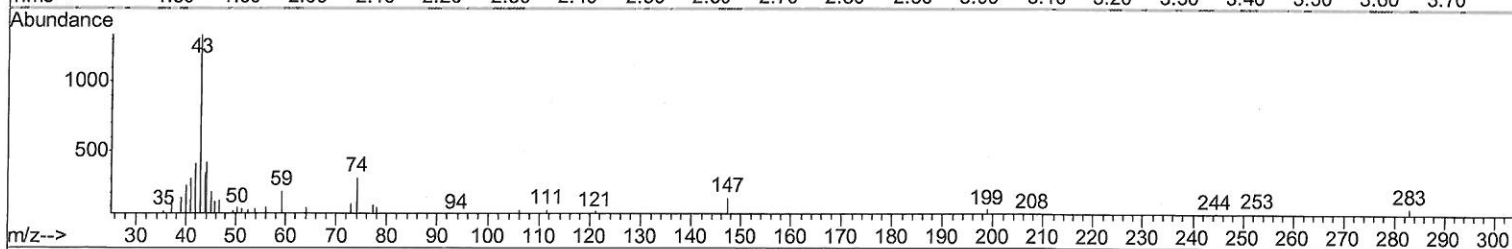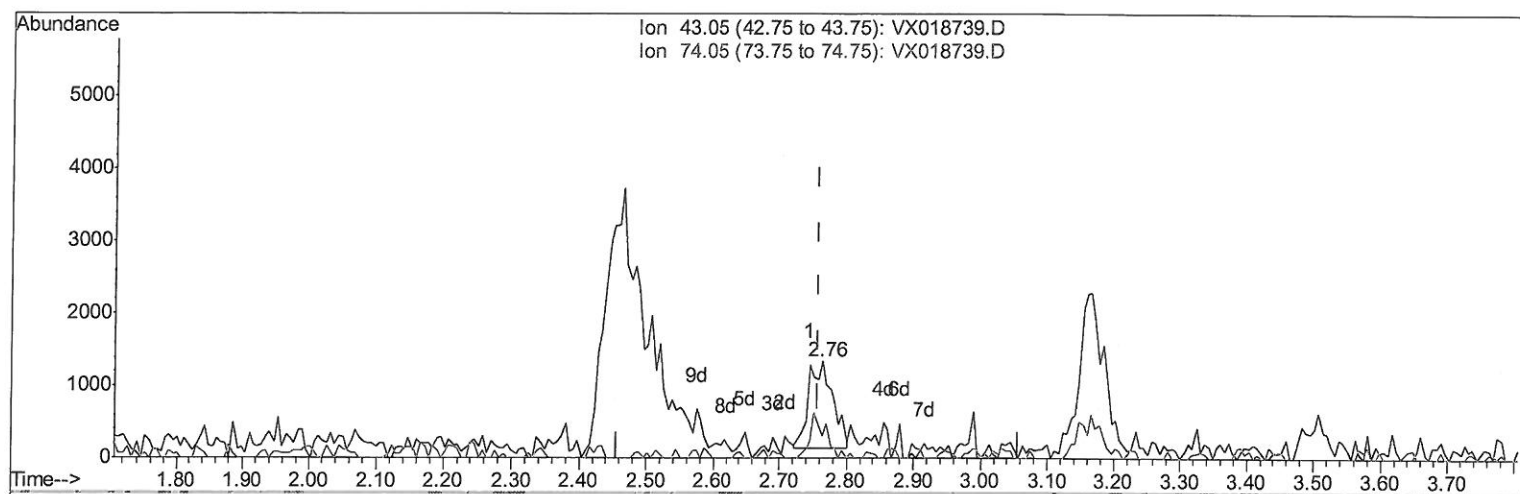

TIC: VX018739.D

(15) Methyl Acetate (T)

2.764min (+0.007) 0.44ug/L m

response 3027

Ion	Exp%	Act%
-----	------	------

43.05	100	100
-------	-----	-----

74.05	27.40	33.14#
-------	-------	--------

0.00	0.00	0.00
------	------	------

0.00	0.00	0.00
------	------	------

7 MD
10/06/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100220\
 Data File : VX018739.D
 Acq On : 02 Oct 2020 10:55
 Operator : JC/SP
 Sample : VSTD00165
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD00165

Manual Integrations
 APPROVED

MMDadoda
 10/6/2020 1:25:19 PM

Quant Time: Oct 02 11:57:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 11:50:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	194294	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	177566	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	92932	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	10380	0.80	ug/L	0.00
7) Chloroethane-d5	1.70	69	8997	0.89	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.34	63	23685	0.88	ug/L	0.00
20) 2-Butanone-d5	4.56	46	26415	7.84	ug/L	0.00
24) Chloroform-d	5.14	84	26653	0.99	ug/L	0.00
26) 1,2-Dichloroethane-d4	6.03	65	15935	1.05	ug/L	0.00
32) Benzene-d6	6.05	84	43305	0.92	ug/L	0.00
36) 1,2-Dichloropropane-d6	7.37	67	12751	0.88	ug/L	0.00
41) Toluene-d8	8.70	98	41966	0.93	ug/L	0.00
45) trans-1,3-Dichloropropene-	8.99	79	7050	1.08	ug/L	0.00
48) 2-Hexanone-d5	9.43	63	18753	7.25	ug/L	0.00
59) 1,1,2,2-Tetrachloroethane-	11.23	84	9627	0.86	ug/L	0.00
65) 1,2-Dichlorobenzene-d4	12.36	152	15594	0.89	ug/L	0.00

Target Compounds

					Qvalue	
2) Dichlorodifluoromethane	1.18	85	12799	0.620	ug/L	97
3) Chloromethane	1.31	50	9583	0.580	ug/L	84
5) Vinyl chloride	1.39	62	10409	0.623	ug/L	95
6) Bromomethane	1.64	94	5718	0.590	ug/L	88
8) Chloroethane	1.72	64	6141	0.653	ug/L	86
9) Trichlorofluoromethane	1.92	101	21828	0.784	ug/L	95
10) 1,1,2-Trichloro-1,2,2-trif	2.37	101	9853	0.668	ug/L	87
12) 1,1-Dichloroethene	2.36	96	9042	0.661	ug/L	89
13) Acetone	2.46	43	15700m	6.564	ug/L	} 99
14) Carbon disulfide	2.55	76	28583	0.586	ug/L	
15) Methyl Acetate	2.76	43	3027m	0.435	ug/L	
16) Methylene chloride	2.83	84	12740	0.667	ug/L	91
17) Methyl tert-butyl Ether	3.17	73	23643	0.646	ug/L	96
18) trans-1,2-Dichloroethene	3.15	96	10204	0.656	ug/L	83
19) 1,1-Dichloroethane	3.67	63	17878	0.646	ug/L #	96
21) 2-Butanone	4.65	43	20220	5.010	ug/L #	67
22) cis-1,2-Dichloroethene	4.56	96	10181	0.628	ug/L #	94
23) Bromochloromethane	4.98	128	5803	0.763	ug/L	77
25) Chloroform	5.17	83	19297	0.639	ug/L	96
27) 1,2-Dichloroethane	6.16	62	15123	0.774	ug/L #	89
29) 1,1,1-Trichloroethane	5.46	97	20277	0.739	ug/L	97
30) Cyclohexane	5.55	56	13879	0.607	ug/L	99
31) Carbon tetrachloride	5.74	117	19128	0.754	ug/L	100
33) Benzene	6.11	78	35247	0.615	ug/L	100
34) Trichloroethene	7.19	95	10935	0.647	ug/L	92
35) Methylcyclohexane	7.44	83	14702	0.623	ug/L	97
37) 1,2-Dichloropropane	7.48	63	8799	0.613	ug/L #	93
38) Bromodichloromethane	7.87	83	14723	0.720	ug/L	94
39) cis-1,3-Dichloropropene	8.42	75	13537	0.605	ug/L	96
40) 4-Methyl-2-pentanone	8.62	43	48852	5.311	ug/L	97

MD
10/06/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100220\
 Data File : VX018739.D
 Acq On : 02 Oct 2020 10:55
 Operator : JC/SP
 Sample : VSTD00165
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD00165

Manual Integrations
 APPROVED

MMDadoda
 10/6/2020 1:25:19 PM

Quant Time: Oct 02 11:57:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 11:50:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

42) Toluene	8.76	91	37880	0.608	ug/L	96
43) 1,3,5-Trimethylbenzene	11.49	105	32370	0.567	ug/L	99
44) 1,2,4-Trimethylbenzene	11.79	105	31881	0.547	ug/L	94
46) trans-1,3-Dichloropropene	9.02	75	13600	0.681	ug/L	88
47) 1,1,2-Trichloroethane	9.20	97	6844	0.631	ug/L	93
49) Tetrachloroethene	9.32	164	9913	0.724	ug/L	87
50) 2-Hexanone	9.48	43	35894	5.449	ug/L	97
51) Dibromochloromethane	9.56	129	9987	0.666	ug/L	91
52) 1,2-Dibromoethane	9.65	107	6553	0.622	ug/L	82
53) Chlorobenzene	10.12	112	26961	0.656	ug/L	98
54) Ethylbenzene	10.23	91	41928	0.612	ug/L	98
55) m,p-xylene	10.34	106	15223	0.584	ug/L	96
56) o-xylene	10.68	106	14960	0.593	ug/L	96
57) Styrene	10.70	104	24682	0.582	ug/L	100
58) Isopropylbenzene	11.00	105	39501	0.581	ug/L	93
60) 1,1,2,2-Tetrachloroethane	11.25	83	7207	0.605	ug/L #	93
62) Bromoform	10.84	173	5748	0.667	ug/L	98
63) 1,3-Dichlorobenzene	12.01	146	21534	0.651	ug/L	94
64) 1,4-Dichlorobenzene	12.08	146	21063	0.637	ug/L	99
66) 1,2-Dichlorobenzene	12.38	146	20737	0.667	ug/L	96
67) 1,2-Dibromo-3-chloropropan	12.98	75	1668	0.615	ug/L	94
68) 1,3,5-Trichlorobenzene	13.15	180	16274	0.659	ug/L	97
69) 1,2,4-trichlorobenzene	13.63	180	12581	0.580	ug/L #	94
70) Naphthalene	13.82	128	20260	0.518	ug/L	97
71) 1,2,3-Trichlorobenzene	14.01	180	11565	0.572	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed