

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018759.D
Acq On : 02 Oct 2020 19:54
Operator : JC/SP
Sample : L4239-06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
BG3N6

Manual Integrations
APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 08:17:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

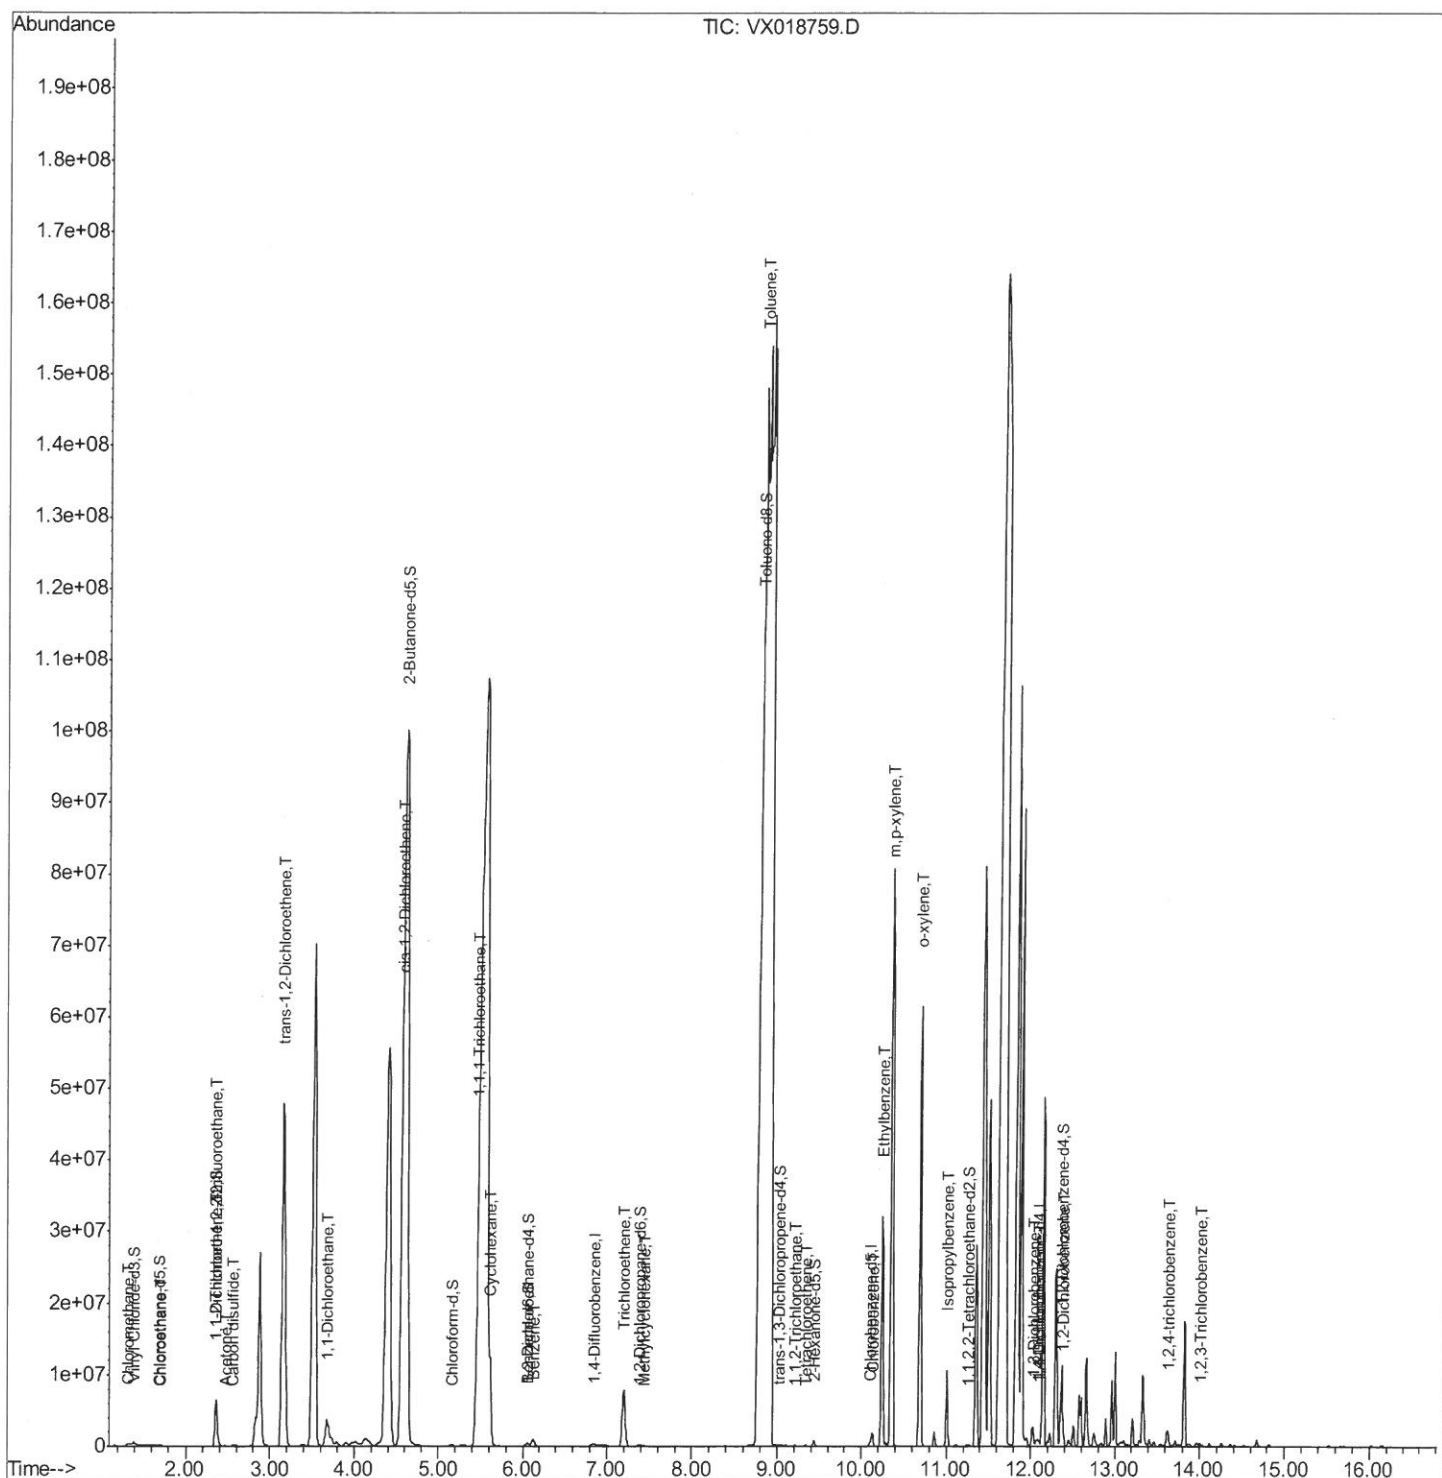

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018759.D
Acq On : 02 Oct 2020 19:54
Operator : JC/SP
Sample : L4239-06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
BG3N6

Manual Integrations
APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

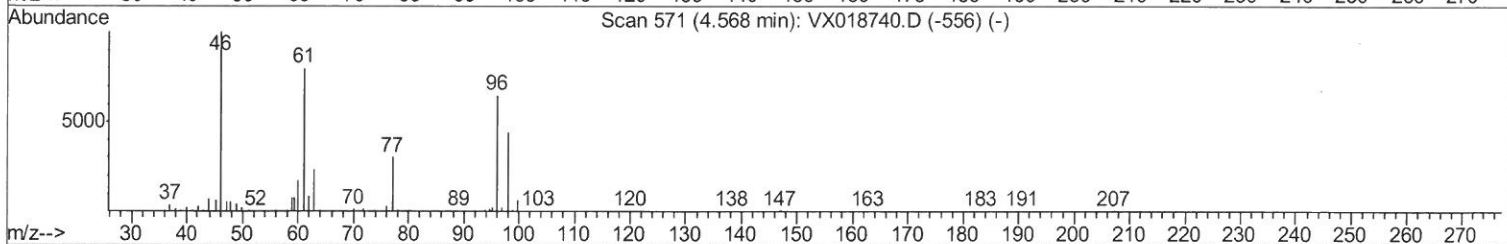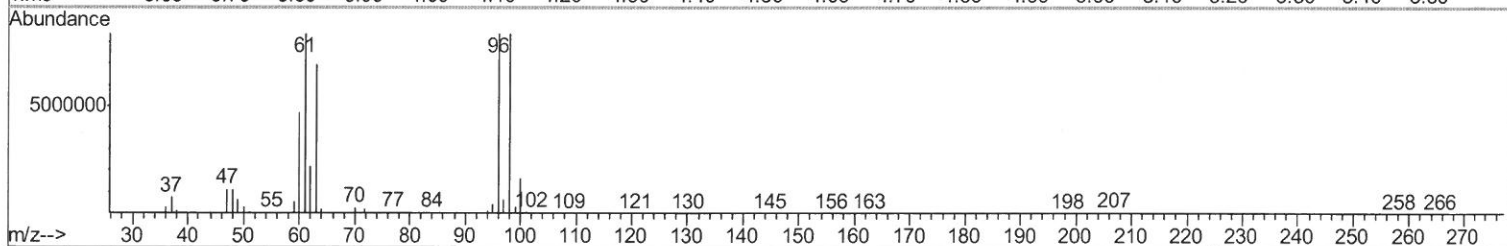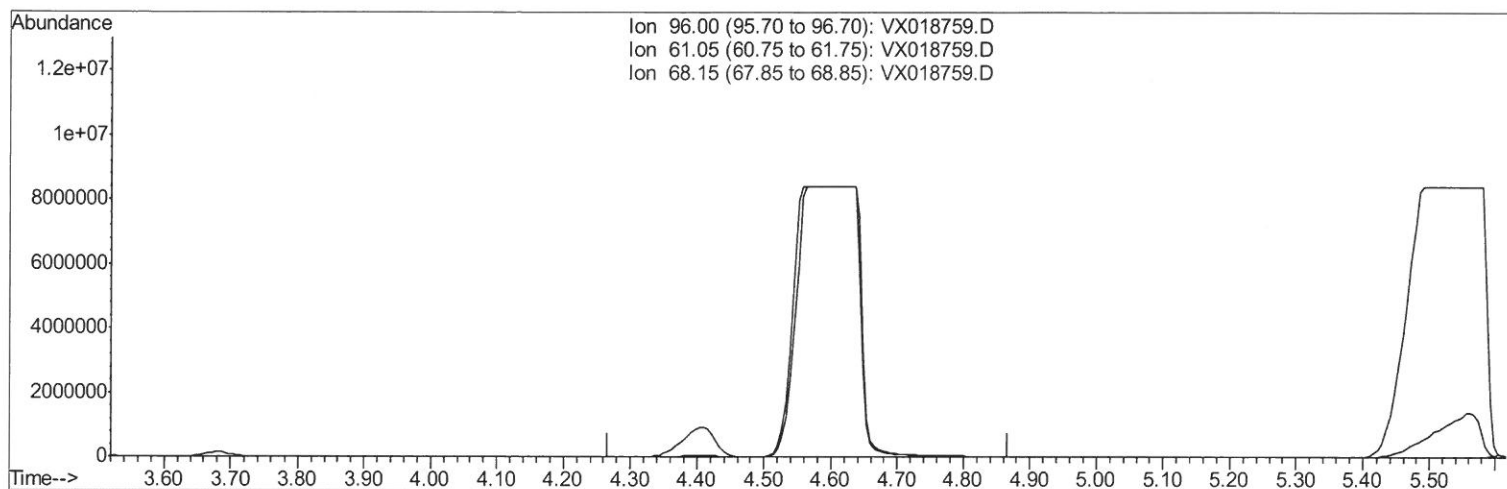

(22) cis-1,2-Dichloroethene (T)

4.568min (-4.568) 0.00ug/L

response 0

Ion	Exp%	Act%
96.00	100	0.00
61.05	123.10	0.00#
68.15	0.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018759.D
Acq On : 02 Oct 2020 19:54
Operator : JC/SP
Sample : L4239-06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
BG3N6

Manual Integrations
APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

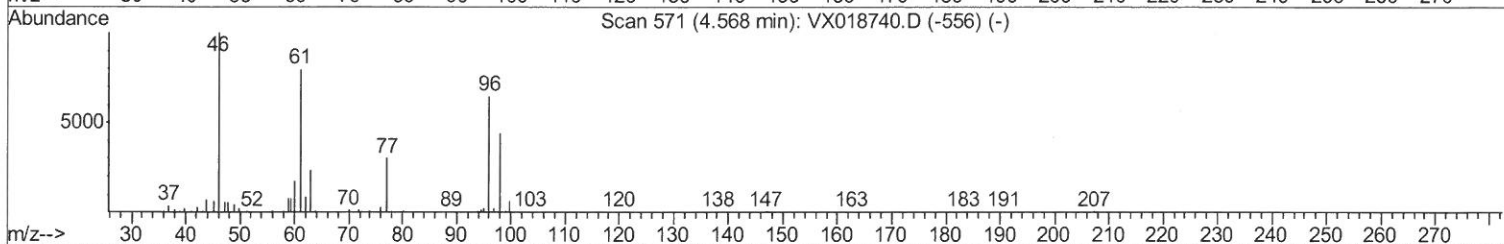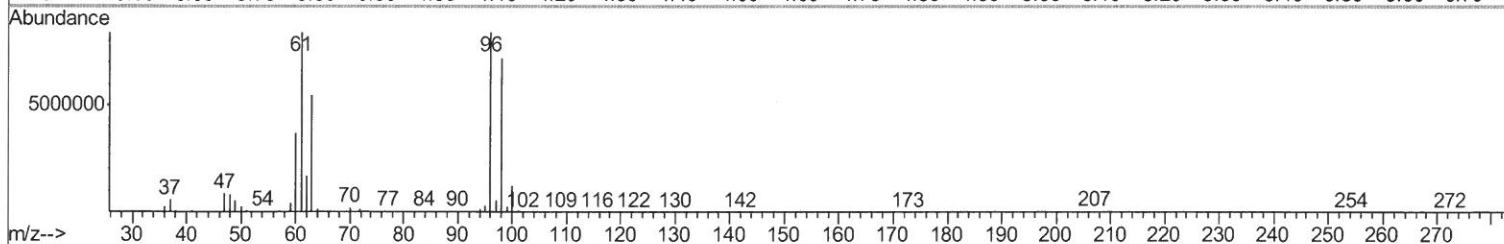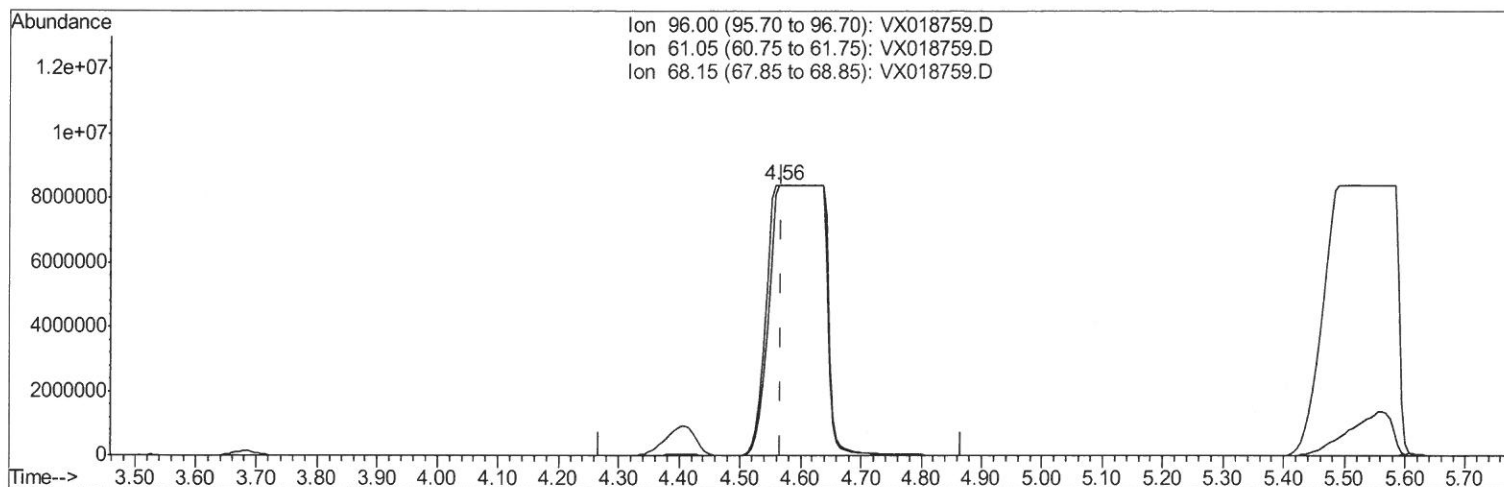

TIC: VX018759.D

(22) cis-1,2-Dichloroethene (T)

4.562min (-0.006) 2753.05ug/L m

response 52271878

Ion	Exp%	Act%
96.00	100	100
61.05	123.10	100.00
68.15	0.50	0.01#
0.00	0.00	0.00

7 MD
10/20/20

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018759.D
Acq On : 02 Oct 2020 19:54
Operator : JC/SP
Sample : L4239-06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
BG3N6

Manual Integrations
APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

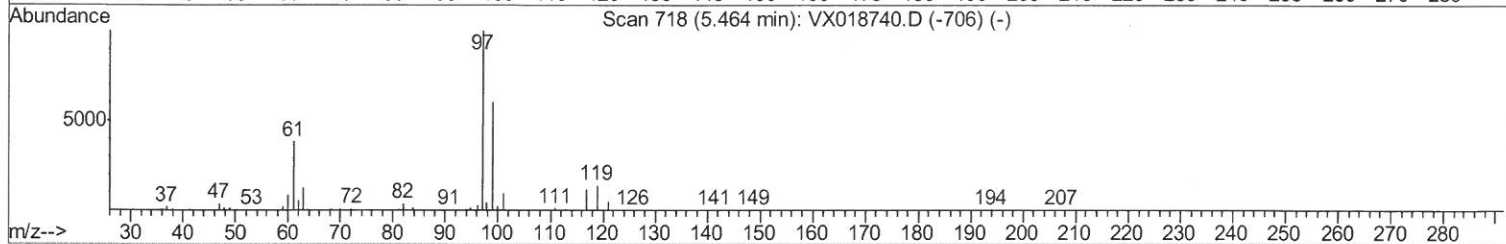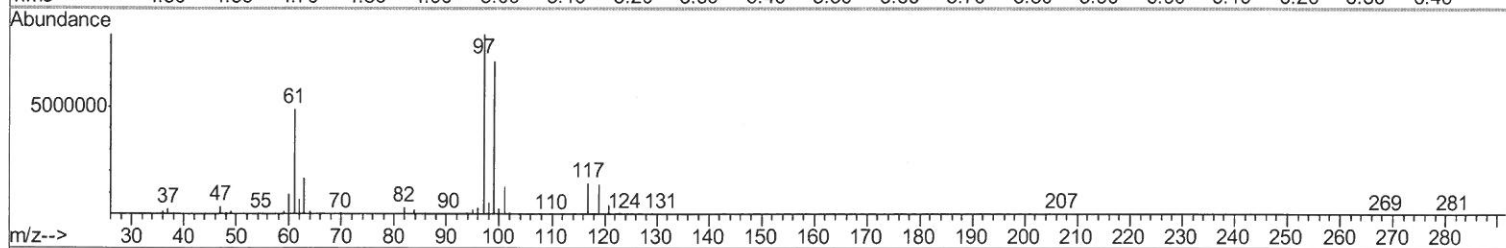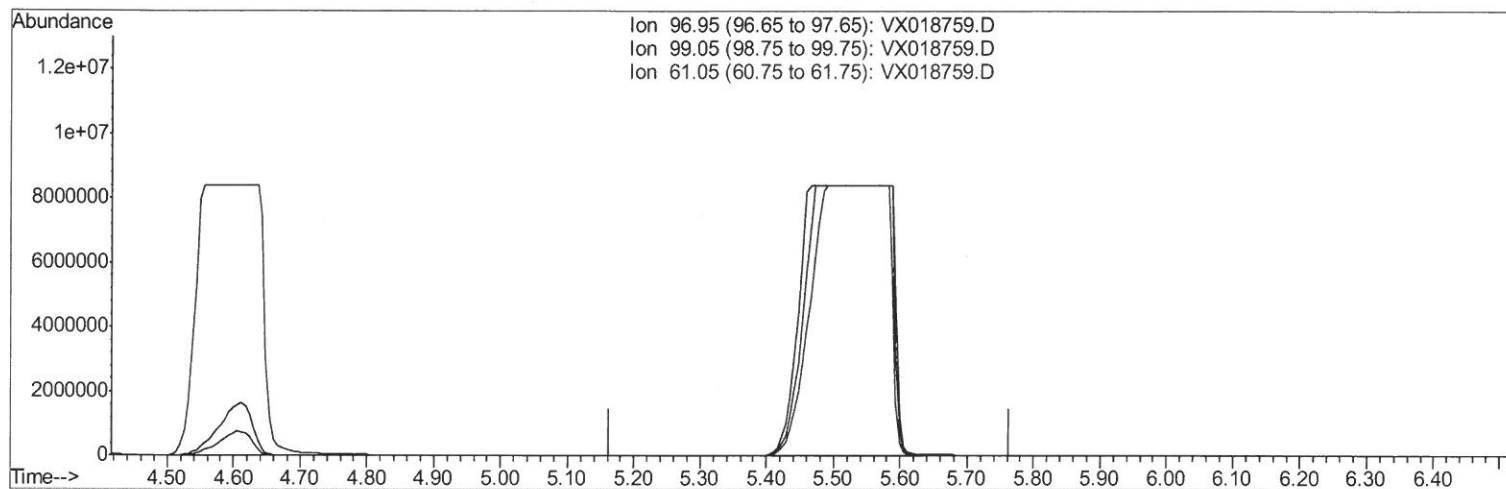

(29) 1,1,1-Trichloroethane (T)

5.464min (-5.464) 0.00ug/L

response 0

Ion	Exp%	Act%
96.95	100	0.00
99.05	64.10	0.00#
61.05	41.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018759.D
Acq On : 02 Oct 2020 19:54
Operator : JC/SP
Sample : L4239-06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
BG3N6

Manual Integrations
APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

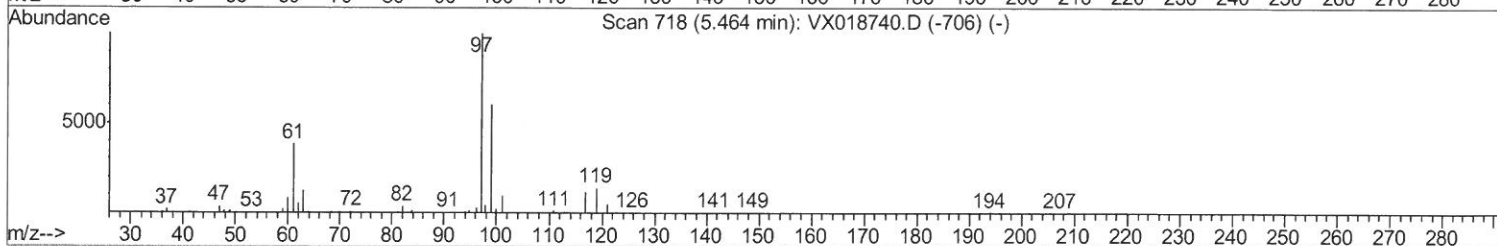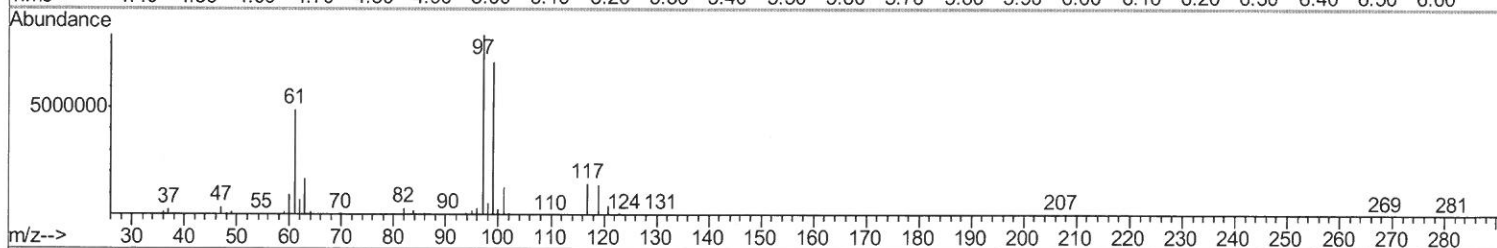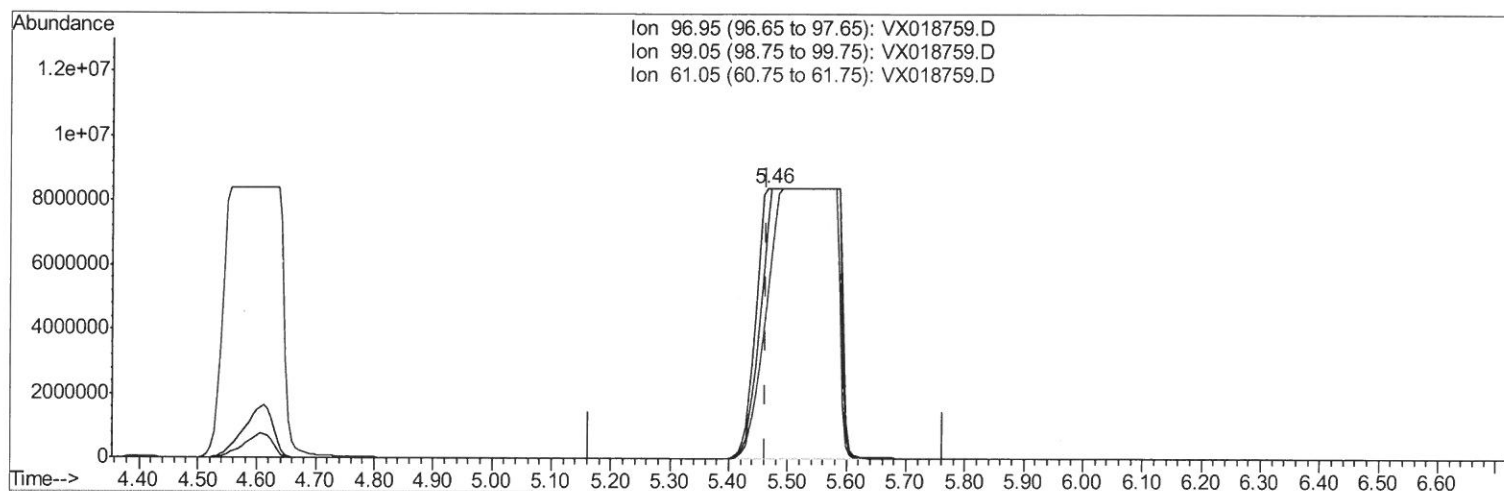

TIC: VX018759.D

(29) 1,1,1-Trichloroethane (T)

5.465min (+0.001) 2050.17ug/L m

response 76286711

Ion Exp% Act%

96.95 100 100

99.05 64.10 0.00#

61.05 41.60 0.00#

0.00 0.00 0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018759.D
Acq On : 02 Oct 2020 19:54
Operator : JC/SP
Sample : L4239-06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
BG3N6

Manual Integrations
APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

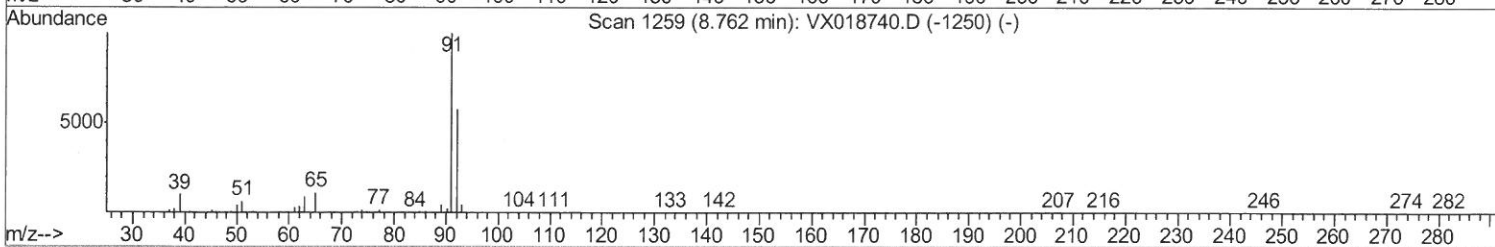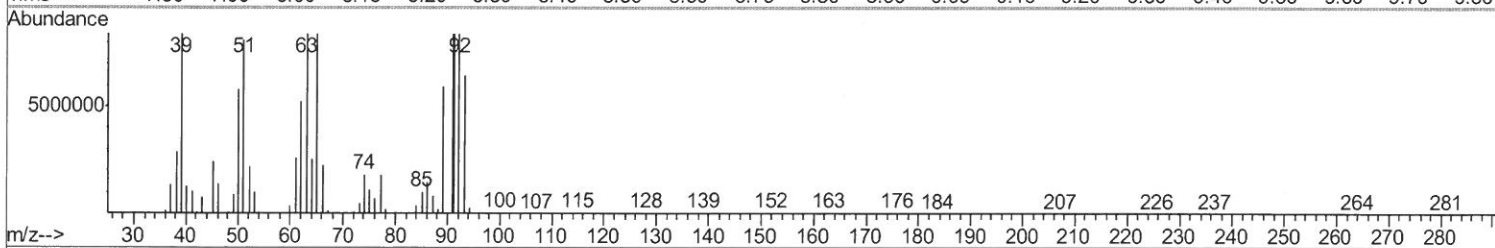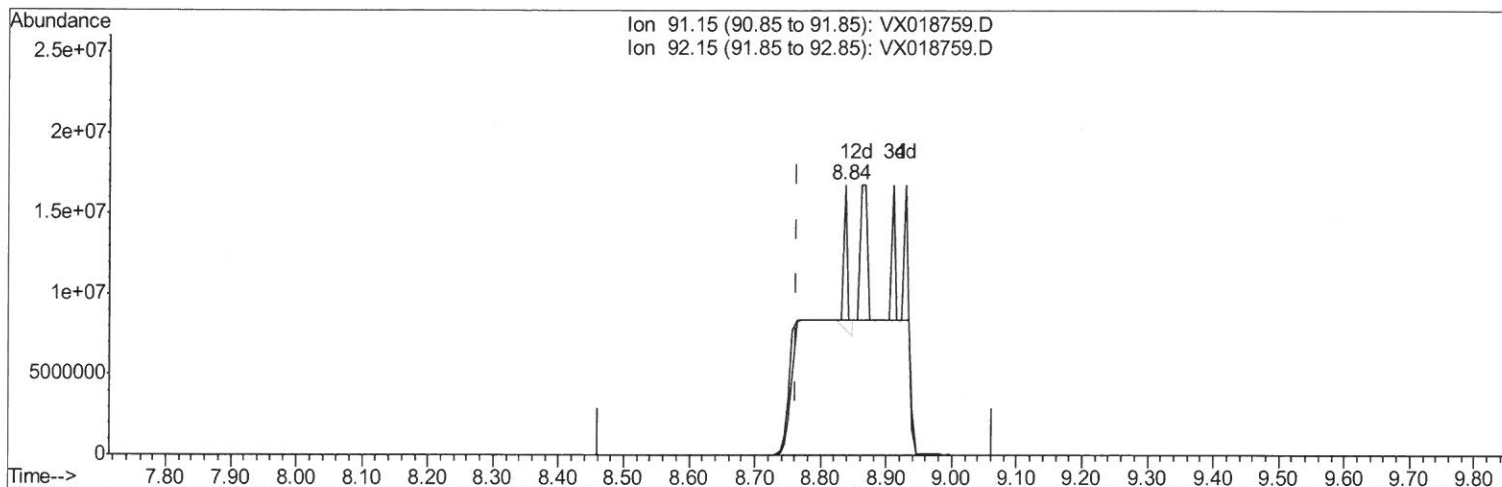

TIC: VX018759.D

(42) Toluene (T)

8.836min (+0.074) 52.26ug/L

response 3766622

Ion	Exp%	Act%
91.15	100	100
92.15	57.60	50.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
 Data File : VX018759.D
 Acq On : 02 Oct 2020 19:54
 Operator : JC/SP
 Sample : L4239-06
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1




Instrument :
 MSVOA_X
ClientSampleId :
 BG3N6

Manual Integrations
APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 14:11:08 2020
 Response via : Initial Calibration

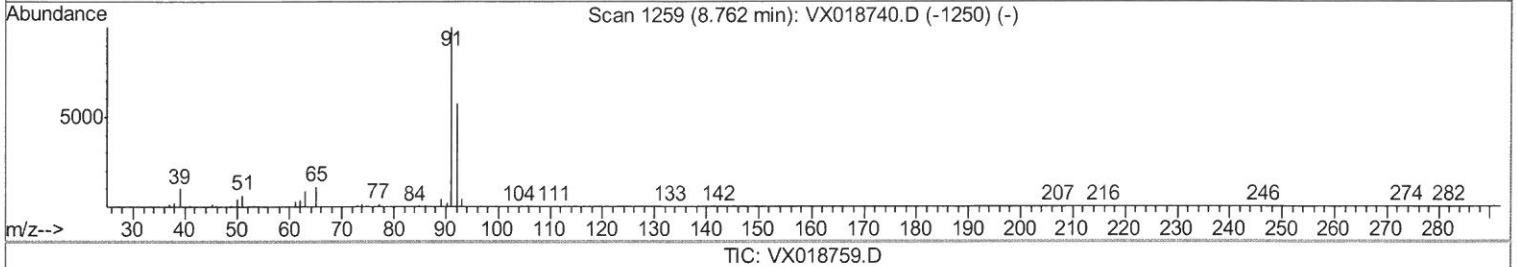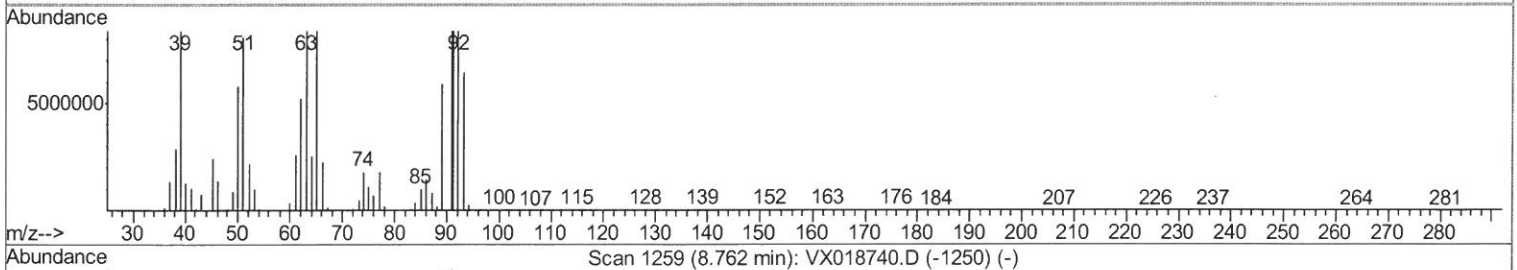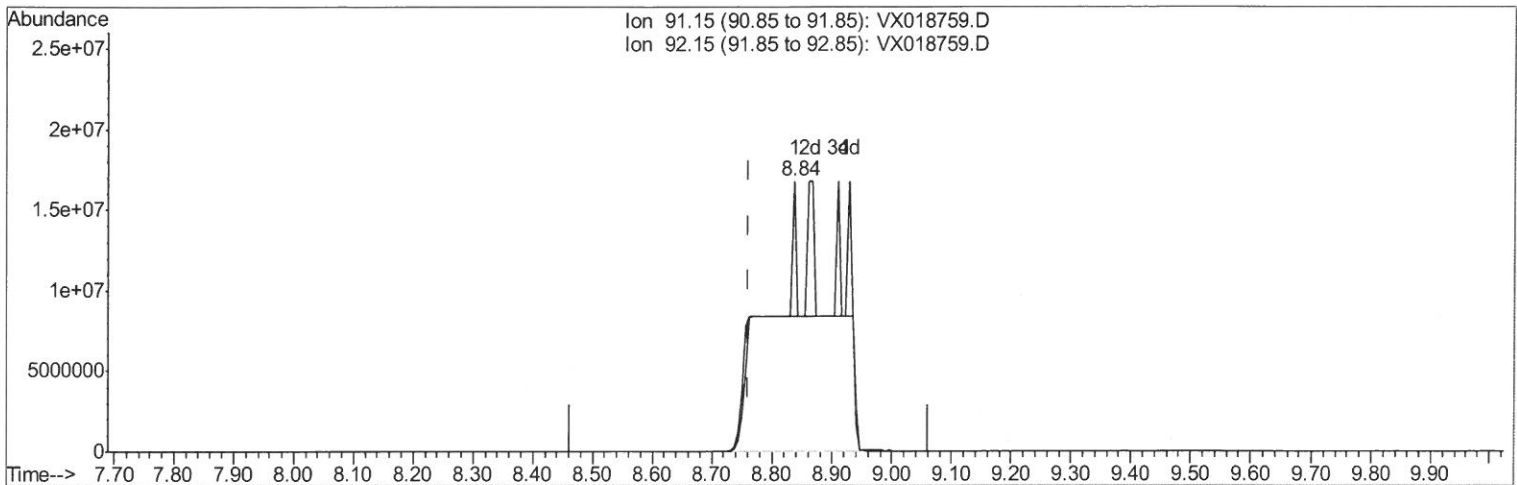

(42) Toluene (T)

8.836min (+0.074) 1530.16ug/L m

response 110287162

Ion	Exp%	Act%
91.15	100	100
92.15	57.60	100.00#
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
10/20/20

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018759.D
Acq On : 02 Oct 2020 19:54
Operator : JC/SP
Sample : L4239-06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1




Instrument :
MSVOA_X
ClientSampleId :
BG3N6

Manual Integrations APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

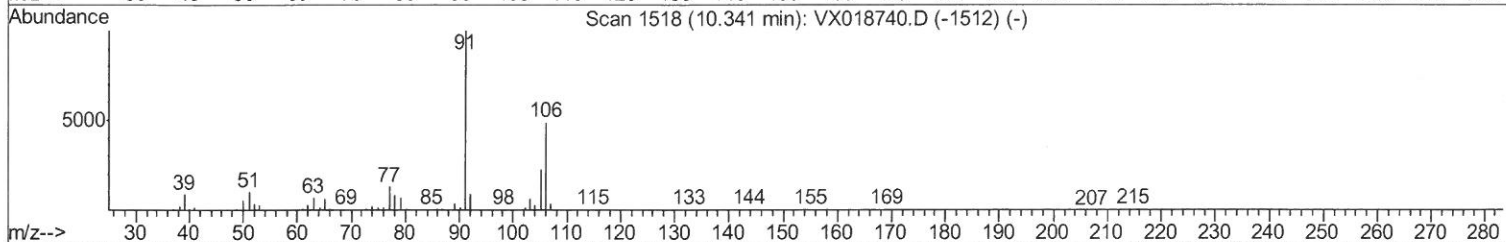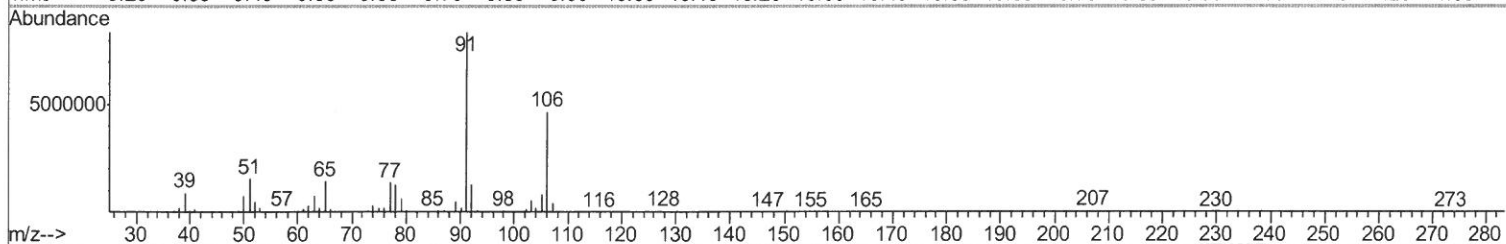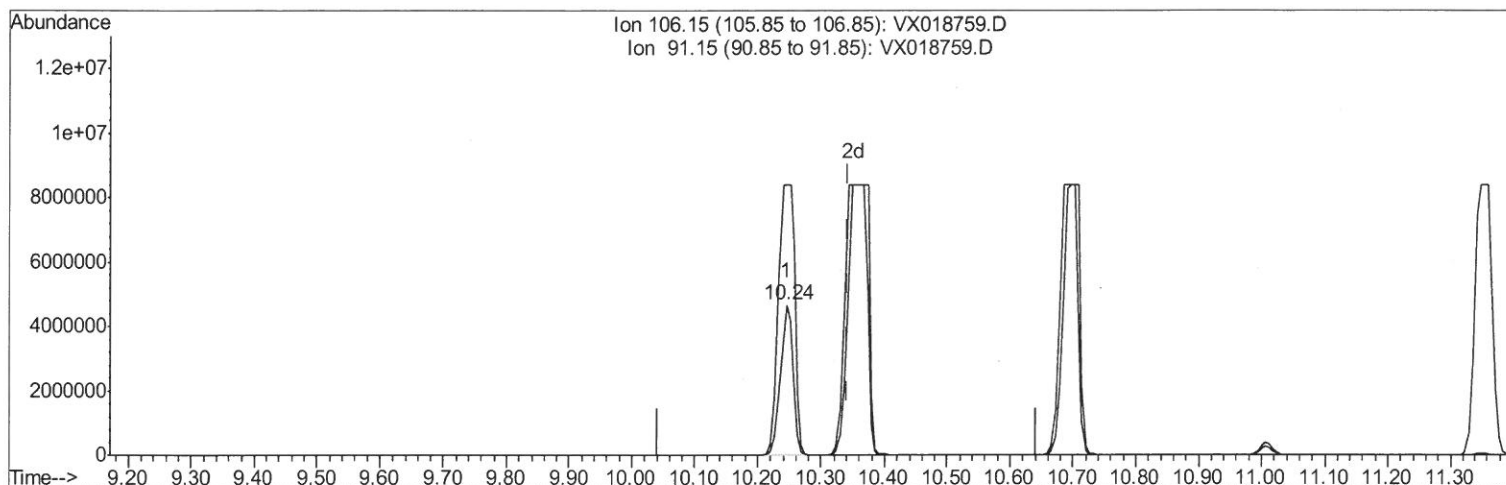

TIC: VX018759.D

(55) m,p-xylene (T)

10.244min (-0.097) 203.06ug/L

response 6399465

Ion	Exp%	Act%
106.15	100	100
91.15	204.80	179.68
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
 Data File : VX018759.D
 Acq On : 02 Oct 2020 19:54
 Operator : JC/SP
 Sample : L4239-06
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1




Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6

Manual Integrations
 APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 05:23:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 14:11:08 2020
 Response via : Initial Calibration

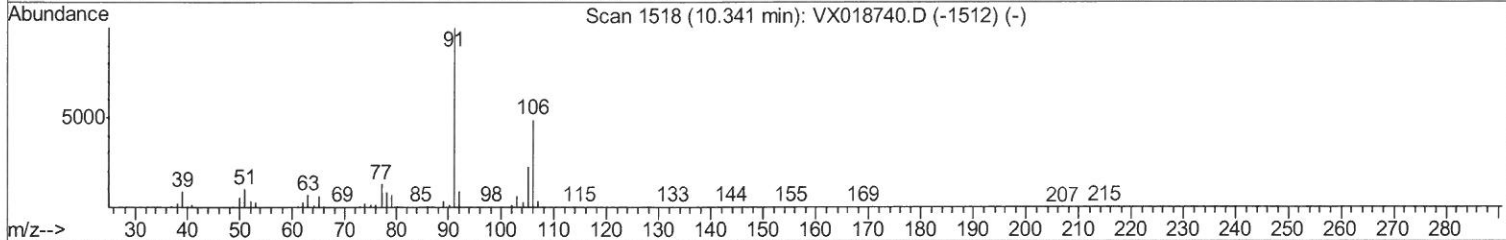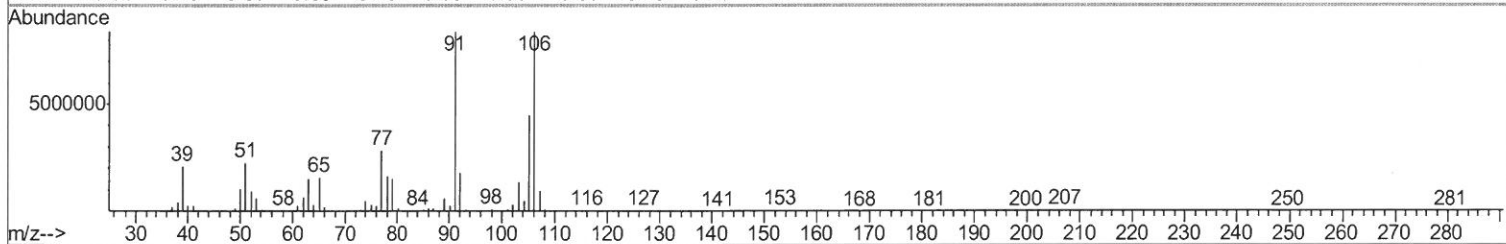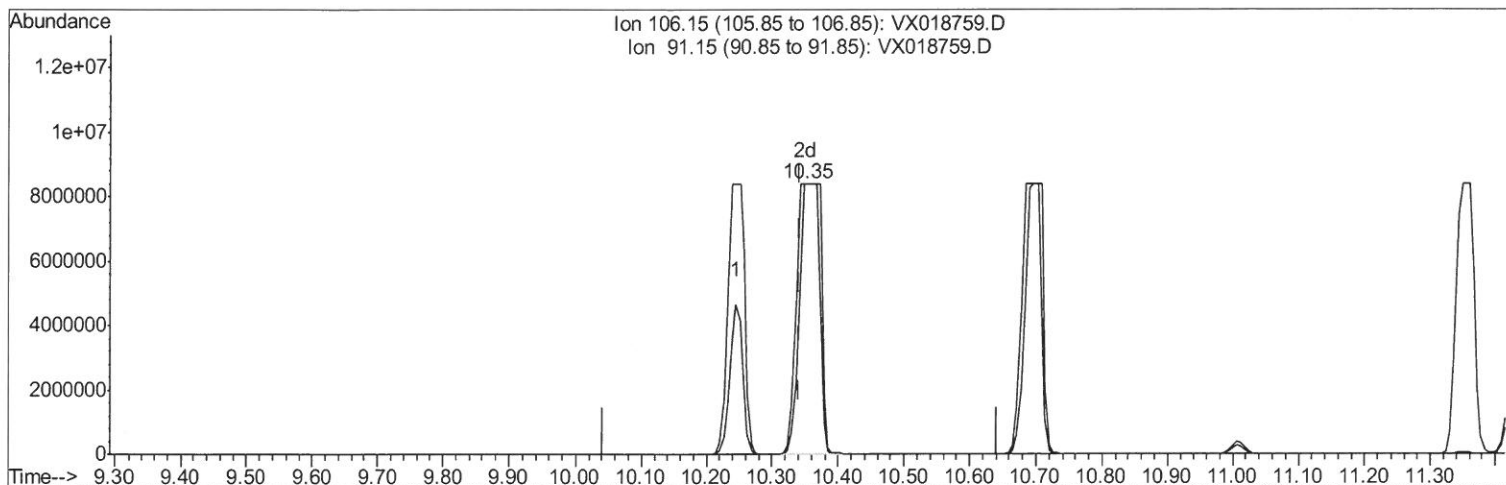

TIC: VX018759.D

(55) m,p-xylene (T)

10.348min (+0.007) 556.47ug/L m

response 17537531

Ion	Exp%	Act%
106.15	100	100
91.15	204.80	100.00#
0.00	0.00	0.00
0.00	0.00	0.00

7 MB
 10/20/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
 Data File : VX018759.D
 Acq On : 02 Oct 2020 19:54
 Operator : JC/SP
 Sample : L4239-06
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6

Manual Integrations
 APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 08:17:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 14:11:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.84	114	345172	5.00	ug/L	0.01
28) Chlorobenzene-d5	10.10	117	314542	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.09	152	164120	5.00	ug/L	0.02

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	112371	5.57	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	111.40%		
7) Chloroethane-d5	1.70	69	80585	5.11	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	102.20%		
11) 1,1-Dichloroethene-d2	2.36	63	1527568	33.58	ug/L	0.01
Spiked Amount 5.000	Range 60 - 125		Recovery =	671.60%#		
20) 2-Butanone-d5	4.62	46	280859	53.10	ug/L	0.07
Spiked Amount 50.000	Range 40 - 130		Recovery =	106.20%		
24) Chloroform-d	5.16	84	216300	4.43	ug/L	0.02
Spiked Amount 5.000	Range 70 - 125		Recovery =	88.60%		
26) 1,2-Dichloroethane-d4	6.04	65	124269	4.17	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	83.40%		
32) Benzene-d6	6.06	84	437238	5.59	ug/L	0.01
Spiked Amount 5.000	Range 70 - 125		Recovery =	111.80%		
36) 1,2-Dichloropropane-d6	7.38	67	133078	5.89	ug/L	0.01
Spiked Amount 5.000	Range 60 - 140		Recovery =	117.80%		
41) Toluene-d8	8.80	98	408353	5.30	ug/L	0.10
Spiked Amount 5.000	Range 70 - 130		Recovery =	106.00%		
45) trans-1,3-Dichloropropene-	9.02	79	55561	4.57	ug/L	0.03
Spiked Amount 5.000	Range 55 - 130		Recovery =	91.40%		
48) 2-Hexanone-d5	9.44	63	233765	57.37	ug/L	0.01
Spiked Amount 50.000	Range 45 - 130		Recovery =	114.74%		
59) 1,1,2,2-Tetrachloroethane-	11.26	84	93960	5.11	ug/L	0.02
Spiked Amount 5.000	Range 65 - 120		Recovery =	102.20%		
65) 1,2-Dichlorobenzene-d4	12.37	152	157532	5.20	ug/L	0.01
Spiked Amount 5.000	Range 80 - 120		Recovery =	104.00%		

Target Compounds

					Ovalue	
3) Chloromethane	1.31	50	23141	1.386	ug/L #	81
8) Chloroethane	1.72	64	185579	16.428	ug/L #	61
10) 1,1,2-Trichloro-1,2,2-trif	2.36	101	11202	0.578	ug/L #	55
12) 1,1-Dichloroethene	2.36	96	2470125	143.659	ug/L #	54
13) Acetone	2.47	43	61446	21.280	ug/L	91
14) Carbon disulfide	2.56	76	573402	10.656	ug/L	100
18) trans-1,2-Dichloroethene	3.15	96	1223369	66.448	ug/L	90
19) 1,1-Dichloroethane	3.68	63	4789239	146.326	ug/L	97
22) cis-1,2-Dichloroethene	4.56	96	52271878m	2753.050	ug/L	94
29) 1,1,1-Trichloroethane	5.46	97	76286711m	2050.168	ug/L	100
30) Cyclohexane	5.61	56	6081352	235.640	ug/L	97
33) Benzene	6.12	78	1171217	17.781	ug/L	97
34) Trichloroethene	7.20	95	3453251	177.566	ug/L	75
35) Methylcyclohexane	7.45	83	28780	1.044	ug/L #	97
42) Toluene	8.84	91	110287162m	1530.162	ug/L	92
47) 1,1,2-Trichloroethane	9.21	97	29681	2.383	ug/L	
49) Tetrachloroethene	9.34	164	14243	0.838	ug/L	

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
 Data File : VX018759.D
 Acq On : 02 Oct 2020 19:54
 Operator : JC/SP
 Sample : L4239-06
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6

Manual Integrations
 APPROVED

MMDadoda

10/6/2020 1:25:44 PM

Quant Time: Oct 03 08:17:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 14:11:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
53) Chlorobenzene	10.13	112	838378	17.005	ug/L	94
54) Ethylbenzene	10.24	91	15097143	186.855	ug/L #	82
55) m,p-xylene	10.35	106	17537531m	556.470	ug/L	
56) o-xylene	10.70	106	14083704	483.570	ug/L #	26
58) Isopropylbenzene	11.01	105	5661438	69.435	ug/L	98
63) 1,3-Dichlorobenzene	12.04	146	37614	0.943	ug/L	96
64) 1,4-Dichlorobenzene	12.10	146	158261	3.978	ug/L	94
66) 1,2-Dichlorobenzene	12.38	146	600593	16.125	ug/L	98
69) 1,2,4-trichlorobenzene	13.63	180	318945	12.512	ug/L	94
71) 1,2,3-Trichlorobenzene	14.01	180	93516	4.077	ug/L	93

7 MD
10/22/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed