

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100220\
 Data File : VX018744.D
 Acq On : 02 Oct 2020 13:35
 Operator : JC/SP
 Sample : VX1002WBL01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK77

Quant Time: Oct 03 05:46:39 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 14:11:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	220436	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	209545	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	101831	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	52907	4.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.20%
7) Chloroethane-d5	1.70	69	41682	4.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.80%
11) 1,1-Dichloroethene-d2	2.34	63	97751	3.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.40%
20) 2-Butanone-d5	4.56	46	152224	45.07	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.14%
24) Chloroform-d	5.14	84	126964	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.40%
26) 1,2-Dichloroethane-d4	6.03	65	78812	4.14	ug/L	-0.01
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
32) Benzene-d6	6.04	84	222252	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.40%
36) 1,2-Dichloropropane-d6	7.37	67	64300	4.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.40%
41) Toluene-d8	8.70	98	204315	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.60%
45) trans-1,3-Dichloropropene-	8.99	79	31211	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
48) 2-Hexanone-d5	9.43	63	117239	43.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.38%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	52166	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.20%
65) 1,2-Dichlorobenzene-d4	12.36	152	82942	4.42	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.40%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	4810	0.361 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100220\
Data File : VX018744.D
Acq On : 02 Oct 2020 13:35
Operator : JC/SP
Sample : VX1002WBL01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK77

Quant Time: Oct 03 05:46:39 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

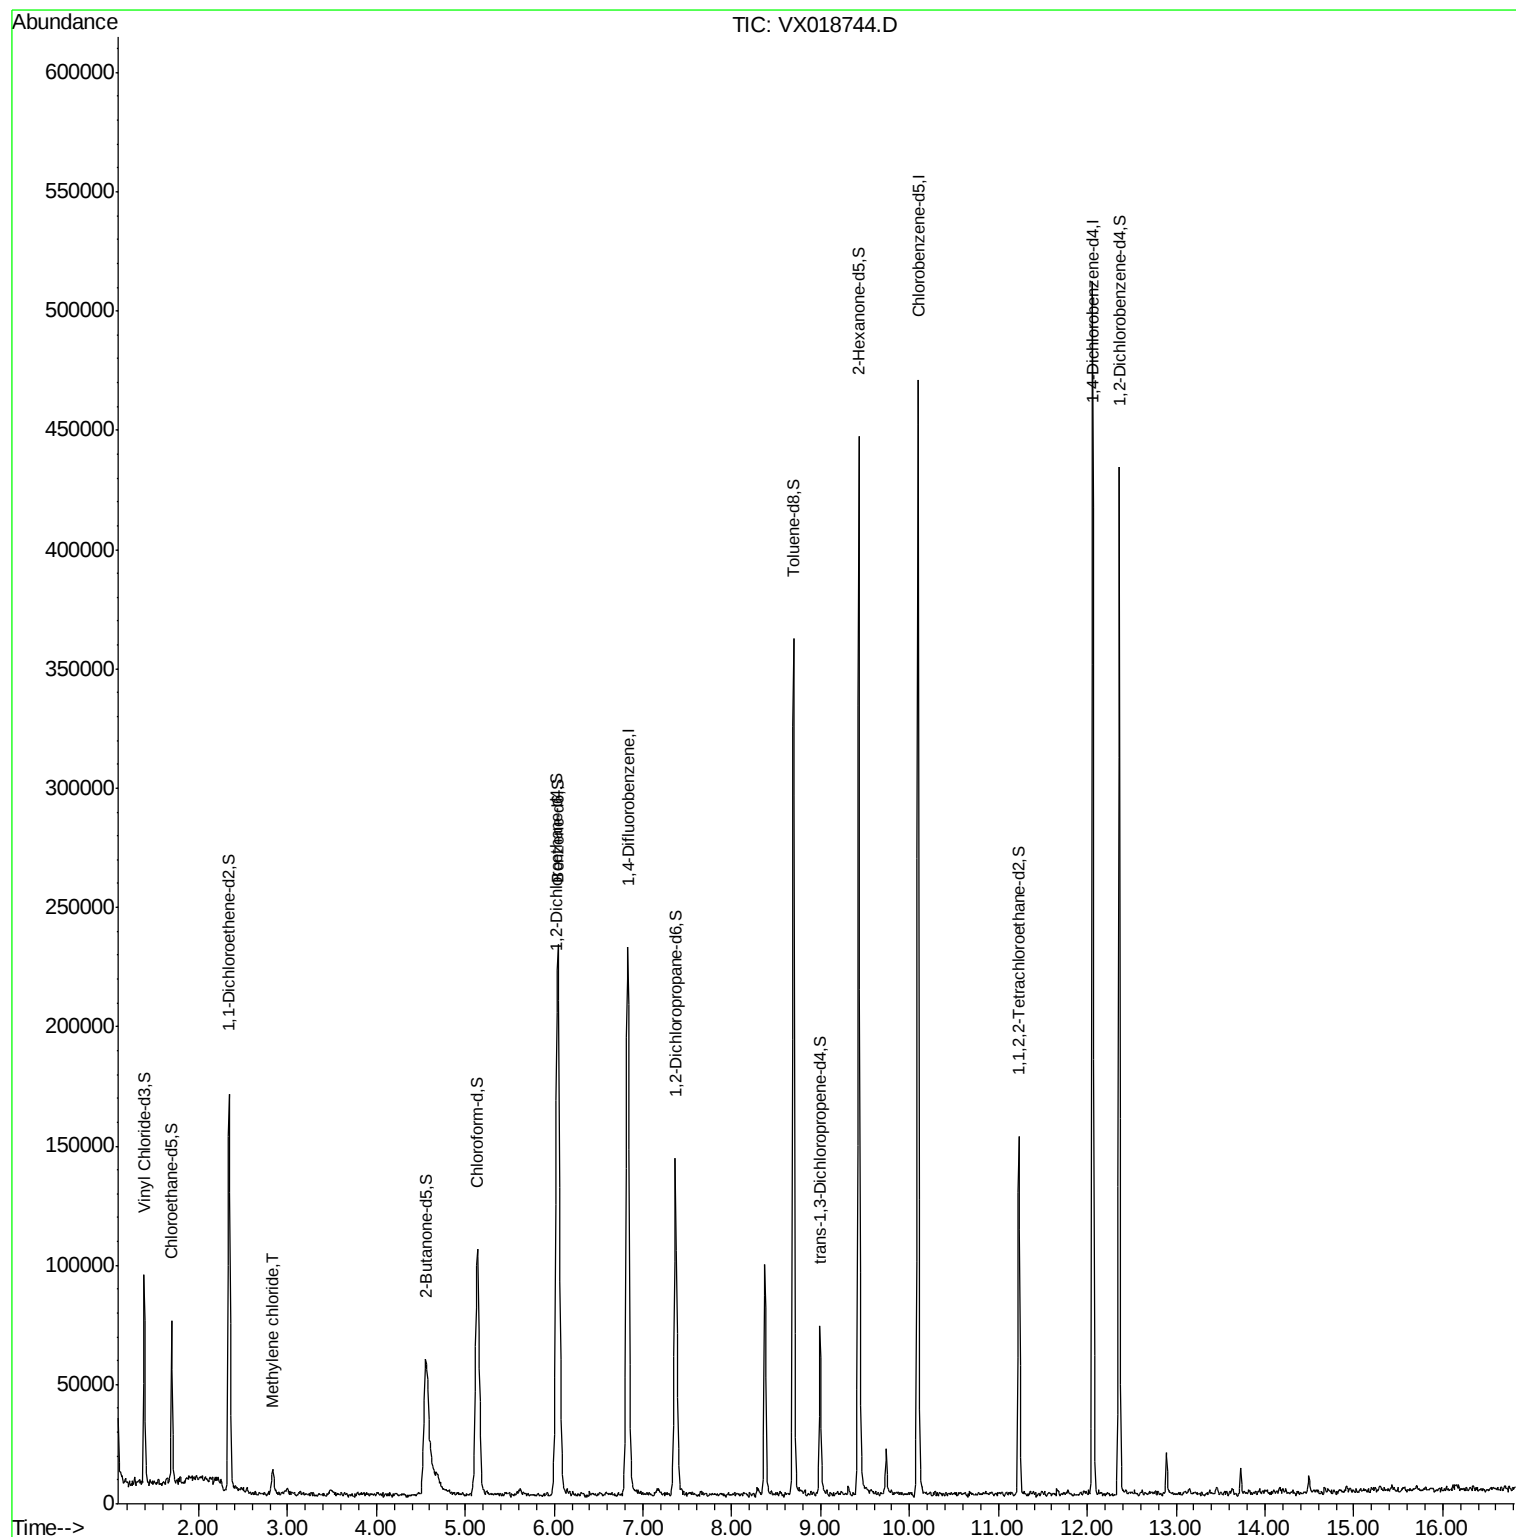

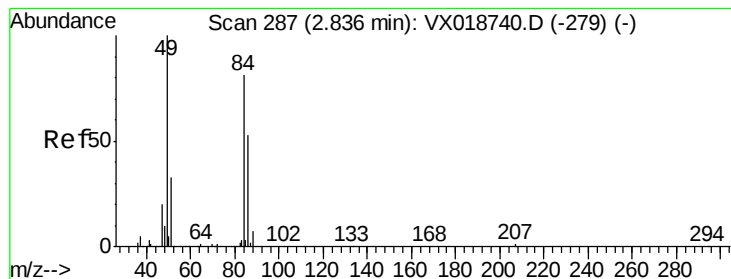

#16
 Methvlene chloride
 Concen: 0.361 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. -0.01 min
 Lab File: VX018744.D
 Acq: 02 Oct 2020 13:35

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK77

Tot Ion: 84 Resp: 4810
 Ion Ratio Lower Upper
 84 100
 86 69.7 45.6 84.8
 49 121.1 85.8 159.3

