

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100220\
 Data File : VX018748.D
 Acq On : 02 Oct 2020 15:27
 Operator : JC/SP
 Sample : L4208-06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK01

Quant Time: Oct 03 06:24:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 02 14:11:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	189750	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	182839	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	91111	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	51752	4.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.40%
7) Chloroethane-d5	1.70	69	43922	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.20%
11) 1,1-Dichloroethene-d2	2.34	63	98953	3.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.20%
20) 2-Butanone-d5	4.56	46	154041	52.98	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.96%
24) Chloroform-d	5.14	84	129961	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	6.03	65	80651	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	6.05	84	226320	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	7.37	67	67245	5.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.40%
41) Toluene-d8	8.70	98	216319	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
45) trans-1,3-Dichloropropene-	8.99	79	33255	4.70	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.00%
48) 2-Hexanone-d5	9.43	63	124783	52.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.36%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	51840	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
65) 1,2-Dichlorobenzene-d4	12.36	152	87249	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%


Target Compounds					Qvalue
16) Methylene chloride	2.84	84	4673	0.408 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100220\
Data File : VX018748.D
Acq On : 02 Oct 2020 15:27
Operator : JC/SP
Sample : L4208-06
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK01

Quant Time: Oct 03 06:24:17 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 02 14:11:08 2020
Response via : Initial Calibration

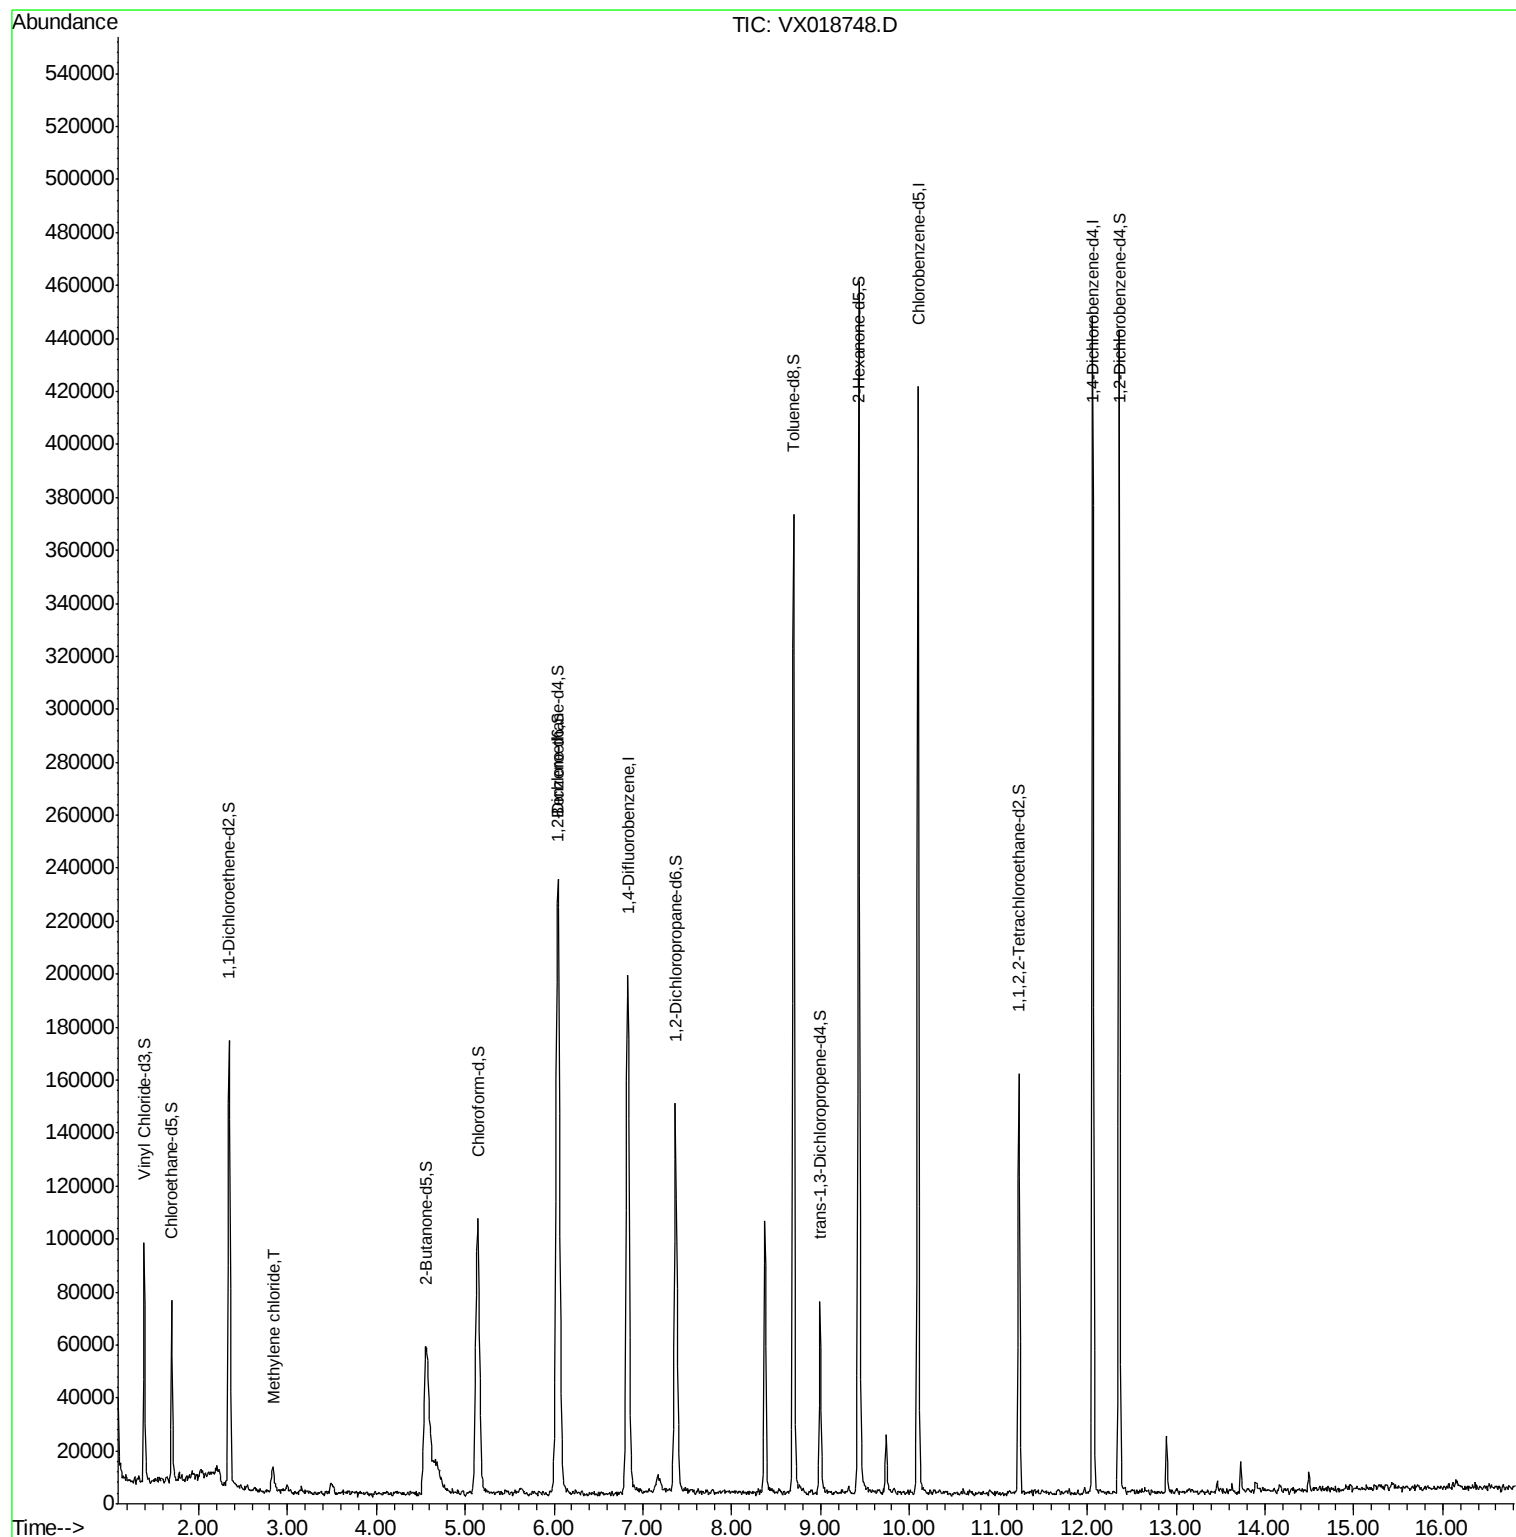

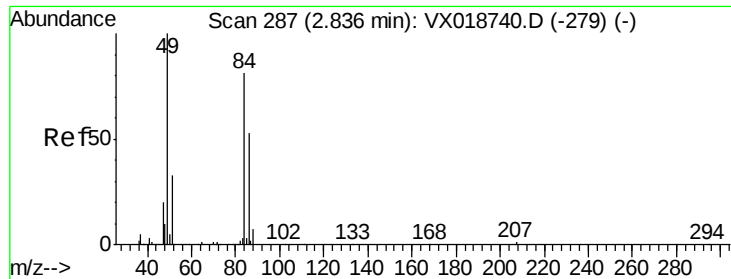

#16
Methylene chloride
Concen: 0.408 ug/L
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX018748.D
Acq: 02 Oct 2020 15:27

Instrument :
MSVOA_X
ClientSampleId :
VHBLK01

Tgt Ion: 84 Resp: 4673
Ion Ratio Lower Upper
84 100
86 59.3 45.6 84.8
49 115.4 85.8 159.3

