


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100220\
 Data File : VX018737.D
 Acq On : 02 Oct 2020 09:52
 Operator : JC/SP
 Sample : BFB76
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB76

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 02 14:11:08 2020

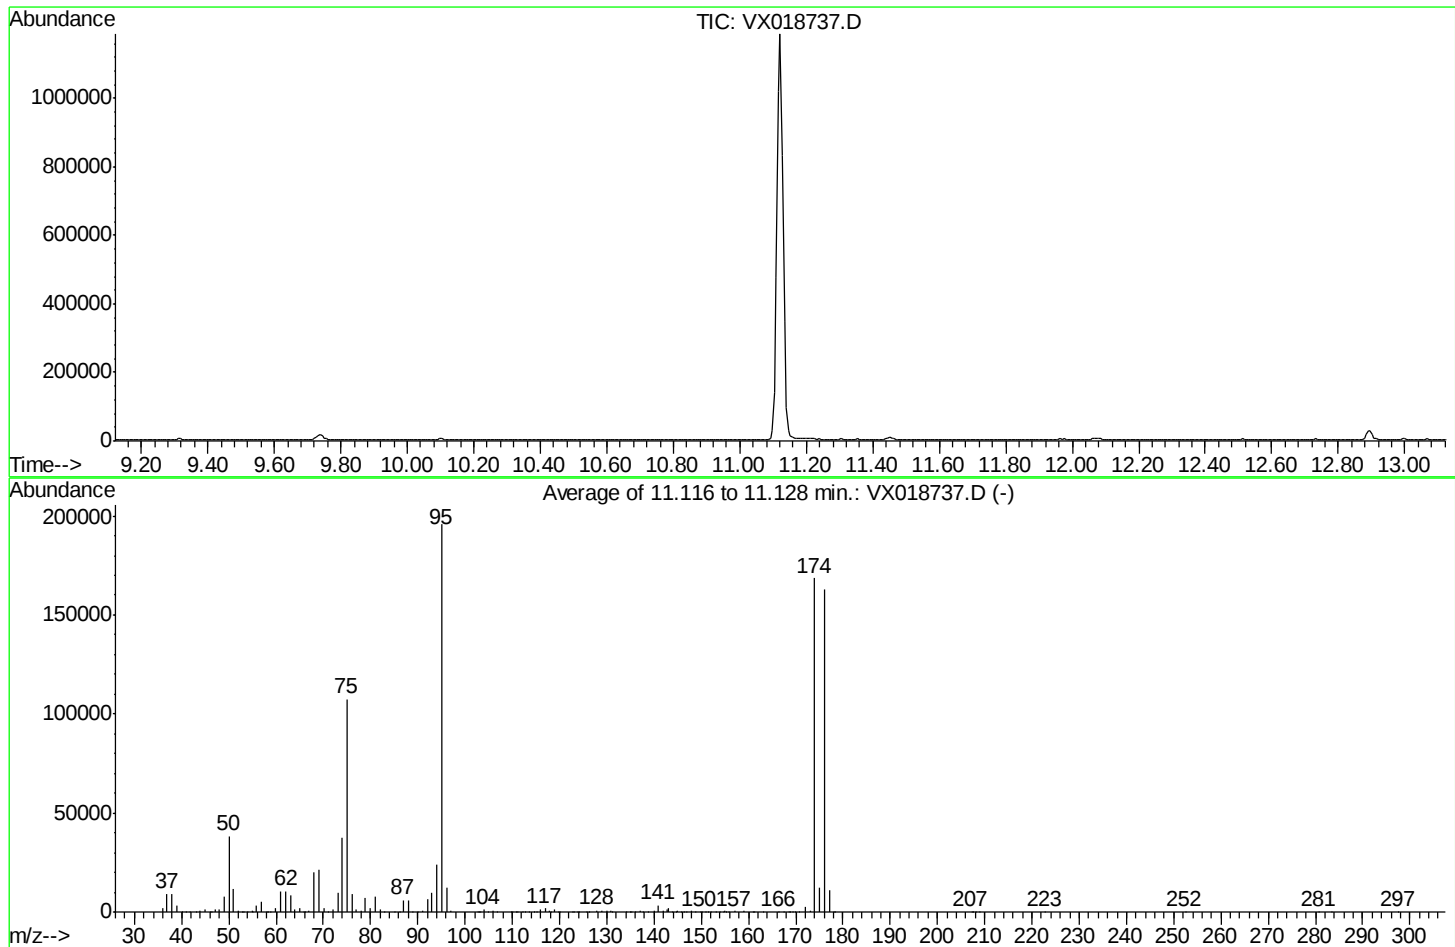

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	38439	PASS
75	95	30	80	54.9	107378	PASS
95	95	100	100	100.0	195754	PASS
96	95	5	9	6.3	12312	PASS
173	174	0.00	2	0.6	953	PASS
174	95	50	120	86.1	168490	PASS
175	174	5	9	7.4	12505	PASS
176	174	95	101	96.7	162922	PASS
177	176	5	9	6.6	10755	PASS

m/z	Abundance
36.00	2000.0
37.00	10994.0
38.00	9582.0
39.00	4224.0
40.10	323.0
40.80	124.0
43.00	285.0
44.00	1537.0
45.00	2004.0
46.00	487.0
47.20	2130.0
47.90	1230.0
49.00	9325.0
50.00	43272.0
51.00	13150.0
52.00	474.0
52.90	487.0
54.00	102.0
54.90	651.0
55.90	3684.0
57.00	5550.0
58.10	328.0
59.90	2390.0
61.10	10841.0
62.00	11828.0
63.10	9462.0
64.00	1225.0
65.10	2125.0
66.00	256.0
66.90	509.0
68.00	23256.0
69.00	23464.0
70.00	2185.0
70.90	122.0
72.00	1499.0
73.00	11381.0
74.00	38904.0
75.00	113568.0
76.00	10324.0
77.10	1186.0
78.00	750.0
78.90	7315.0
79.90	2271.0
80.90	8149.0
82.00	1887.0
82.90	130.0
85.00	66.0
86.00	419.0
86.90	6622.0
88.00	5915.0
88.80	365.0
90.00	54.0
90.90	720.0
92.00	6310.0
93.00	10250.0
94.00	25376.0
95.00	199488.0
96.10	12535.0
97.10	482.0
102.60	137.0
103.00	93.0
104.00	1113.0
104.80	450.0
106.00	951.0
106.90	353.0
109.60	89.0
110.10	268.0
110.80	188.0
112.00	175.0
112.80	171.0
113.40	169.0
114.70	307.0
115.10	299.0
115.90	986.0
116.90	2008.0
117.80	1106.0
119.00	1275.0
119.70	101.0
120.10	70.0
122.70	105.0
124.10	264.0
125.70	64.0
128.00	920.0
128.90	465.0
129.90	746.0
130.80	404.0
134.10	126.0
135.20	290.0
135.90	195.0
137.00	393.0
138.10	81.0
138.80	123.0

Instrument :
MSVOA_X
ClientSampleId :
BFB76

140.10	411.0
140.90	3164.0
142.00	258.0
142.80	3086.0
144.70	869.0
145.80	502.0
146.80	148.0
148.00	627.0
150.10	152.0
151.40	92.0
152.00	215.0
153.00	166.0
154.10	170.0
154.90	557.0
155.90	229.0
157.00	348.0
158.90	321.0
160.90	367.0
168.50	81.0
169.20	169.0
169.90	176.0
170.80	673.0
172.00	2961.0
174.00	155584.0
175.00	12414.0
176.00	145664.0
177.10	9876.0
178.20	310.0
207.00	201.0
280.90	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB76

m/z	Abundance
35.20	224.0
36.00	2394.0
37.00	10562.0
38.00	11006.0
39.00	4148.0
40.00	301.0
40.90	169.0
41.80	146.0
42.80	127.0
44.00	1325.0
45.10	1899.0
46.20	394.0
47.10	1303.0
48.00	1673.0
49.00	9284.0
50.00	43896.0
51.00	13695.0
52.00	852.0
53.10	302.0
54.00	168.0
54.90	688.0
55.90	3948.0
57.00	6791.0
58.20	395.0
58.90	57.0
60.00	2287.0
61.00	12993.0
62.10	12724.0
63.00	9744.0
64.10	1251.0
65.10	1934.0
65.80	407.0
67.00	839.0
68.00	23960.0
69.00	24360.0
70.10	1858.0
70.90	78.0
71.90	1168.0
73.00	11489.0
74.00	45208.0
75.00	125104.0
76.00	9358.0
76.90	994.0
77.90	661.0
78.90	8047.0
79.90	2237.0
80.90	8759.0
81.90	1987.0
83.00	464.0
86.10	446.0
87.00	6601.0
87.90	8063.0
90.00	109.0
90.90	1279.0
92.00	8066.0
93.00	12167.0
94.00	28400.0
95.00	230464.0
96.00	15610.0
97.10	519.0
102.60	175.0
103.20	331.0
103.90	903.0
104.90	376.0
105.90	1061.0
106.70	350.0
110.10	101.0
110.80	308.0
112.00	351.0
112.80	329.0
115.00	310.0
115.80	1312.0
116.90	1759.0
117.80	627.0
118.10	636.0
119.00	2007.0
122.70	79.0
123.10	97.0
124.00	233.0
125.70	156.0
126.20	123.0
127.90	1059.0
129.00	649.0
129.90	870.0
130.80	341.0
131.20	269.0
134.10	148.0
134.90	735.0
136.00	65.0
137.00	683.0
138.60	95.0
140.00	281.0

Instrument :
MSVOA_X
ClientSampleId :
BFB76

141.00	4049.0
142.10	673.0
143.00	4455.0
143.90	328.0
144.90	1163.0
145.90	281.0
146.70	107.0
147.80	821.0
148.70	264.0
149.80	378.0
150.10	350.0
150.80	58.0
151.20	55.0
151.90	225.0
153.00	135.0
153.90	297.0
155.00	742.0
155.90	84.0
157.00	495.0
158.90	387.0
161.10	578.0
163.00	53.0
167.50	131.0
168.50	76.0
169.20	133.0
169.80	250.0
172.00	2761.0
174.00	194112.0
175.00	15375.0
176.00	191936.0
177.00	14013.0
178.10	416.0
207.20	179.0
209.00	126.0
252.50	80.0
280.90	105.0
297.50	78.0

Instrument :
MSVOA_X
ClientSampleId :
BFB76

m/z	Abundance
36.00	1052.0
37.00	6979.0
38.10	5748.0
39.10	2519.0
40.20	325.0
40.90	96.0
41.80	107.0
43.20	140.0
44.00	1390.0
45.10	1114.0
46.20	186.0
47.10	1145.0
47.90	1129.0
49.00	5606.0
50.00	28544.0
51.00	7423.0
52.00	730.0
52.90	235.0
53.90	66.0
55.10	479.0
56.00	2145.0
56.90	4186.0
57.90	282.0
58.30	276.0
60.00	1765.0
61.10	7143.0
62.00	7354.0
63.10	5991.0
64.00	862.0
65.10	1348.0
66.20	207.0
68.00	14087.0
69.00	16624.0
70.00	1065.0
72.00	849.0
73.00	6175.0
74.00	27624.0
75.00	83464.0
76.10	7831.0
77.00	986.0
77.90	370.0
79.00	6010.0
79.90	1761.0
81.00	5570.0
82.10	1006.0
83.00	276.0
85.00	75.0
85.90	116.0
87.00	4451.0
88.00	4328.0
91.00	783.0
92.00	5155.0
93.00	6856.0
94.10	18360.0
95.00	157312.0
96.00	8791.0
97.10	296.0
102.70	206.0
104.00	1005.0
104.80	235.0
106.00	755.0
106.70	304.0
109.90	114.0
111.20	234.0
112.10	210.0
112.80	289.0
114.90	346.0
115.80	937.0
117.00	1662.0
117.80	761.0
119.00	1393.0
119.70	70.0
122.60	56.0
123.80	285.0
126.20	52.0
127.90	722.0
128.80	370.0
129.90	890.0
130.80	468.0
135.10	429.0
136.90	541.0
137.60	84.0
138.70	148.0
139.90	361.0
140.80	2806.0
141.90	450.0
142.90	2390.0
143.80	220.0
144.90	698.0
146.30	279.0
146.90	222.0
148.00	434.0

Instrument :
MSVOA_X
ClientSampleId :
BFB76

148.80	70.0
150.00	397.0
150.80	83.0
151.80	238.0
153.80	174.0
154.70	340.0
155.20	405.0
155.80	182.0
157.10	426.0
159.00	386.0
160.80	185.0
161.20	209.0
162.90	58.0
166.40	61.0
167.50	131.0
168.80	51.0
169.70	86.0
170.80	113.0
172.00	1979.0
173.10	2861.0
174.00	155776.0
175.00	9726.0
176.00	151168.0
177.00	8377.0
177.90	435.0
207.00	320.0
207.60	56.0
208.10	85.0
222.80	50.0
280.70	106.0
283.30	90.0

Instrument :
MSVOA_X
ClientSampleId :
BFB76

m/z	Abundance
35.40	152.0
36.30	85.0
36.80	128.0
37.40	110.0
39.10	154.0
40.50	235.0
41.00	90.0
43.20	88.0
44.10	432.0
45.20	161.0
45.90	72.0
48.60	82.0
50.20	131.0
51.50	114.0
52.20	51.0
53.80	72.0
54.60	95.0
55.10	89.0
55.80	78.0
57.90	51.0
59.30	154.0
61.60	90.0
64.10	52.0
67.80	88.0
68.50	134.0
70.30	53.0
71.40	168.0
73.20	54.0
79.90	68.0
105.00	85.0
108.80	117.0
111.80	122.0
134.80	133.0
137.90	58.0
154.60	57.0
155.00	81.0
207.10	200.0
222.30	122.0
281.30	119.0
290.90	80.0

Instrument :
MSVOA_X
ClientSampleId :
BFB76