

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012786.D
Acq On : 03 Oct 2019 16:13
Operator : JC/SP
Sample : K5189-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ135I-20190930

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	41	rBV	384007	486270	52.31%	9.192%
2	1.265	58	62	69	rBV	33593	43454	4.67%	0.821%
3	2.430	248	253	260	rBV	7216	13430	1.44%	0.254%
4	2.594	273	280	295	rBV	52333	98063	10.55%	1.854%
5	5.490	744	755	769	rBV	101690	295165	31.75%	5.579%
6	5.649	769	781	797	rBV	185750	528653	56.87%	9.993%
7	6.051	837	847	862	rBV	124393	326247	35.10%	6.167%
8	6.850	969	978	993	rBV	295913	695234	74.79%	13.142%
9	8.709	1276	1283	1301	rBV	579108	929578	100.00%	17.572%
10	10.111	1507	1513	1529	rBV	540962	755706	81.30%	14.285%
11	11.135	1675	1681	1692	rBV	391590	522015	56.16%	9.868%
12	12.074	1829	1835	1844	rBV	480954	596389	64.16%	11.273%


Sum of corrected areas: 5290204

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012786.D
Acq On : 03 Oct 2019 16:13
Operator : JC/SP
Sample : K5189-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ135I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

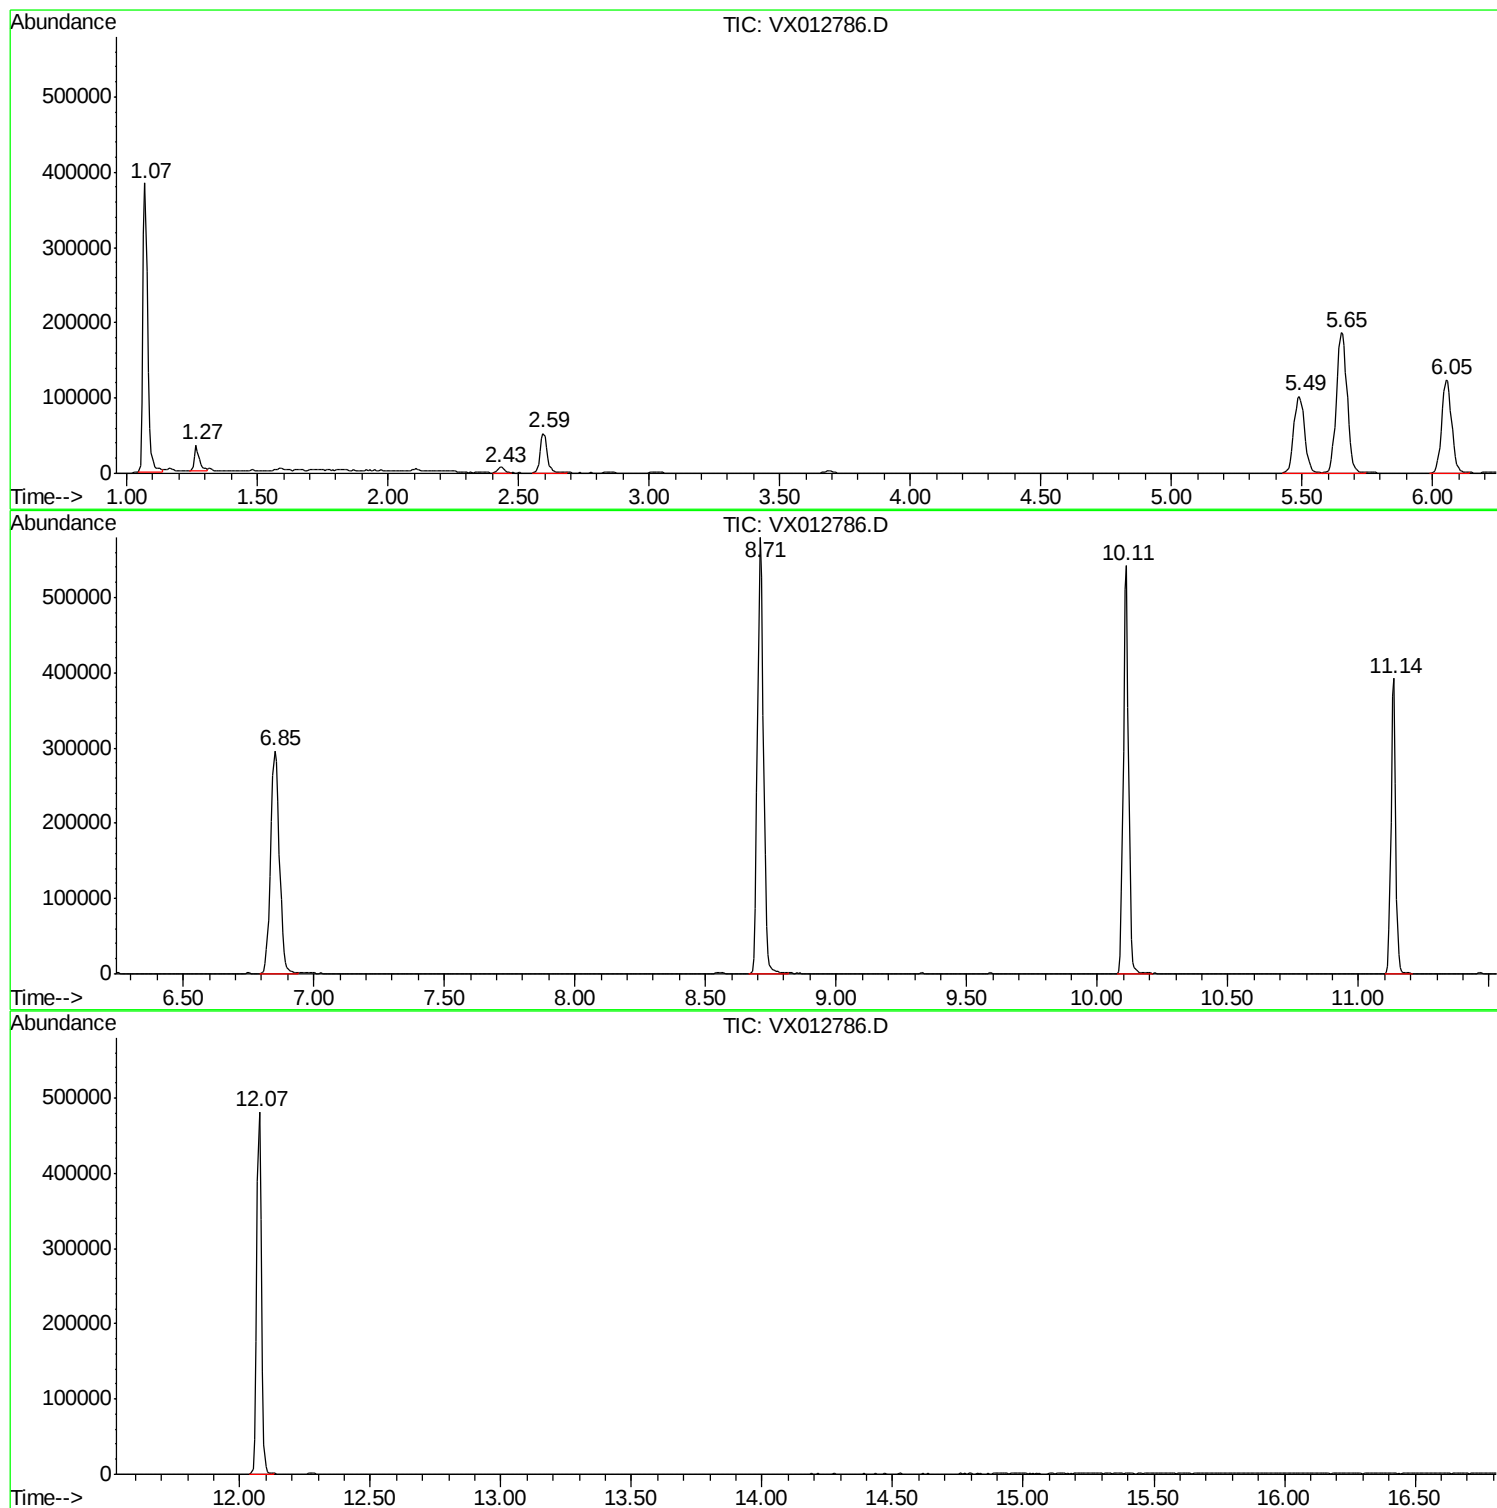

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012786.D
Acq On : 03 Oct 2019 16:13
Operator : JC/SP
Sample : K5189-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ135I-20190930










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	9.27 ug/l	98063	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2		Hvdrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		Hvdrazine, ethyl-	60	C2H8N2	000624-80-6	9
4		Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4
5		Formamide	45	CH3NO	000075-12-7	4

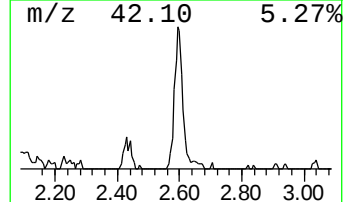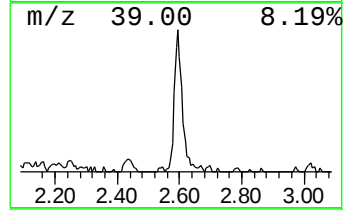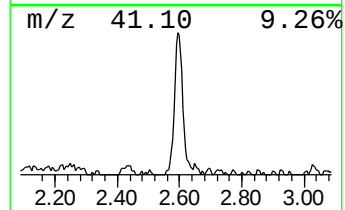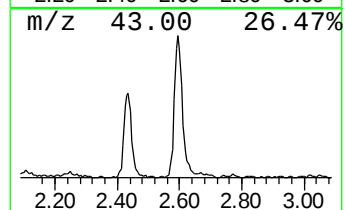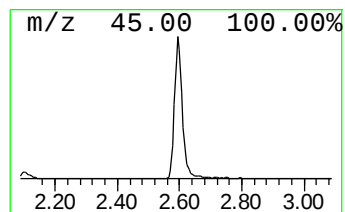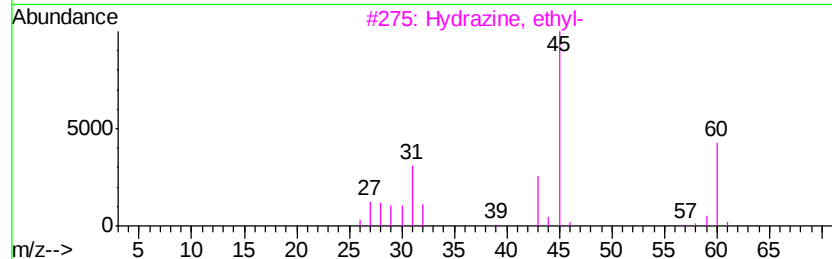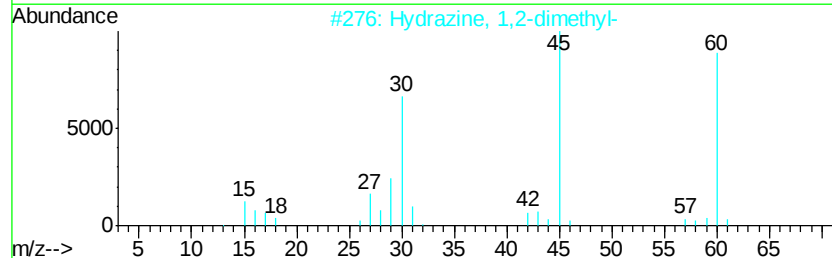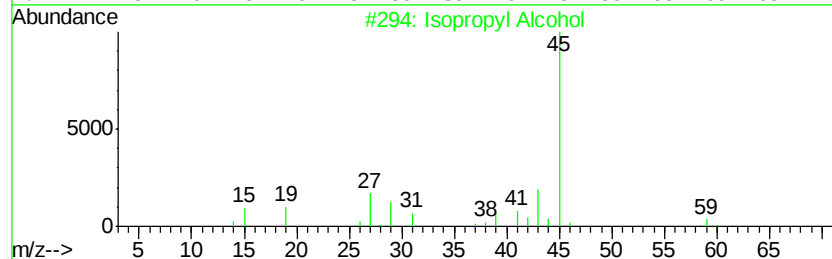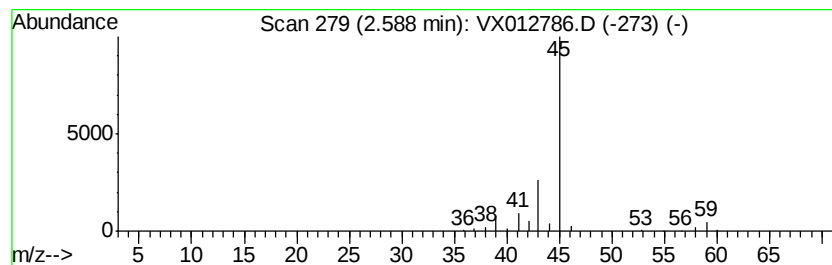

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100319\
Data File : VX012786.D
Acq On : 03 Oct 2019 16:13
Operator : JC/SP
Sample : K5189-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ135I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	9.3	ug/l	98063	1	5.65	528653	50.0