

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100319\
 Data File : VX012787.D
 Acq On : 03 Oct 2019 16:36
 Operator : JC/SP
 Sample : K5189-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ134I-20190930

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	411577	499572	52.52%	8.958%
2	1.265	58	62	72	rBV	35388	48320	5.08%	0.866%
3	2.594	272	280	296	rBV	92747	170739	17.95%	3.062%
4	5.490	743	755	770	rBV3	103933	298911	31.42%	5.360%
5	5.654	770	782	800	rVV2	191182	537808	56.54%	9.644%
6	6.051	837	847	864	rBV	125278	333644	35.07%	5.983%
7	6.849	967	978	998	rBV	299802	715201	75.19%	12.825%
8	8.709	1276	1283	1300	rBV	594662	951237	100.00%	17.058%
9	9.330	1380	1385	1392	rBV2	23837	35229	3.70%	0.632%
10	10.111	1507	1513	1527	rBV	571586	787992	82.84%	14.131%
11	11.135	1675	1681	1693	rBV	422800	549925	57.81%	9.861%
12	12.074	1829	1835	1849	rBV	524069	647955	68.12%	11.619%


Sum of corrected areas: 5576533

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012787.D
Acq On : 03 Oct 2019 16:36
Operator : JC/SP
Sample : K5189-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ134I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

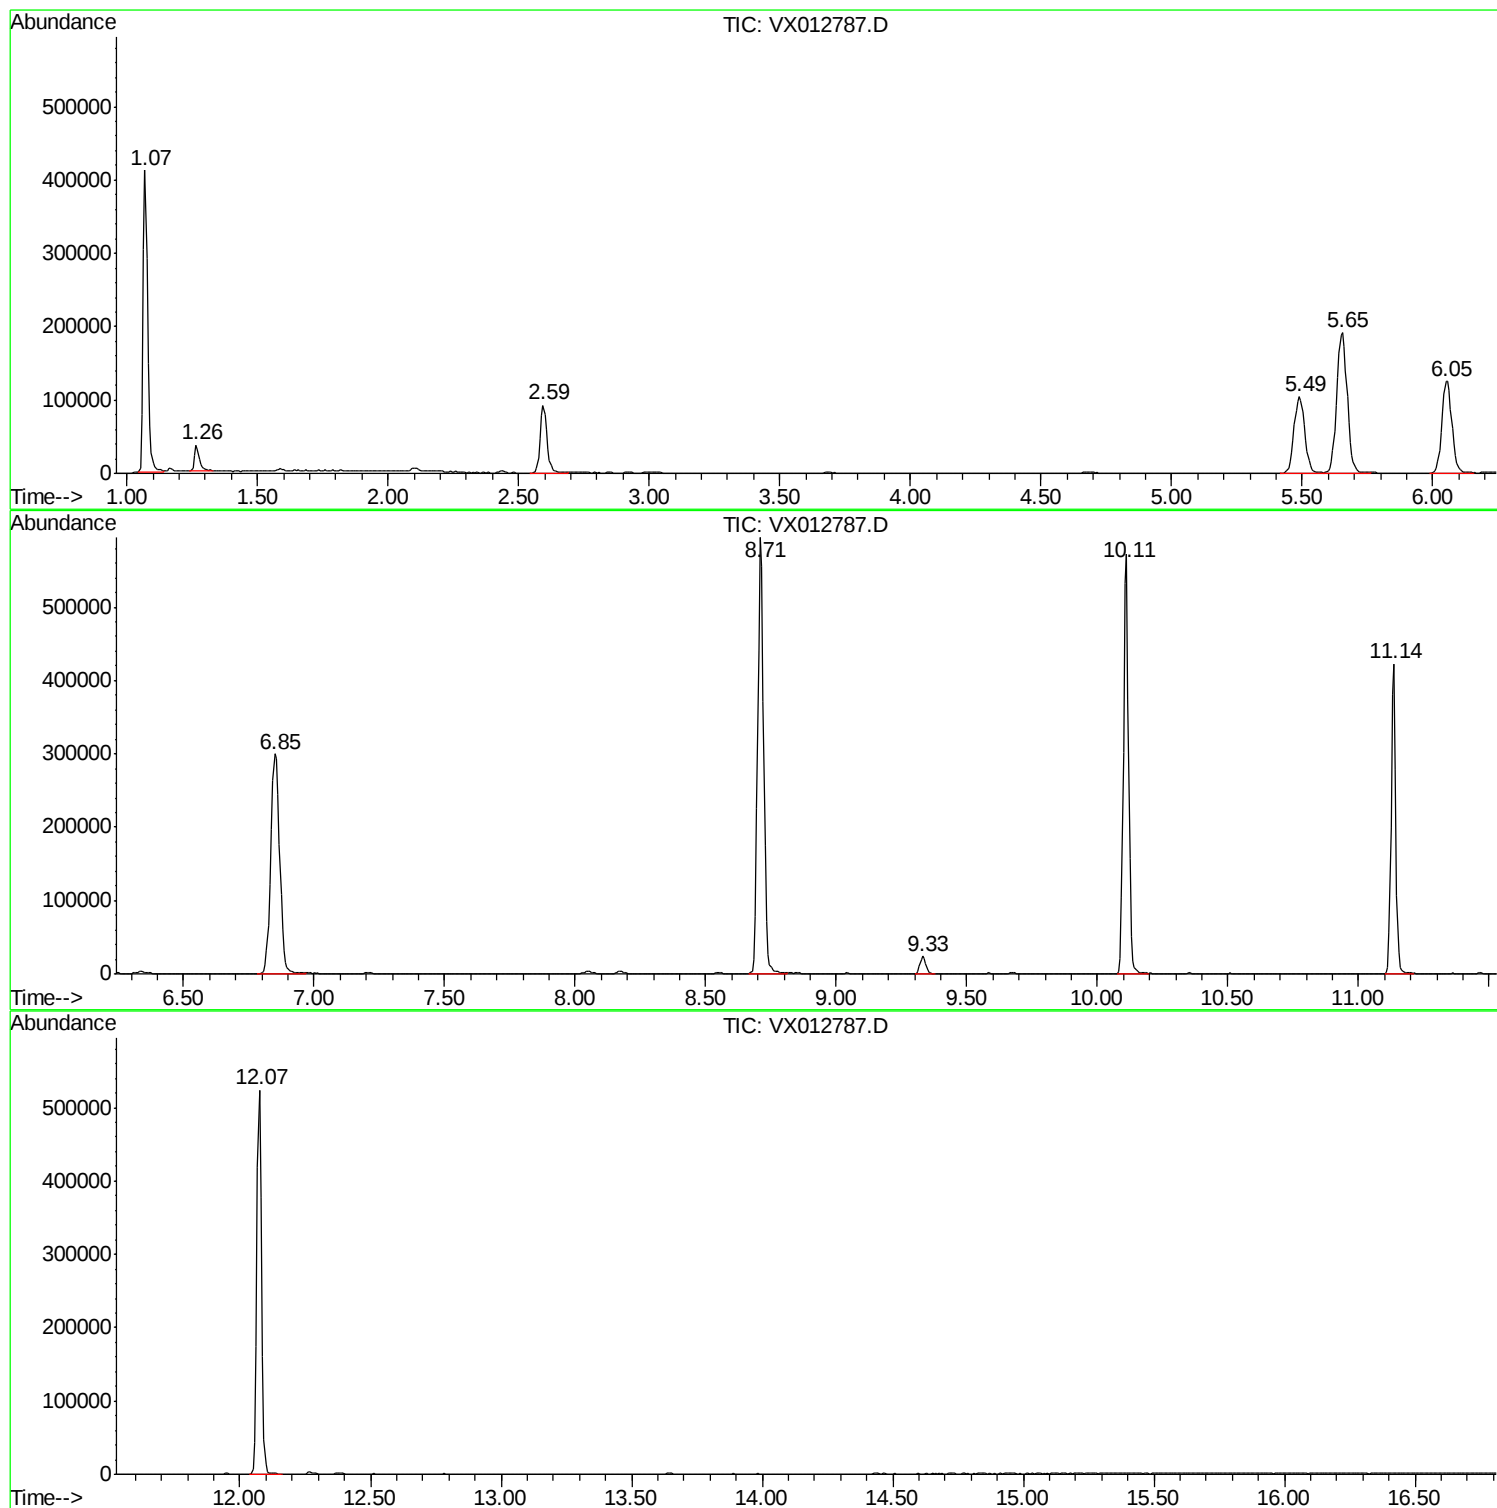

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012787.D
Acq On : 03 Oct 2019 16:36
Operator : JC/SP
Sample : K5189-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ134I-20190930










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	15.87 ug/l	170739	Pentafluorobenzene	5.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	80
2			Hvdrazine, ethyl-	60	C2H8N2	000624-80-6	40
3			Hvdrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

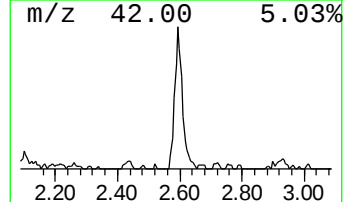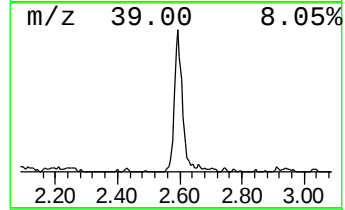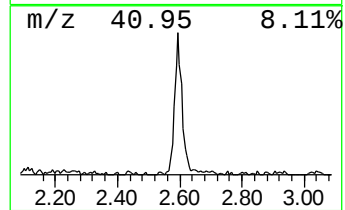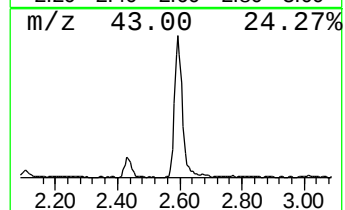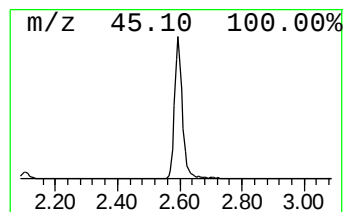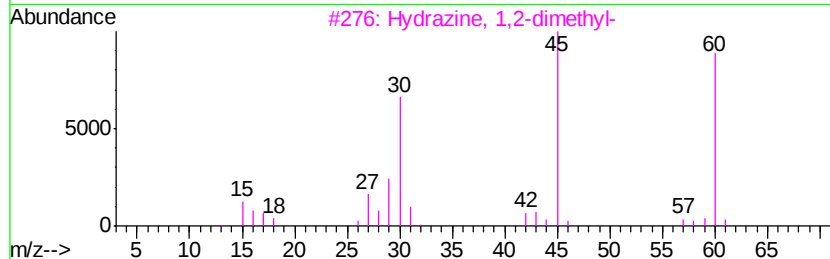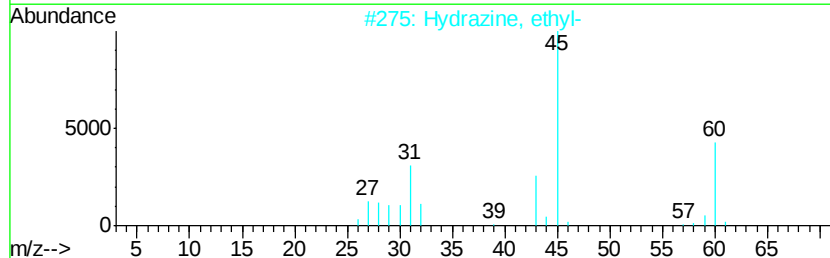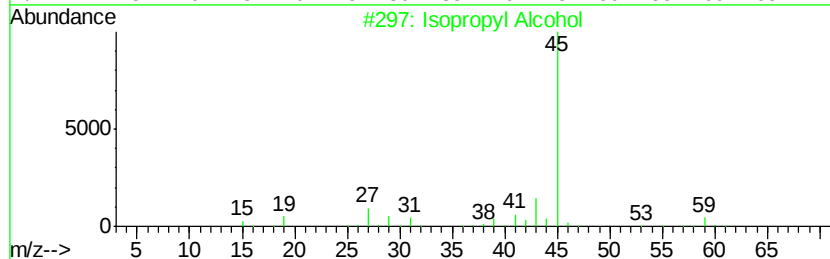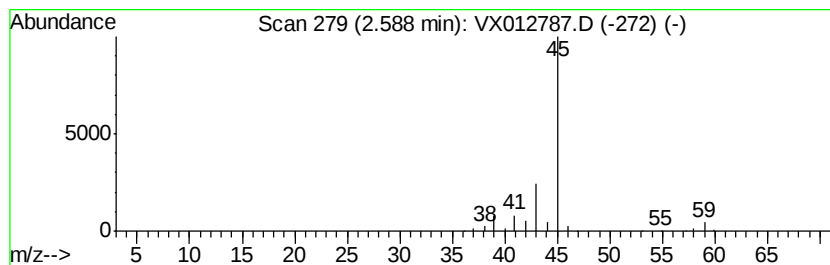

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100319\
Data File : VX012787.D
Acq On : 03 Oct 2019 16:36
Operator : JC/SP
Sample : K5189-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ134I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	15.9	ug/l	170739	1	5.65	537808	50.0