

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100319\
 Data File : VX012790.D
 Acq On : 03 Oct 2019 17:46
 Operator : JC/SP
 Sample : K5189-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ133I-20190930

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	394493	486219	52.95%	9.450%
2	1.265	58	62	68	rBV	35445	44691	4.87%	0.869%
3	2.436	248	254	262	rVB	6955	12867	1.40%	0.250%
4	2.594	273	280	295	rBV	33863	62820	6.84%	1.221%
5	5.490	741	755	771	rBV2	100871	291127	31.70%	5.658%
6	5.649	771	781	795	rBV	182167	516672	56.26%	10.042%
7	6.051	837	847	864	rBV	122602	323251	35.20%	6.282%
8	6.849	967	978	992	rBV	288528	685983	74.70%	13.332%
9	8.709	1276	1283	1300	rBV	589778	918299	100.00%	17.847%
10	10.111	1507	1513	1528	rVB	529693	742041	80.81%	14.422%
11	11.135	1675	1681	1691	rBV	391467	505649	55.06%	9.827%
12	12.074	1829	1835	1845	rBV	453082	555721	60.52%	10.800%


Sum of corrected areas: 5145340

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012790.D
Acq On : 03 Oct 2019 17:46
Operator : JC/SP
Sample : K5189-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ133I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

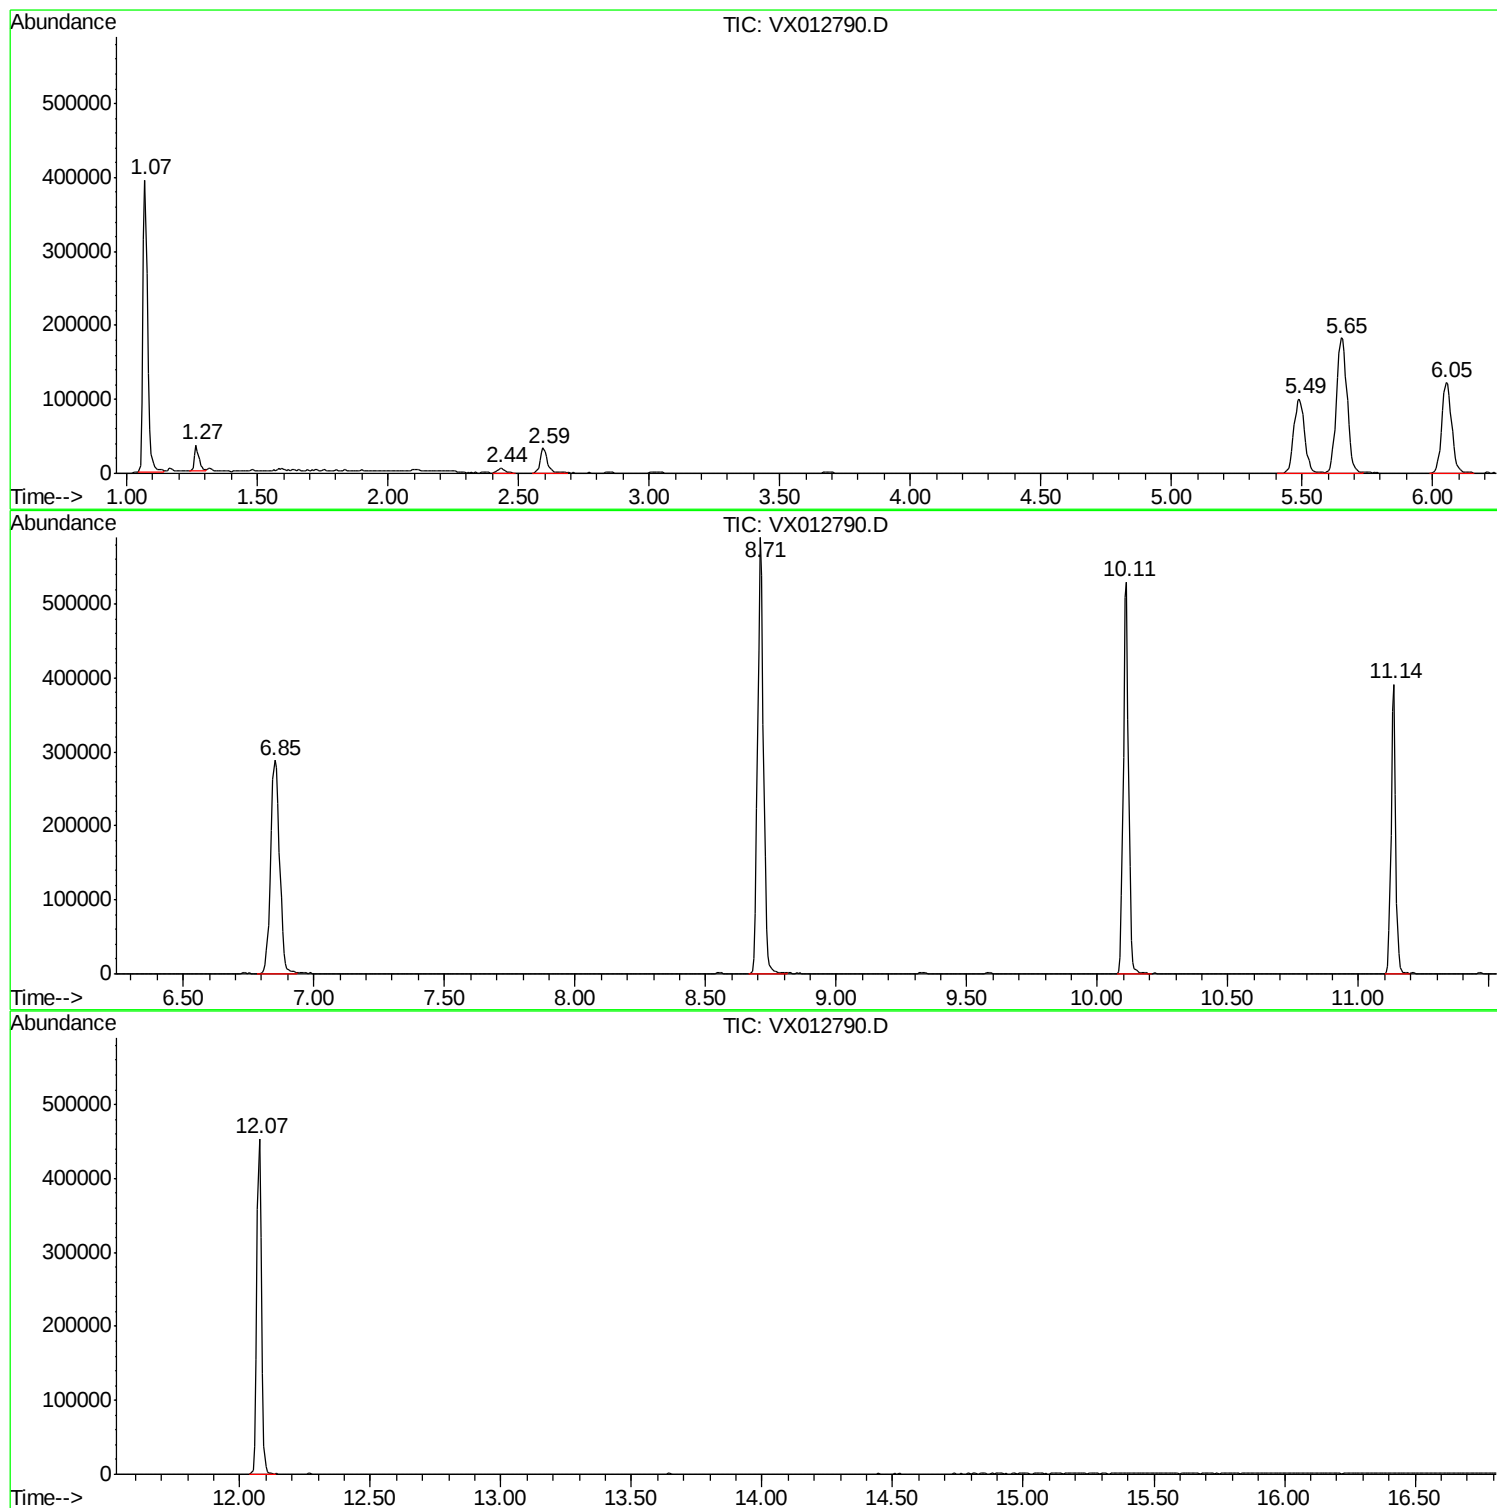

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012790.D
Acq On : 03 Oct 2019 17:46
Operator : JC/SP
Sample : K5189-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ133I-20190930










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	6.08 ug/l	62820	Pentafluorobenzene	5.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	43
3			Formic acid, 1-methylethyl ester	88	C4H8O2	000625-55-8	40
4			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
5			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

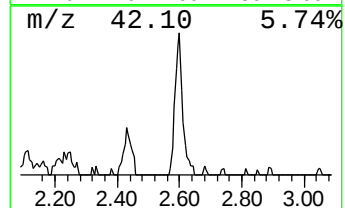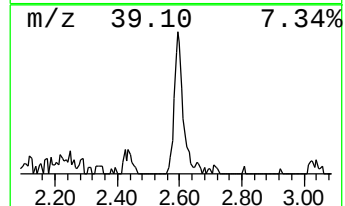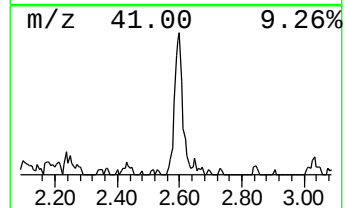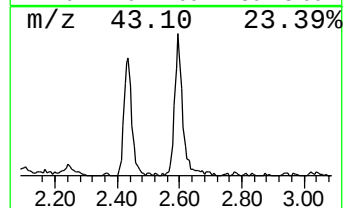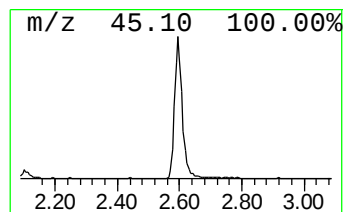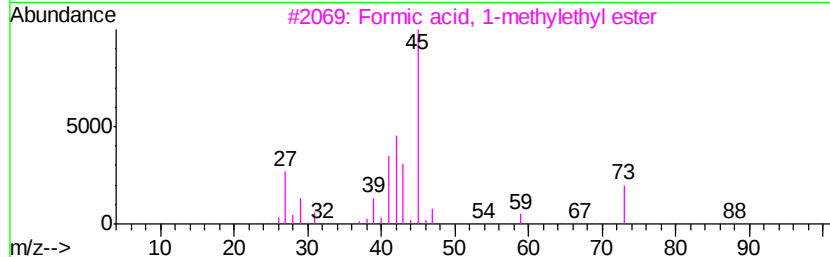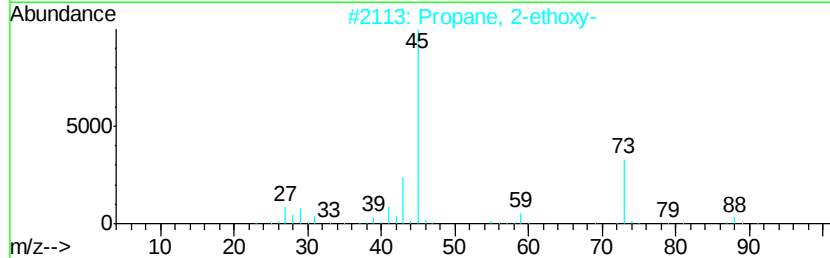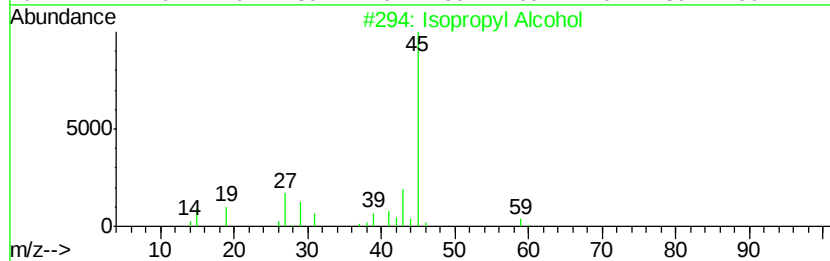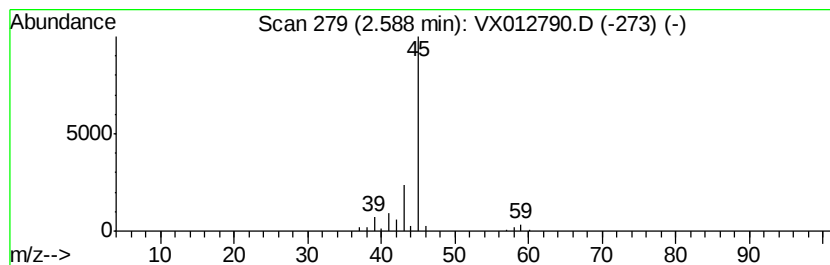

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100319\
Data File : VX012790.D
Acq On : 03 Oct 2019 17:46
Operator : JC/SP
Sample : K5189-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ133I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	6.1	ug/l	62820	1	5.65	516672	50.0