

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100319\
 Data File : VX012793.D
 Acq On : 03 Oct 2019 18:56
 Operator : JC/SP
 Sample : K5189-12
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-MW128I-20190930

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	41	rBV	317133	387548	40.88%	7.287%
2	1.265	58	62	69	rBV	30252	39413	4.16%	0.741%
3	2.429	247	253	262	rBV	6674	12178	1.28%	0.229%
4	2.594	273	280	292	rBV	46948	85310	9.00%	1.604%
5	5.490	743	755	768	rBV2	105021	297497	31.38%	5.594%
6	5.654	768	782	795	rBV	188618	535732	56.51%	10.074%
7	6.057	836	848	861	rBV	124127	330052	34.81%	6.206%
8	6.849	967	978	996	rBV	301681	712011	75.10%	13.388%
9	8.709	1277	1283	1302	rBV	605094	948062	100.00%	17.827%
10	10.111	1507	1513	1523	rBV	569649	787293	83.04%	14.804%
11	11.135	1675	1681	1692	rBV	433643	548346	57.84%	10.311%
12	12.074	1830	1835	1847	rVB	530184	634704	66.95%	11.935%


Sum of corrected areas: 5318146

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012793.D
Acq On : 03 Oct 2019 18:56
Operator : JC/SP
Sample : K5189-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-MW128I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

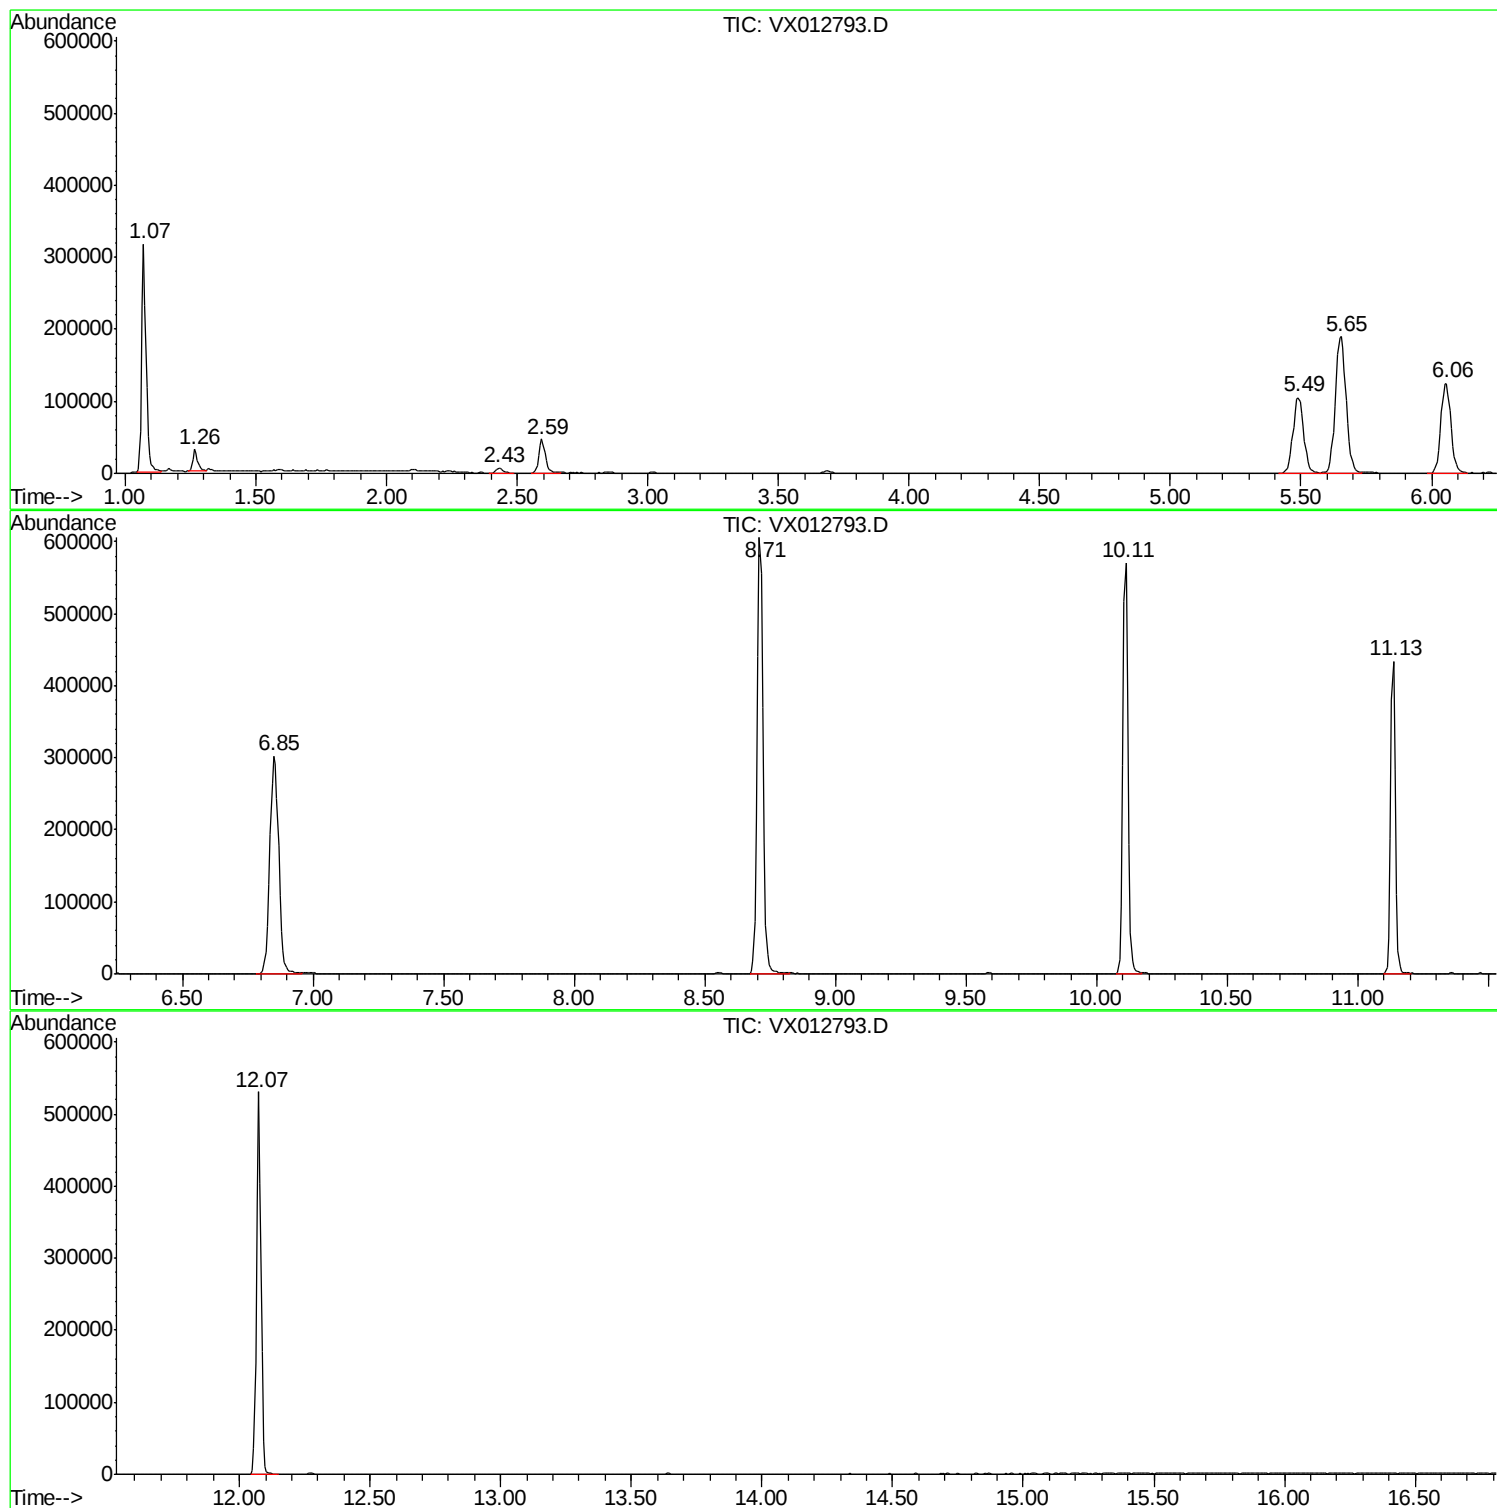

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012793.D
Acq On : 03 Oct 2019 18:56
Operator : JC/SP
Sample : K5189-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-MW128I-20190930










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	7.96 ug/l	85310	Pentafluorobenzene	5.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Hvdrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3			Hvdrazine, ethyl-	60	C2H8N2	000624-80-6	9
4			Formamide	45	CH3NO	000075-12-7	4
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

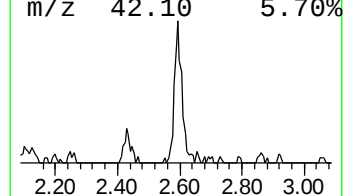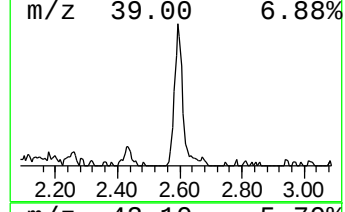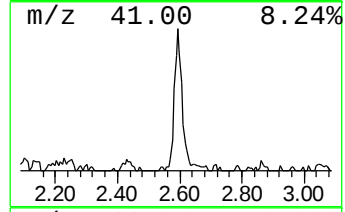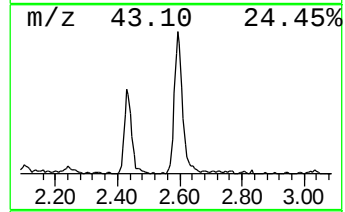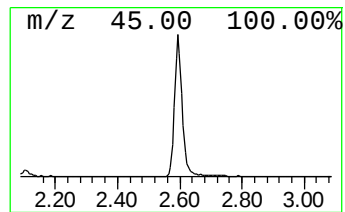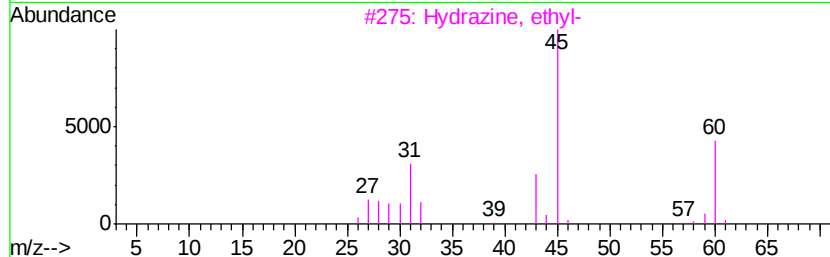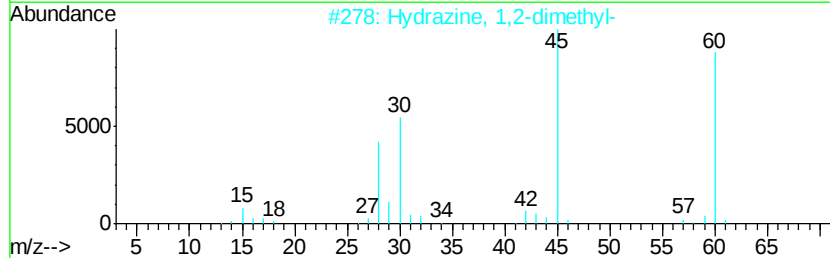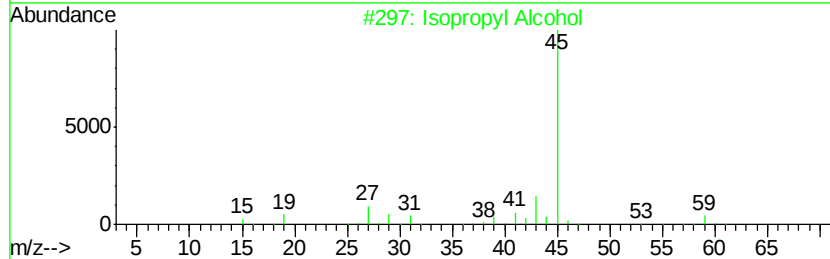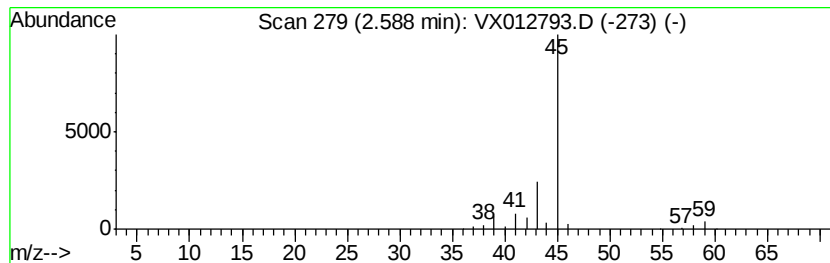

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100319\
Data File : VX012793.D
Acq On : 03 Oct 2019 18:56
Operator : JC/SP
Sample : K5189-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-MW128I-20190930

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	8.0	ug/l	85310	1	5.65	535732	50.0