

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100319\
 Data File : VX012796.D
 Acq On : 03 Oct 2019 20:06
 Operator : JC/SP
 Sample : K5189-15
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ179I-20191001

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	38	rBV	388457	480110	50.10%	8.725%
2	1.265	58	62	66	rBV	30415	37403	3.90%	0.680%
3	2.430	248	253	261	rVB	6011	10077	1.05%	0.183%
4	2.594	273	280	294	rBV	48528	90635	9.46%	1.647%
5	5.490	743	755	767	rBV	106613	302683	31.58%	5.500%
6	5.649	770	781	801	rVV2	188620	540864	56.43%	9.829%
7	6.051	836	847	859	rBV	127727	335212	34.98%	6.092%
8	6.850	968	978	997	rBV	301386	720981	75.23%	13.102%
9	8.709	1276	1283	1300	rBV	608985	958384	100.00%	17.416%
10	10.111	1507	1513	1523	rBV	568715	802123	83.70%	14.577%
11	11.135	1675	1681	1694	rBV	431694	566807	59.14%	10.300%
12	12.074	1829	1835	1845	rBV	543051	657565	68.61%	11.950%


Sum of corrected areas: 5502844

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012796.D
Acq On : 03 Oct 2019 20:06
Operator : JC/SP
Sample : K5189-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ179I-20191001

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

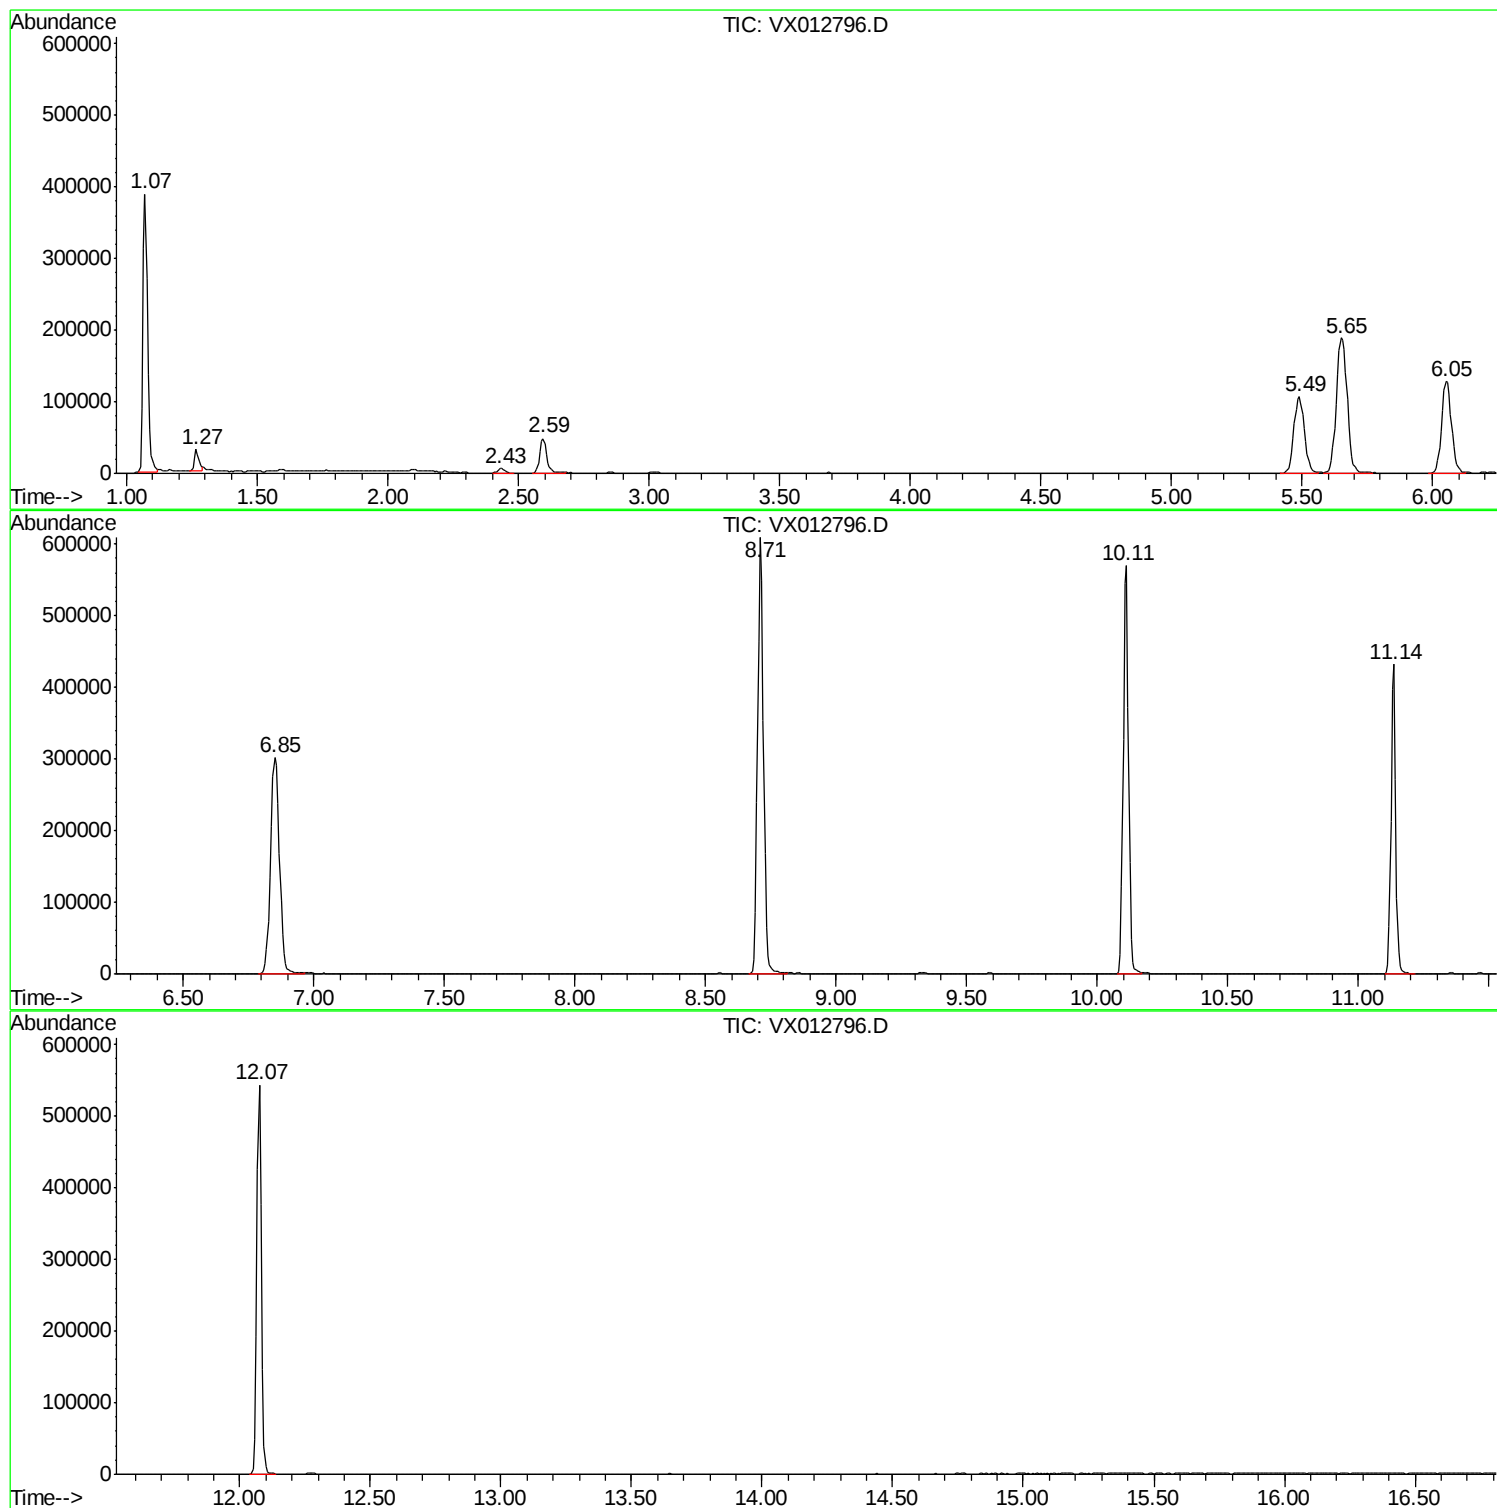

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012796.D
Acq On : 03 Oct 2019 20:06
Operator : JC/SP
Sample : K5189-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ179I-20191001










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	8.38 ug/l	90635	Pentafluorobenzene	5.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	90
2			Hvdrazine, ethyl-	60	C2H8N2	000624-80-6	40
3			Hvdrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			Formamide	45	CH3NO	000075-12-7	5
5			1-Butene, 4-methoxy	86	C5H10O	004696-30-4	4

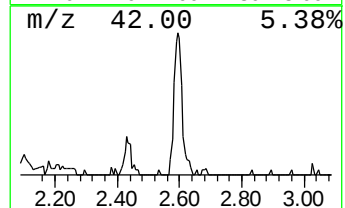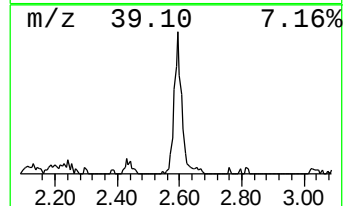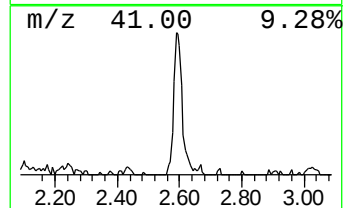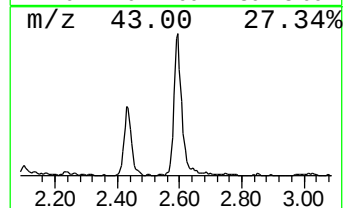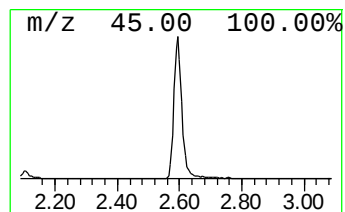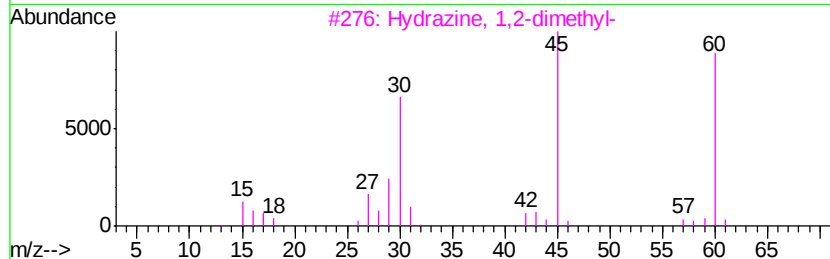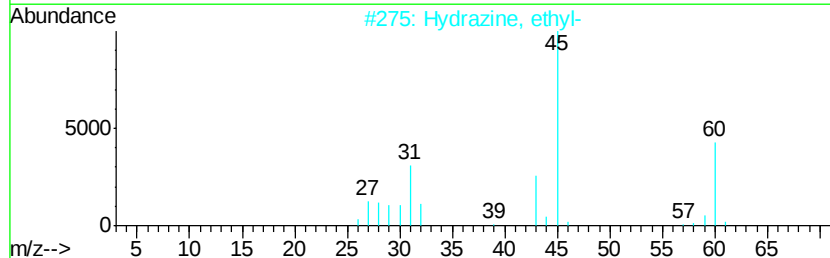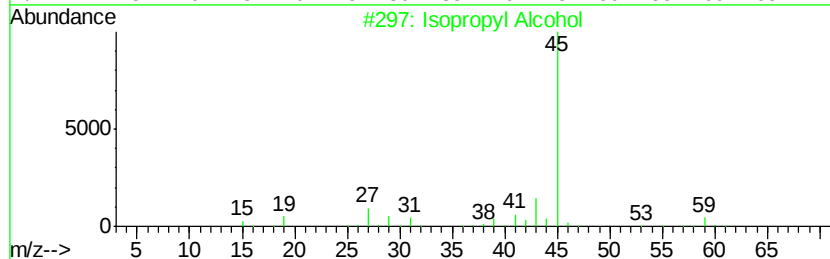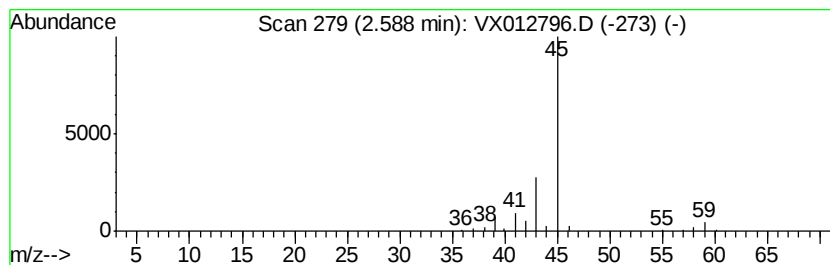

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_X\DATA\VX100319\
Data File : VX012796.D
Acq On : 03 Oct 2019 20:06
Operator : JC/SP
Sample : K5189-15
Misc : 5.0mL/MSV0A_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSV0A_X
ClientSampleId :
SA-PZ179I-20191001

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	8.4	ug/l	90635	1	5.65	540864	50.0