

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012797.D
Acq On : 03 Oct 2019 20:30
Operator : JC/SP
Sample : K5189-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ180I-20191001

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	38	rBV	342782	421540	45.55%	8.107%
2	1.265	58	62	69	rBV	31150	41690	4.50%	0.802%
3	2.430	248	253	262	rVB	7799	13269	1.43%	0.255%
4	2.594	273	280	292	rBV	47322	89610	9.68%	1.723%
5	5.490	744	755	769	rBV2	101116	292286	31.58%	5.621%
6	5.655	771	782	796	rVV	187301	526130	56.85%	10.119%
7	6.051	835	847	862	rBV	125562	328178	35.46%	6.312%
8	6.850	969	978	993	rBV	296002	699232	75.55%	13.448%
9	8.709	1275	1283	1295	rBV	587429	925546	100.00%	17.801%
10	10.111	1507	1513	1530	rVB	537154	761374	82.26%	14.643%
11	11.135	1675	1681	1693	rBV	404525	519003	56.08%	9.982%
12	12.074	1830	1835	1842	rBV	476811	581680	62.85%	11.187%


Sum of corrected areas: 5199538

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012797.D
Acq On : 03 Oct 2019 20:30
Operator : JC/SP
Sample : K5189-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ180I-20191001

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

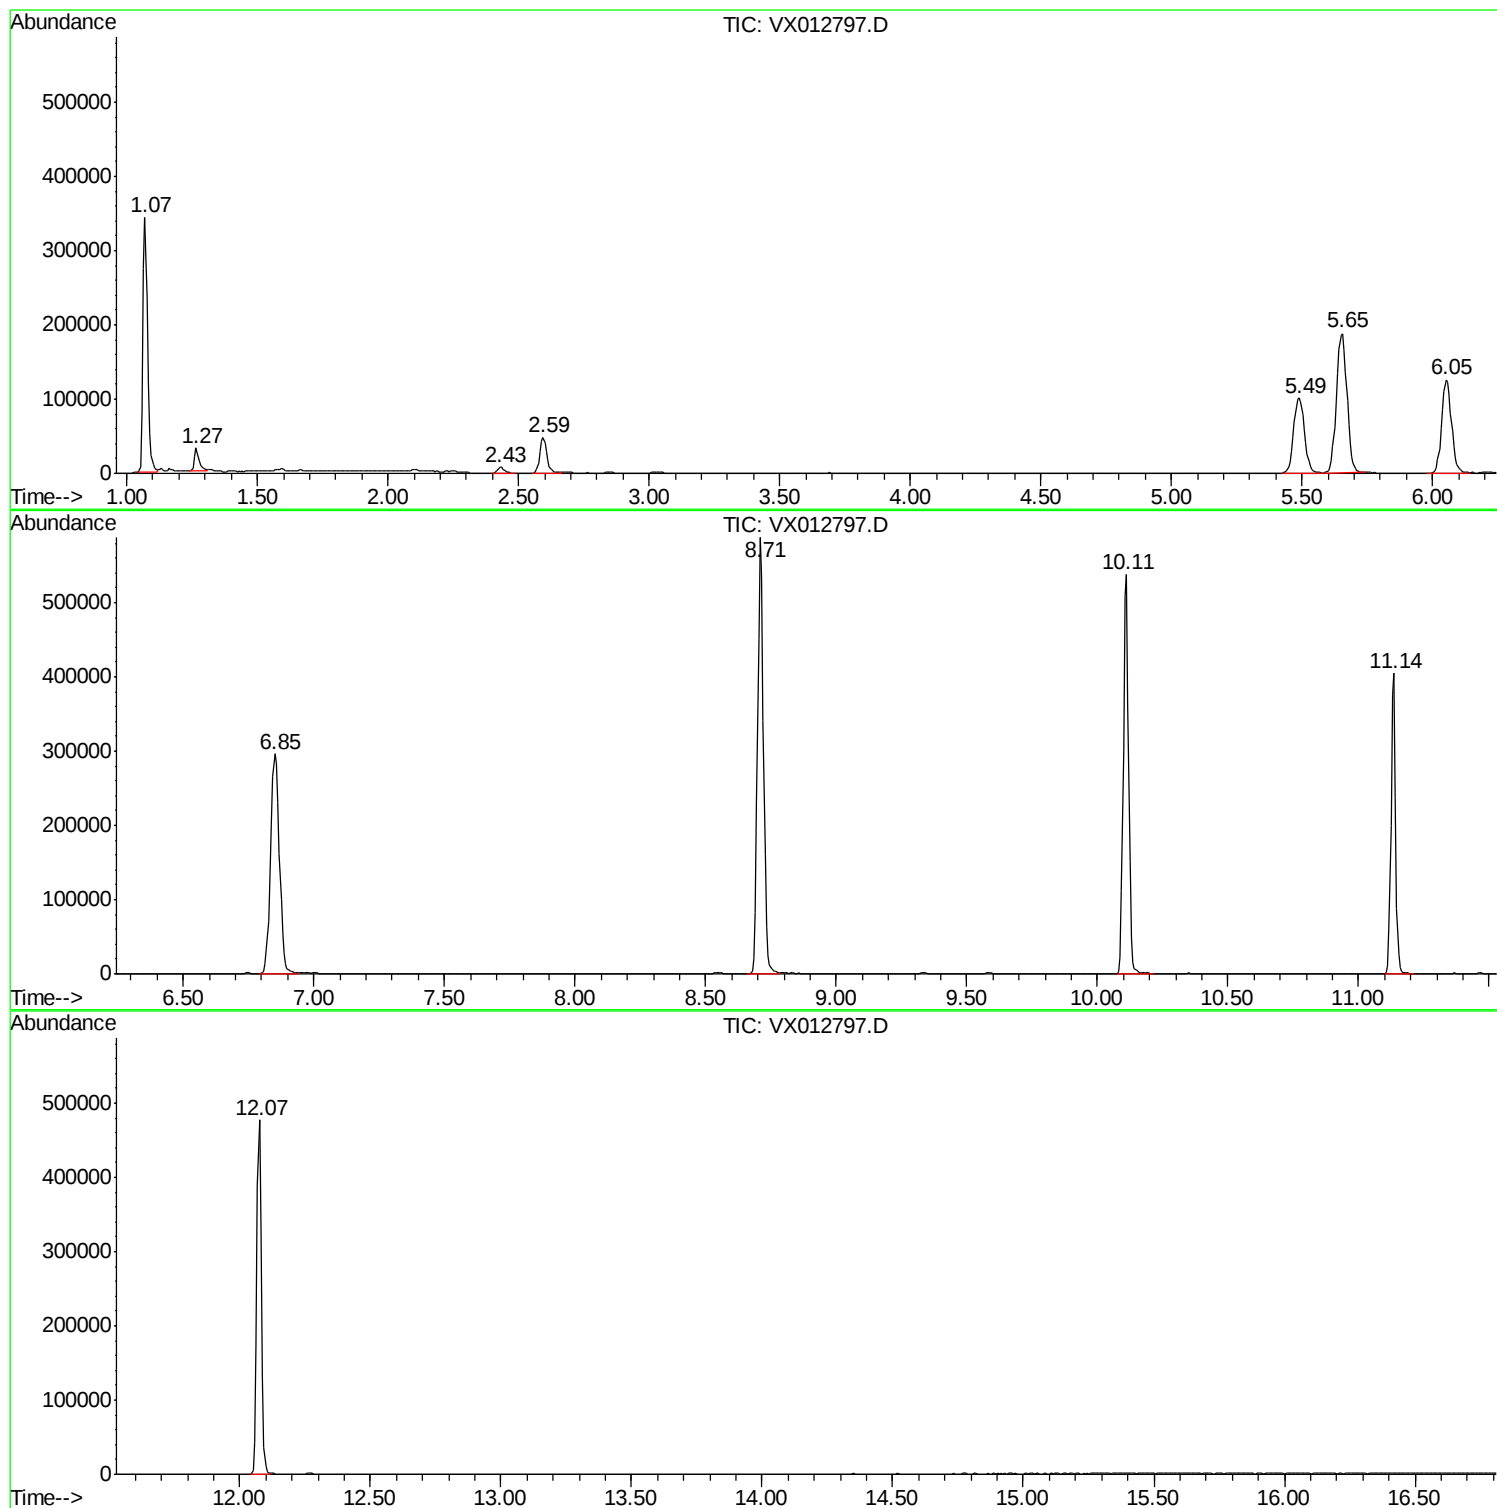

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100319\
Data File : VX012797.D
Acq On : 03 Oct 2019 20:30
Operator : JC/SP
Sample : K5189-16
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ180I-20191001










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	8.52 ug/l	89610	Pentafluorobenzene	5.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Hvdrazine, ethyl-	60	C2H8N2	000624-80-6	40
3			Hvdrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4			Ethylamine	45	C2H7N	000075-04-7	7
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

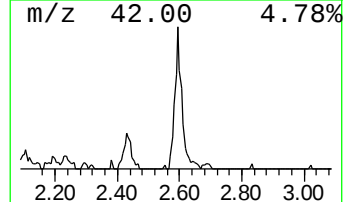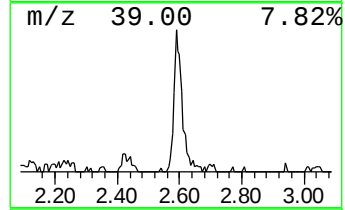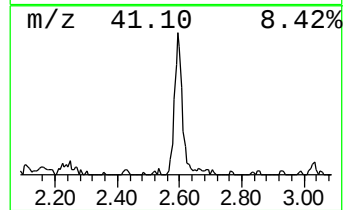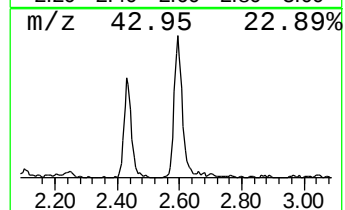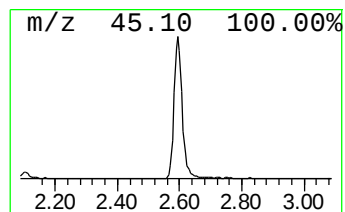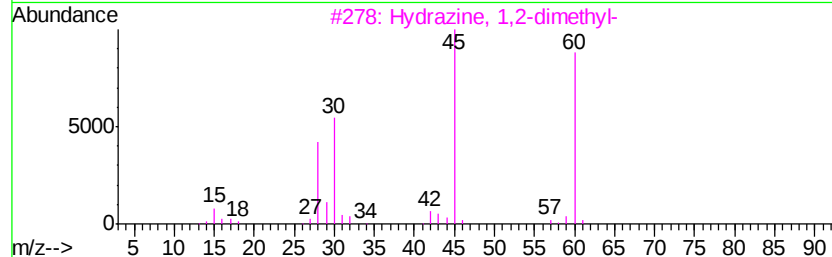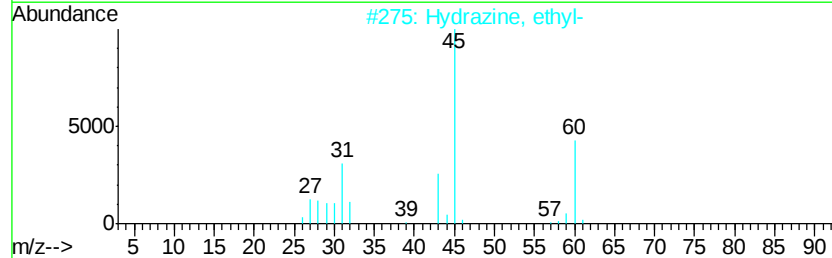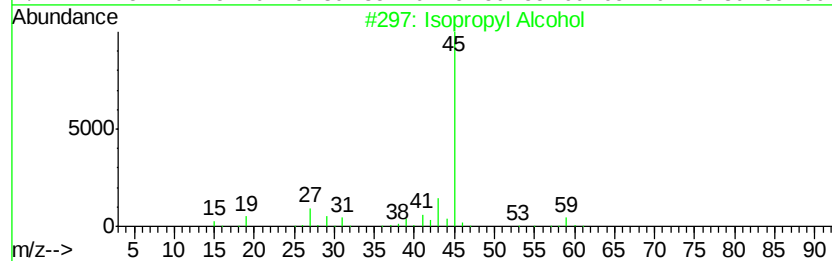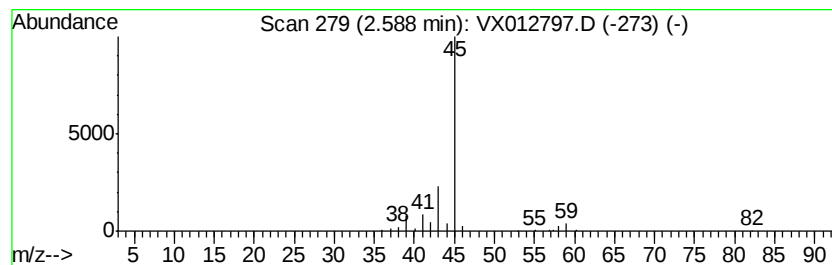

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100319\
Data File : VX012797.D
Acq On : 03 Oct 2019 20:30
Operator : JC/SP
Sample : K5189-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ180I-20191001

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	8.5	ug/l	89610	1	5.65	526130	50.0