

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
 Data File : VX031841.D
 Acq On : 03 Oct 2022 18:16
 Operator : JC/MD
 Sample : N4864-09 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 04 07:07:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 04 06:59:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	91532	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	136364	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	148692	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	109127	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	82467	50.289	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 100.580%	
35) Dibromofluoromethane	5.385	113	77498	47.834	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 95.660%	
50) Toluene-d8	8.647	98	276720	47.745	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 95.480%	
62) 4-Bromofluorobenzene	11.079	95	98897	47.384	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 94.760%	


Target Compounds				Qvalue		
5) Bromomethane	1.618	94	613	Below Cal	#	75
6) Chloroethane	1.636	64	87	Below Cal	#	43
10) Methyl Iodide	2.459	142	341	0.261	ug/l #	79
11) Tert butyl alcohol	3.001	59	109	0.477	ug/l #	73
16) Acetone	2.386	43	231	Below Cal	#	45
17) Carbon Disulfide	2.514	76	761	Below Cal	#	75
20) Methylene Chloride	2.788	84	425	0.296	ug/l #	76
25) 2-Butanone	4.580	43	183	0.243	ug/l #	49
36) 1,1-Dichloropropene	5.550	75	6330	3.151	ug/l #	52
38) Carbon Tetrachloride	5.550	117	8773	3.518	ug/l #	19
39) Methylcyclohexane	7.373	83	1031	0.418	ug/l #	72
43) Isopropyl Acetate	6.251	43	781	0.318	ug/l #	61
52) Toluene	8.720	92	834	0.205	ug/l	87
55) 1,1,2-Trichloroethane	9.104	97	456	0.281	ug/l #	15
67) Ethyl Benzene	10.195	91	295172	39.773	ug/l	97
68) m/p-Xylenes	10.299	106	49360	16.110	ug/l	91
69) o-Xylene	10.646	106	2456	0.832	ug/l	95
73) Isopropylbenzene	10.963	105	17328	2.248	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	48292	24.323	ug/l #	37
78) n-propylbenzene	11.305	91	83594	9.922	ug/l	98
79) 2-Chlorotoluene	11.396	91	9948	1.954	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	33131	5.147	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	48292	83.497	ug/l #	11
82) 4-Chlorotoluene	11.451	91	4118	0.701	ug/l #	44
83) tert-Butylbenzene	11.756	119	63386	9.743	ug/l #	61
84) 1,2,4-Trimethylbenzene	11.750	105	507615	79.238	ug/l	95
85) sec-Butylbenzene	11.750	105	507615	64.813	ug/l #	56
86) p-Isopropyltoluene	12.085	119	12167	1.780	ug/l #	1
89) n-Butylbenzene	12.329	91	11810	2.187	ug/l #	25
90) Hexachloroethane	12.530	117	5586	4.530	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	12.963	75	335	0.726	ug/l #	3
95) Naphthalene	13.774	128	210744	28.774	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031841.D
Acq On : 03 Oct 2022 18:16
Operator : JC/MD
Sample : N4864-09 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Oct 04 07:07:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 04 06:59:30 2022
Response via : Initial Calibration

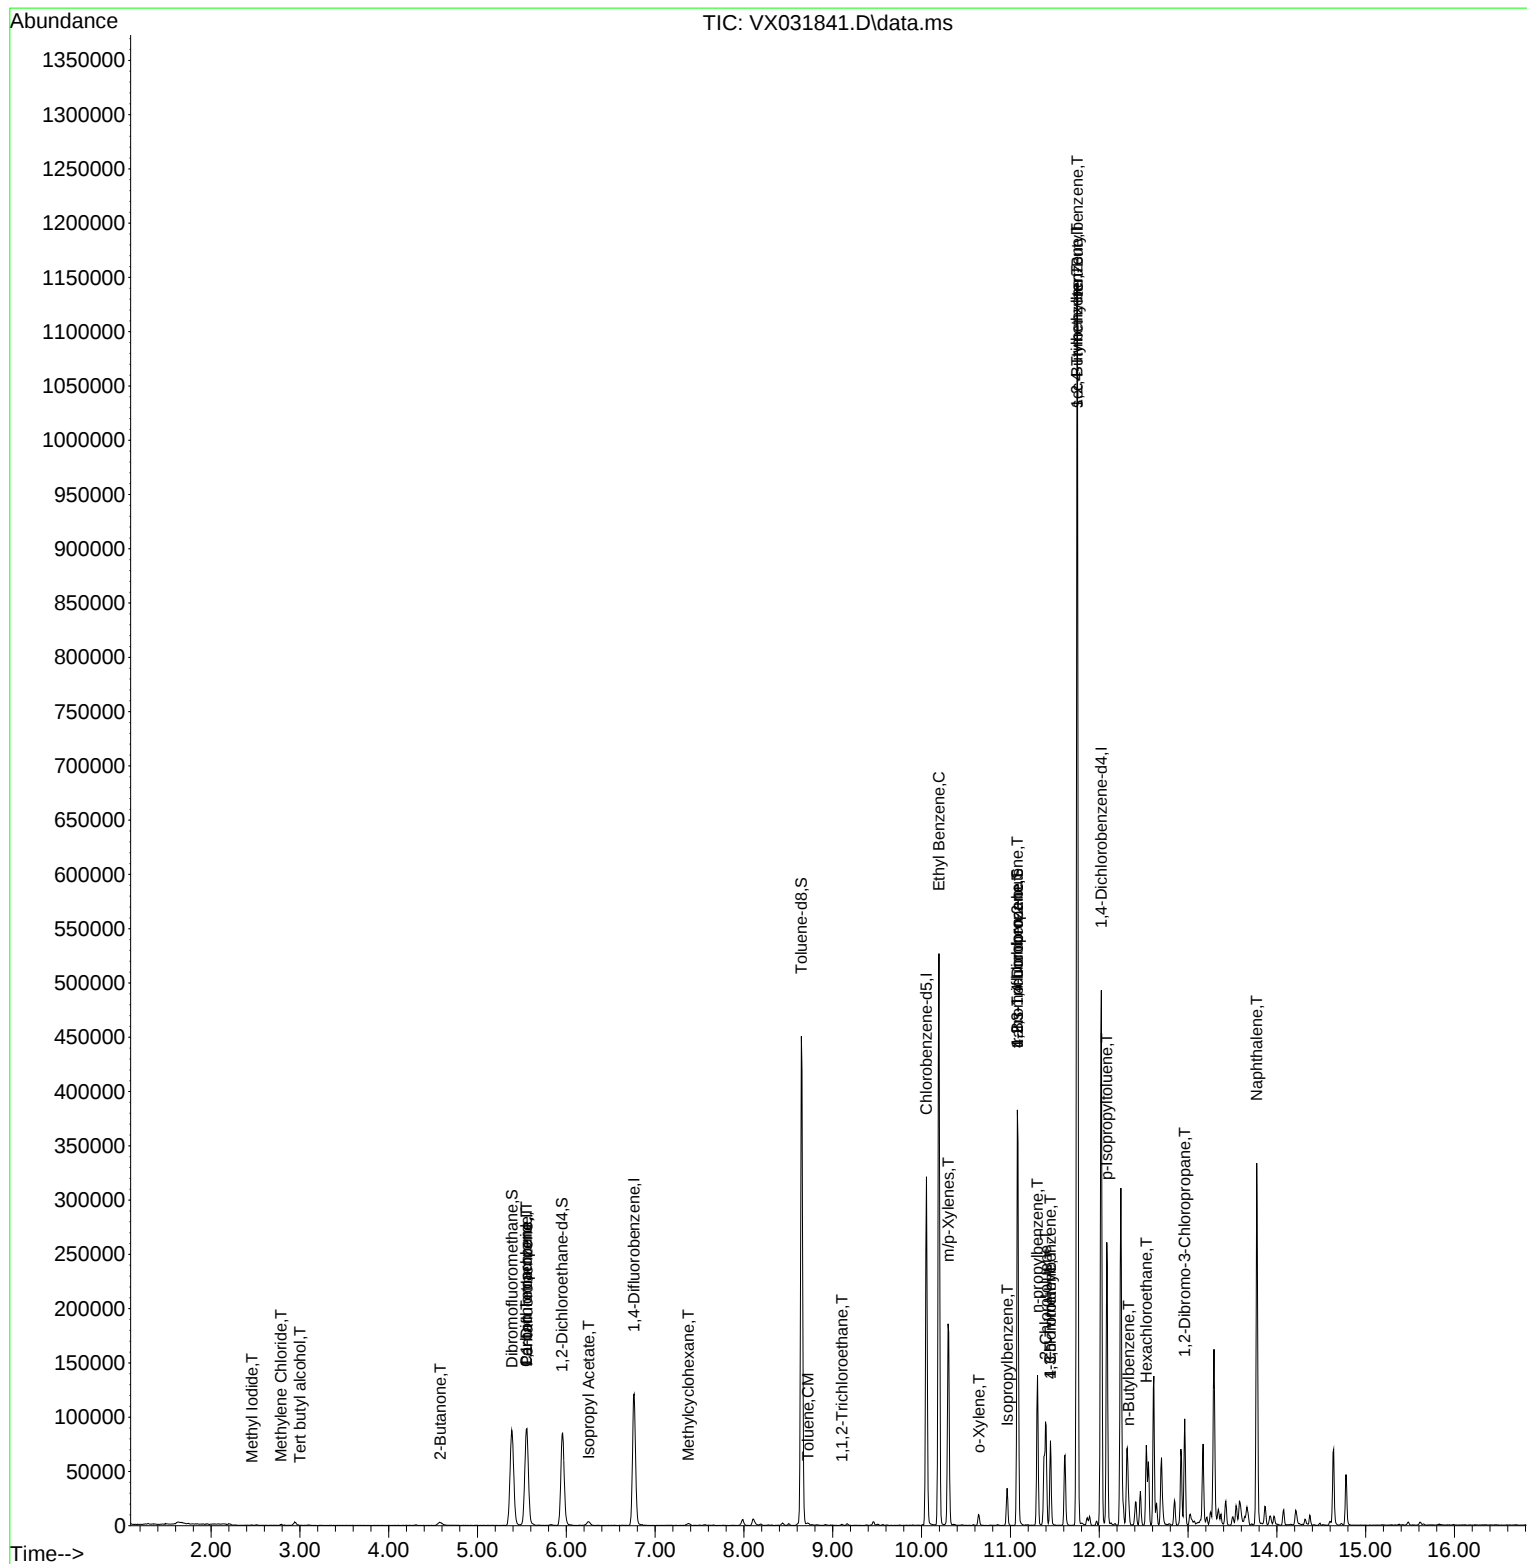






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 91532
Ion Ratio Lower Upper
168 100
99 54.7 48.8 73.2



#5
Bromomethane
Concen: Below Cal
RT: 1.618 min Scan# 87
Delta R.T. 0.007 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16


Tgt Ion: 94 Resp: 613
Ion Ratio Lower Upper
94 100
96 69.4 74.4 111.6#

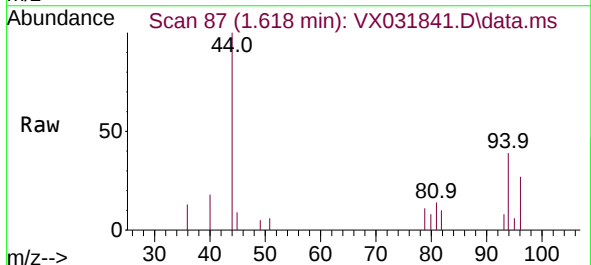



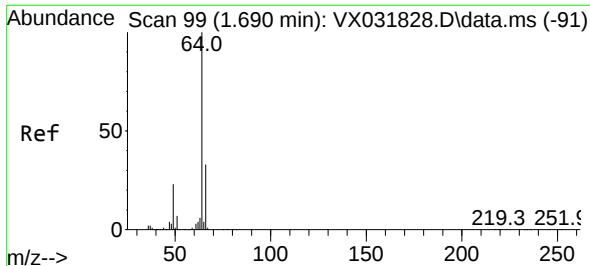


#6
Chloroethane
Concen: Below Cal
RT: 1.636 min Scan# 90
Delta R.T. -0.049 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Instrument :
MSVOA_X
ClientSampleId :



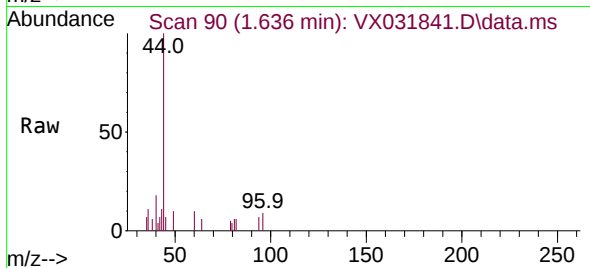



Tgt Ion: 64 Resp: 87
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#

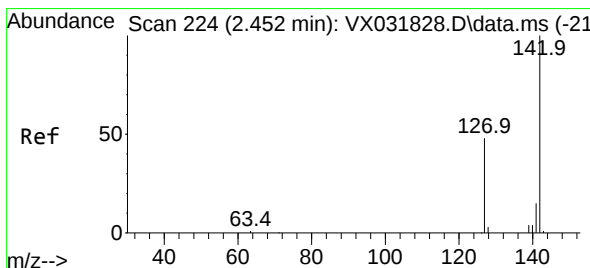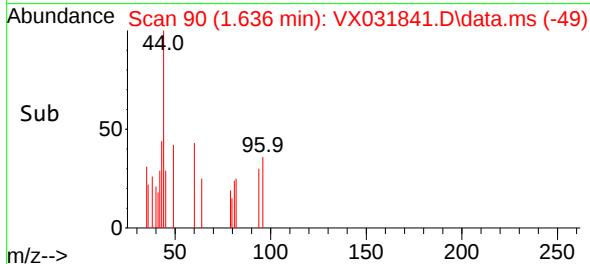

#10
Methyl Iodide
Concen: 0.261 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 142 Resp: 341
Ion Ratio Lower Upper
142 100
127 36.1 37.4 56.0#
141 0.0 11.6 17.4#

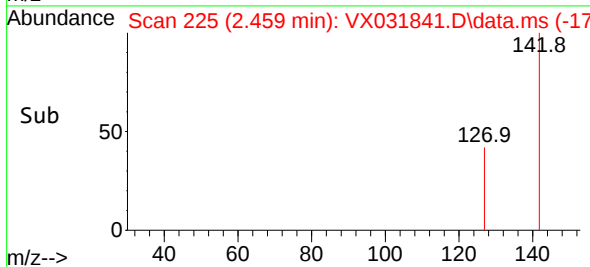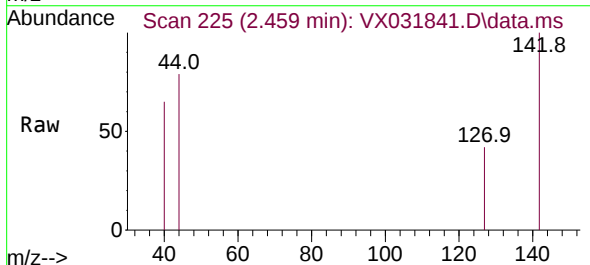



#11

Tert butyl alcohol

Concen: 0.477 ug/l

RT: 3.001 min Scan# 31

Delta R.T. -0.080 min

Lab File: VX031841.D

Acq: 03 Oct 2022 18:16

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 59 Resp: 109

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

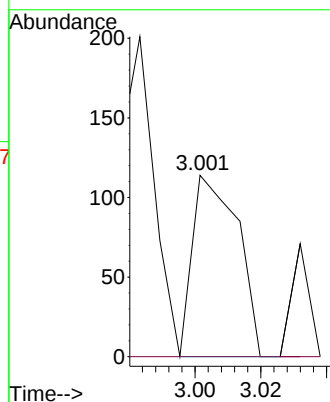

#16

Acetone

Concen: Below Cal

RT: 2.386 min Scan# 213

Delta R.T. -0.006 min

Lab File: VX031841.D




Acq: 03 Oct 2022 18:16


Tgt Ion: 43 Resp: 231

Ion Ratio Lower Upper

43 100


58 0.0 23.8 35.8#

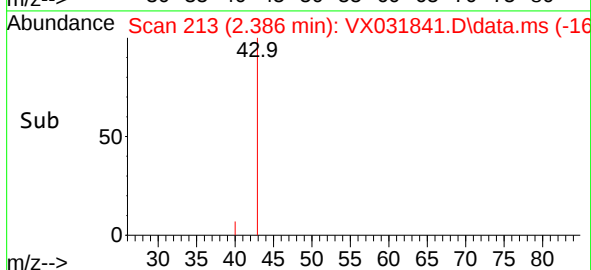






#17
Carbon Disulfide
Concen: Below Cal
RT: 2.514 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 76 Resp: 761
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

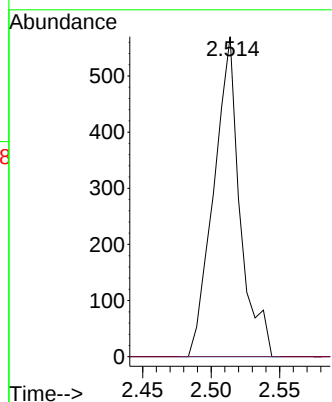

#20
Methylene Chloride
Concen: 0.296 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 84 Resp: 425
Ion Ratio Lower Upper
84 100
49 92.1 105.9 158.9#
51 29.8 32.2 48.2#
86 69.9 50.8 76.2



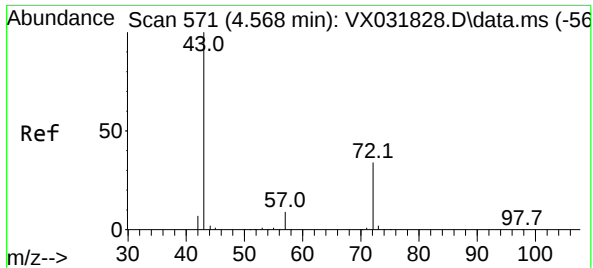

#25

2-Butanone

Concen: 0.243 ug/l

RT: 4.580 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX031841.D

Acq: 03 Oct 2022 18:16

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 183

Ion Ratio Lower Upper

43 100

72 0.0 21.1 31.7#

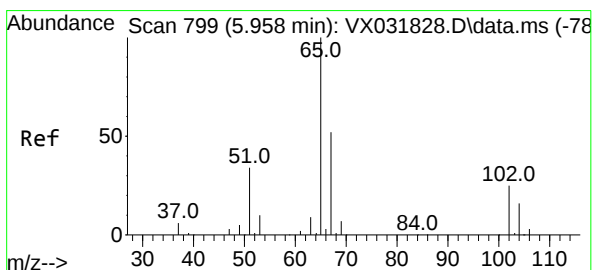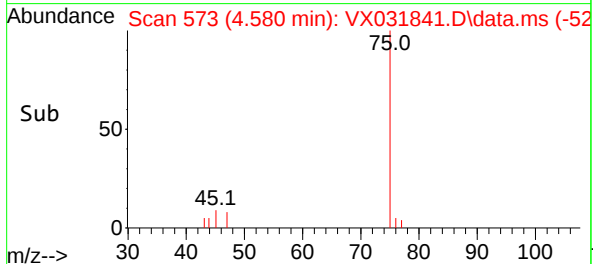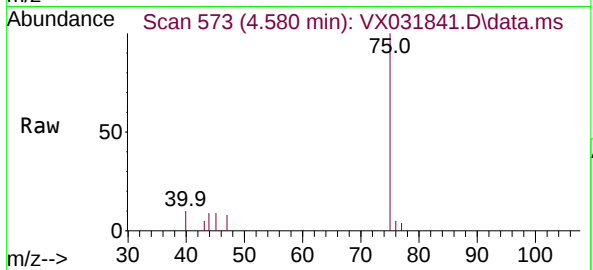

#33

1,2-Dichloroethane-d4

Concen: 50.289 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX031841.D




Acq: 03 Oct 2022 18:16


Tgt Ion: 65 Resp: 82467

Ion Ratio Lower Upper

65 100

67 50.6 0.0 102.4


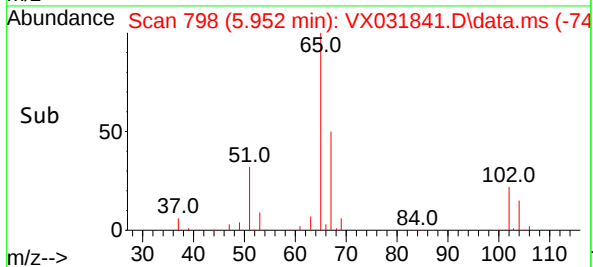

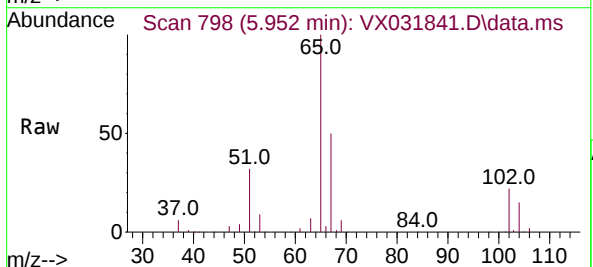




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 136364
Ion Ratio Lower Upper
114 100
63 15.9 0.0 42.6
88 15.0 0.0 33.0



#35
Dibromofluoromethane
Concen: 47.834 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion:113 Resp: 77498
Ion Ratio Lower Upper
113 100
111 100.5 82.4 123.6
192 19.3 14.1 21.1


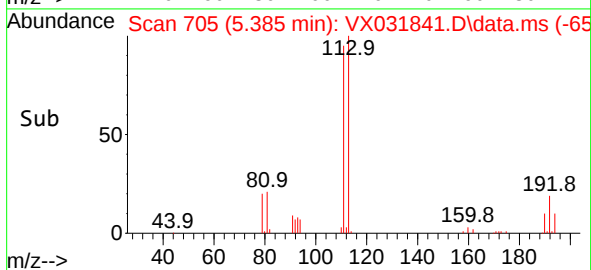






#36
1,1-Dichloropropene
Concen: 3.151 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.146 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 6330
Ion Ratio Lower Upper
75 100
110 11.1 17.5 52.5#
77 0.0 24.9 37.3#

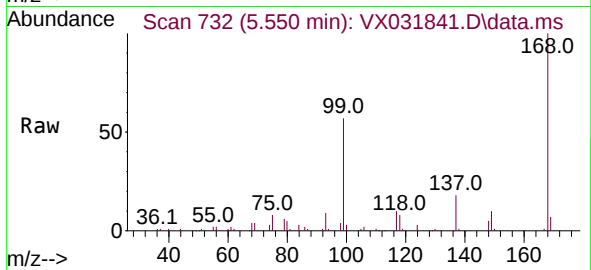

#38
Carbon Tetrachloride
Concen: 3.518 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 117 Resp: 8773
Ion Ratio Lower Upper
117 100
119 7.1 74.6 112.0#
121 0.0 25.3 37.9#



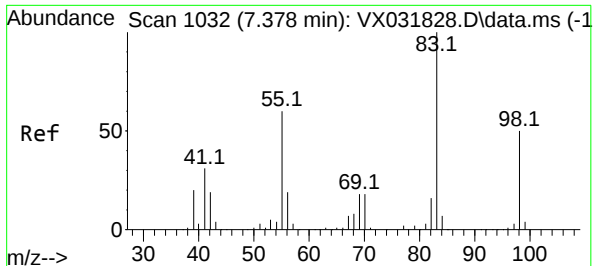

#39

Methylcyclohexane

Concen: 0.418 ug/l

RT: 7.373 min Scan# 1031

Delta R.T. -0.006 min

Lab File: VX031841.D

Acq: 03 Oct 2022 18:16

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 1031

Ion Ratio Lower Upper

83 100

55 47.7 61.0 91.4#

98 34.6 37.7 56.5#

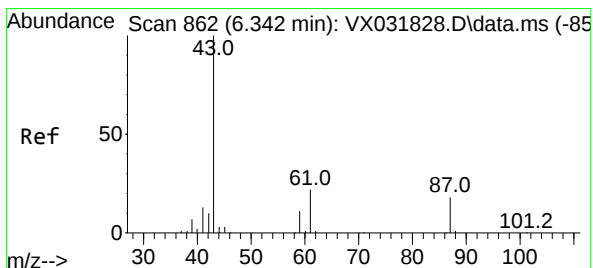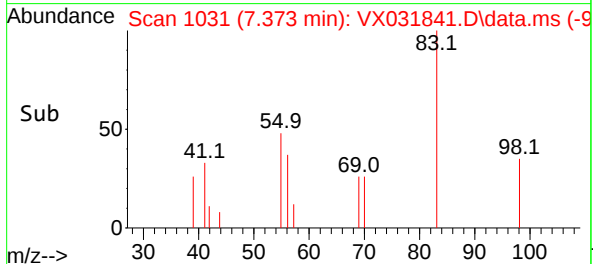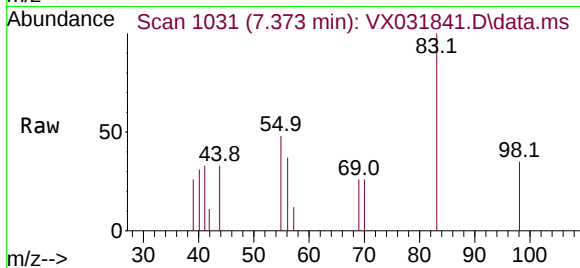

#43

Isopropyl Acetate

Concen: 0.318 ug/l

RT: 6.251 min Scan# 847

Delta R.T. -0.091 min

Lab File: VX031841.D

Acq: 03 Oct 2022 18:16




Tgt Ion: 43 Resp: 781


Ion Ratio Lower Upper

43 100

61 0.0 15.3 22.9#

87 0.0 10.6 15.8#

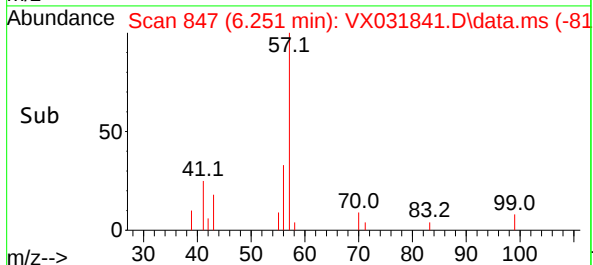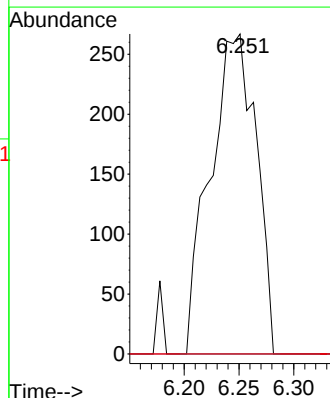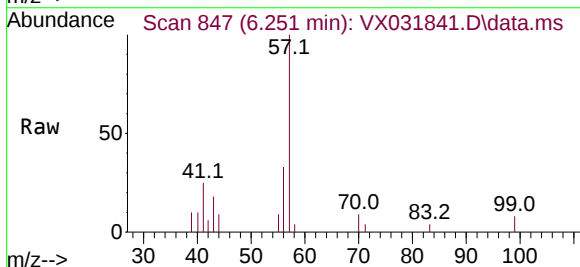



#50

Toluene-d8

Concen: 47.745 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX031841.D

Acq: 03 Oct 2022 18:16

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 98 Resp: 276720

Ion Ratio Lower Upper

98 100

100 66.8 52.5 78.7

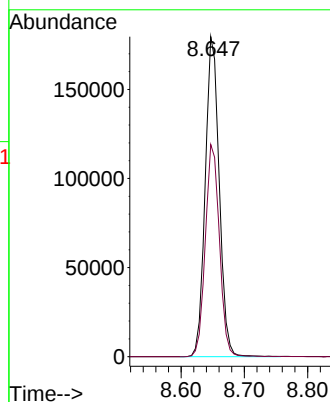

#52

Toluene

Concen: 0.205 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX031841.D




Acq: 03 Oct 2022 18:16


Tgt Ion: 92 Resp: 834

Ion Ratio Lower Upper

92 100


91 189.2 137.1 205.7

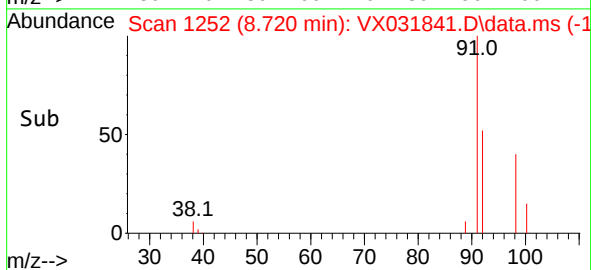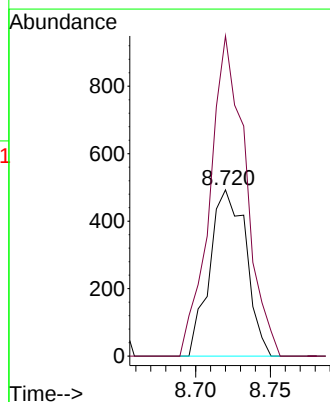






#55
 1,1,2-Trichloroethane
 Concen: 0.281 ug/l
 RT: 9.104 min Scan# 11
 Delta R.T. -0.049 min
 Lab File: VX031841.D
 Acq: 03 Oct 2022 18:16

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion:	97	Resp:	456
Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.0	103.6#
85	0.0	44.1	66.1#
99	0.0	51.3	76.9#



#62
 4-Bromofluorobenzene
 Concen: 47.384 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.000 min
 Lab File: VX031841.D
 Acq: 03 Oct 2022 18:16

Tgt Ion:	95	Resp:	98897
Ion	Ratio	Lower	Upper
95	100		
174	87.4	0.0	153.2
176	84.3	0.0	144.0









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 148692
Ion Ratio Lower Upper
117 100
82 49.6 46.8 70.2
119 31.5 26.4 39.6

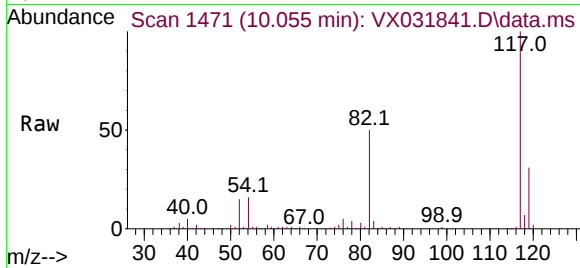

#67
Ethyl Benzene
Concen: 39.773 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 91 Resp: 295172
Ion Ratio Lower Upper
91 100
106 33.4 25.2 37.8




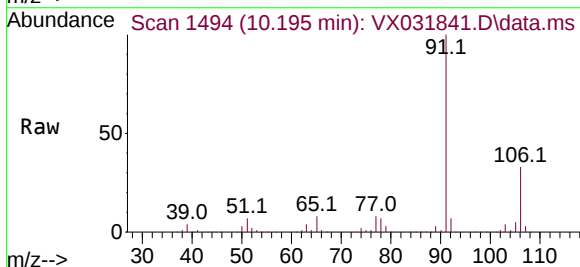




#68
m/p-Xylenes
Concen: 16.110 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 49360
Ion Ratio Lower Upper
106 100
91 188.2 161.0 241.4

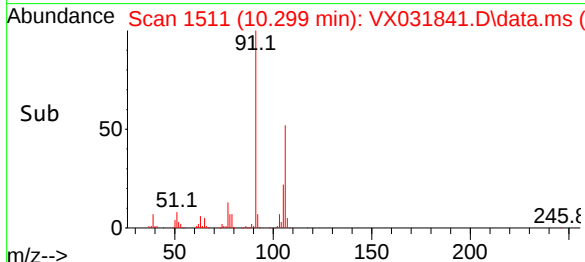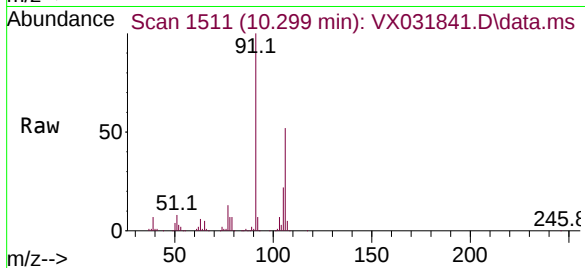

#69
o-Xylene
Concen: 0.832 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion:106 Resp: 2456
Ion Ratio Lower Upper
106 100
91 206.9 107.2 321.6


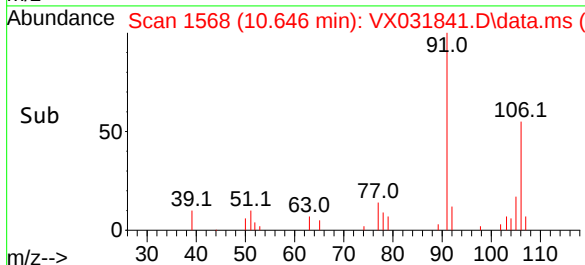

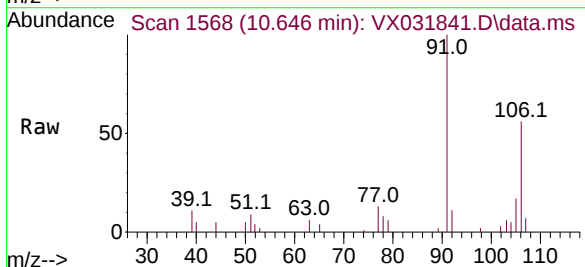


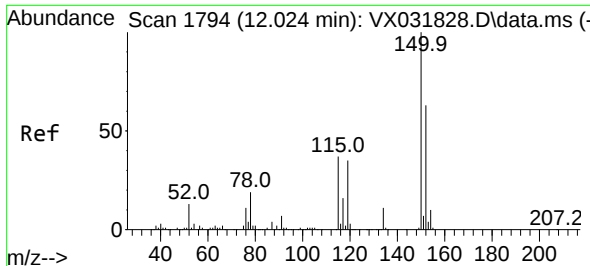

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 109127
Ion Ratio Lower Upper
152 100
115 56.5 43.4 130.1
150 153.7 0.0 346.8

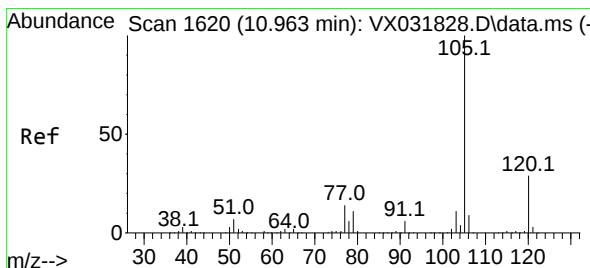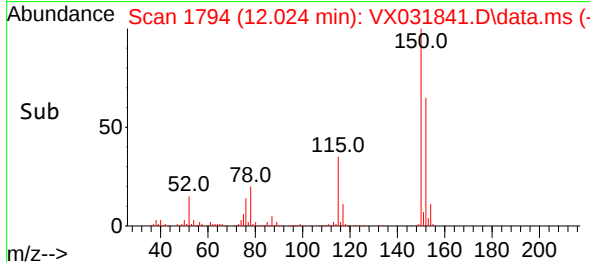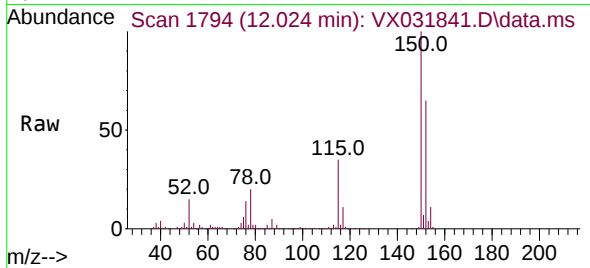

#73
Isopropylbenzene
Concen: 2.248 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion:105 Resp: 17328
Ion Ratio Lower Upper
105 100
120 29.6 13.7 41.0


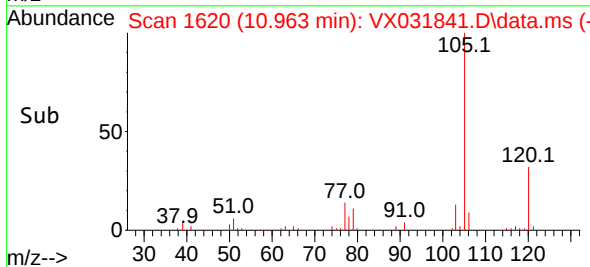

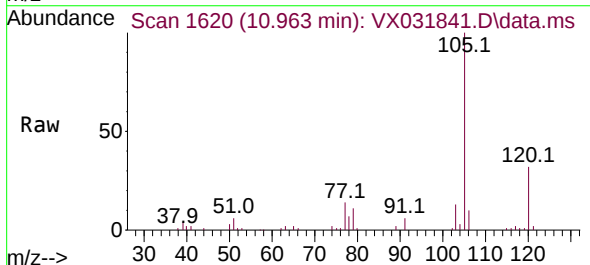




#76
1,2,3-Trichloropropane
Concen: 24.323 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 48292
Ion Ratio Lower Upper
75 100
77 1.1 20.3 60.9#



#78
n-propylbenzene
Concen: 9.922 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 91 Resp: 83594
Ion Ratio Lower Upper
91 100
120 24.8 11.8 35.4









#79
2-Chlorotoluene
Concen: 1.954 ug/l
RT: 11.396 min Scan# 1
Delta R.T. 0.030 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 9948
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#

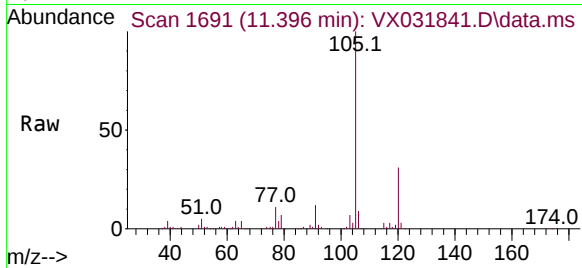

#80
1,3,5-Trimethylbenzene
Concen: 5.147 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 105 Resp: 33131
Ion Ratio Lower Upper
105 100
120 50.7 24.5 73.5


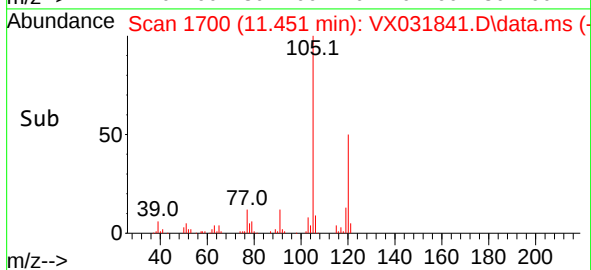

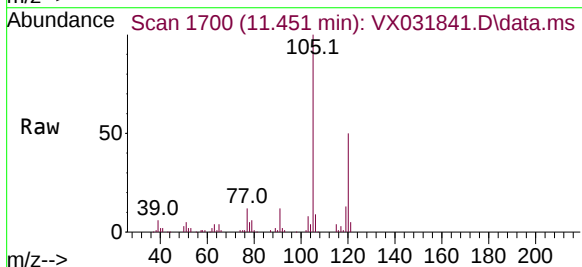




#81
trans-1,4-Dichloro-2-butene
Concen: 83.497 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 48292
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

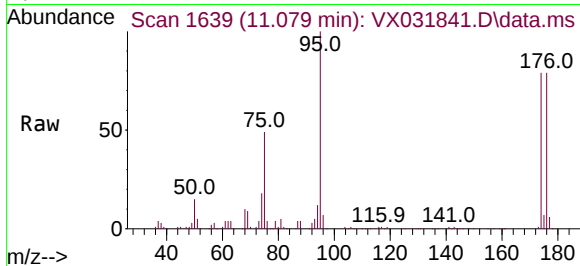

#82
4-Chlorotoluene
Concen: 0.701 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 91 Resp: 4118
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#




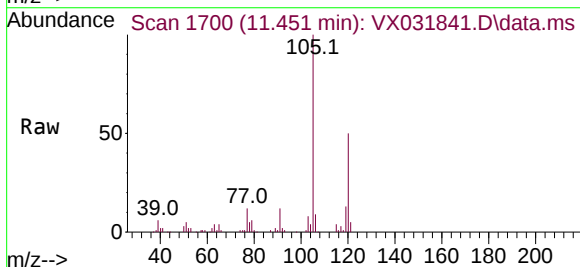




#83
tert-Butylbenzene
Concen: 9.743 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.043 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 63386
Ion Ratio Lower Upper
119 100
91 84.8 29.2 87.6
134 0.0 11.6 34.8#

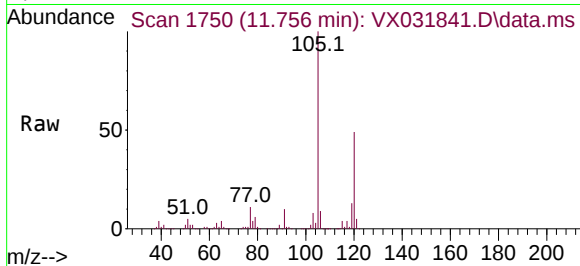

#84
1,2,4-Trimethylbenzene
Concen: 79.238 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion:105 Resp: 507615
Ion Ratio Lower Upper
105 100
120 48.3 22.6 67.8




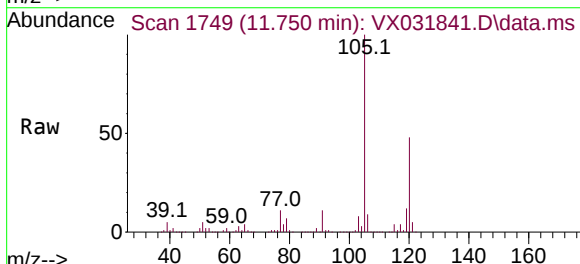




#85
 sec-Butylbenzene
 Concen: 64.813 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX031841.D
 Acq: 03 Oct 2022 18:16




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 507615
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#

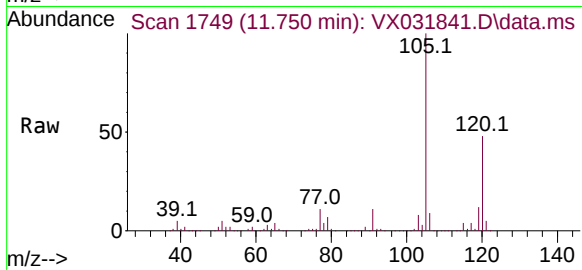

#86
 p-Isopropyltoluene
 Concen: 1.780 ug/l
 RT: 12.085 min Scan# 1804
 Delta R.T. 0.073 min
 Lab File: VX031841.D
 Acq: 03 Oct 2022 18:16

Tgt Ion:119 Resp: 12167
 Ion Ratio Lower Upper
 119 100
 134 0.0 13.4 40.2#
 91 100.3 12.4 37.2#

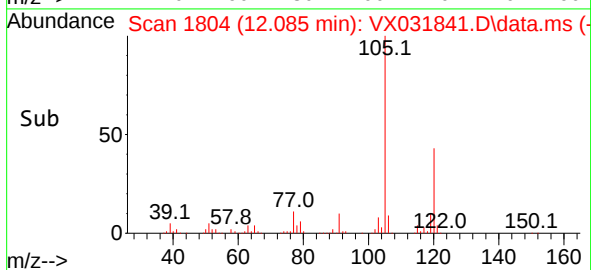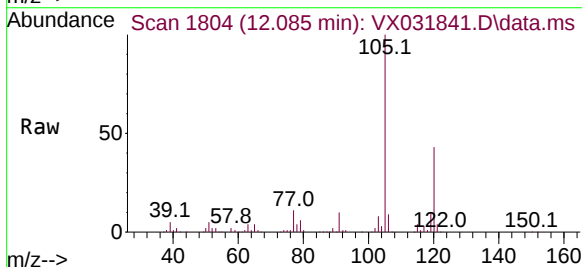



#89

n-Butylbenzene

Concen: 2.187 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX031841.D





Acq: 03 Oct 2022 18:16

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 91	Resp: 11810
Ion Ratio	Lower Upper
91	100
92	35.8 27.0 81.0
134	117.1 13.3 39.9#

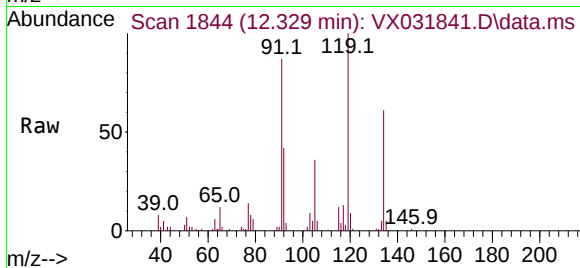

#90

Hexachloroethane

Concen: 4.530 ug/l




RT: 12.530 min Scan# 1877


Delta R.T. -0.012 min

Lab File: VX031841.D

Acq: 03 Oct 2022 18:16

Tgt Ion: 117	Resp: 5586
Ion Ratio	Lower Upper
117	100
201	0.0 34.8 104.4#


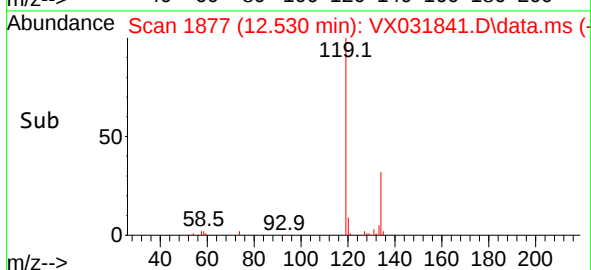

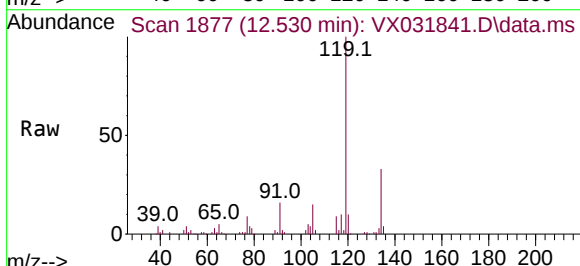


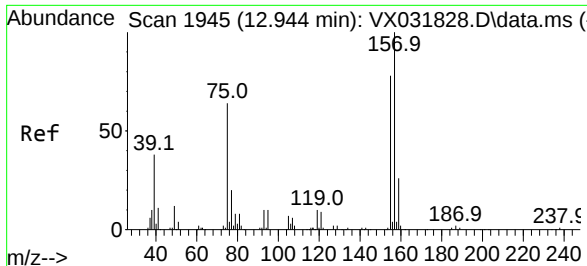

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.726 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 335
Ion Ratio Lower Upper
75 100
155 0.0 40.3 120.8#
157 0.0 51.5 154.5#

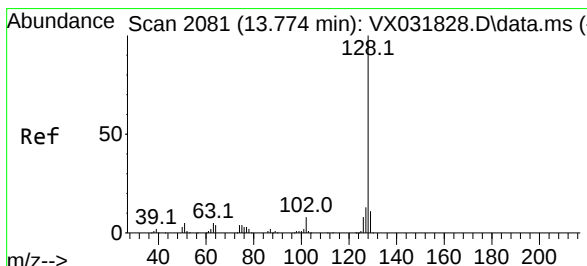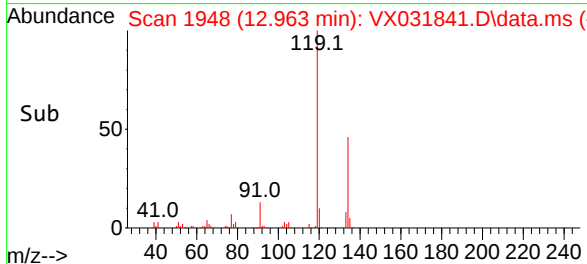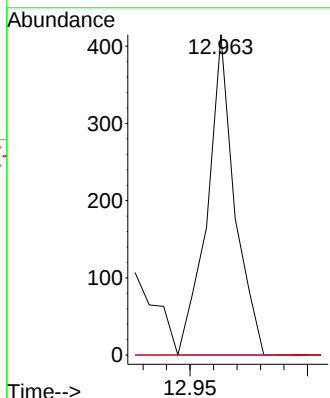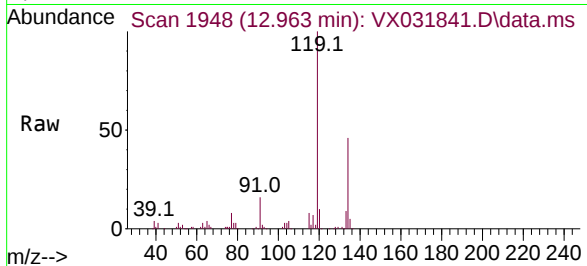

#95
Naphthalene
Concen: 28.774 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX031841.D
Acq: 03 Oct 2022 18:16

Tgt Ion: 128 Resp: 210744
Ion Ratio Lower Upper
128 100
127 12.7 10.4 15.6
129 11.0 8.8 13.2

