

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
 Data File : VX031858.D
 Acq On : 04 Oct 2022 00:49
 Operator : JC/MD
 Sample : N4887-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 220928033-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
 Title : SW846 8260

Signal : TIC: VX031858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.392	206	214	225	rBV	58901	119500	6.88%	1.118%
2	2.995	297	313	339	rBV	381443	1556720	89.67%	14.565%
3	4.581	558	573	589	rBV	496450	1736113	100.00%	16.244%
4	5.007	632	643	663	rVB2	188426	602740	34.72%	5.639%
5	5.385	694	705	720	rVV3	104659	302807	17.44%	2.833%
6	5.550	720	732	750	rVB	113953	327102	18.84%	3.060%
7	5.958	789	799	806	rBV	93786	250059	14.40%	2.340%
8	6.038	806	812	821	rVB2	30780	80534	4.64%	0.754%
9	6.257	838	848	858	rBV3	11728	42600	2.45%	0.399%
10	6.763	922	931	942	rBV	144436	346824	19.98%	3.245%
11	8.647	1234	1240	1247	rBV	509833	796597	45.88%	7.453%
12	8.714	1247	1251	1261	rVB	35395	60393	3.48%	0.565%
13	9.378	1352	1360	1366	rVB2	14931	26296	1.51%	0.246%
14	10.055	1461	1471	1484	rBV	366102	509549	29.35%	4.768%
15	10.195	1490	1494	1504	rBV2	32744	51039	2.94%	0.478%
16	10.299	1504	1511	1517	rVB	50790	78241	4.51%	0.732%
17	10.640	1563	1567	1576	rBV2	32802	53009	3.05%	0.496%
18	11.031	1626	1631	1634	rBV	22856	31673	1.82%	0.296%
19	11.079	1634	1639	1646	rVB	448567	567182	32.67%	5.307%
20	11.506	1704	1709	1715	rBV	16450	26086	1.50%	0.244%
21	11.750	1744	1749	1755	rVB	21167	29321	1.69%	0.274%
22	12.024	1788	1794	1801	rBV	558448	728000	41.93%	6.811%
23	12.244	1824	1830	1839	rBV	22758	40768	2.35%	0.381%
24	12.415	1853	1858	1863	rBV	50479	68220	3.93%	0.638%
25	12.908	1927	1939	1943	rBV	100841	160724	9.26%	1.504%
26	12.957	1943	1947	1952	rVB5	15516	32448	1.87%	0.304%
27	13.475	2027	2032	2035	rBV	75832	110550	6.37%	1.034%
28	13.512	2035	2038	2046	rVV	137407	212755	12.25%	1.991%
29	13.591	2046	2051	2058	rVB5	20106	38970	2.24%	0.365%
30	13.731	2070	2074	2077	rBV	57966	90104	5.19%	0.843%
31	13.774	2077	2081	2090	rVV	614075	819753	47.22%	7.670%
32	13.865	2093	2096	2101	rVV	23332	32707	1.88%	0.306%
33	13.926	2102	2106	2116	rVB5	14240	30755	1.77%	0.288%
34	14.097	2129	2134	2141	rBV2	22469	39956	2.30%	0.374%
35	14.311	2165	2169	2175	rBV	19347	35156	2.02%	0.329%
36	14.640	2218	2223	2234	rVB	53961	90044	5.19%	0.842%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031858.D
Acq On : 04 Oct 2022 00:49
Operator : JC/MD
Sample : N4887-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220928033-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M

Title : SW846 8260

37	14.780	2241	2246	2251	rBV2	44236	61893	3.57%	0.579%
38	15.060	2287	2292	2303	rBV	31767	52026	3.00%	0.487%
39	15.207	2308	2316	2322	rVB2	16716	30143	1.74%	0.282%
40	16.091	2453	2461	2473	rBV	102882	178761	10.30%	1.673%
41	16.328	2492	2500	2506	rVB2	16335	31068	1.79%	0.291%
42	16.688	2549	2559	2568	rBV	108343	208781	12.03%	1.953%




Sum of corrected areas: 10687967

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031858.D
Acq On : 04 Oct 2022 00:49
Operator : JC/MD
Sample : N4887-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220928033-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

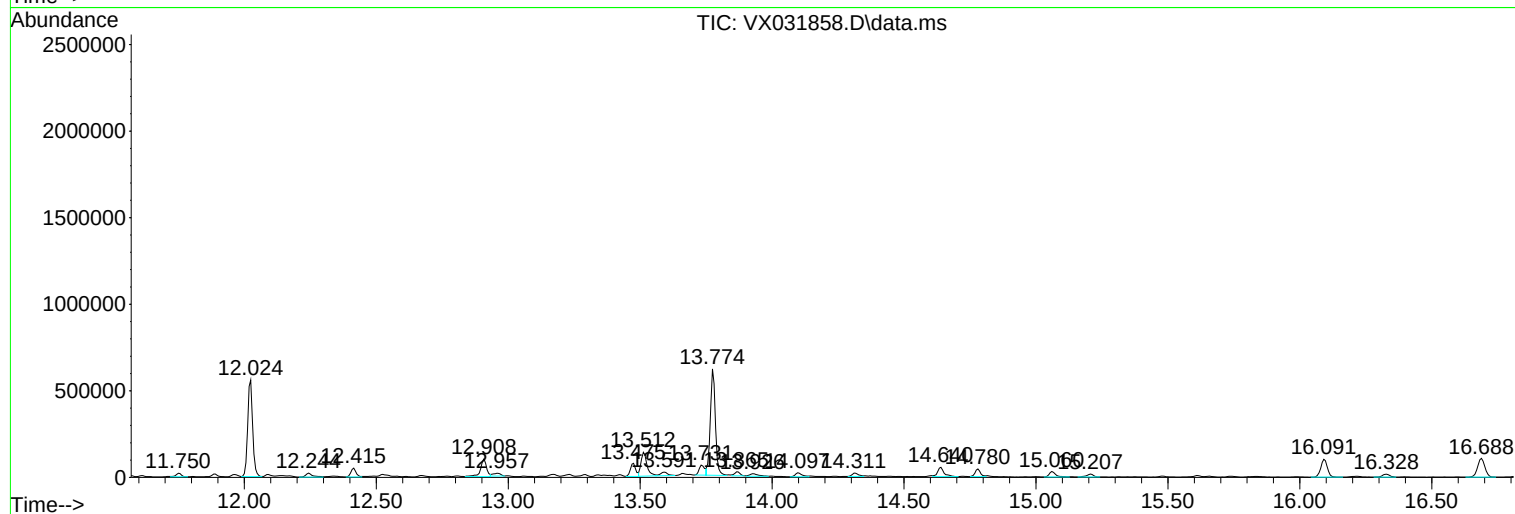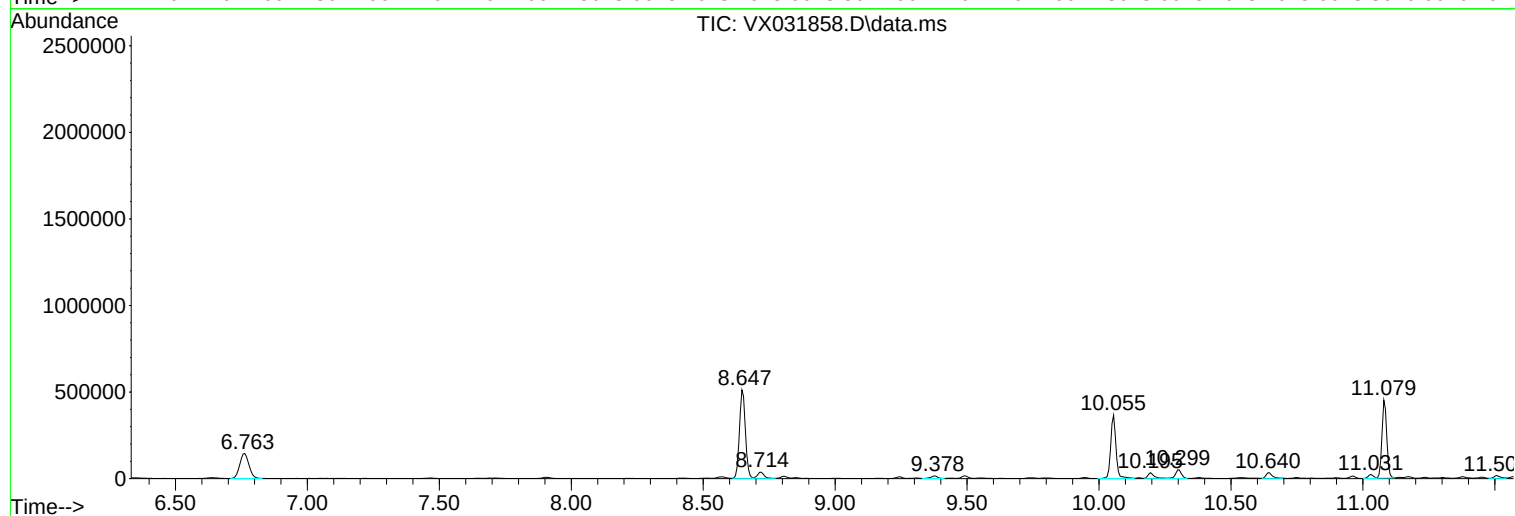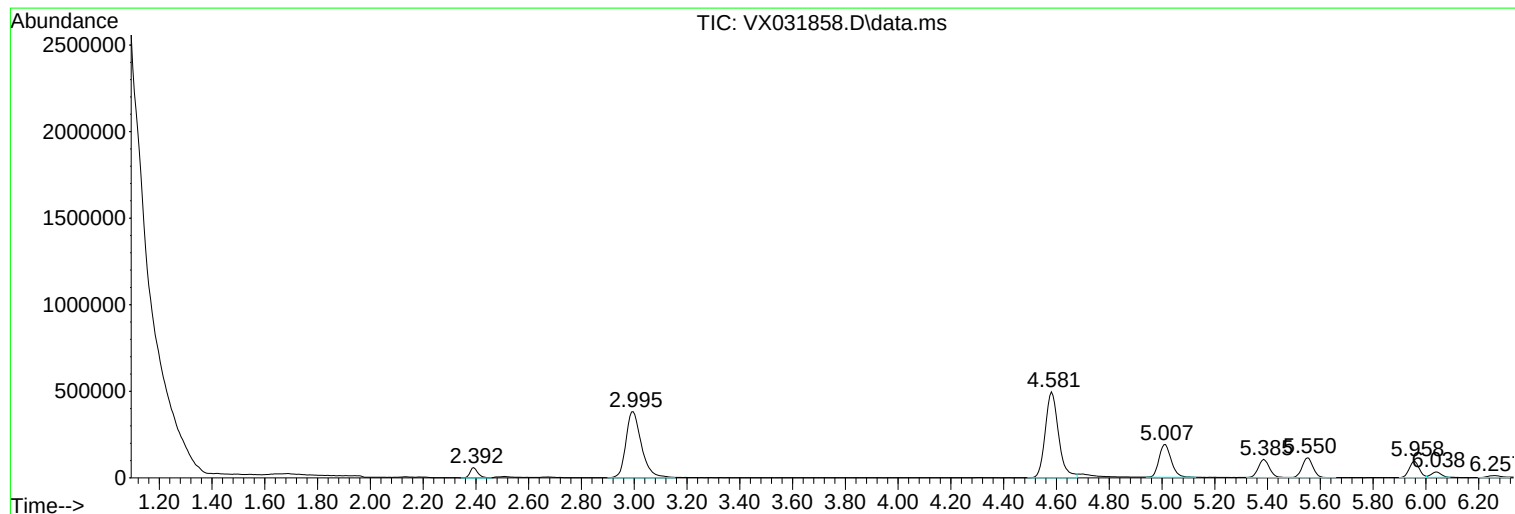

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031858.D
Acq On : 04 Oct 2022 00:49
Operator : JC/MD
Sample : N4887-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220928033-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031858.D
Acq On : 04 Oct 2022 00:49
Operator : JC/MD
Sample : N4887-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220928033-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------