

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
 Data File : VX031859.D
 Acq On : 04 Oct 2022 01:12
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
 Title : SW846 8260

Signal : TIC: VX031859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	720	rBV2	98353	283888	44.63%	8.252%
2	5.550	721	732	747	rVB	80751	227368	35.75%	6.609%
3	5.958	789	799	808	rBV2	92484	246938	38.82%	7.178%
4	6.044	808	813	823	rVB3	8716	22423	3.53%	0.652%
5	6.763	919	931	943	rBV	118646	284445	44.72%	8.268%
6	8.647	1233	1240	1248	rBV	396900	636073	100.00%	18.489%
7	8.720	1248	1252	1258	rVB2	6617	11032	1.73%	0.321%
8	10.055	1465	1471	1482	rBV	287201	383506	60.29%	11.148%
9	11.079	1634	1639	1651	rBV	335946	436533	68.63%	12.689%
10	12.024	1788	1794	1805	rBV	400443	488943	76.87%	14.212%
11	12.414	1853	1858	1863	rBV2	11844	14196	2.23%	0.413%
12	12.860	1908	1931	1933	rBV3	47841	159178	25.03%	4.627%
13	13.774	2073	2081	2094	rVV	100715	148364	23.32%	4.313%
14	13.872	2094	2097	2105	rVB3	4067	6594	1.04%	0.192%
15	14.146	2130	2142	2153	rBV5	7599	28829	4.53%	0.838%
16	14.640	2219	2223	2229	rVB	6001	8581	1.35%	0.249%
17	15.060	2286	2292	2298	rBV	10283	16676	2.62%	0.485%
18	16.091	2455	2461	2467	rBV	8952	16555	2.60%	0.481%
19	16.688	2552	2559	2565	rBV	10346	20128	3.16%	0.585%




Sum of corrected areas: 3440250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031859.D
Acq On : 04 Oct 2022 01:12
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

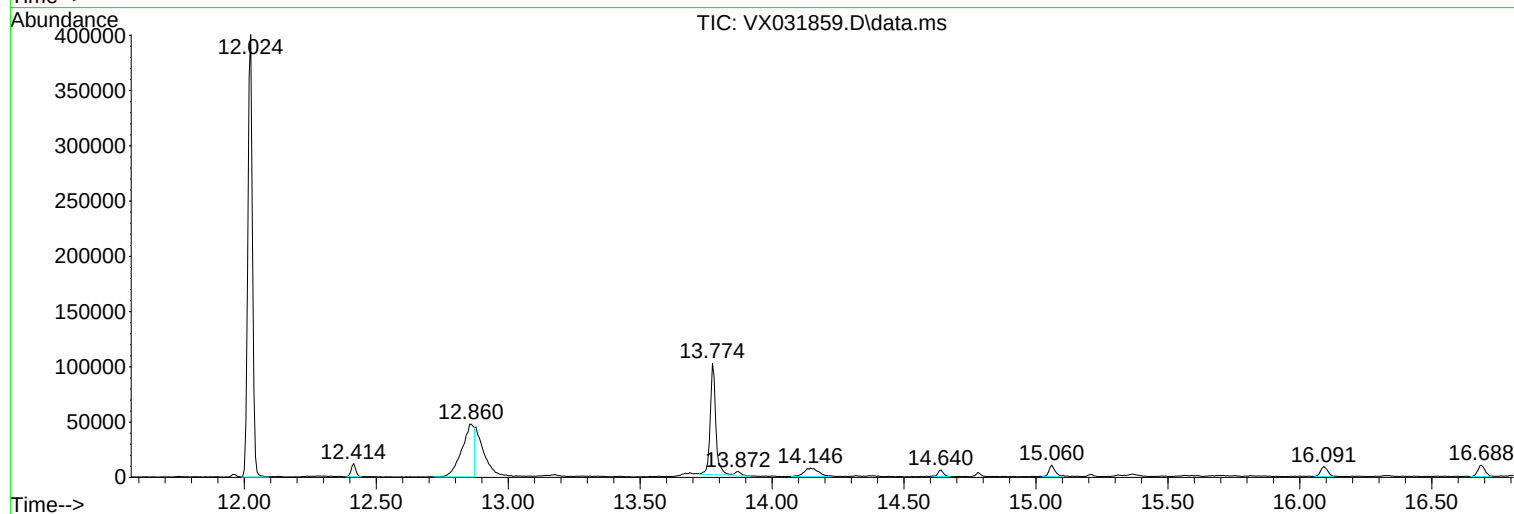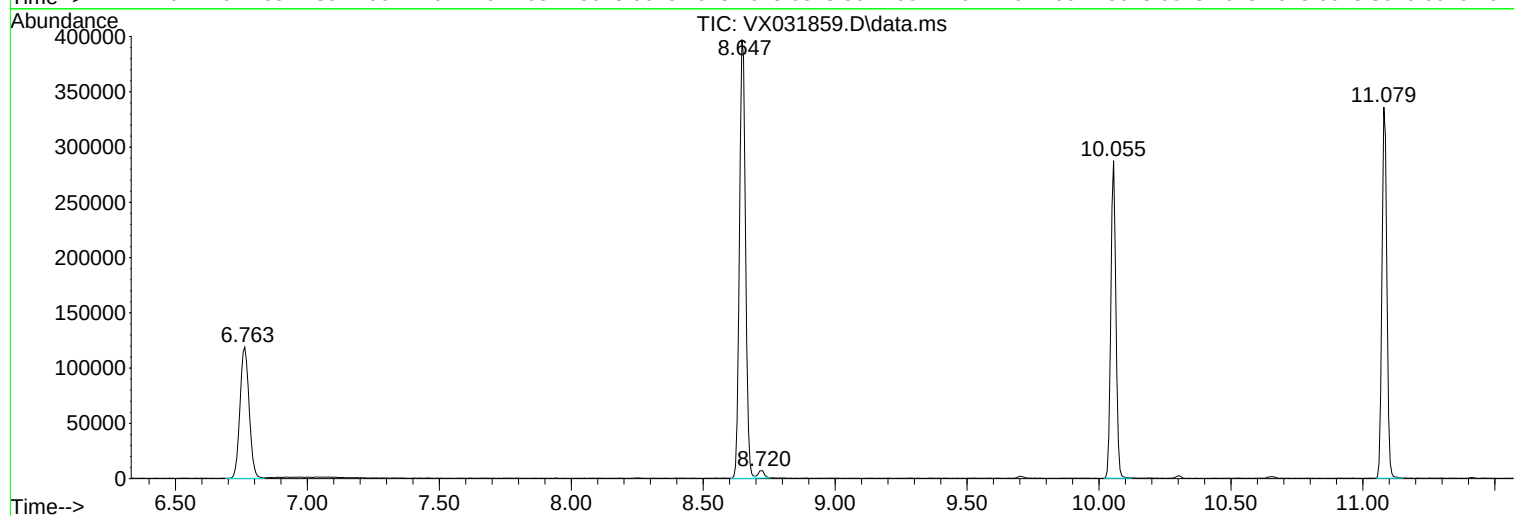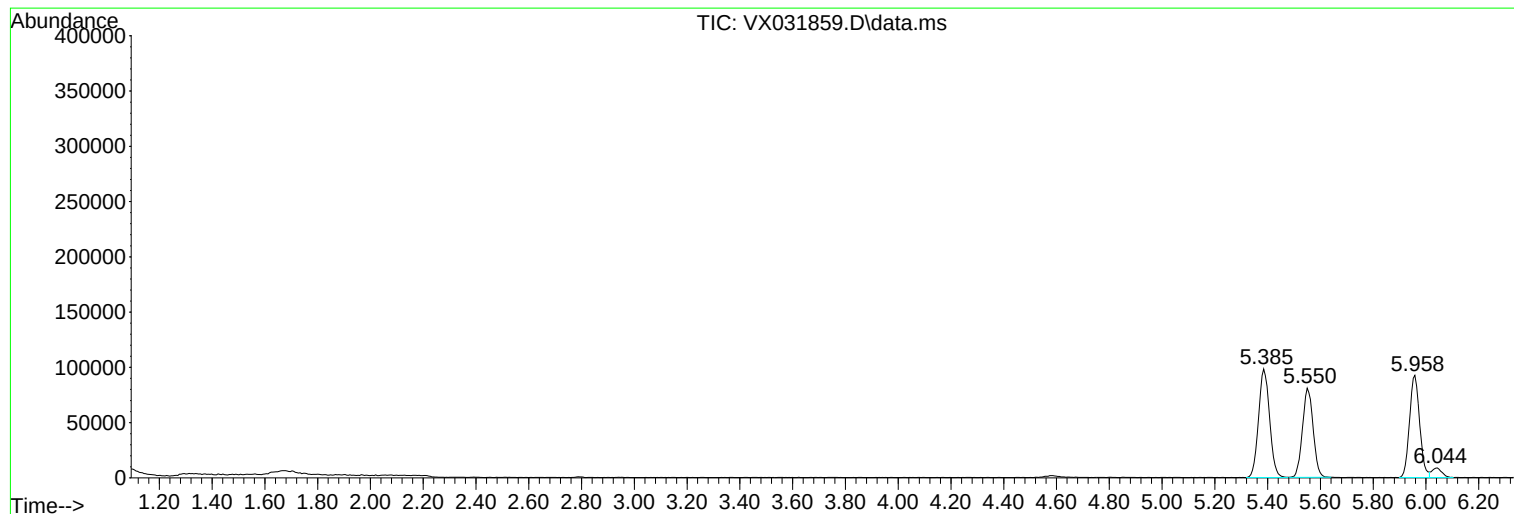

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031859.D
Acq On : 04 Oct 2022 01:12
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.860	16.28 ug/l	159178	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorene	166	C13H10	000086-73-7	96
2			1,3-Benzodioxole-5-carboxylic acid	166	C8H6O4	000094-53-1	59
3			3-Trifluoromethylbenzhydryl chlo...	270	C14H10ClF3	067240-79-3	56
4			1H-Phenylene	166	C13H10	000203-80-5	53
5			Benzene, 5-heptene-1,3-diyn-1-yl-	166	C13H10	013678-98-3	50

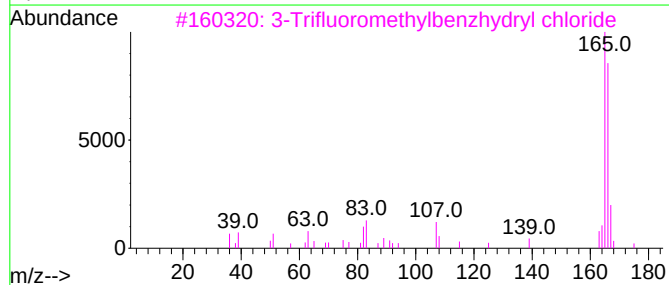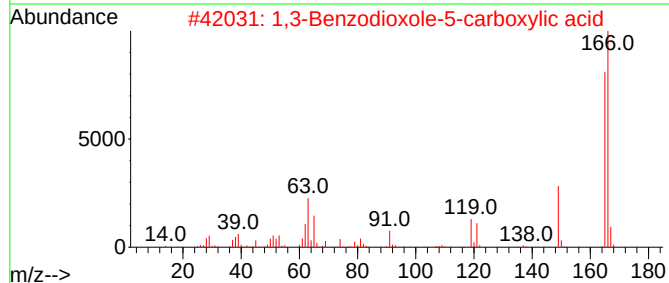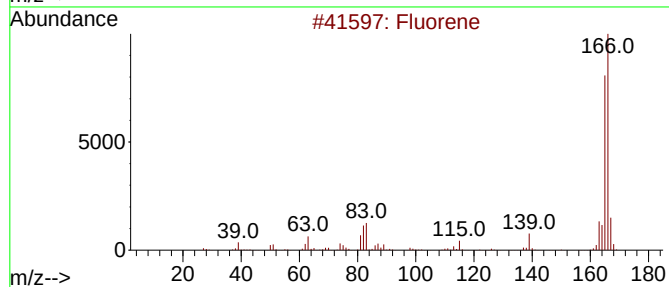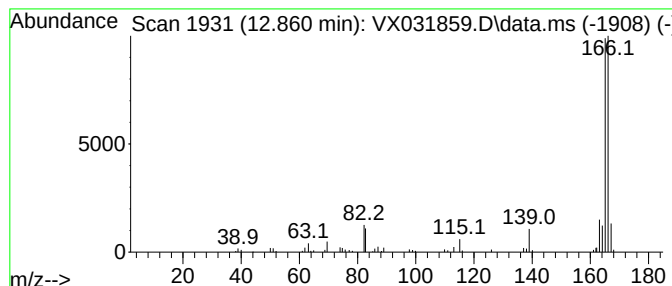

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031859.D
Acq On : 04 Oct 2022 01:12
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorene	12.860	16.3	ug/l	159178	4	12.024	488943	50.0