
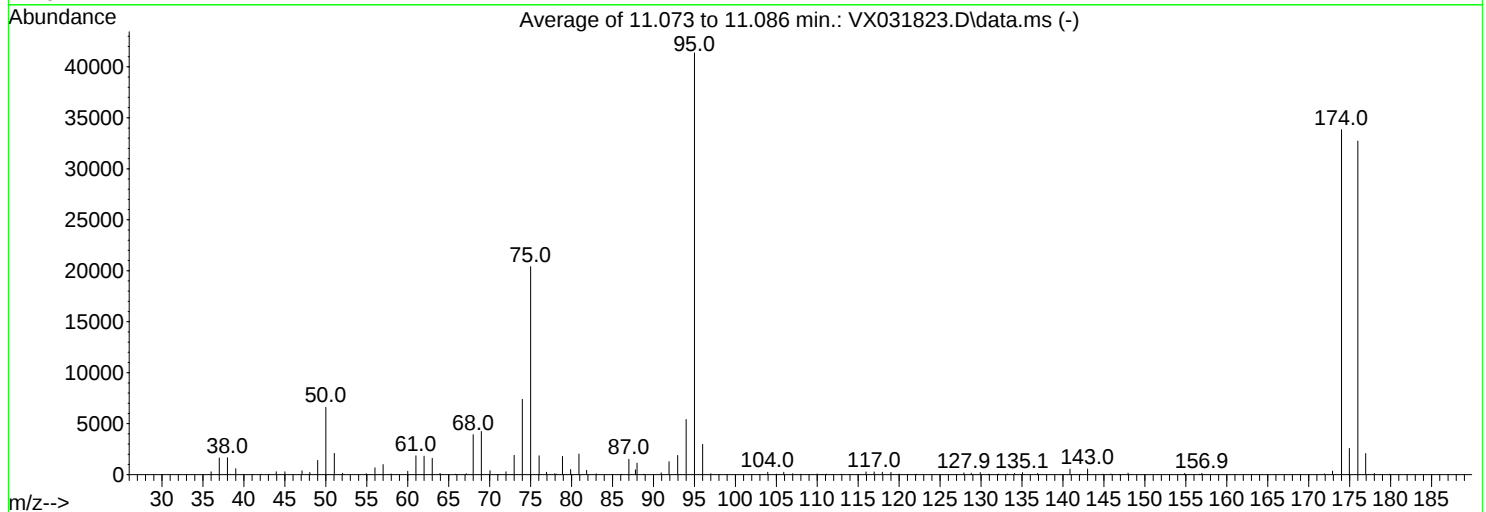


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031823.D
Acq On : 03 Oct 2022 09:08
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Title : SW846 8260
Last Update : Tue Oct 04 06:59:30 2022

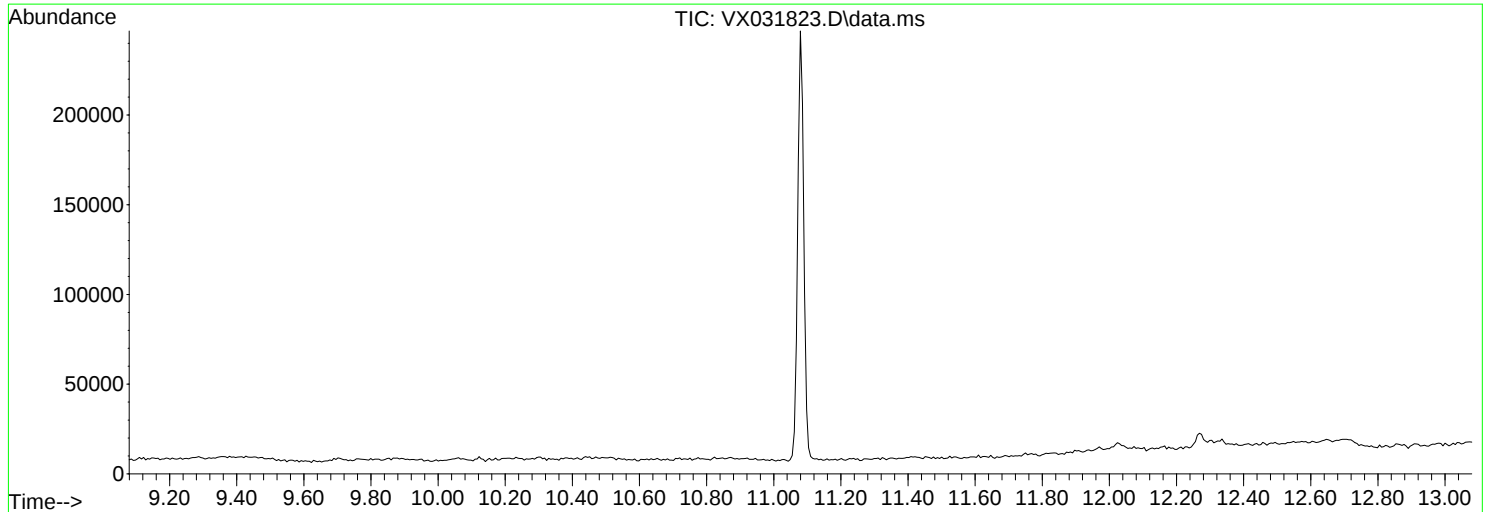

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	6608	PASS
75	95	30	60	49.3	20396	PASS
95	95	100	100	100.0	41373	PASS
96	95	5	9	7.2	2968	PASS
173	174	0.00	2	1.0	346	PASS
174	95	50	100	81.8	33840	PASS
175	174	5	9	7.6	2576	PASS
176	174	95	101	96.7	32723	PASS
177	176	5	9	6.4	2078	PASS