
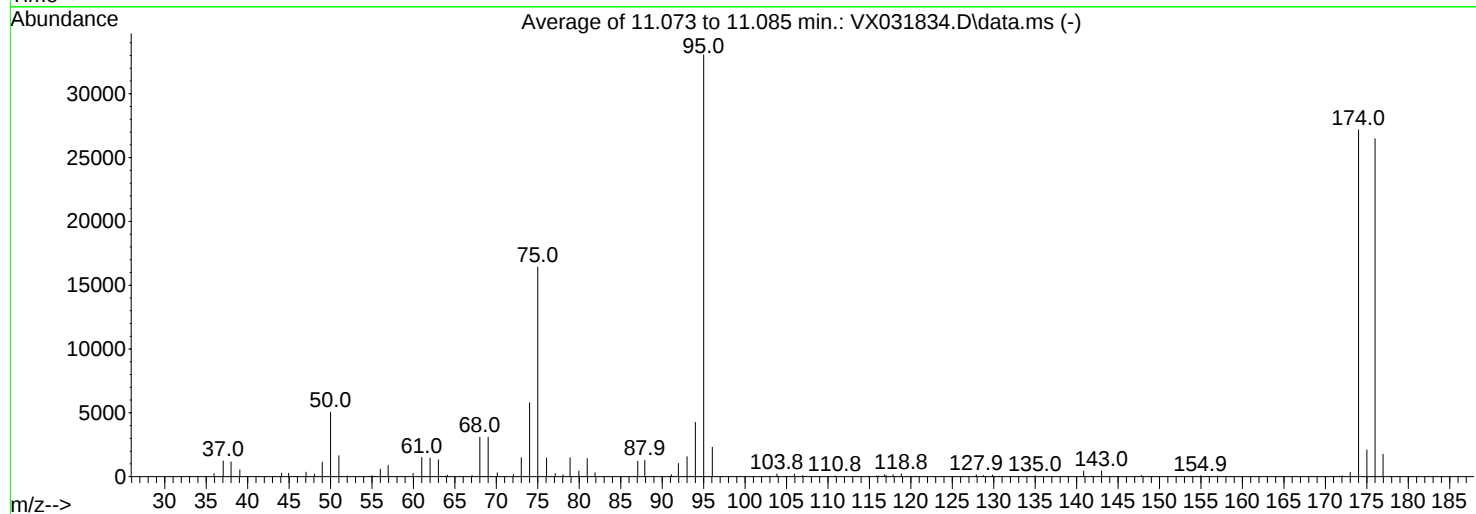


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100322\
Data File : VX031834.D
Acq On : 03 Oct 2022 14:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Title : SW846 8260
Last Update : Tue Oct 04 06:59:30 2022

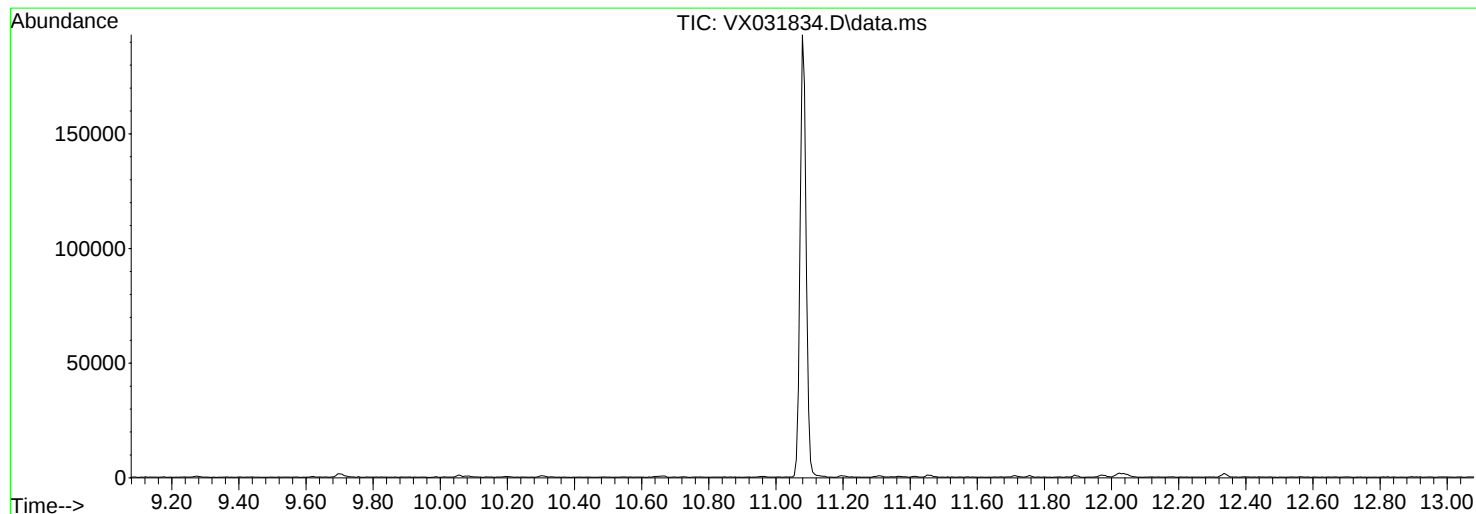

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	5051	PASS
75	95	30	60	49.7	16433	PASS
95	95	100	100	100.0	33051	PASS
96	95	5	9	7.0	2302	PASS
173	174	0.00	2	1.3	342	PASS
174	95	50	100	82.2	27168	PASS
175	174	5	9	7.7	2091	PASS
176	174	95	101	97.5	26483	PASS
177	176	5	9	6.6	1758	PASS