

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
 Data File : VX043250.D
 Acq On : 03 Oct 2024 10:34
 Operator : JC/MD
 Sample : P4231-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT101D1-20240924

Quant Time: Oct 04 01:27:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 16:50:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	82876	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	161117	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	142155	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	61992	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	72937	53.888	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 107.780%	
35) Dibromofluoromethane	5.385	113	52591	47.331	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 94.660%	
50) Toluene-d8	8.647	98	193229	50.182	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.360%	
62) 4-Bromofluorobenzene	11.079	95	70683	50.528	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 101.060%	


Target Compounds				Qvalue		
2) Dichlorodifluoromethane	1.166	85	1127	1.169	ug/l	97
5) Bromomethane	1.599	94	135	0.332	ug/l #	60
7) Trichlorofluoromethane	1.868	101	298	0.201	ug/l	91
9) 1,1,2-Trichlorotrifluo...	2.319	101	13449	14.504	ug/l	98
11) Tert butyl alcohol	2.947	59	24743	96.066	ug/l #	75
12) 1,1-Dichloroethene	2.313	96	4600	4.996	ug/l	95
13) Acrolein	2.233	56	56	0.230	ug/l #	1
15) Acrylonitrile	2.953	53	460	0.875	ug/l #	16
16) Acetone	2.392	43	880	1.557	ug/l	95
18) Methyl Acetate	2.703	43	383	0.270	ug/l #	51
19) Methyl tert-butyl Ether	2.934	73	1394	0.423	ug/l	93
20) Methylene Chloride	2.782	84	260	0.249	ug/l #	76
23) Vinyl Acetate	3.757	43	20	6.345	ug/l #	71
24) 1,1-Dichloroethane	3.611	63	1733	0.978	ug/l #	81
25) 2-Butanone	4.593	43	876	1.130	ug/l #	49
26) 2,2-Dichloropropane	4.593	77	993	0.589	ug/l #	54
27) cis-1,2-Dichloroethene	4.501	96	2091	1.830	ug/l	88
28) Bromochloromethane	5.086	49	141	0.202	ug/l #	10
30) Chloroform	5.099	83	2103	1.080	ug/l	89
31) Cyclohexane	5.544	56	2127	1.456	ug/l #	27
32) 1,1,1-Trichloroethane	5.367	97	508	0.284	ug/l #	46
36) 1,1-Dichloropropene	5.544	75	7238	5.156	ug/l #	49
38) Carbon Tetrachloride	5.678	117	1333	0.802	ug/l	85
39) Methylcyclohexane	7.117	83	3084	1.747	ug/l #	1
44) Trichloroethene	7.123	130	225418	199.694	ug/l	94
49) 1,4-Dioxane	7.684	88	483	18.188	ug/l	99
51) 4-Methyl-2-Pentanone	8.647	43	1050	0.621	ug/l #	1
55) 1,1,2-Trichloroethane	9.165	97	723	0.682	ug/l #	80
60) Dibromochloromethane	9.281	129	481	0.391	ug/l #	11
64) Tetrachloroethene	9.275	164	426	0.432	ug/l	89
76) 1,2,3-Trichloropropane	11.079	75	39176	28.491	ug/l #	33
81) trans-1,4-Dichloro-2-b...	11.079	75	39176	73.838	ug/l #	8

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
Data File : VX043250.D
Acq On : 03 Oct 2024 10:34
Operator : JC/MD
Sample : P4231-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924

Quant Time: Oct 04 01:27:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 16:50:57 2024
Response via : Initial Calibration




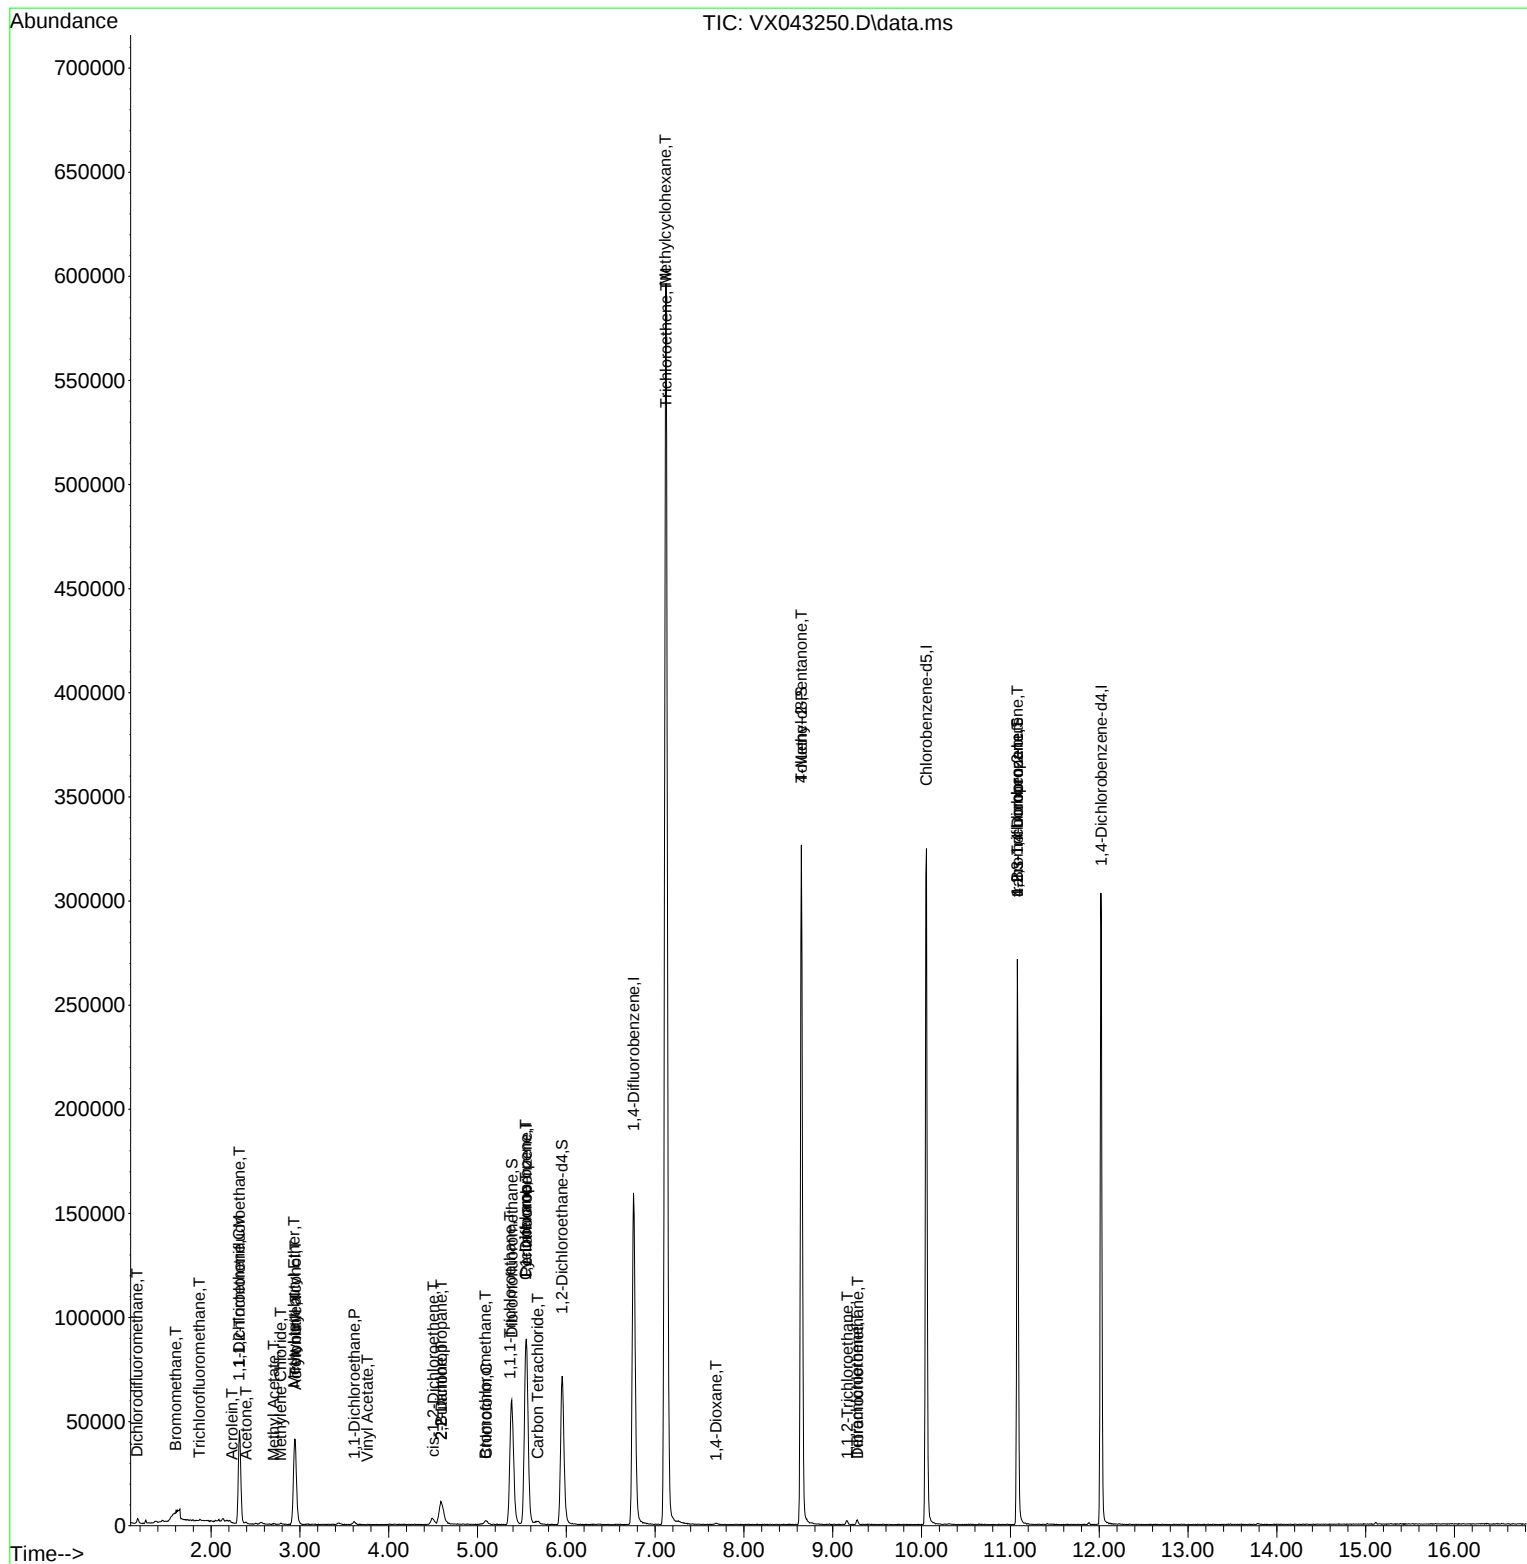




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument : MSVOA_X
ClientSampleId : TT101D1-20240924


Tgt Ion:168 Resp: 82876
Ion Ratio Lower Upper
168 100
99 63.9 49.7 74.5

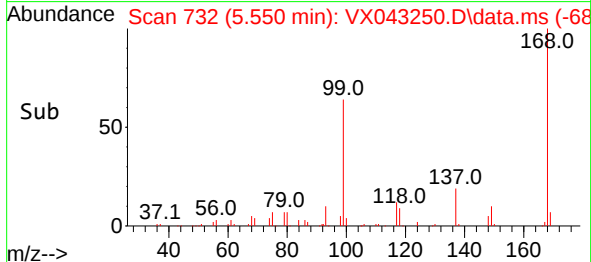

#2
Dichlorodifluoromethane
Concen: 1.169 ug/l
RT: 1.166 min Scan# 13
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 85 Resp: 1127
Ion Ratio Lower Upper
85 100
87 32.4 17.1 51.2







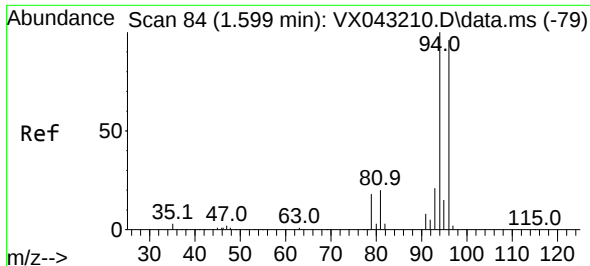

#5
Bromomethane
Concen: 0.332 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion: 94 Resp: 135
Ion Ratio Lower Upper
94 100
96 57.1 76.6 115.0#

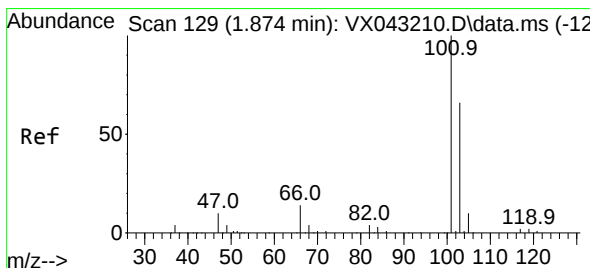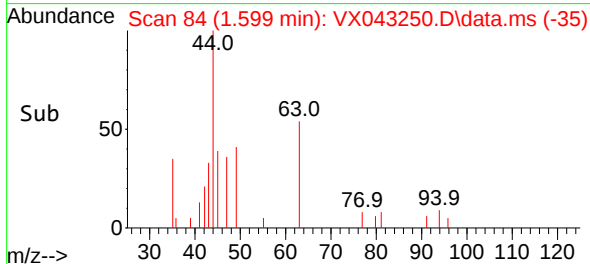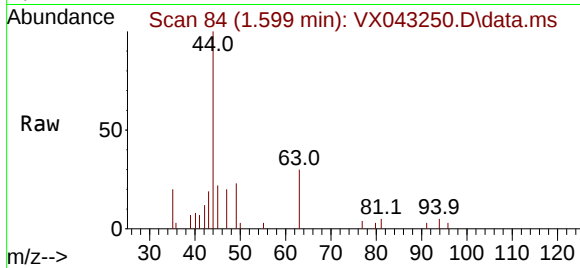

#7
Trichlorofluoromethane
Concen: 0.201 ug/l
RT: 1.868 min Scan# 128
Delta R.T. -0.006 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 101 Resp: 298
Ion Ratio Lower Upper
101 100
103 59.0 52.7 79.1


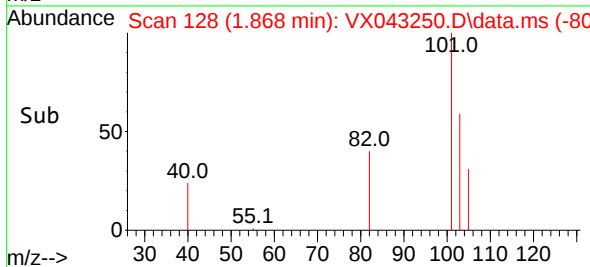

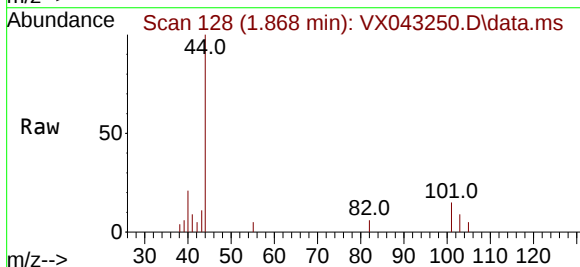




#9
1,1,2-Trichlorotrifluoroethane
Concen: 14.504 ug/l
RT: 2.319 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion:101 Resp: 13449
Ion Ratio Lower Upper
101 100
85 44.6 37.0 55.6
151 74.0 60.0 90.0



#11
Tert butyl alcohol
Concen: 96.066 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.049 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 59 Resp: 24743
Ion Ratio Lower Upper
59 100
57 1.5 8.6 13.0#





#12

1,1-Dichloroethene

Concen: 4.996 ug/l

RT: 2.313 min Scan# 201

Delta R.T. 0.000 min

Lab File: VX043250.D

Acq: 03 Oct 2024 10:34

Instrument :

MSVOA_X

ClientSampleId :

TT101D1-20240924





Tgt Ion: 96 Resp: 4600

Ion Ratio Lower Upper

96 100

61 155.4 130.6 195.8

98 62.4 51.7 77.5



#13

Acrolein

Concen: 0.230 ug/l

RT: 2.233 min Scan# 188

Delta R.T. -0.006 min

Lab File: VX043250.D




Acq: 03 Oct 2024 10:34


Tgt Ion: 56 Resp: 56

Ion Ratio Lower Upper

56 100

55 201.8 57.4 86.0#

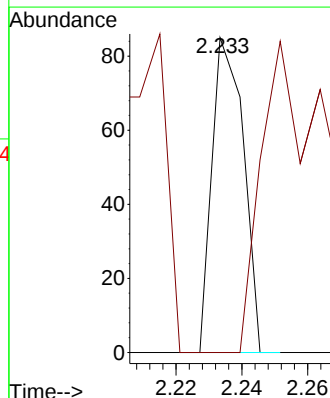



#15

Acrylonitrile

Concen: 0.875 ug/l

RT: 2.953 min Scan# 306

Delta R.T. -0.116 min

Lab File: VX043250.D

Acq: 03 Oct 2024 10:34

Instrument :

MSVOA_X

ClientSampleId :

TT101D1-20240924





Tgt Ion: 53 Resp: 460

Ion Ratio Lower Upper

53 100

52 0.0 67.6 101.4#

51 0.0 30.3 45.5#

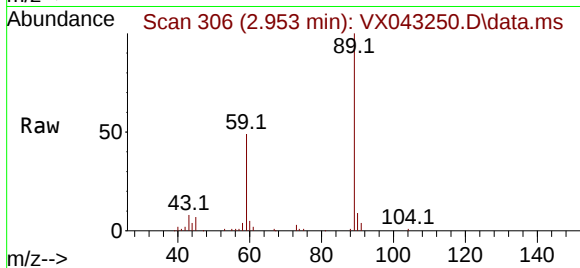

#16

Acetone

Concen: 1.557 ug/l

RT: 2.392 min Scan# 214

Delta R.T. 0.006 min

Lab File: VX043250.D




Acq: 03 Oct 2024 10:34


Tgt Ion: 43 Resp: 880

Ion Ratio Lower Upper

43 100

58 30.7 22.6 33.8




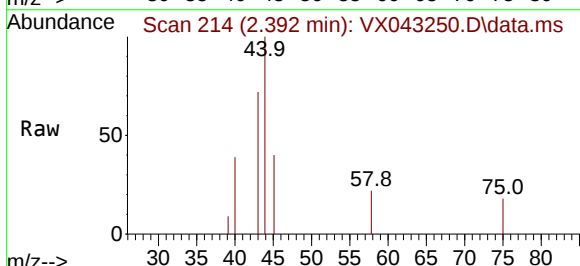




#18
Methyl Acetate
Concen: 0.270 ug/l
RT: 2.703 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion: 43 Resp: 383
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7#



#19
Methyl tert-butyl Ether
Concen: 0.423 ug/l
RT: 2.934 min Scan# 303
Delta R.T. -0.183 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 73 Resp: 1394
Ion Ratio Lower Upper
73 100
57 17.6 16.7 25.1









#20
Methylene Chloride
Concen: 0.249 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion: 84	Resp: 260
Ion Ratio	Lower Upper
84 100	
49 96.3	96.7 145.1#
51 48.2	30.4 45.6#
86 44.0	54.7 82.1#



#23
Vinyl Acetate
Concen: 6.345 ug/l
RT: 3.757 min Scan# 438
Delta R.T. 0.036 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 43	Resp: 20
Ion Ratio	Lower Upper
43 100	
86 0.0	8.8 13.2#

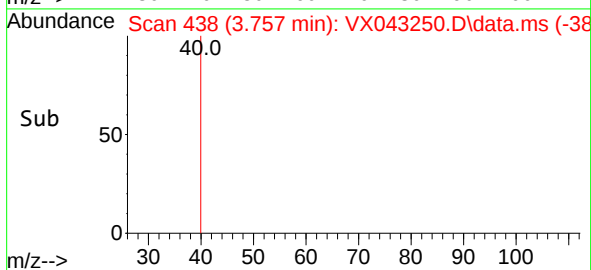



#24

1,1-Dichloroethane

Concen: 0.978 ug/l

RT: 3.611 min Scan# 41

Delta R.T. 0.006 min

Lab File: VX043250.D


Acq: 03 Oct 2024 10:34

Instrument :




MSVOA_X

ClientSampleId :

TT101D1-20240924

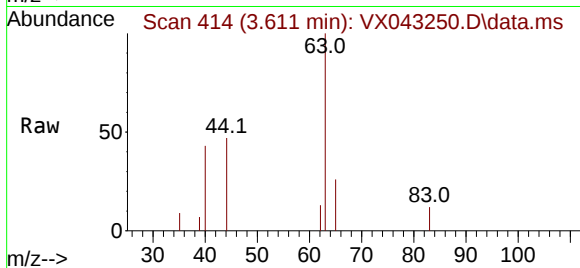

Tgt Ion:	63	Resp:	1733
Ion	Ratio	Lower	Upper
63	100		
98	0.0	3.8	11.2#
100	0.0	2.5	7.4#

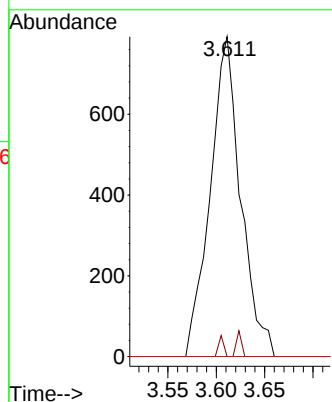

#25

2-Butanone

Concen: 1.130 ug/l




RT: 4.593 min Scan# 575


Delta R.T. 0.031 min

Lab File: VX043250.D

Acq: 03 Oct 2024 10:34

Tgt Ion:	43	Resp:	876
Ion	Ratio	Lower	Upper
43	100		
72	0.0	20.6	31.0#


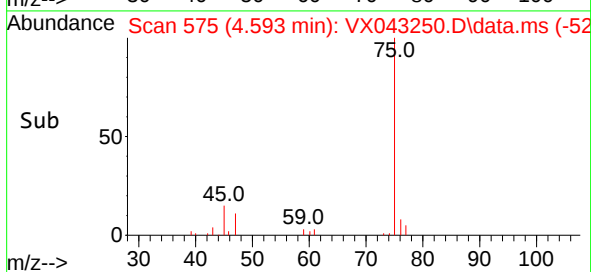
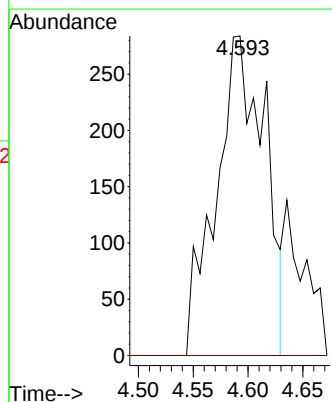
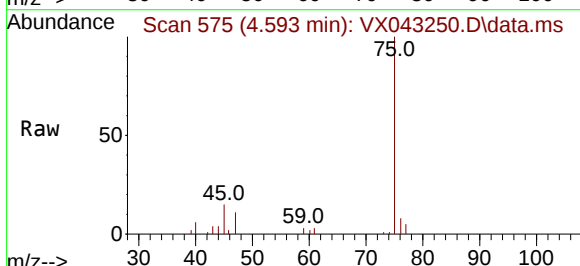




#26
2,2-Dichloropropane
Concen: 0.589 ug/l
RT: 4.593 min Scan# 51
Delta R.T. 0.122 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion: 77 Resp: 993
Ion Ratio Lower Upper
77 100
97 0.0 10.8 32.3#

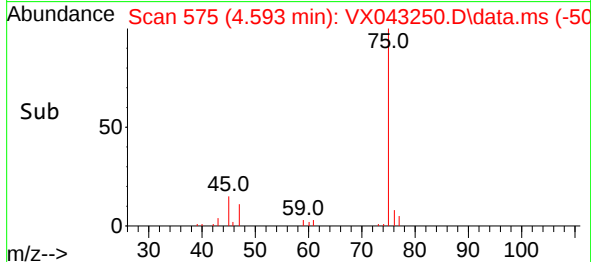

#27
cis-1,2-Dichloroethene
Concen: 1.830 ug/l
RT: 4.501 min Scan# 560
Delta R.T. 0.018 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 96 Resp: 2091
Ion Ratio Lower Upper
96 100
61 127.7 0.0 298.2
98 64.8 0.0 128.6





#28

Bromochloromethane

Concen: 0.202 ug/l

RT: 5.086 min Scan# 61

Delta R.T. 0.189 min

Lab File: VX043250.D

Acq: 03 Oct 2024 10:34

Instrument :

MSVOA_X

ClientSampleId :

TT101D1-20240924





Tgt Ion: 49 Resp: 141

Ion Ratio Lower Upper

49 100

129 0.0 0.0 4.0

130 0.0 65.5 98.3#

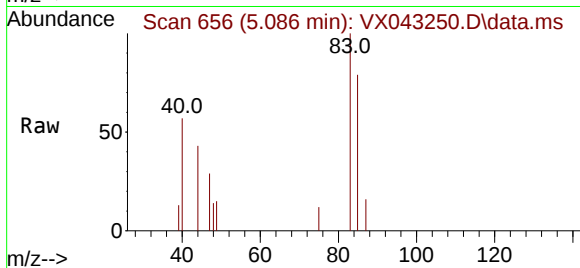

#30

Chloroform

Concen: 1.080 ug/l

RT: 5.099 min Scan# 658

Delta R.T. 0.006 min

Lab File: VX043250.D




Acq: 03 Oct 2024 10:34


Tgt Ion: 83 Resp: 2103

Ion Ratio Lower Upper

83 100


85 56.9 52.5 78.7

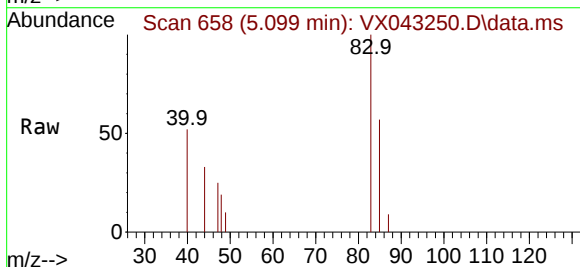






#31
Cyclohexane
Concen: 1.456 ug/l
RT: 5.544 min Scan# 718
Delta R.T. 0.079 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924

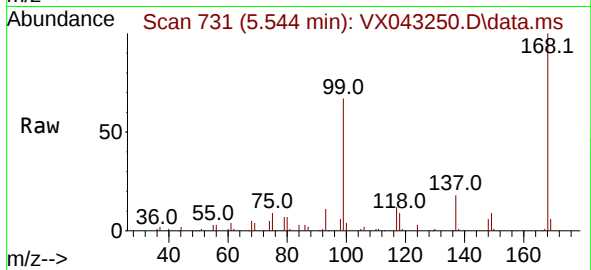

Tgt Ion: 56 Resp: 2127




Ion	Ratio	Lower	Upper
56	100		
69	148.5	25.8	38.6#
84	111.7	71.1	106.7#




#32
1,1,1-Trichloroethane
Concen: 0.284 ug/l
RT: 5.367 min Scan# 702
Delta R.T. -0.012 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 97 Resp: 508

Ion	Ratio	Lower	Upper
97	100		
99	0.0	51.2	76.8#
61	35.4	35.6	53.4#


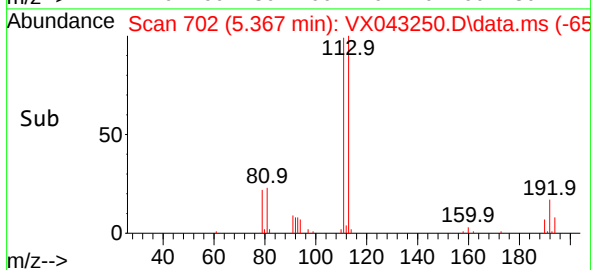






#33
 1,2-Dichloroethane-d4
 Concen: 53.888 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. 0.000 min
 Lab File: VX043250.D
 Acq: 03 Oct 2024 10:34




Instrument :
 MSVOA_X
 ClientSampleId :
 TT101D1-20240924


Tgt Ion: 65 Resp: 72937
 Ion Ratio Lower Upper
 65 100
 67 49.2 0.0 99.0

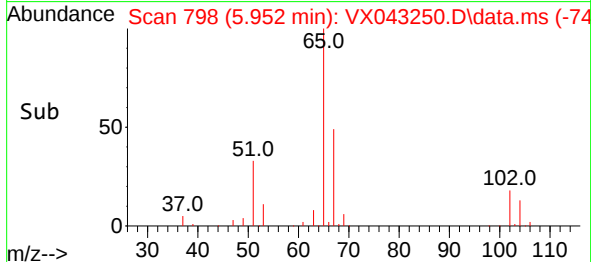

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. 0.000 min
 Lab File: VX043250.D
 Acq: 03 Oct 2024 10:34

Tgt Ion: 114 Resp: 161117
 Ion Ratio Lower Upper
 114 100
 63 20.6 0.0 43.0
 88 16.4 0.0 33.0









#35
Dibromofluoromethane
Concen: 47.331 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion:113 Resp: 52591
Ion Ratio Lower Upper
113 100
111 104.0 83.4 125.0
192 18.5 14.1 21.1



#36
1,1-Dichloropropene
Concen: 5.156 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.146 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 75 Resp: 7238
Ion Ratio Lower Upper
75 100
110 8.7 17.8 53.3#
77 0.0 24.9 37.3#


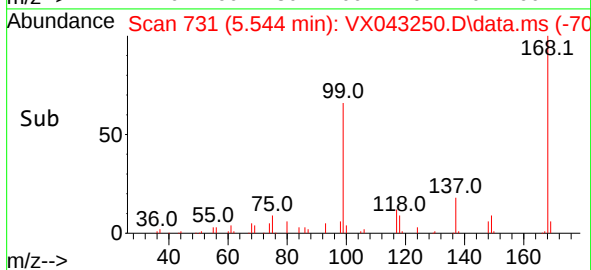






#38
Carbon Tetrachloride
Concen: 0.802 ug/l
RT: 5.678 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion:117 Resp: 1333
Ion Ratio Lower Upper
117 100
119 80.1 77.7 116.5
121 26.8 24.3 36.5

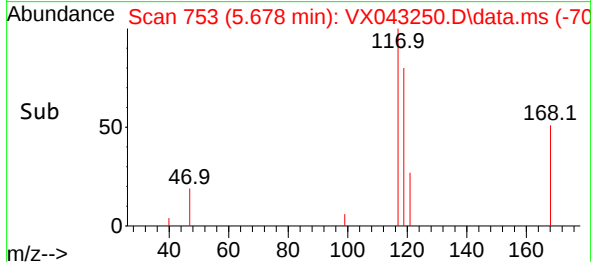

#39
Methylcyclohexane
Concen: 1.747 ug/l
RT: 7.117 min Scan# 989
Delta R.T. -0.256 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 83 Resp: 3084
Ion Ratio Lower Upper
83 100
55 0.0 59.4 89.2#
98 197.1 39.3 58.9#









#44
Trichloroethene
Concen: 199.694 ug/l
RT: 7.123 min Scan# 990
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion:130 Resp: 225418
Ion Ratio Lower Upper
130 100
95 102.1 0.0 192.2

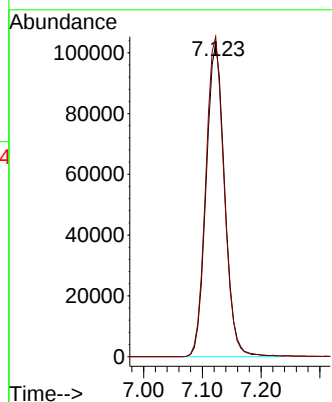

#49
1,4-Dioxane
Concen: 18.188 ug/l
RT: 7.684 min Scan# 1082
Delta R.T. 0.018 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 88 Resp: 483
Ion Ratio Lower Upper
88 100
43 36.6 29.5 44.3
58 67.7 55.2 82.8


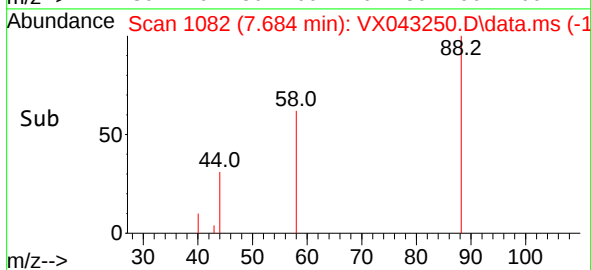






#50
Toluene-d8
Concen: 50.182 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion: 98 Resp: 193229
Ion Ratio Lower Upper
98 100
100 64.9 52.4 78.6

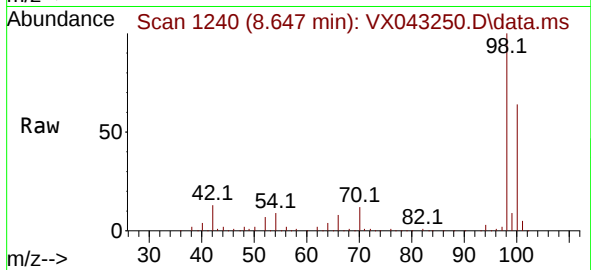

#51
4-Methyl-2-Pentanone
Concen: 0.621 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.073 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 43 Resp: 1050
Ion Ratio Lower Upper
43 100
58 146.2 30.0 45.0#







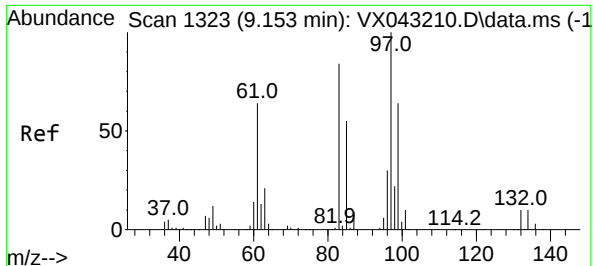

#55
 1,1,2-Trichloroethane
 Concen: 0.682 ug/l
 RT: 9.165 min Scan# 11
 Delta R.T. 0.012 min
 Lab File: VX043250.D
 Acq: 03 Oct 2024 10:34




Instrument :
 MSVOA_X
 ClientSampleId :
 TT101D1-20240924


Tgt Ion: 97	Resp:	723	
Ion	Ratio	Lower	Upper
97	100		
83	55.6	66.9	100.3#
85	57.3	43.9	65.9
99	47.8	51.6	77.4#

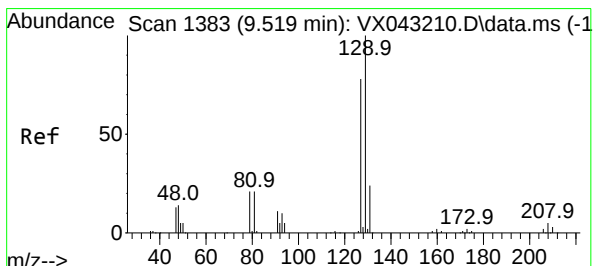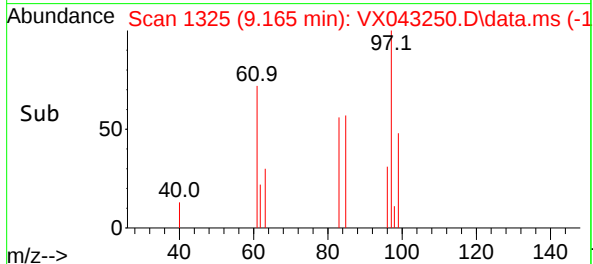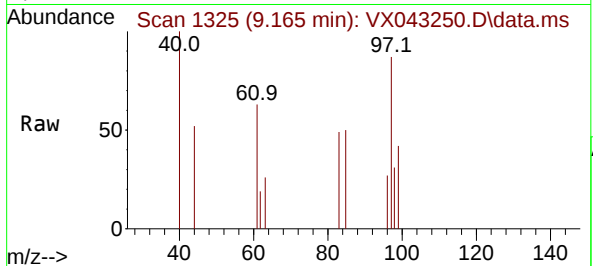

#60
 Dibromochloromethane
 Concen: 0.391 ug/l
 RT: 9.281 min Scan# 1344
 Delta R.T. -0.238 min
 Lab File: VX043250.D
 Acq: 03 Oct 2024 10:34

Tgt Ion:129	Resp:	481	
Ion	Ratio	Lower	Upper
129	100		
127	0.0	38.3	114.9#


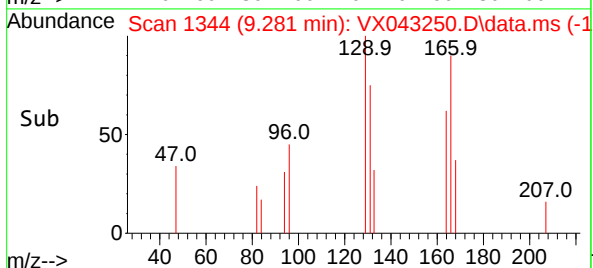
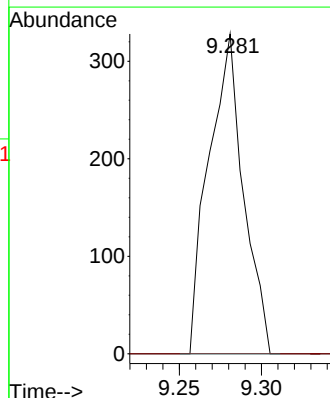
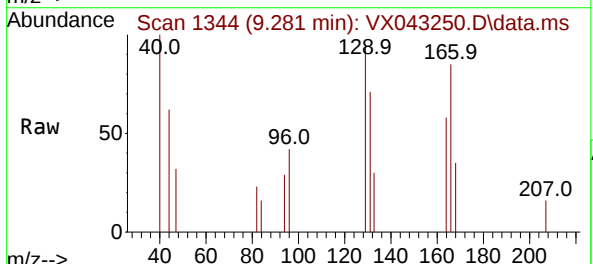




#62
4-Bromofluorobenzene
Concen: 50.528 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924


Tgt Ion: 95 Resp: 70683
Ion Ratio Lower Upper
95 100
174 73.0 0.0 145.0
176 70.6 0.0 143.0

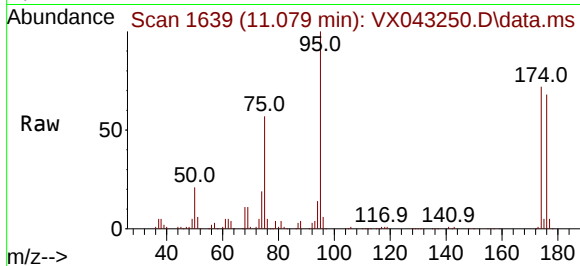

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 117 Resp: 142155
Ion Ratio Lower Upper
117 100
82 55.7 45.0 67.6
119 33.4 25.3 37.9

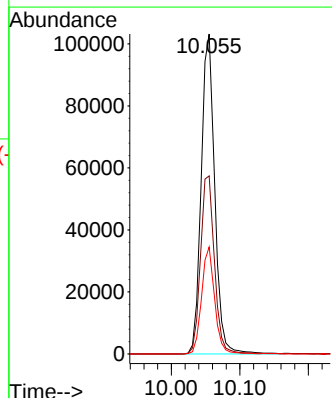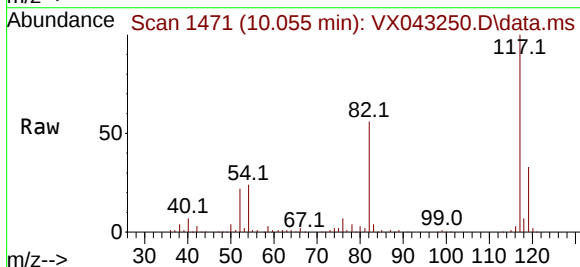







#64
Tetrachloroethene
Concen: 0.432 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924

Tgt Ion:164 Resp: 426




Ion	Ratio	Lower	Upper
164	100		
166	112.8	96.0	144.0
129	86.2	79.4	119.0
131	104.4	72.6	109.0

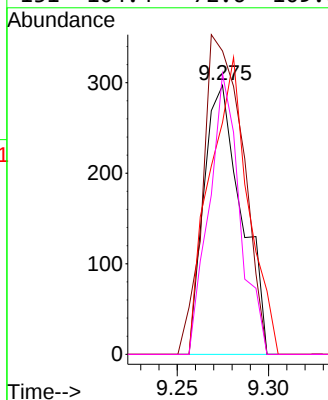


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion:152 Resp: 61992

Ion	Ratio	Lower	Upper
152	100		
115	63.2	44.1	132.3
150	156.3	0.0	347.4



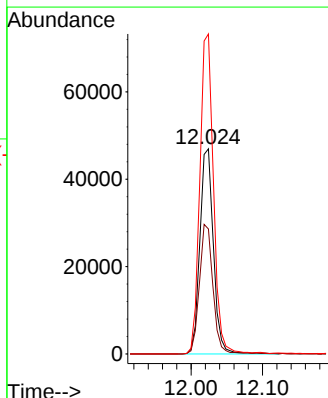





#76
1,2,3-Trichloropropane
Concen: 28.491 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20240924

Tgt Ion: 75 Resp: 39176
Ion Ratio Lower Upper
75 100
77 0.9 22.0 66.0#

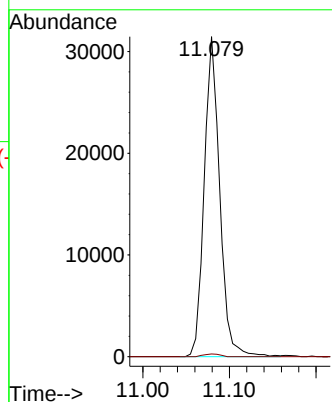

#81
trans-1,4-Dichloro-2-butene
Concen: 73.838 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX043250.D
Acq: 03 Oct 2024 10:34

Tgt Ion: 75 Resp: 39176
Ion Ratio Lower Upper
75 100
53 0.0 83.9 125.9#
89 0.0 38.6 58.0#

