

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
 Data File : VX043245.D
 Acq On : 03 Oct 2024 08:37
 Operator : JC/MD
 Sample : VX1003MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1003MBL01

Quant Time: Oct 04 01:24:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 16:50:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	78813	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	153090	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	139562	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	61287	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	68127	52.929	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.860%
35) Dibromofluoromethane	5.385	113	50413	47.750	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.500%
50) Toluene-d8	8.647	98	186529	50.982	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.960%
62) 4-Bromofluorobenzene	11.079	95	68354	51.425	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	102.860%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
Data File : VX043245.D
Acq On : 03 Oct 2024 08:37
Operator : JC/MD
Sample : VX1003MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01


Quant Time: Oct 04 01:24:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 16:50:57 2024
Response via : Initial Calibration

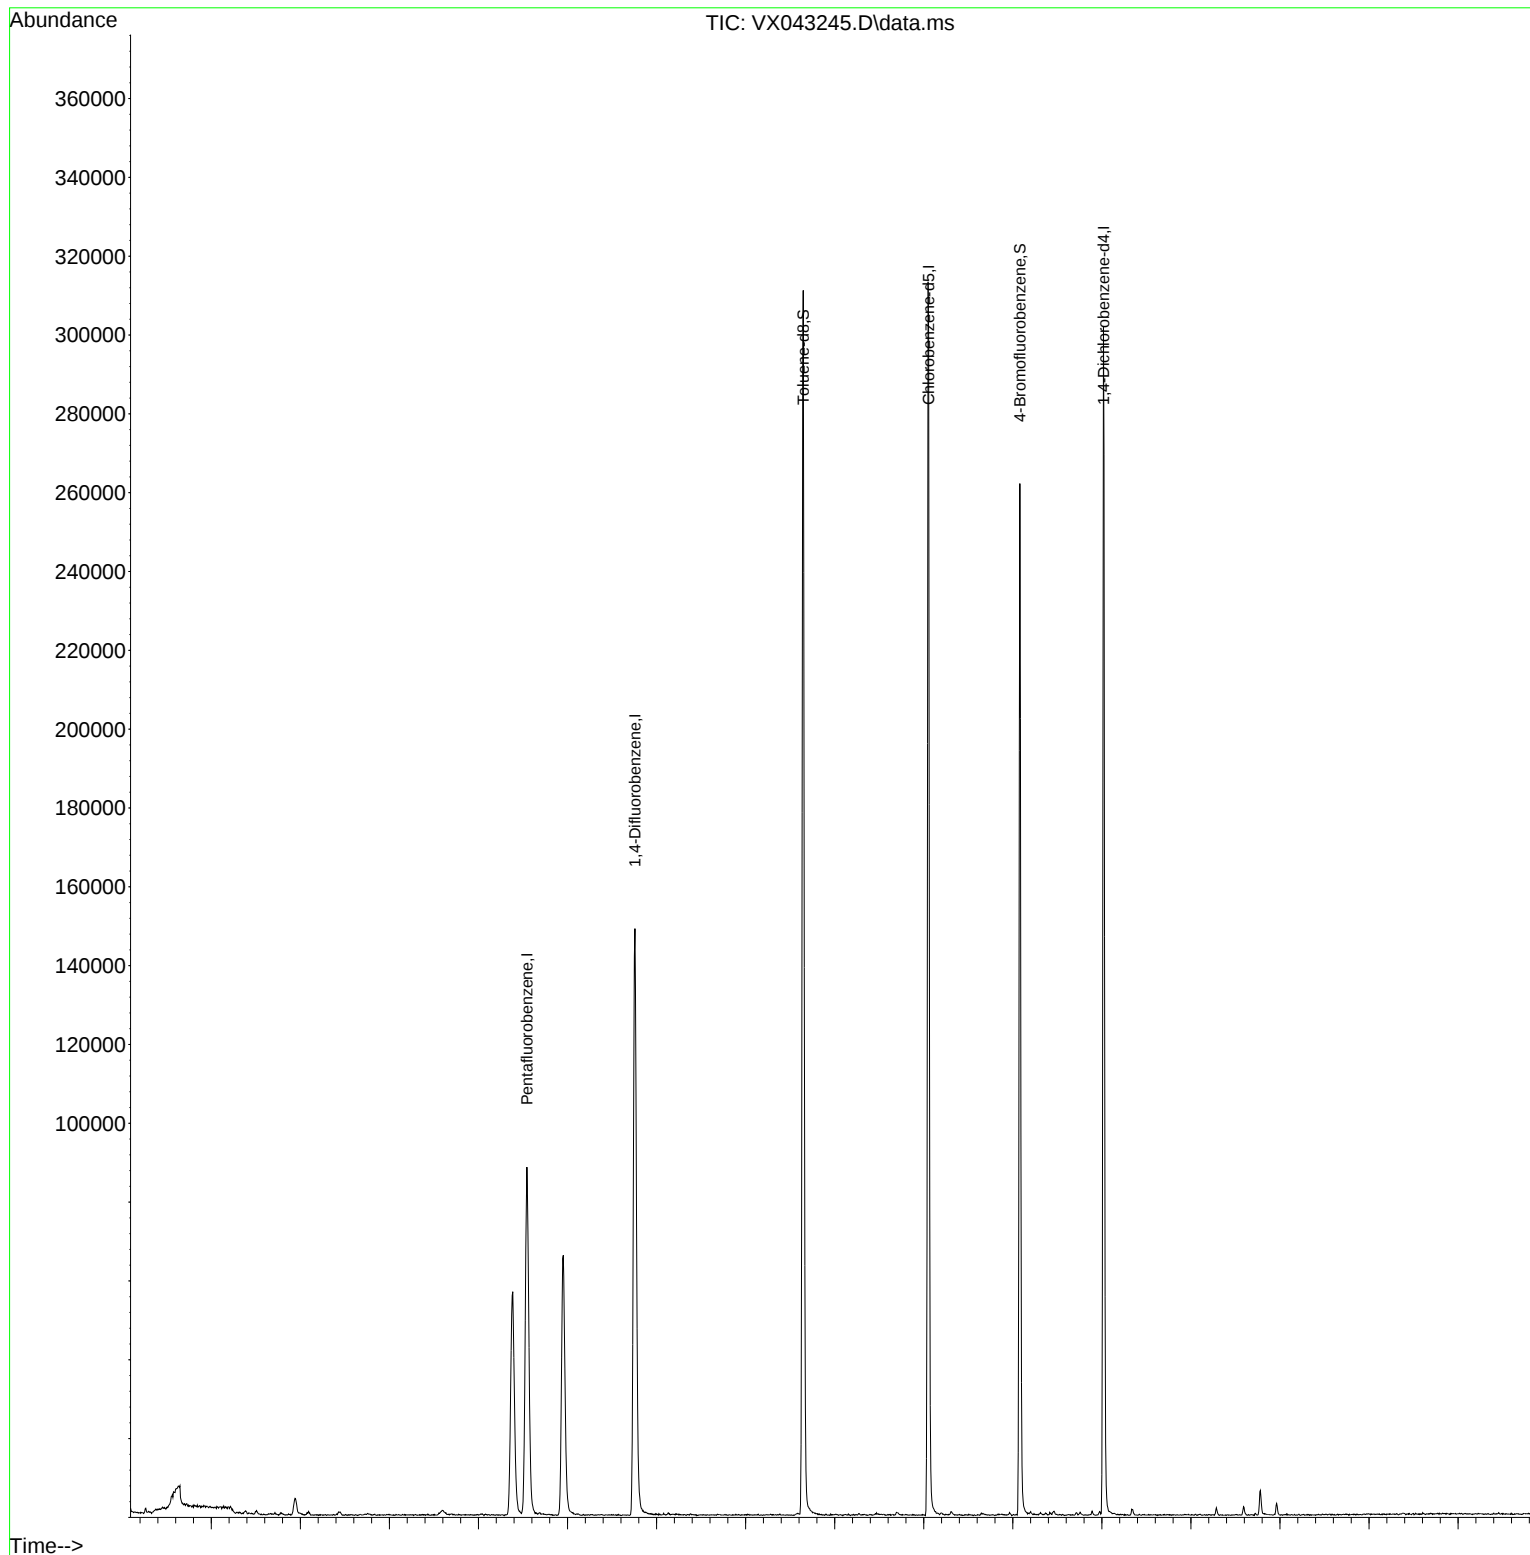



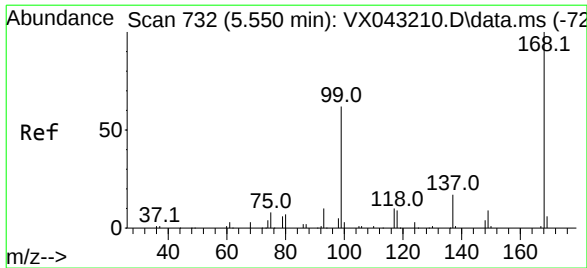


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.006 min
Lab File: VX043245.D
Acq: 03 Oct 2024 08:37

Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01



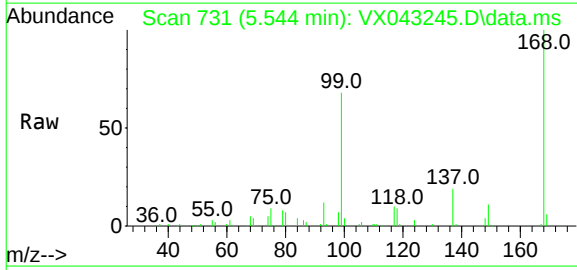



Tgt Ion:168 Resp: 78813
Ion Ratio Lower Upper
168 100
99 68.2 49.7 74.5

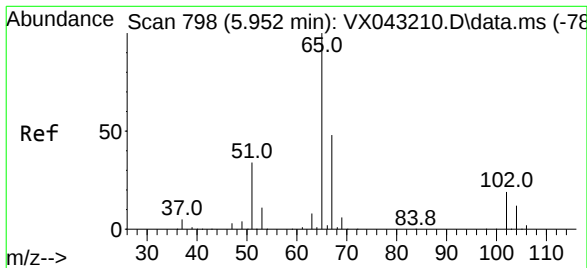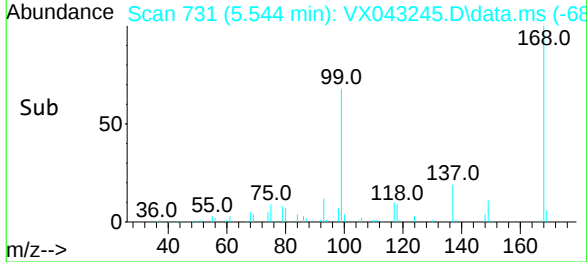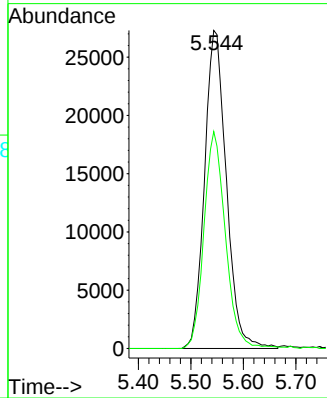

#33
1,2-Dichloroethane-d4
Concen: 52.929 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX043245.D
Acq: 03 Oct 2024 08:37

Tgt Ion: 65 Resp: 68127
Ion Ratio Lower Upper
65 100
67 49.9 0.0 99.0


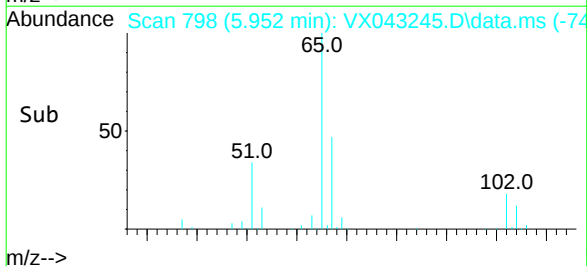
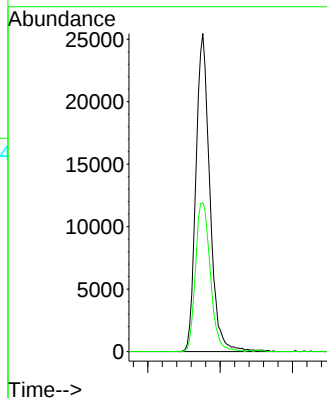
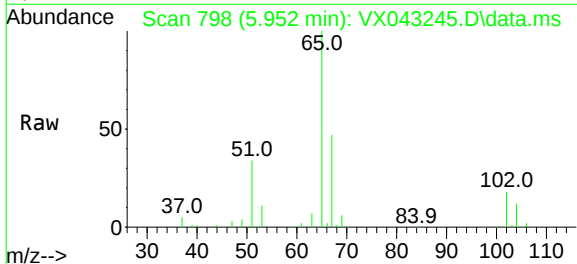


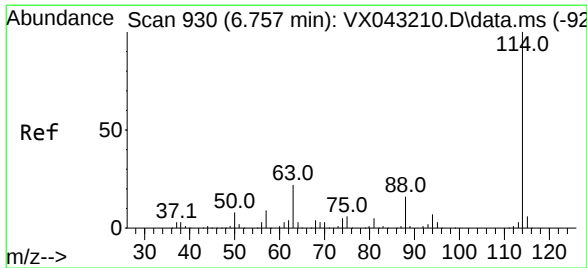

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 93
Delta R.T. -0.000 min
Lab File: VX043245.D
Acq: 03 Oct 2024 08:37




Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01


Tgt Ion:	114	Resp:	153090
Ion	Ratio	Lower	Upper
114	100		
63	20.5	0.0	43.0
88	16.4	0.0	33.0

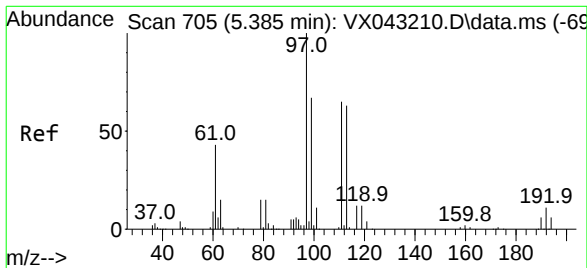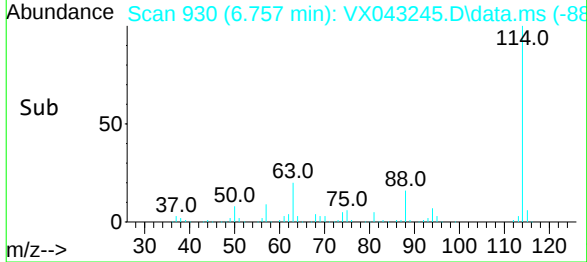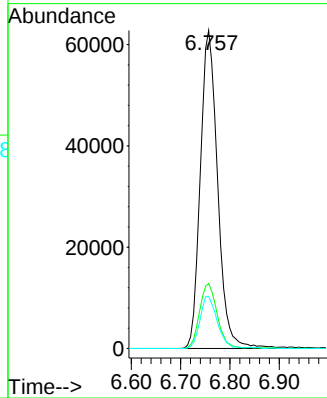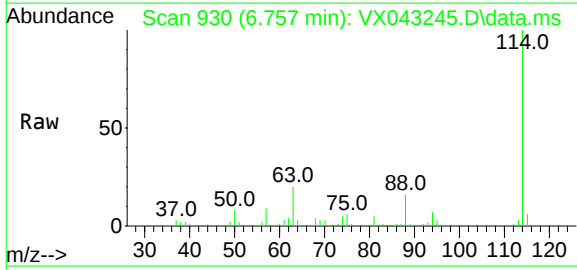

#35
Dibromofluoromethane
Concen: 47.750 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX043245.D
Acq: 03 Oct 2024 08:37

Tgt Ion:	113	Resp:	50413
Ion	Ratio	Lower	Upper
113	100		
111	102.3	83.4	125.0
192	17.7	14.1	21.1


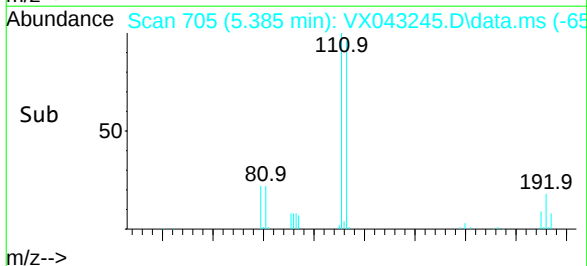
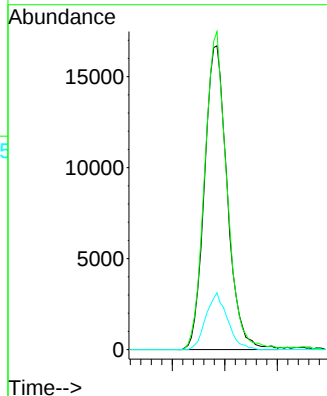
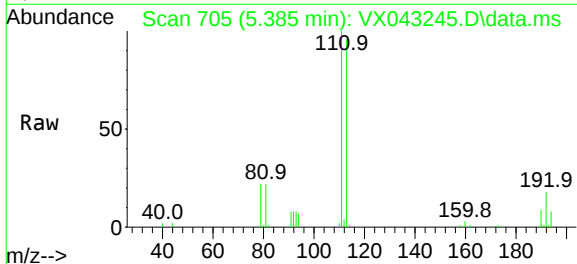


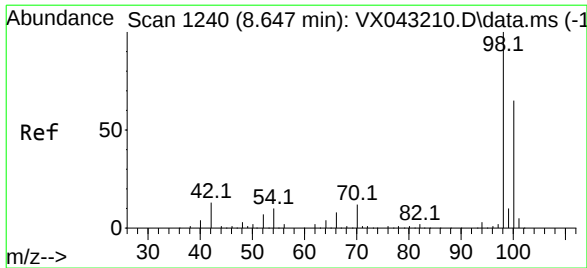

#50
Toluene-d8
Concen: 50.982 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX043245.D
Acq: 03 Oct 2024 08:37




Instrument :
MSVOA_X
ClientSampleId :
VX1003MBL01


Tgt Ion: 98 Resp: 186529
Ion Ratio Lower Upper
98 100
100 64.7 52.4 78.6

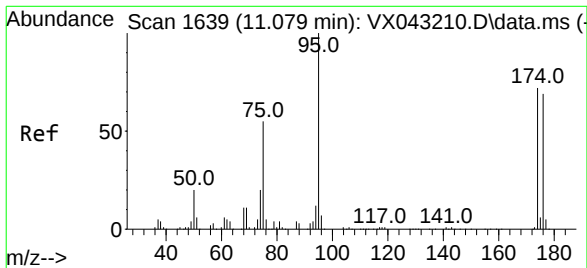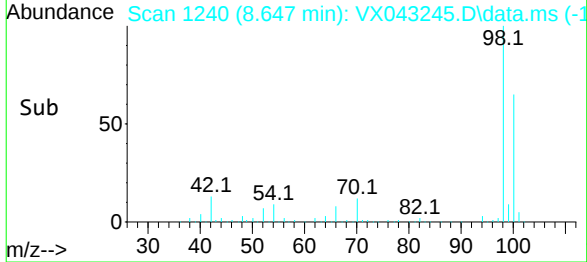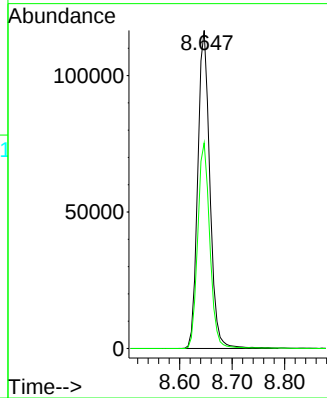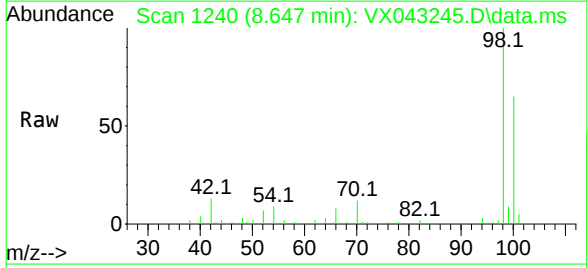

#62
4-Bromofluorobenzene
Concen: 51.425 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX043245.D
Acq: 03 Oct 2024 08:37

Tgt Ion: 95 Resp: 68354
Ion Ratio Lower Upper
95 100
174 73.6 0.0 145.0
176 71.0 0.0 143.0

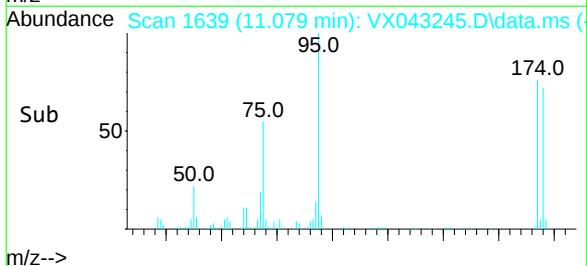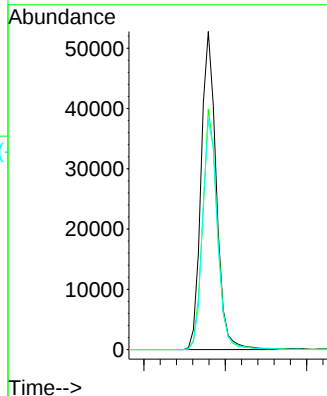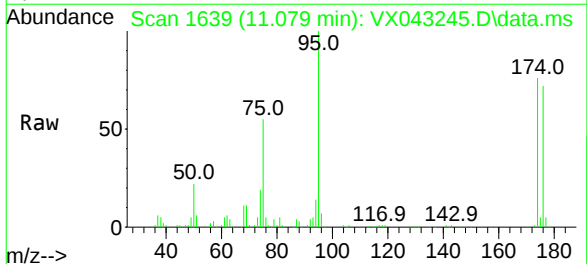

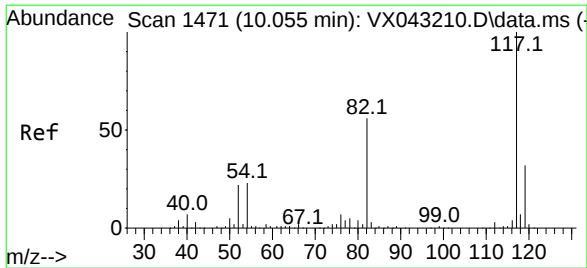

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX043245.D

Acq: 03 Oct 2024 08:37

Instrument :

MSVOA_X

ClientSampleId :

VX1003MBL01





Tgt Ion:117 Resp: 139562

Ion Ratio Lower Upper

117 100

82 54.3 45.0 67.6

119 31.7 25.3 37.9

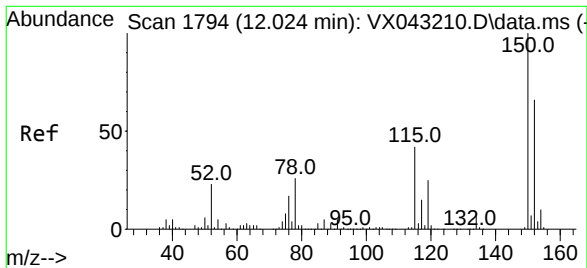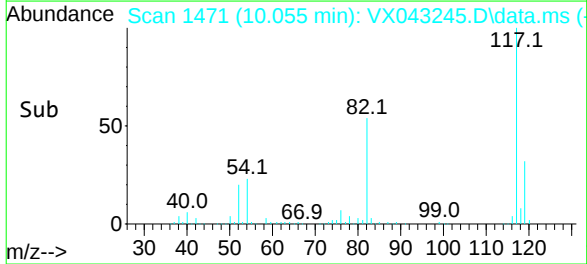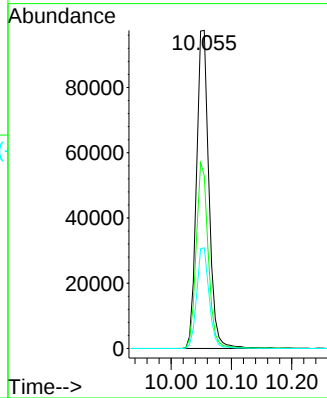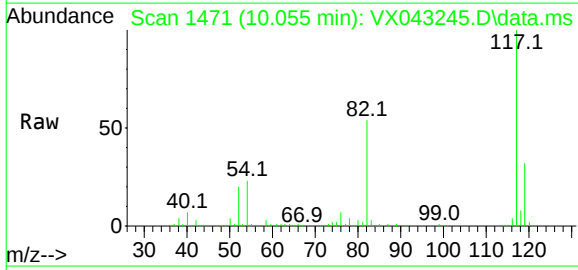

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX043245.D

Acq: 03 Oct 2024 08:37

Tgt Ion:152 Resp: 61287

Ion Ratio Lower Upper

152 100

115 61.7 44.1 132.3

150 154.9 0.0 347.4

