

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
 Data File : VX043265.D
 Acq On : 03 Oct 2024 16:21
 Operator : JC/MD
 Sample : P4263-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Title : SW846 8260

Signal : TIC: VX043265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	34	rBV	26442	37573	7.13%	1.293%
2	1.581	71	81	82	rBV4	3717	8761	1.66%	0.301%
3	5.385	694	705	721	rBV	60728	181213	34.41%	6.236%
4	5.550	723	732	753	rVB	92183	265807	50.47%	9.147%
5	5.952	788	798	815	rBV2	70947	190598	36.19%	6.559%
6	6.763	921	931	948	rBV	157863	386513	73.39%	13.300%
7	8.647	1234	1240	1253	rBV	331395	526682	100.00%	18.123%
8	10.055	1465	1471	1487	rBV	320682	454651	86.32%	15.645%
9	11.079	1634	1639	1651	rBV	260045	344406	65.39%	11.851%
10	12.018	1788	1793	1804	rBV	311916	405087	76.91%	13.939%
11	14.225	2150	2155	2159	rVB3	4129	7200	1.37%	0.248%
12	14.475	2193	2196	2202	rBV6	4288	6513	1.24%	0.224%
13	14.615	2215	2219	2225	rBV4	5454	7737	1.47%	0.266%
14	14.755	2235	2242	2246	rBV4	4725	7177	1.36%	0.247%
15	15.182	2307	2312	2314	rBV3	6143	8191	1.56%	0.282%
16	15.207	2314	2316	2321	rVB3	4232	5908	1.12%	0.203%
17	15.487	2356	2362	2367	rBV2	11123	18833	3.58%	0.648%
18	15.615	2378	2383	2386	rBV2	5631	8837	1.68%	0.304%
19	15.652	2386	2389	2394	rVB2	4088	6074	1.15%	0.209%
20	16.091	2455	2461	2465	rBV5	3853	7721	1.47%	0.266%
21	16.371	2499	2507	2514	rBV3	11925	20604	3.91%	0.709%




Sum of corrected areas: 2906086

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
Data File : VX043265.D
Acq On : 03 Oct 2024 16:21
Operator : JC/MD
Sample : P4263-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

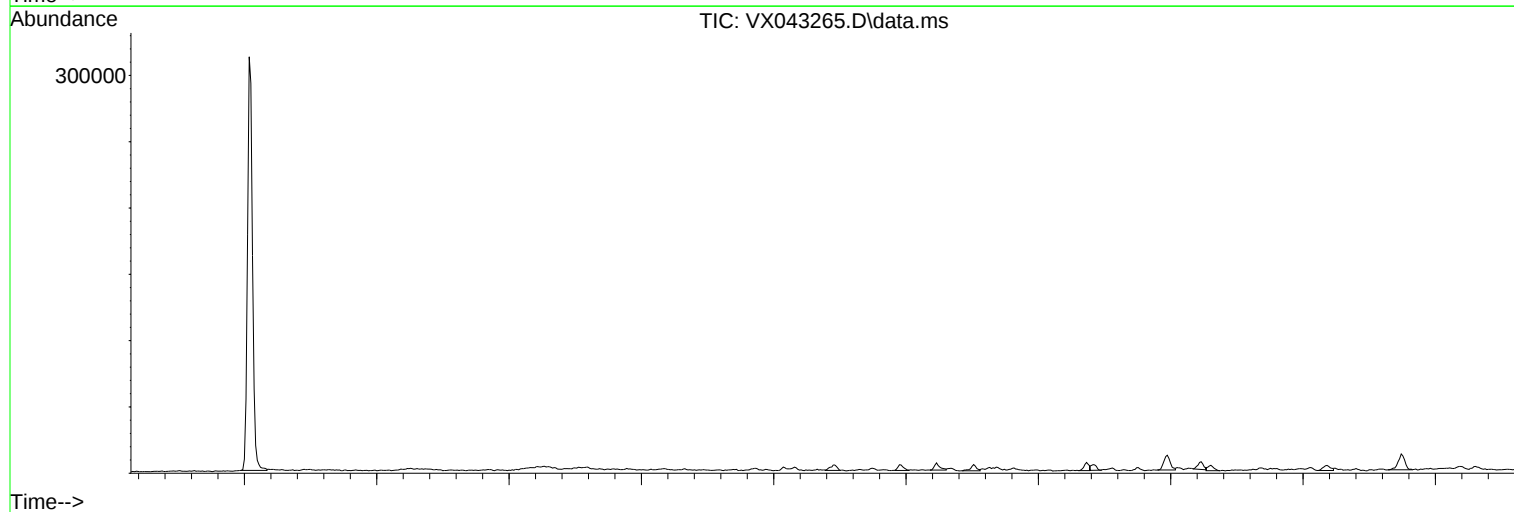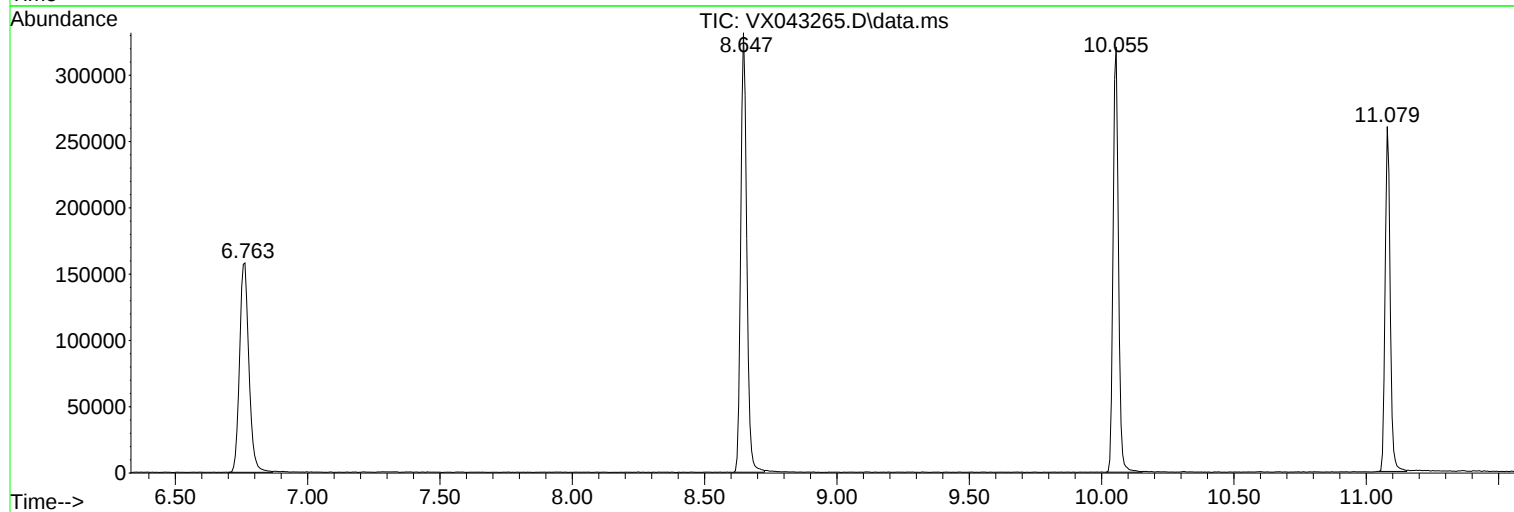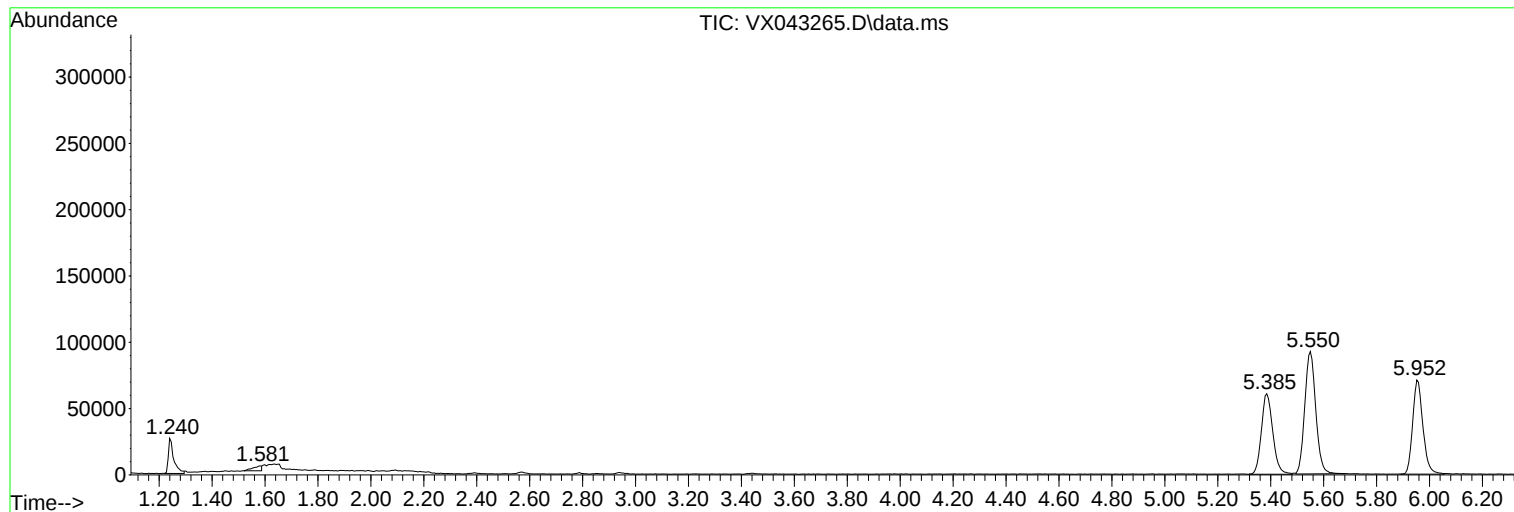

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
Data File : VX043265.D
Acq On : 03 Oct 2024 16:21
Operator : JC/MD
Sample : P4263-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.240	7.07 ug/l	37573	Pentafluorobenzene	5.550

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Sulfur dioxide	64	O2S	007446-09-5	83
2	Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3	Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
4	Ethyl Chloride	64	C2H5Cl	000075-00-3	3
5	Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	3

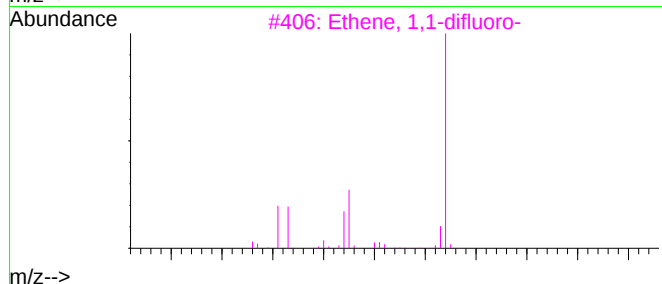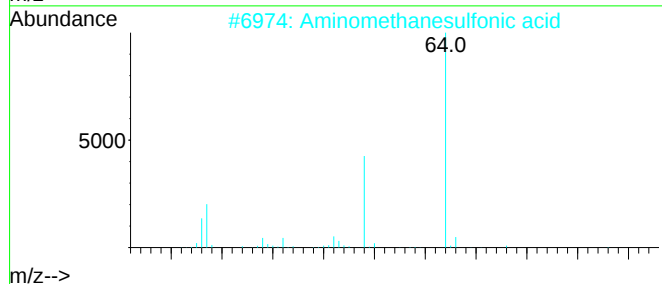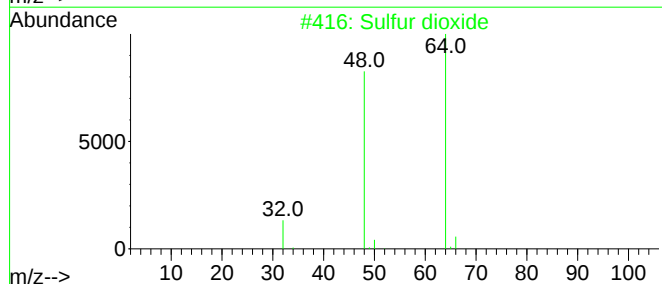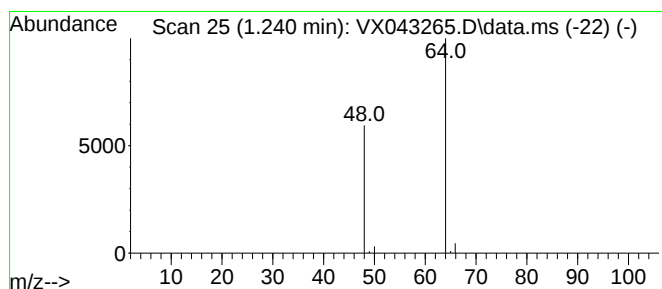

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100324\
Data File : VX043265.D
Acq On : 03 Oct 2024 16:21
Operator : JC/MD
Sample : P4263-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.240	7.1	ug/l	37573	1	5.550	265807	50.0