

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\WX100418\  
 Data File : VX005060.D  
 Acq On : 05 Oct 2018 10:44  
 Operator : JC/MD  
 Sample : J5207-25  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 98 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW512-4145

Quant Time: Oct 05 11:35:58 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X092618W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Oct 03 04:00:03 2018  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc      | Units   | Dev(Min) |
|-------------------------------|--------|------|----------|-----------|---------|----------|
| -----                         |        |      |          |           |         |          |
| Internal Standards            |        |      |          |           |         |          |
| 1) Pentafluorobenzene         | 5.665  | 168  | 213663   | 50.00     | ug/l    | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.860  | 114  | 329670   | 50.00     | ug/l    | 0.00     |
| 63) Chlorobenzene-d5          | 10.116 | 117  | 326750   | 50.00     | ug/l    | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.079 | 152  | 176738   | 50.00     | ug/l    | 0.00     |
|                               |        |      |          |           |         |          |
| System Monitoring Compounds   |        |      |          |           |         |          |
| 33) 1,2-Dichloroethane-d4     | 6.061  | 65   | 166656   | 54.60     | ug/l    | 0.00     |
| Spiked Amount 50.000          |        |      | Recovery | =         | 109.20% |          |
| 35) Dibromofluoromethane      | 5.501  | 113  | 139079   | 49.78     | ug/l    | 0.00     |
| Spiked Amount 50.000          |        |      | Recovery | =         | 99.56%  |          |
| 50) Toluene-d8                | 8.720  | 98   | 476252   | 51.27     | ug/l    | 0.00     |
| Spiked Amount 50.000          |        |      | Recovery | =         | 102.54% |          |
| 62) 4-Bromofluorobenzene      | 11.140 | 95   | 171321   | 51.20     | ug/l    | 0.00     |
| Spiked Amount 50.000          |        |      | Recovery | =         | 102.40% |          |
|                               |        |      |          |           |         |          |
| Target Compounds              |        |      |          |           |         | Qvalue   |
| 3) Chloromethane              | 1.325  | 50   | 1011     | 0.29      | ug/l #  | 83       |
| 5) Bromomethane               | 1.629  | 94   | 606      | 0.31      | ug/l #  | 57       |
| 6) Chloroethane               | 1.727  | 64   | 261      | Below Cal | #       | 45       |
| 11) Tert butyl alcohol        | 3.019  | 59   | 4308     | 5.05      | ug/l #  | 83       |
| 12) 1,1-Dichloroethene        | 2.373  | 96   | 574      | 0.25      | ug/l #  | 80       |
| 13) Acrolein                  | 2.294  | 56   | 266      | 0.44      | ug/l #  | 10       |
| 16) Acetone                   | 2.446  | 43   | 16954    | 9.51      | ug/l    | 90       |
| 17) Carbon Disulfide          | 2.574  | 76   | 5743     | 0.83      | ug/l    | 98       |
| 18) Methyl Acetate            | 2.776  | 43   | 1452     | 0.32      | ug/l    | 93       |
| 20) Methylene Chloride        | 2.855  | 84   | 1003     | Below Cal |         | 91       |
| 24) 1,1-Dichloroethane        | 3.696  | 63   | 17852    | 3.52      | ug/l    | 98       |
| 25) 2-Butanone                | 4.702  | 43   | 3756     | 1.43      | ug/l #  | 86       |
| 36) 1,1-Dichloropropene       | 5.665  | 75   | 14403    | 3.78      | ug/l #  | 46       |
| 38) Carbon Tetrachloride      | 5.665  | 117  | 18997    | 4.74      | ug/l #  | 18       |
| 39) Methylcyclohexane         | 7.458  | 83   | 850      | 0.22      | ug/l #  | 80       |
| 52) Toluene                   | 8.787  | 92   | 5301     | 0.81      | ug/l    | 92       |
| 56) Ethyl methacrylate        | 9.274  | 69   | 25       | 2.87      | ug/l #  | 1        |
| 58) 2-Chloroethyl Vinyl ether | 8.348  | 63   | 19       | 14.25     | ug/l #  | 49       |
| 68) m/p-Xylenes               | 10.360 | 106  | 2080     | 0.40      | ug/l    | 95       |
| 69) o-Xylene                  | 10.701 | 106  | 961      | 0.20      | ug/l    | 79       |
| 70) Styrene                   | 10.713 | 104  | 83       | 2.15      | ug/l #  | 1        |
| 74) N-ethyl acetate           | 10.908 | 43   | 309      | 1.80      | ug/l #  | 1        |
| 76) 1,2,3-Trichloropropane    | 11.140 | 75   | 83941    | 21.19     | ug/l #  | 35       |
| 80) 1,3,5-Trimethylbenzene    | 11.506 | 105  | 566      | Below Cal |         | 87       |
| 81) trans-1,4-Dichloro-2-b... | 11.140 | 75   | 83941    | 57.48     | ug/l #  | 10       |
| 84) 1,2,4-Trimethylbenzene    | 11.810 | 105  | 1828     | Below Cal |         | 94       |
| 95) Naphthalene               | 13.834 | 128  | 946      | 0.78      | ug/l #  | 90       |
| -----                         |        |      |          |           |         |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100418\  
Data File : VX005060.D  
Acq On : 05 Oct 2018 10:44  
Operator : JC/MD  
Sample : J5207-25  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 98 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145

Quant Time: Oct 05 11:35:58 2018  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X092618W.M  
Quant Title : SW846 8260  
QLast Update : Wed Oct 03 04:00:03 2018  
Response via : Initial Calibration




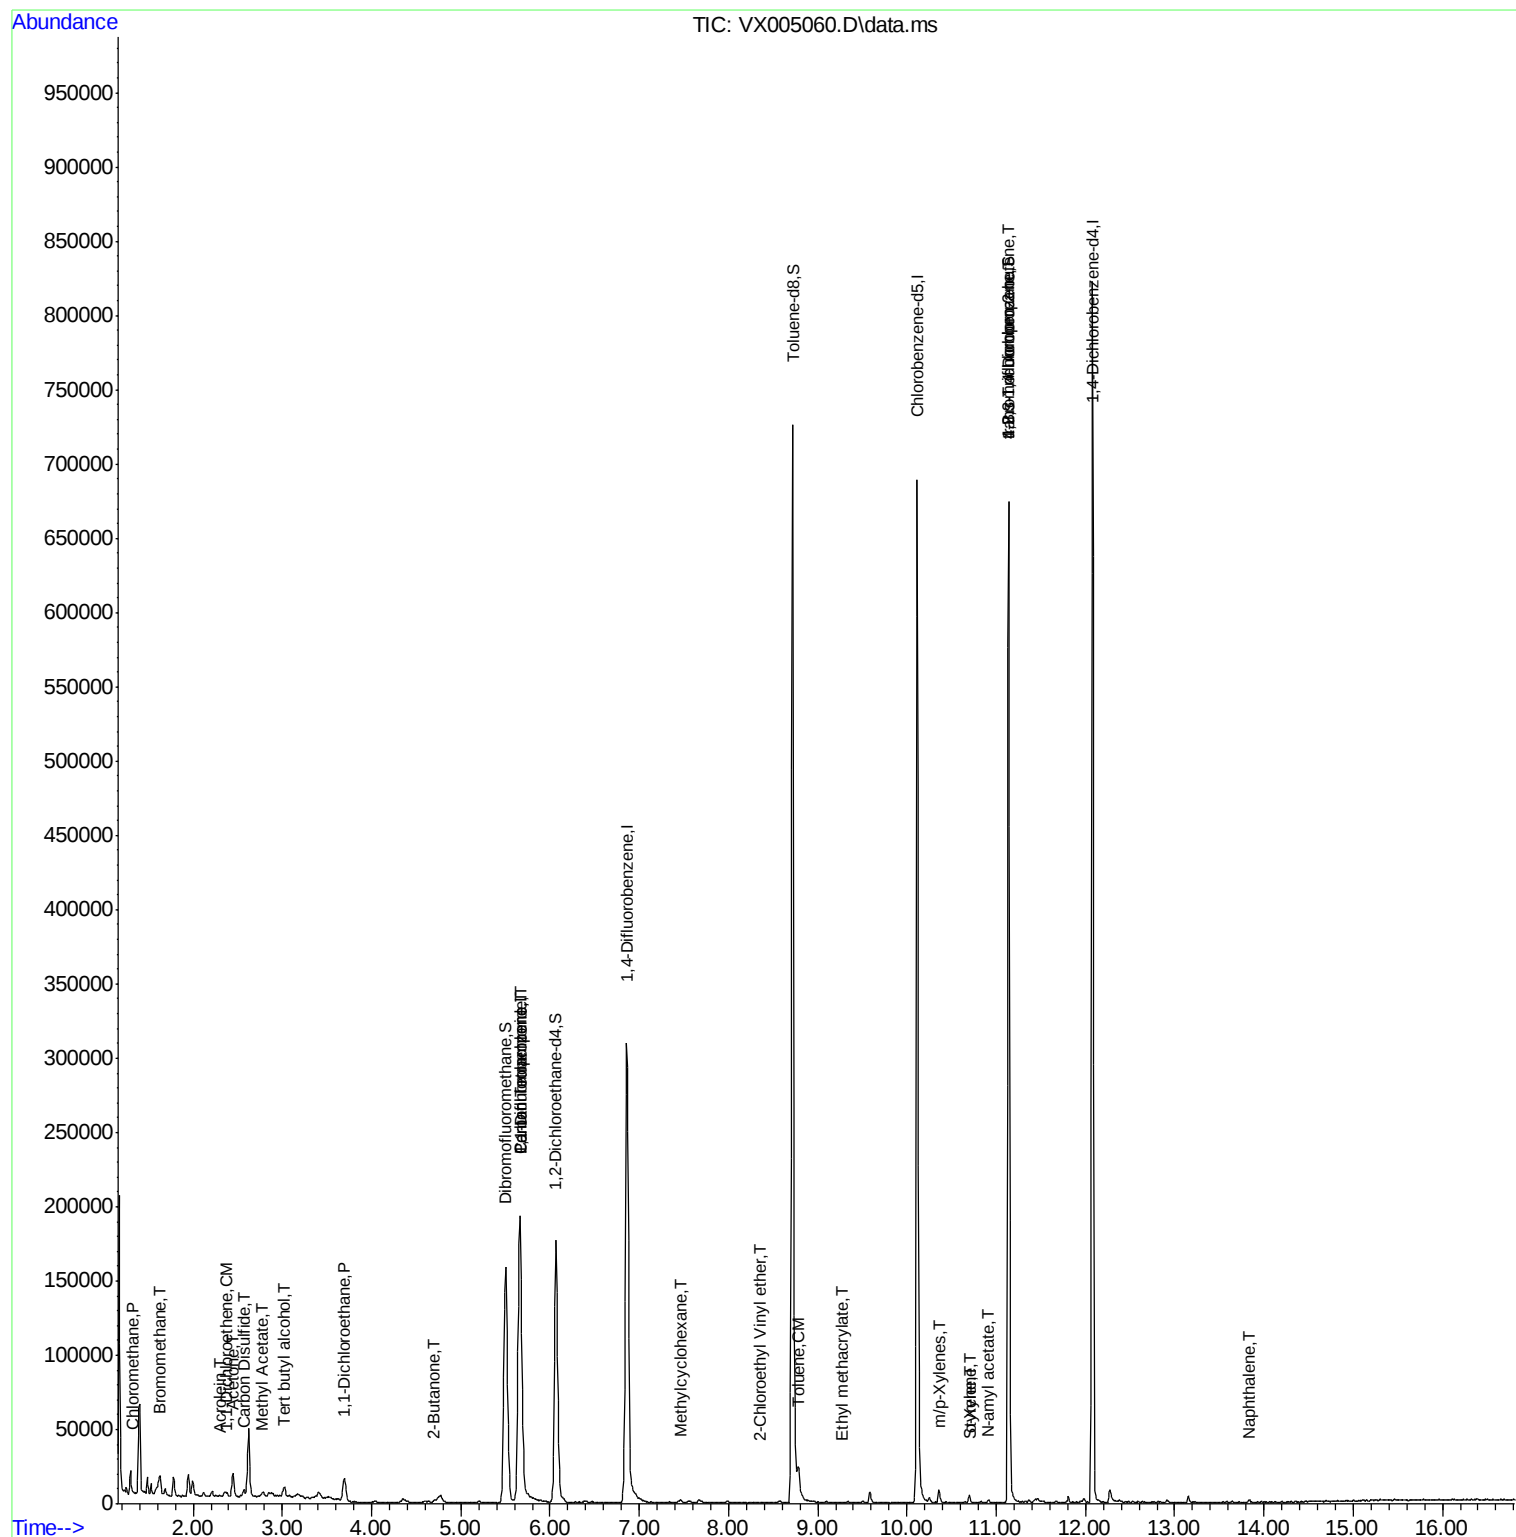


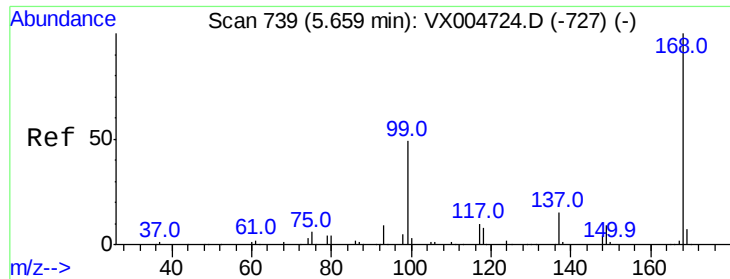

#1  
Pentafluorobenzene  
Concen: 50.00 ug/l  
RT: 5.665 min Scan# 74  
Delta R.T. 0.006 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44




Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145


Tot Ion:168 Resp: 213663  
Ion Ratio Lower Upper  
168 100  
99 50.2 39.3 58.9

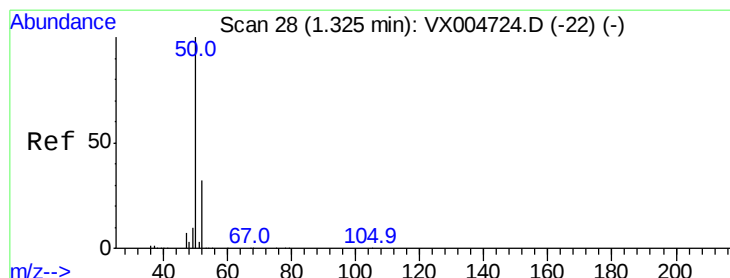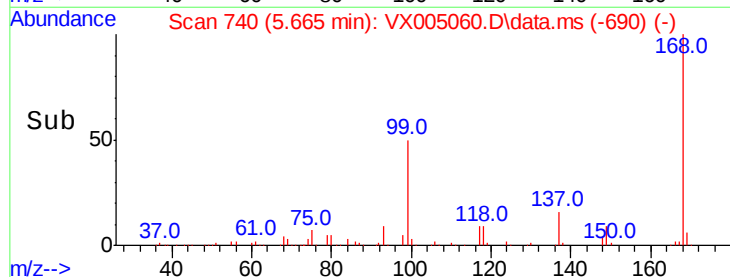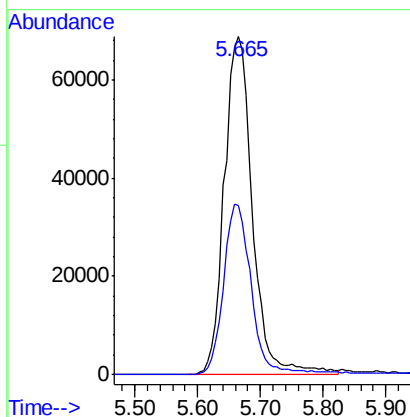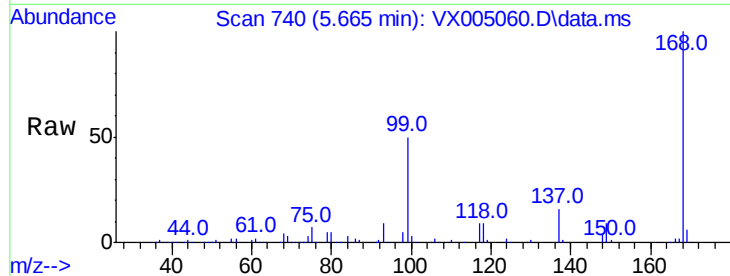

#3  
Chloromethane  
Concen: 0.29 ug/l  
RT: 1.325 min Scan# 28  
Delta R.T. 0.000 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44

Tgt Ion: 50 Resp: 1011  
Ion Ratio Lower Upper  
50 100  
52 41.8 25.8 38.6#

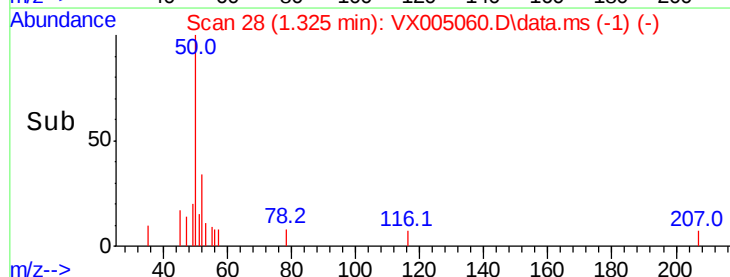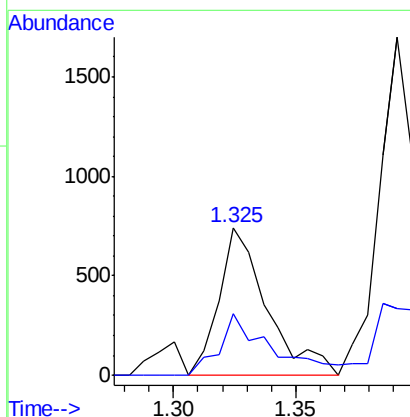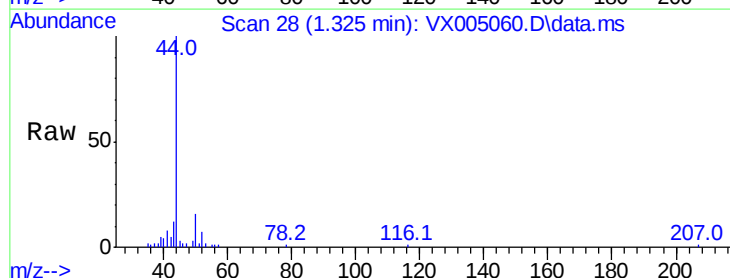



#5

Bromomethane

Concen: 0.31 ug/l

RT: 1.629 min Scan# 78

Delta R.T. -0.006 min

Lab File: VX005060.D

Acq: 05 Oct 2018 10:44

Instrument :

MSVOA\_X

ClientSampleId :





SA-TW512-4145

Tot Ion: 94 Resp: 606

Ion Ratio Lower Upper

94 100

96 56.6 79.5 119.3#

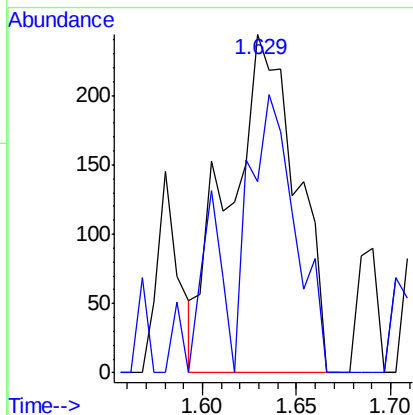

#6

Chloroethane

Concen: Below Cal

RT: 1.727 min Scan# 94

Delta R.T. 0.012 min

Lab File: VX005060.D




Acq: 05 Oct 2018 10:44


Tgt Ion: 64 Resp: 261

Ion Ratio Lower Upper

64 100

66 0.0 23.8 35.6#



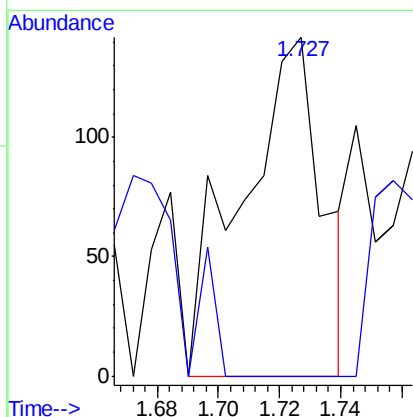





#11  
Tert butyl alcohol  
Concen: 5.05 ug/l  
RT: 3.019 min Scan# 30  
Delta R.T. -0.061 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44




Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145


Tot Ion: 59 Resp: 4308  
Ion Ratio Lower Upper  
59 100  
57 4.1 8.6 12.8#

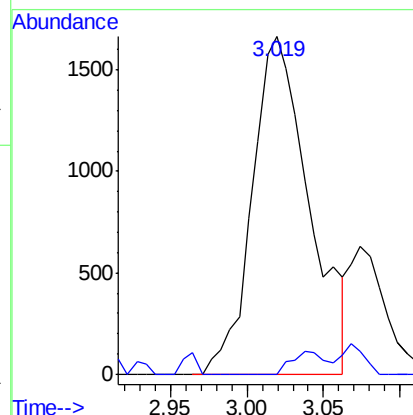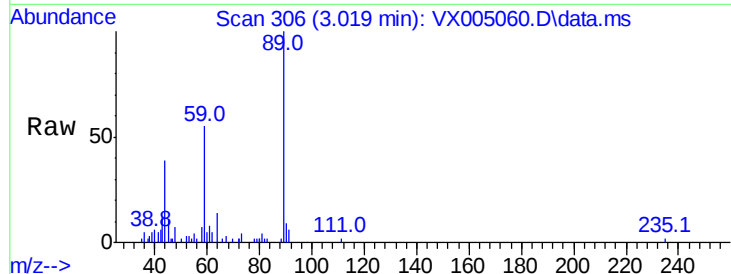

#12  
1,1-Dichloroethene  
Concen: 0.25 ug/l  
RT: 2.373 min Scan# 200  
Delta R.T. 0.006 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44

Tgt Ion: 96 Resp: 574  
Ion Ratio Lower Upper  
96 100  
61 139.2 130.2 195.4  
98 46.7 53.4 80.0#

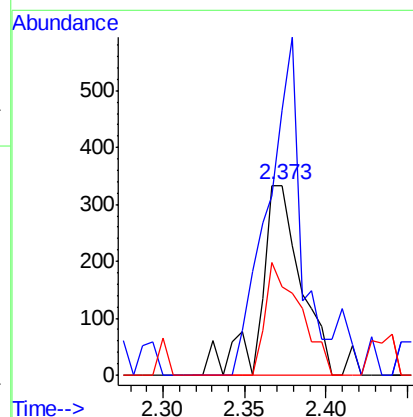

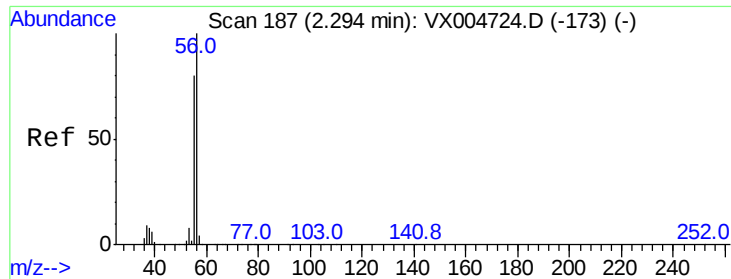

#13

Acrolein

Concen: 0.44 ug/l

RT: 2.294 min Scan# 18

Delta R.T. -0.000 min

Lab File: VX005060.D

Acq: 05 Oct 2018 10:44

Instrument :

MSVOA\_X

ClientSampleId :





SA-TW512-4145

Tot Ion: 56 Resp: 266

Ion Ratio Lower Upper

56 100

55 0.0 63.4 95.2#

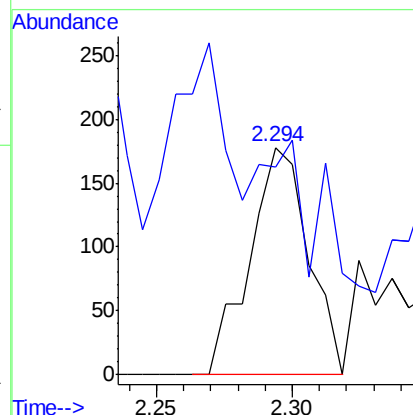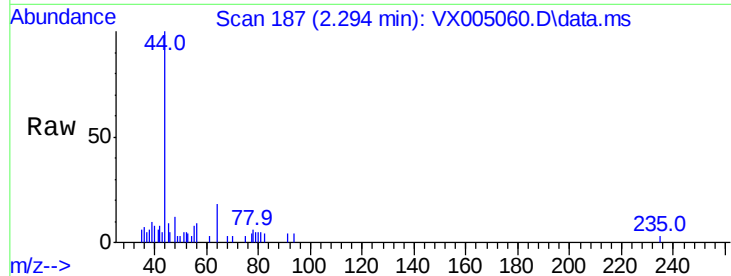

#16

Acetone

Concen: 9.51 ug/l

RT: 2.446 min Scan# 212

Delta R.T. 0.000 min

Lab File: VX005060.D




Acq: 05 Oct 2018 10:44


Tgt Ion: 43 Resp: 16954

Ion Ratio Lower Upper

43 100

58 32.3 21.8 32.6


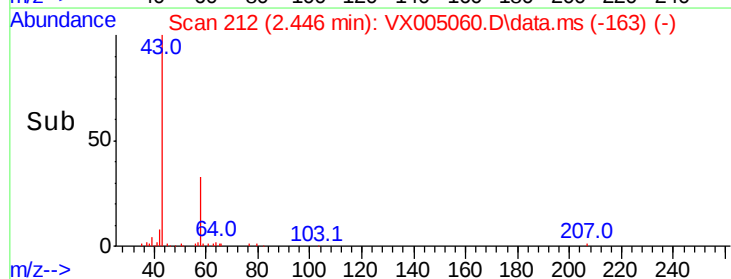
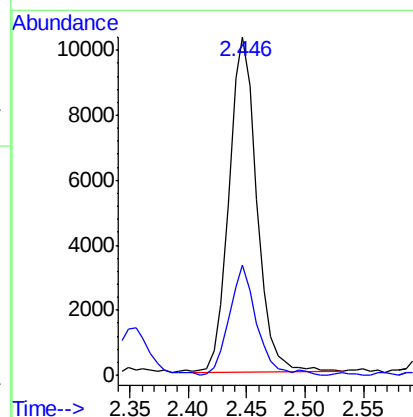





#17  
Carbon Disulfide  
Concen: 0.83 ug/l  
RT: 2.574 min Scan# 231  
Delta R.T. 0.006 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44




Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145


Tot Ion: 76 Resp: 5743  
Ion Ratio Lower Upper  
76 100  
78 8.2 7.0 10.6

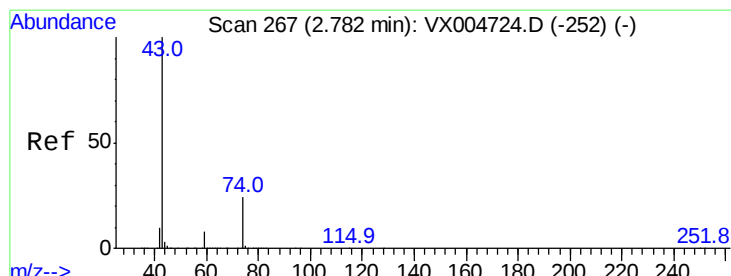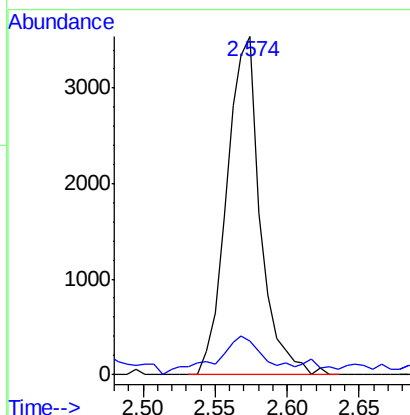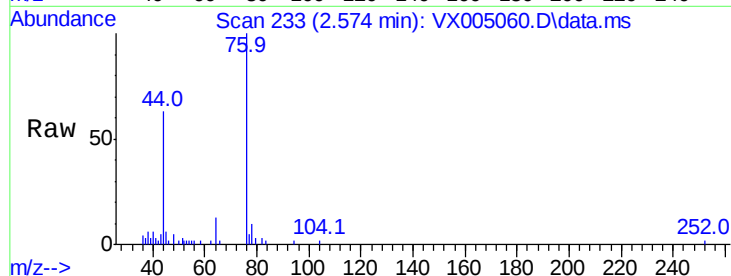

#18  
Methyl Acetate  
Concen: 0.32 ug/l  
RT: 2.776 min Scan# 266  
Delta R.T. -0.006 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44

Tgt Ion: 43 Resp: 1452  
Ion Ratio Lower Upper  
43 100  
74 18.8 17.8 26.8



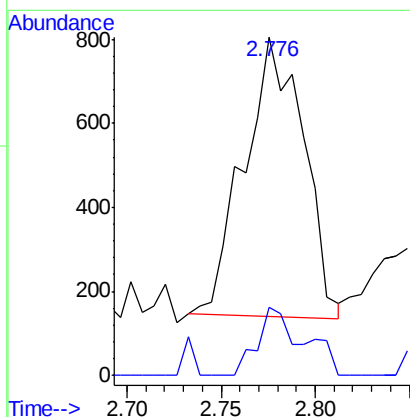





#20  
Methvlene Chloride  
Concen: Below Cal  
RT: 2.855 min Scan# 27  
Delta R.T. 0.000 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44




Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145


Tot Ion: 84 Resp: 1003  
Ion Ratio Lower Upper  
84 100  
49 106.3 92.3 138.5  
51 47.5 31.8 47.6  
86 54.2 48.5 72.7

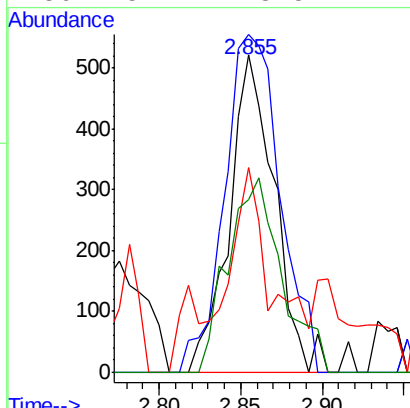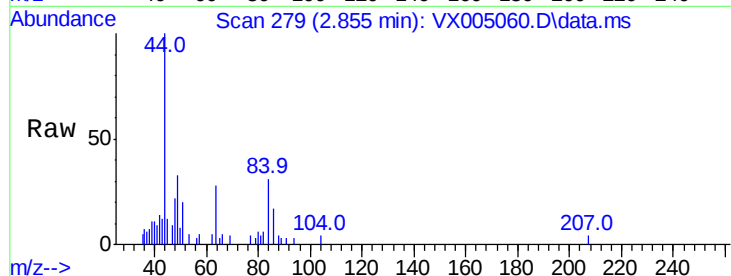

#24  
1,1-Dichloroethane  
Concen: 3.52 ug/l  
RT: 3.696 min Scan# 417  
Delta R.T. 0.000 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44

Tgt Ion: 63 Resp: 17852  
Ion Ratio Lower Upper  
63 100  
98 5.7 3.0 9.2  
100 5.2 2.0 5.8

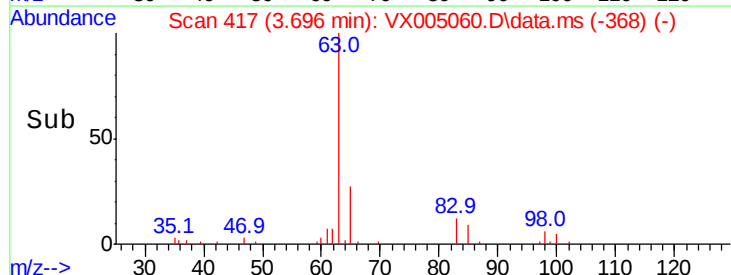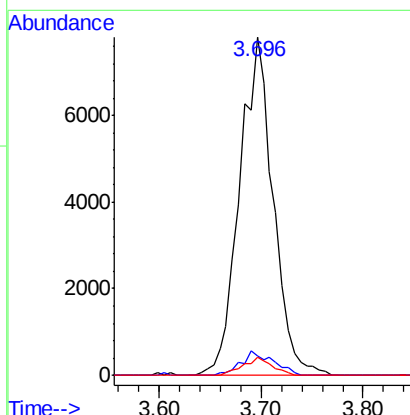

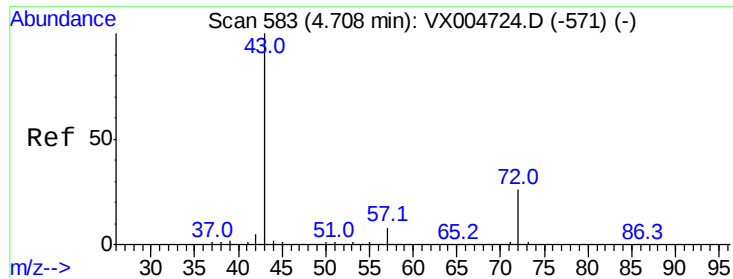

#25

2-Butanone

Concen: 1.43 ug/l

RT: 4.702 min Scan# 58

Delta R.T. -0.006 min

Lab File: VX005060.D

Acq: 05 Oct 2018 10:44

Instrument :

MSVOA\_X

ClientSampleId :





SA-TW512-4145

Tot Ion: 43 Resp: 3756

Ion Ratio Lower Upper

43 100

72 18.7 20.8 31.2#

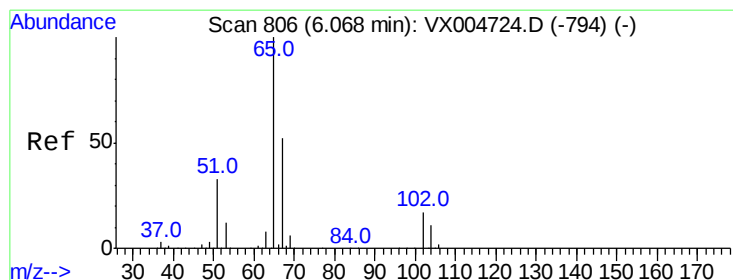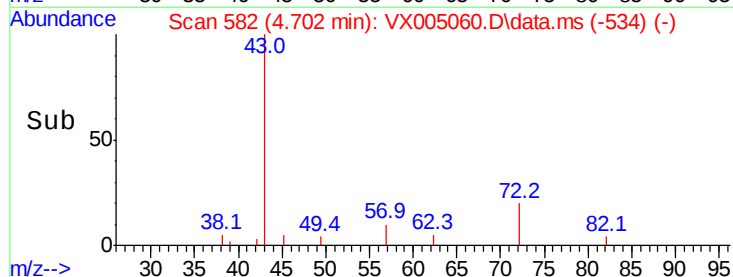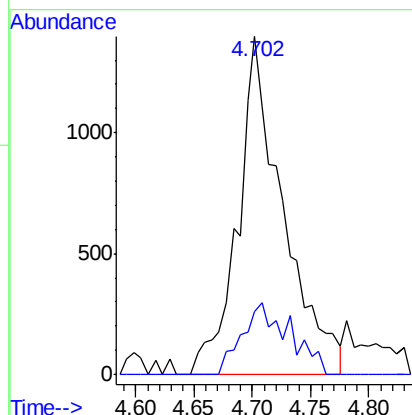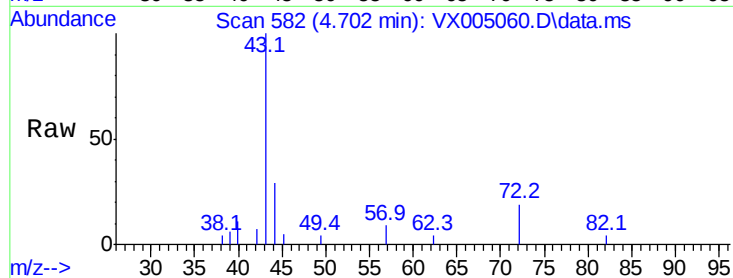

#33

1,2-Dichloroethane-d4

Concen: 54.60 ug/l

RT: 6.061 min Scan# 805

Delta R.T. -0.006 min

Lab File: VX005060.D




Acq: 05 Oct 2018 10:44


Tgt Ion: 65 Resp: 166656

Ion Ratio Lower Upper

65 100

67 53.4 0.0 107.4


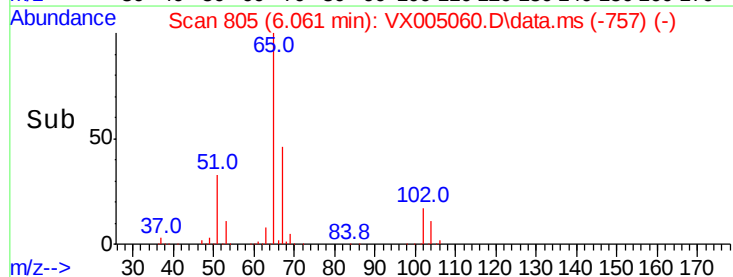
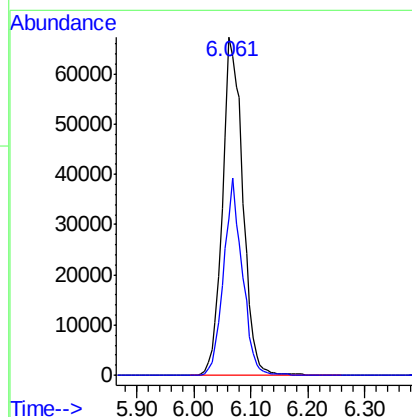
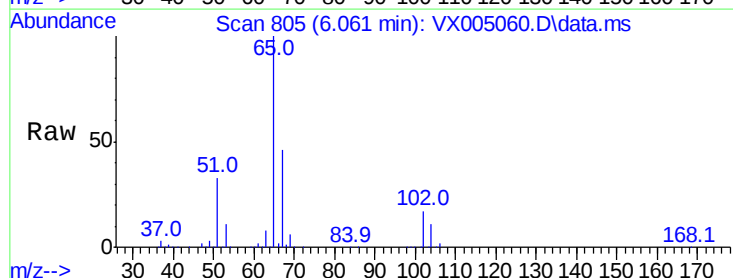


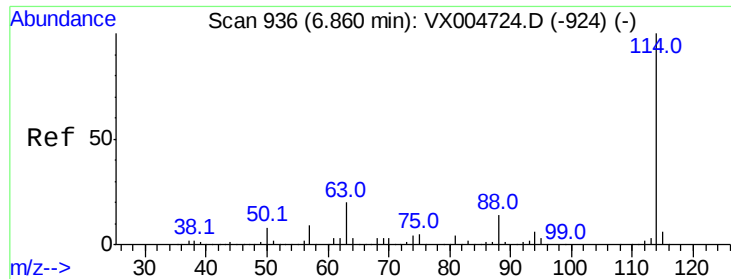

#34  
 1,4-Difluorobenzene  
 Concen: 50.00 ug/l  
 RT: 6.860 min Scan# 93  
 Delta R.T. 0.000 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW512-4145


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 114     | 100   |       |       |
| 63      | 20.9  | 0.0   | 39.8  |
| 88      | 15.9  | 0.0   | 27.0  |

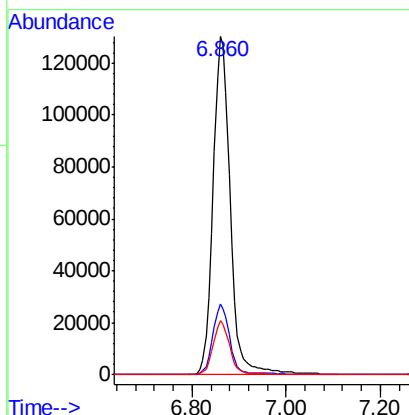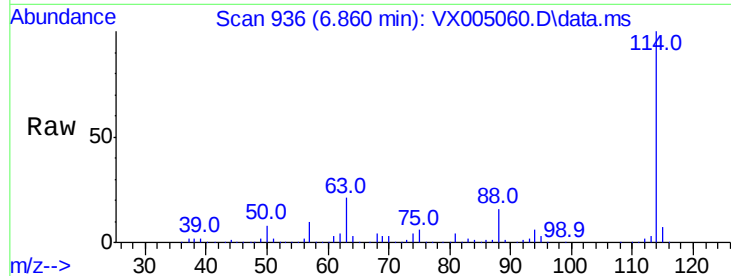

#35  
 Dibromofluoromethane  
 Concen: 49.78 ug/l  
 RT: 5.501 min Scan# 713  
 Delta R.T. 0.000 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 113     | 100   |       |       |
| 111     | 100.8 | 77.0  | 115.4 |
| 192     | 24.0  | 17.0  | 25.6  |



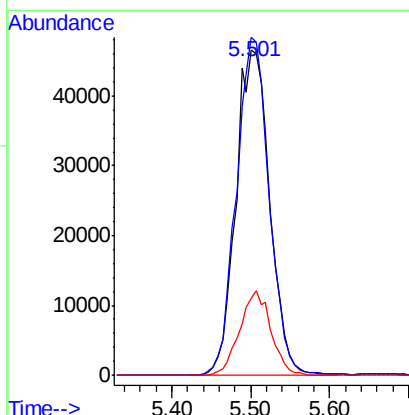



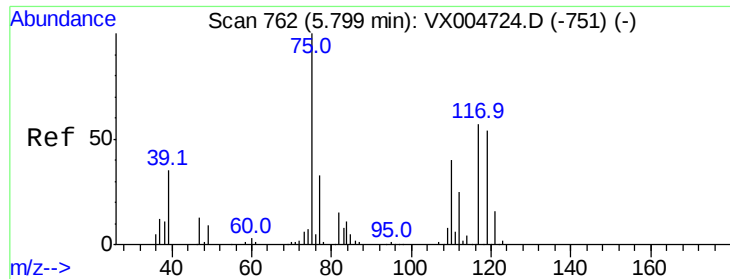

#36  
 1,1-Dichloropropene  
 Concen: 3.78 ug/l  
 RT: 5.665 min Scan# 740  
 Delta R.T. -0.134 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW512-4145


Tot Ion: 75 Resp: 14403  
 Ion Ratio Lower Upper  
 75 100  
 110 9.6 20.0 59.9#  
 77 0.0 27.1 40.7#

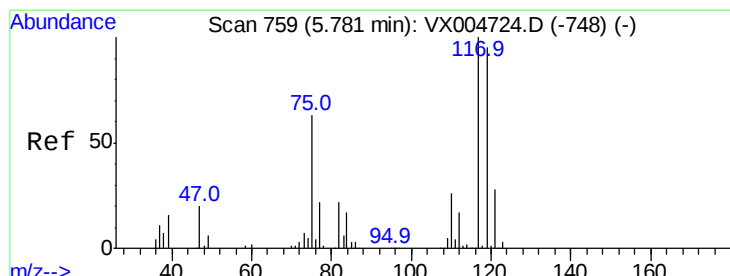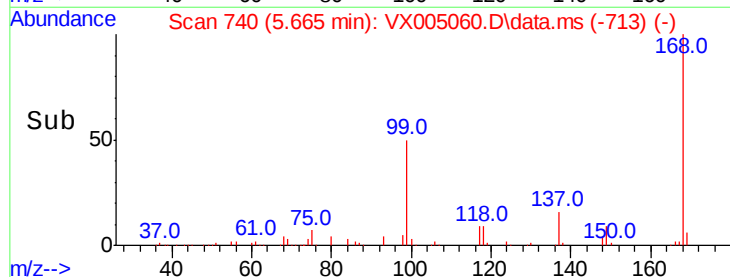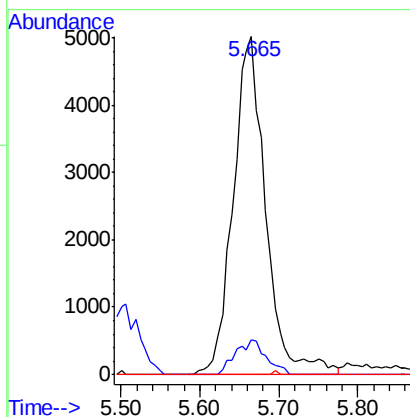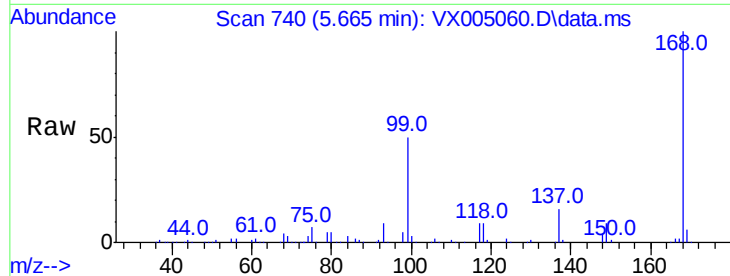

#38  
 Carbon Tetrachloride  
 Concen: 4.74 ug/l  
 RT: 5.665 min Scan# 740  
 Delta R.T. -0.116 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44

Tgt Ion: 117 Resp: 18997  
 Ion Ratio Lower Upper  
 117 100  
 119 6.1 75.2 112.8#  
 121 0.0 22.5 33.7#


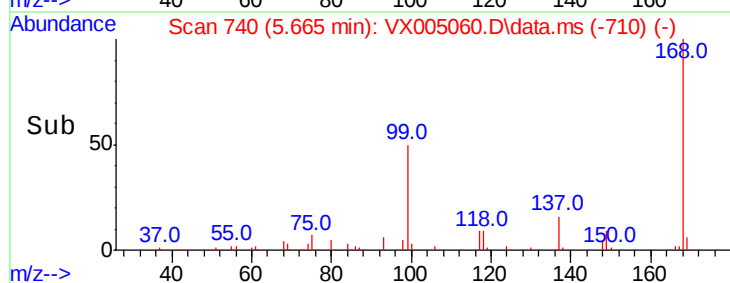
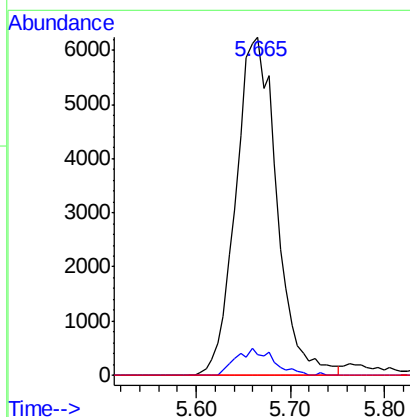
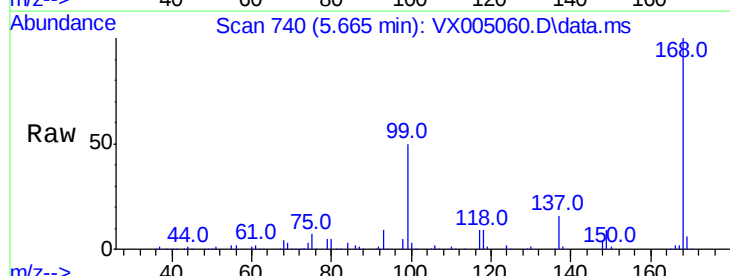


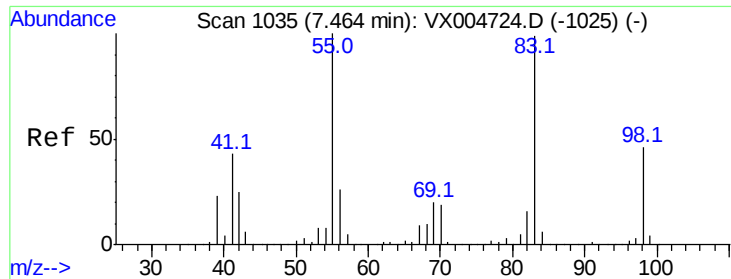

#39  
Methylcyclohexane  
Concen: 0.22 ug/l  
RT: 7.458 min Scan# 1034  
Delta R.T. -0.006 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44




Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145


Tot Ion: 83 Resp: 850  
Ion Ratio Lower Upper  
83 100  
55 76.7 81.1 121.7#  
98 52.7 37.3 55.9

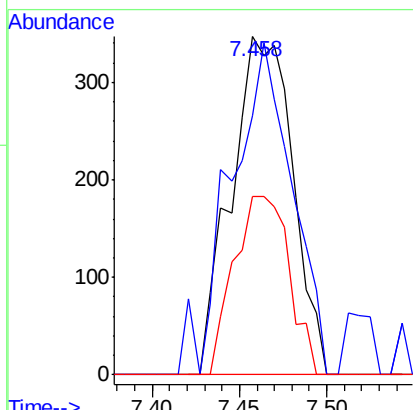

#50  
Toluene-d8  
Concen: 51.27 ug/l  
RT: 8.720 min Scan# 1241  
Delta R.T. 0.000 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44

Tgt Ion: 98 Resp: 476252  
Ion Ratio Lower Upper  
98 100  
100 63.8 51.9 77.9

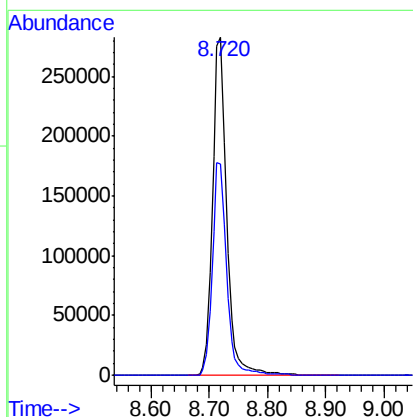

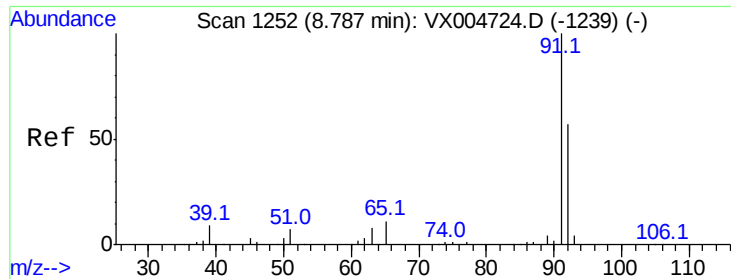

#52

Toluene

Concen: 0.81 ug/l

RT: 8.787 min Scan# 12

Delta R.T. 0.000 min

Lab File: VX005060.D

Acq: 05 Oct 2018 10:44

Instrument :

MSVOA\_X

ClientSampleId :





SA-TW512-4145

Tot Ion: 92 Resp: 5301

Ion Ratio Lower Upper

92 100

91 160.2 136.7 205.1

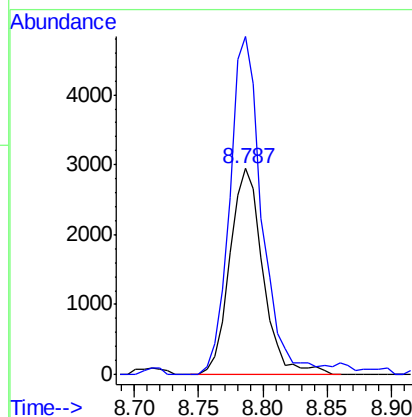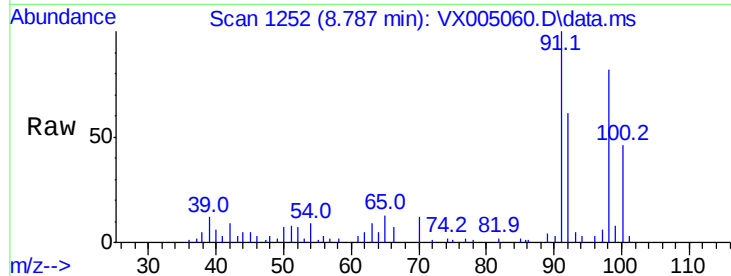

#56

Ethyl methacrylate

Concen: 2.87 ug/l

RT: 9.274 min Scan# 1332

Delta R.T. 0.091 min

Lab File: VX005060.D

Acq: 05 Oct 2018 10:44




Tgt Ion: 69 Resp: 25


Ion Ratio Lower Upper

69 100

41 296.0 56.9 85.3#

39 212.0 28.4 42.6#



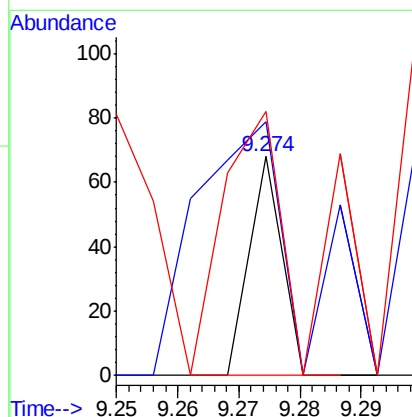



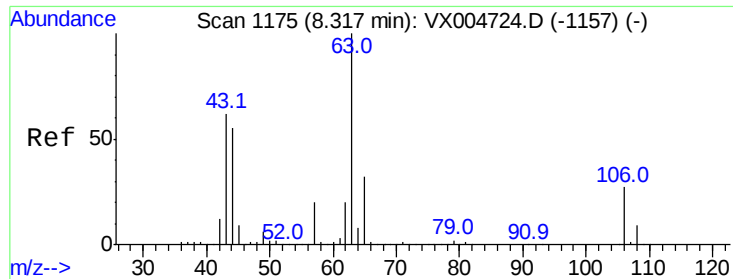

#58  
 2-Chloroethyl Vinyl ether  
 Concen: 14.25 ug/l  
 RT: 8.348 min Scan# 1175  
 Delta R.T. 0.030 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW512-4145


Tot Ion: 63 Resp: 19  
 Ion Ratio Lower Upper  
 63 100  
 106 0.0 21.0 31.6#

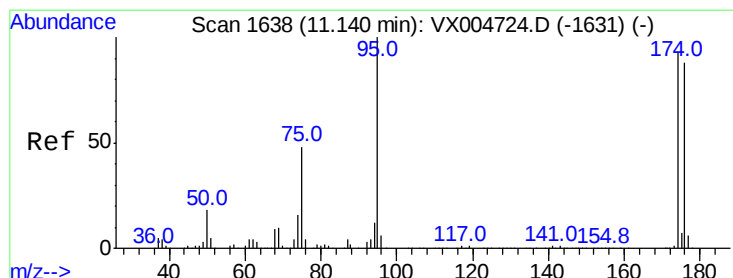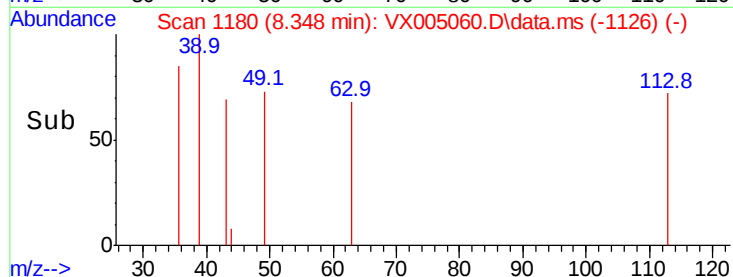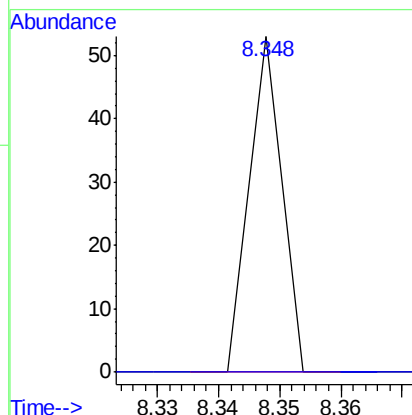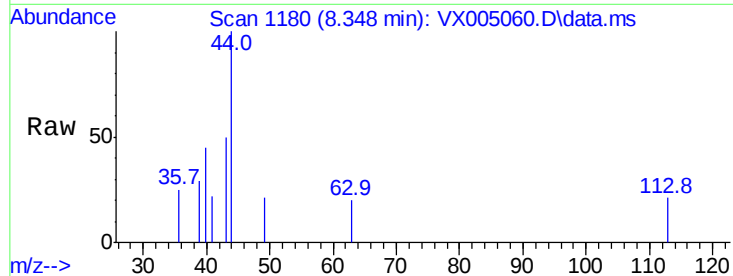

#62  
 4-Bromofluorobenzene  
 Concen: 51.20 ug/l  
 RT: 11.140 min Scan# 1638  
 Delta R.T. 0.000 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44

Tgt Ion: 95 Resp: 171321  
 Ion Ratio Lower Upper  
 95 100  
 174 93.2 0.0 185.0  
 176 88.8 0.0 180.2


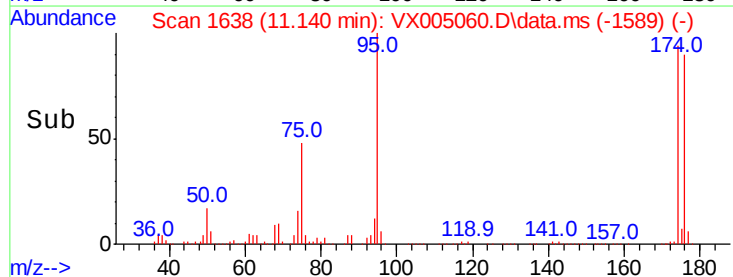
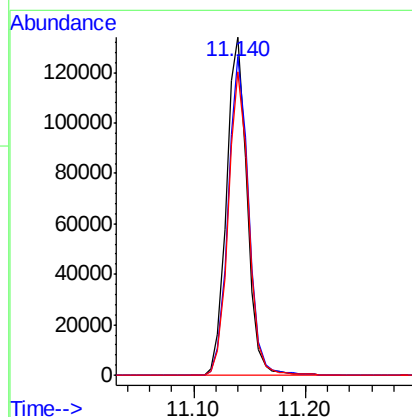
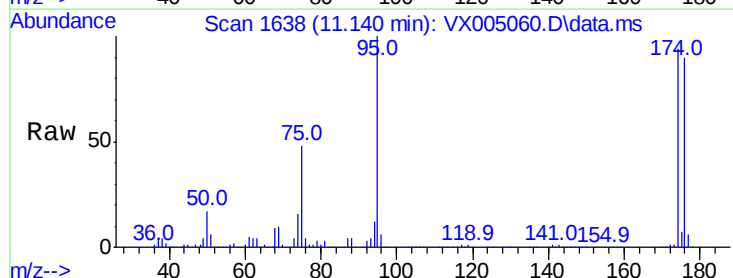


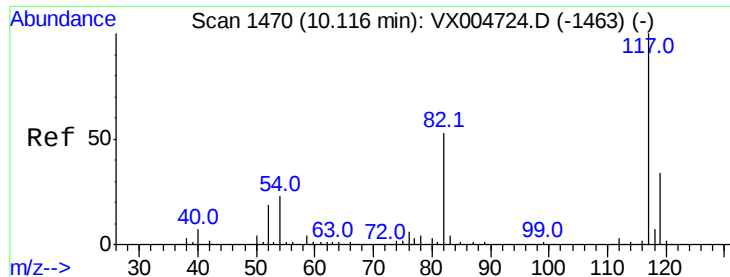

#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 10.116 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44




Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145


Tot Ion:117 Resp: 326750  
Ion Ratio Lower Upper  
117 100  
82 53.2 42.2 63.4  
119 31.9 27.4 41.0

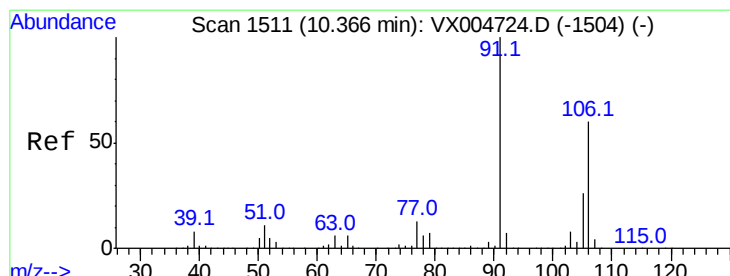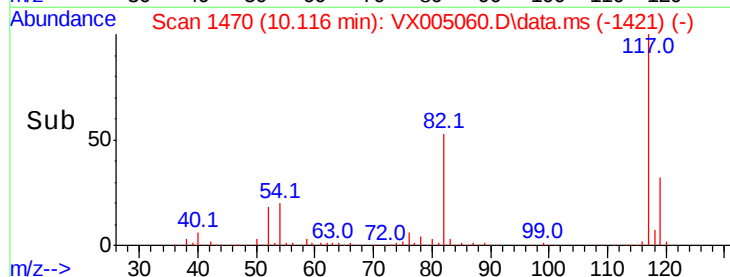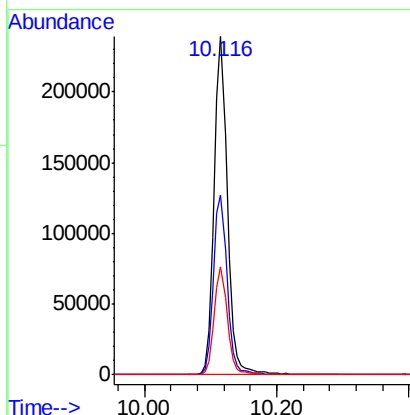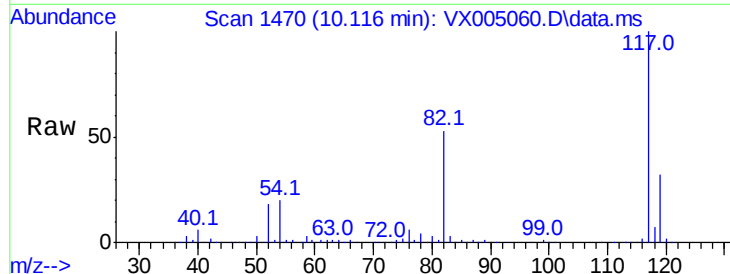

#68  
m/p-Xylenes  
Concen: 0.40 ug/l  
RT: 10.360 min Scan# 1510  
Delta R.T. -0.006 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44

Tgt Ion:106 Resp: 2080  
Ion Ratio Lower Upper  
106 100  
91 189.8 157.5 236.3


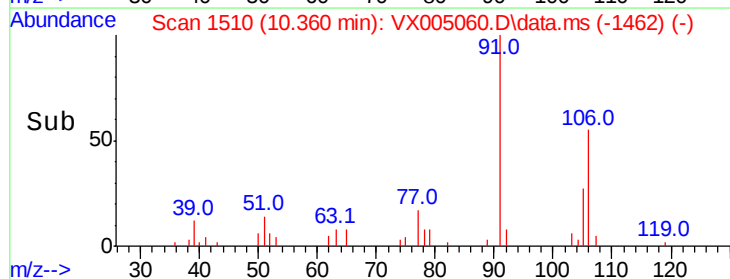
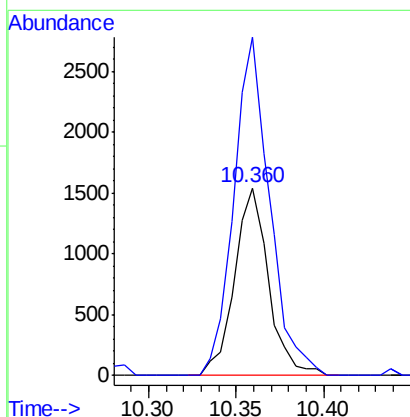
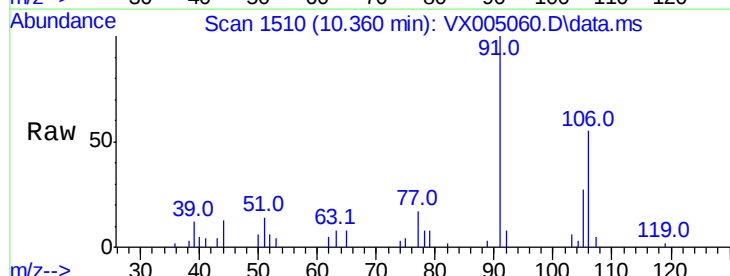


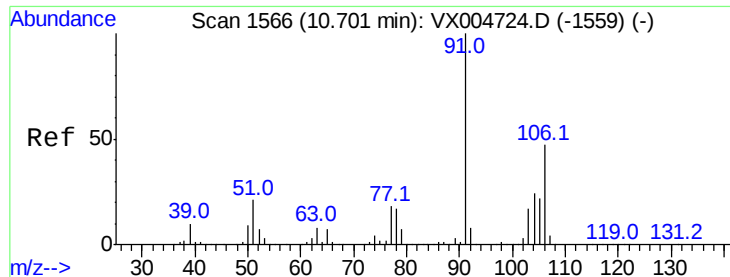

#69  
o-Xylene  
Concen: 0.20 ug/l  
RT: 10.701 min Scan# 1566  
Delta R.T. 0.000 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44




Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW512-4145


Tot Ion:106 Resp: 961  
Ion Ratio Lower Upper  
106 100  
91 249.2 108.3 324.8

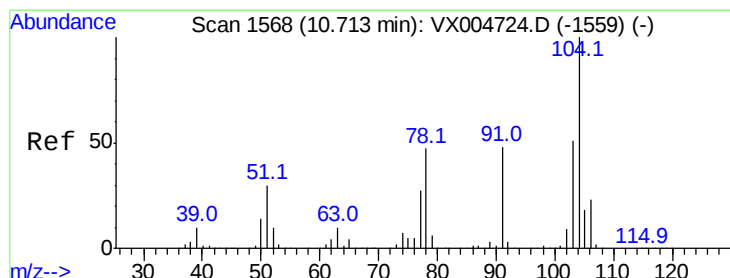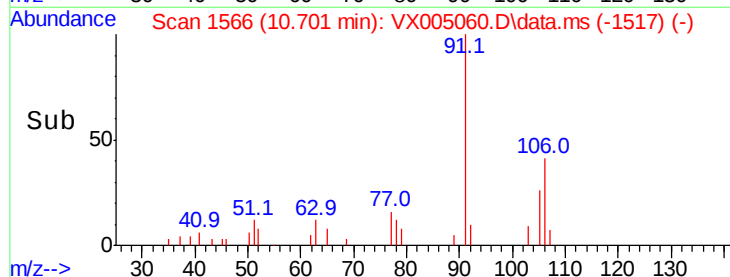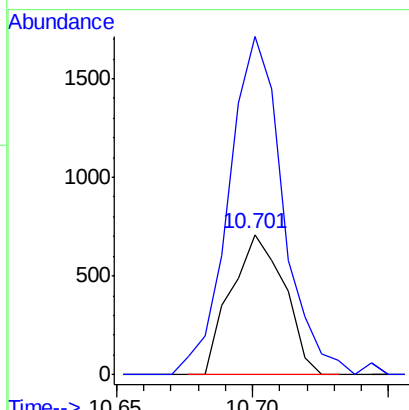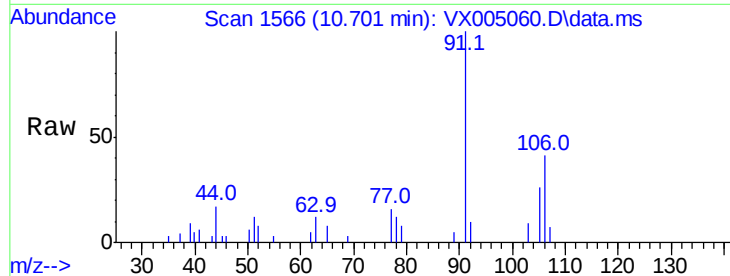

#70  
Styrene  
Concen: 2.15 ug/l  
RT: 10.713 min Scan# 1568  
Delta R.T. 0.000 min  
Lab File: VX005060.D  
Acq: 05 Oct 2018 10:44

Tgt Ion:104 Resp: 83  
Ion Ratio Lower Upper  
104 100  
78 294.0 40.0 60.0#  
103 330.1 44.3 66.5#


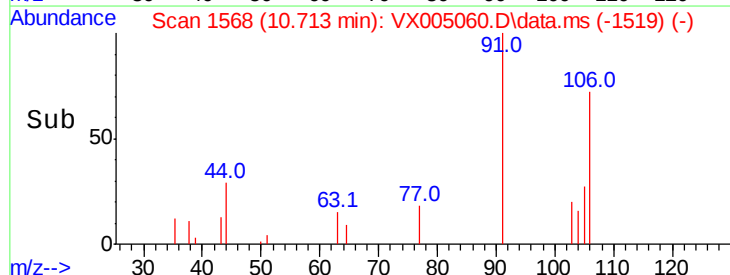
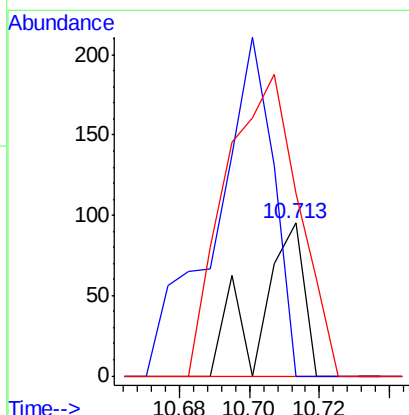
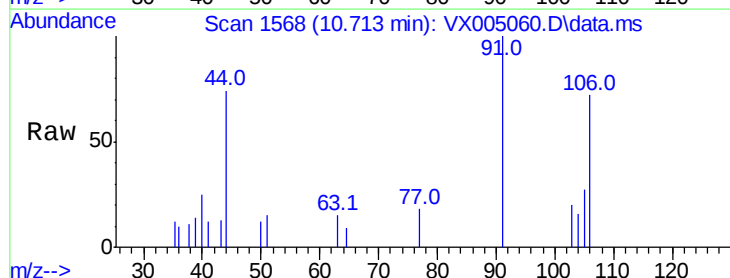


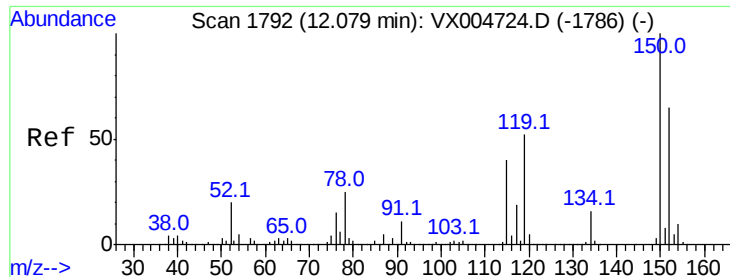

#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.00 ug/l  
 RT: 12.079 min Scan# 1792  
 Delta R.T. 0.000 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW512-4145


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 152     | 100   |       |       |
| 115     | 55.7  | 40.2  | 120.6 |
| 150     | 155.5 | 0.0   | 351.0 |

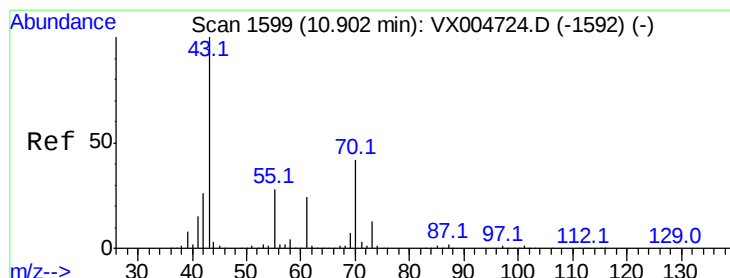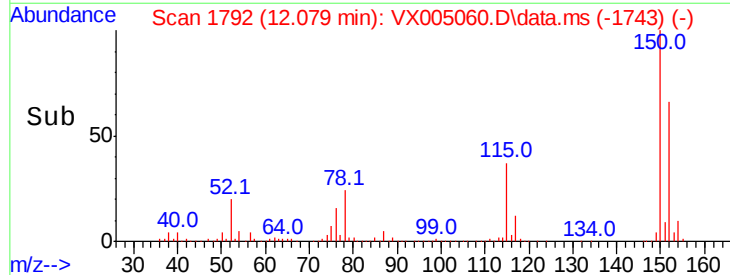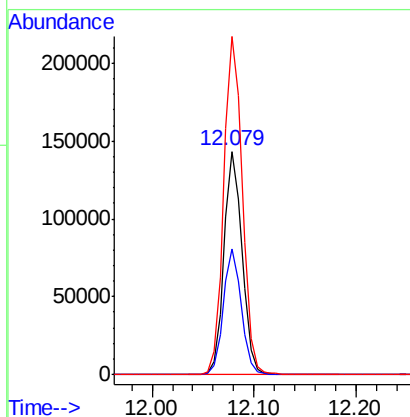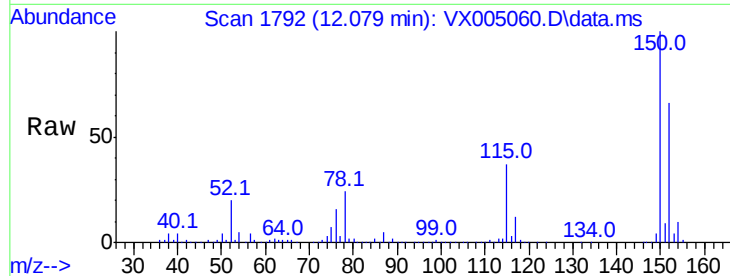

#74  
 N-ethyl acetate  
 Concen: 1.80 ug/l  
 RT: 10.908 min Scan# 1600  
 Delta R.T. 0.006 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 43      | 100   |       |       |
| 70      | 117.2 | 32.6  | 48.8# |
| 55      | 150.5 | 21.6  | 32.4# |
| 61      | 0.0   | 19.1  | 28.7# |


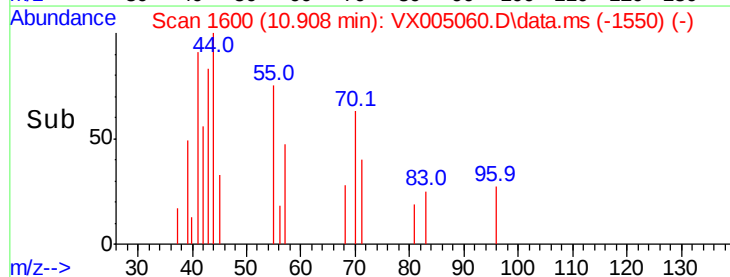
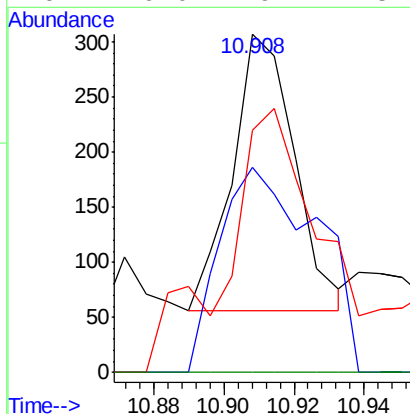
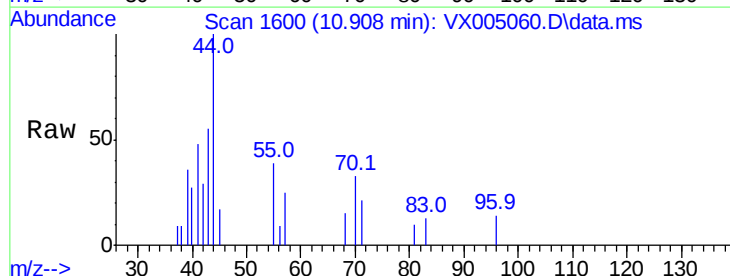


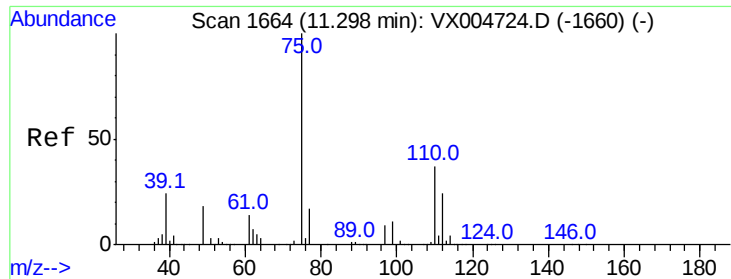

#76  
 1,2,3-Trichloropropane  
 Concen: 21.19 ug/l  
 RT: 11.140 min Scan# 1638  
 Delta R.T. -0.159 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW512-4145


Tot Ion: 75 Resp: 83941  
 Ion Ratio Lower Upper  
 75 100  
 77 1.3 21.4 64.3#

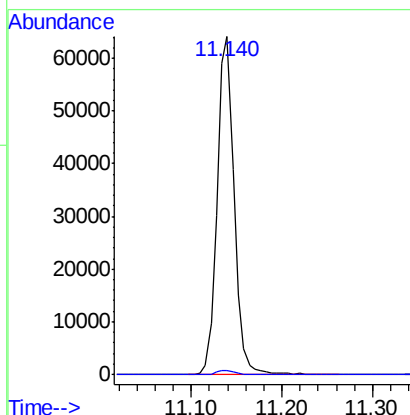

#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 57.48 ug/l  
 RT: 11.140 min Scan# 1638  
 Delta R.T. 0.061 min  
 Lab File: VX005060.D  
 Acq: 05 Oct 2018 10:44

Tgt Ion: 75 Resp: 83941  
 Ion Ratio Lower Upper  
 75 100  
 53 0.3 80.2 120.4#  
 89 0.0 37.1 55.7#

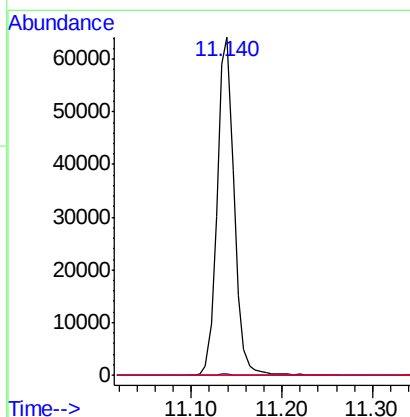

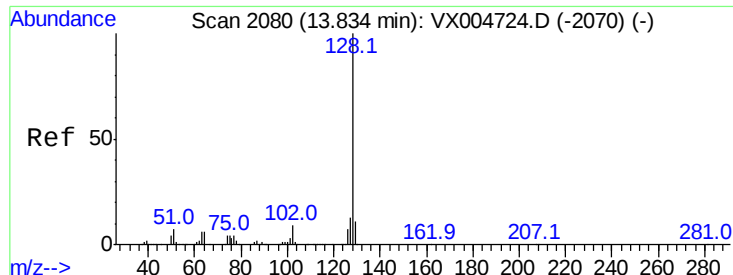

#95

Naphthalene

Concen: 0.78 ug/l

RT: 13.834 min Scan# 20

Delta R.T. 0.000 min

Lab File: VX005060.D

Acq: 05 Oct 2018 10:44

Instrument :

MSVOA\_X

ClientSampleId :

SA-TW512-4145

Tot Ion:128 Resp: 946

Ion Ratio Lower Upper

128 100

127 18.6 10.4 15.6#

129 12.6 8.7 13.1

