

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100418\
 Data File : VX005015.D
 Acq On : 04 Oct 2018 12:41
 Operator : JC/MD
 Sample : J5214-04DL 1000X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 N48719DL

Manual Integrations
 APPROVED

MMDadoda
 10/5/2018 3:24:49 PM

Quant Time: Oct 05 13:25:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 03 04:00:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	243865	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	408369	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	398623	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	231278	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.07	65	175819	50.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.94%	
35) Dibromofluoromethane	5.50	113	151716	43.84	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.68%	
50) Toluene-d8	8.72	98	577170	50.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.32%	
62) 4-Bromofluorobenzene	11.14	95	233553	56.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.68%	

MMDadoda

10/5/2018 3:24:49 PM

Target Compounds

						Qvalue
16) Acetone	2.45	43	112108	55.122	ug/l	93
25) 2-Butanone	4.70	43	130176	43.423	ug/l	100
39) Methylcyclohexane	7.46	83	10499	2.177	ug/l #	83
40) Benzene	6.14	78	30027	2.031	ug/l	95
42) 1,2-Dichloroethane	6.20	62	4032	0.772	ug/l	85
51) 4-Methyl-2-Pentanone	8.65	43	15467	2.715	ug/l	99
52) Toluene	8.79	92	179377	22.082	ug/l	97
59) 2-Hexanone	9.50	43	31495	6.635	ug/l	96
67) Ethyl Benzene	10.26	91	870433	53.636	ug/l	97
68) m/p-Xylenes	10.36	106	1960258	309.111	ug/l	97
69) o-Xylene	10.70	106	1033675	177.463	ug/l	99
73) Isopropylbenzene	11.02	105	174020	11.937	ug/l	99
78) n-propylbenzene	11.36	91	1001006	59.846	ug/l	99
80) 1,3,5-Trimethylbenzene	11.51	105	1958374	146.957	ug/l	99
84) 1,2,4-Trimethylbenzene	11.81	105	7282242	530.407	ug/l	97
85) sec-Butylbenzene	11.94	105	81541m	5.578	ug/l	
86) p-Isopropyltoluene	12.02	119	164020	12.383	ug/l	98
95) Naphthalene	13.83	128	3405415	175.190	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100418\
Data File : VX005015.D
Acq On : 04 Oct 2018 12:41
Operator : JC/MD
Sample : J5214-04DL 1000X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleID :
N48719DL

Manual Integrations
APPROVED

MMDadoda
10/5/2018 3:24:49 PM

Quant Time: Oct 05 13:25:17 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 03 04:00:03 2018
Response via : Initial Calibration

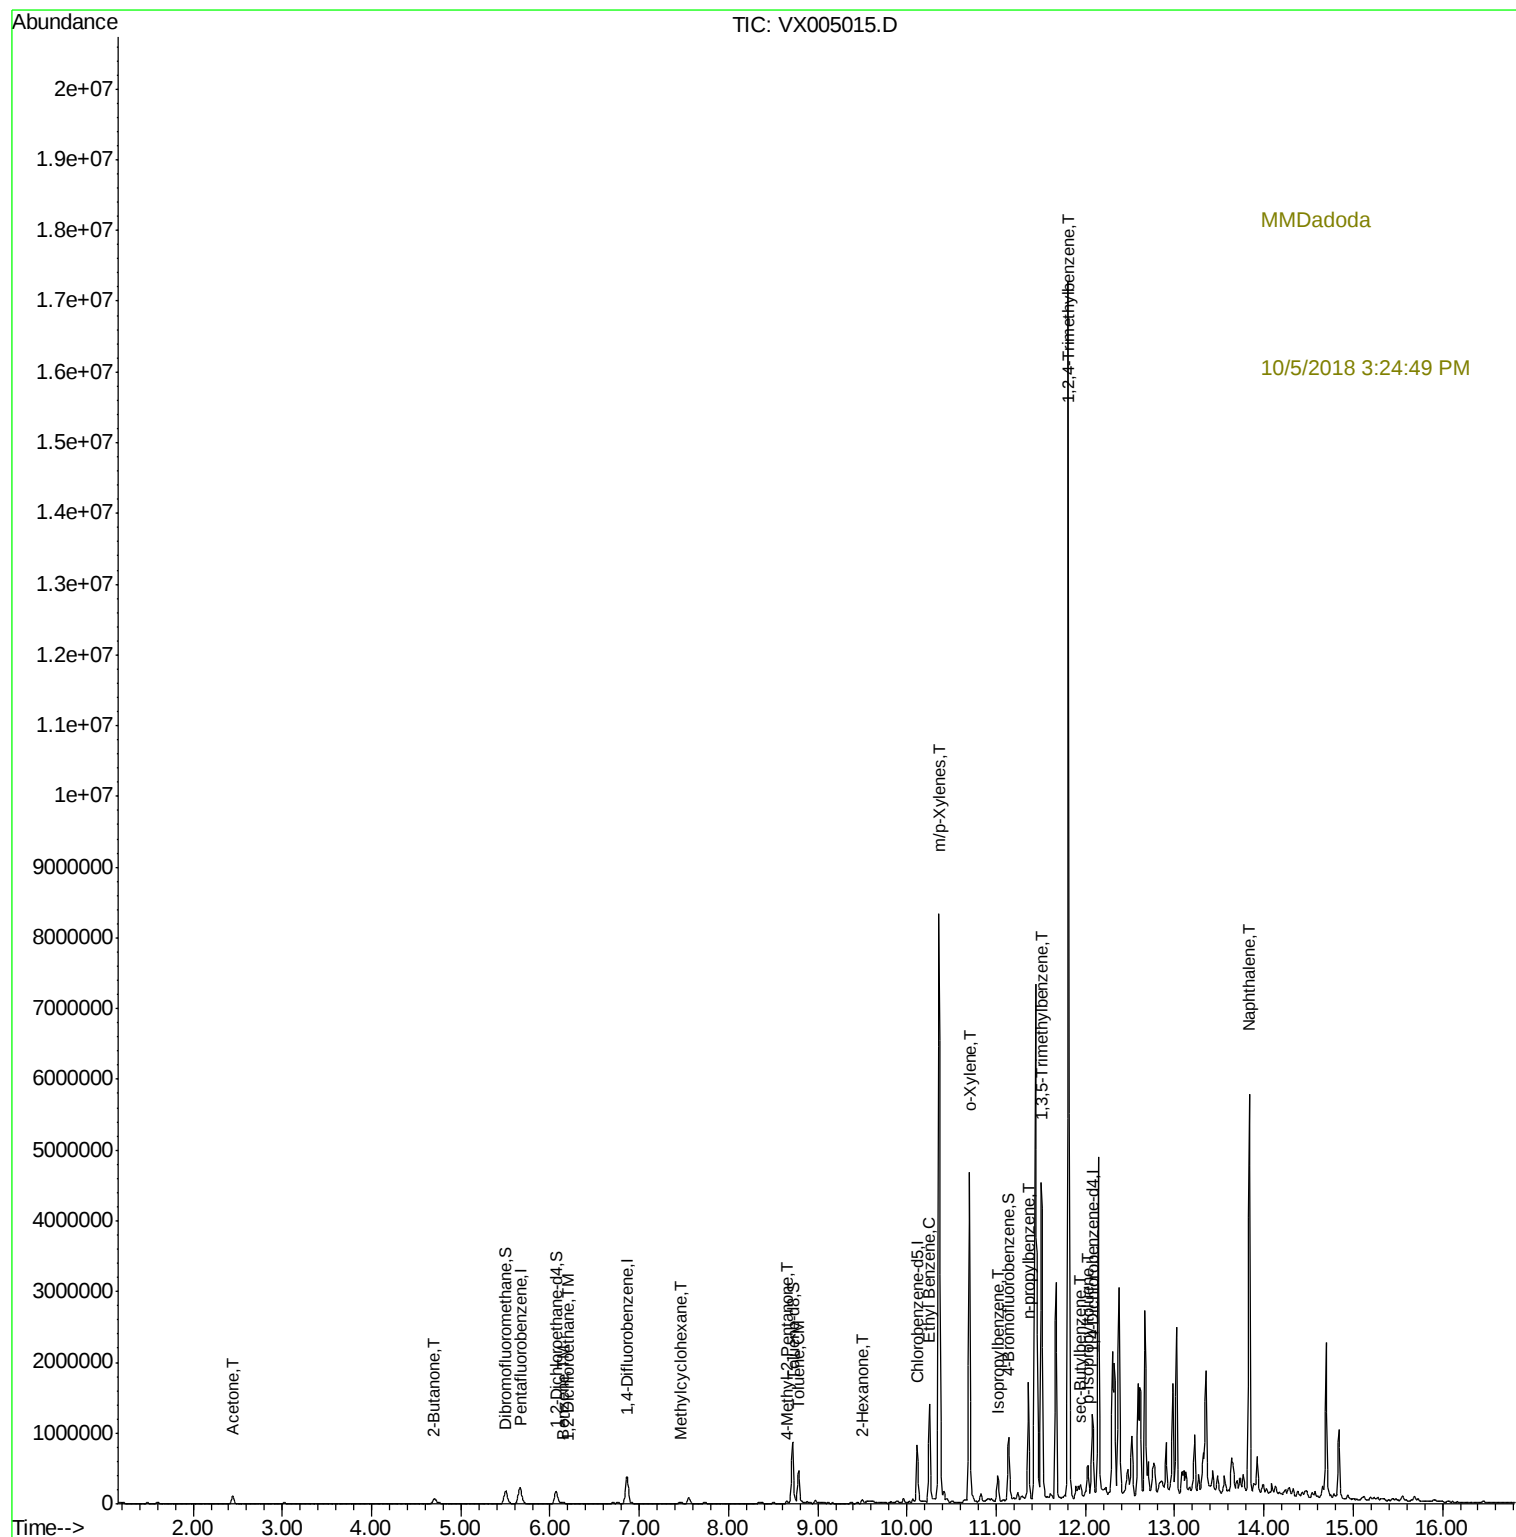

MMDadoda

10/5/2018 3:24:49 PM