

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100418\
 Data File : VX005032.D
 Acq On : 04 Oct 2018 21:22
 Operator : JC/MD
 Sample : J5207-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-TW507-4347

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.611	68	75	76	rBV7	8248	15258	1.12%	0.214%
2	2.446	208	212	219	rVB	9027	14785	1.09%	0.207%
3	2.623	234	241	248	rBV	79218	140281	10.34%	1.964%
4	3.025	298	307	314	rVB	15662	36516	2.69%	0.511%
5	4.775	581	594	606	rBV2	15090	51120	3.77%	0.716%
6	5.501	701	713	727	rBV2	167586	482598	35.57%	6.756%
7	5.665	729	740	756	rBV	207127	606004	44.67%	8.483%
8	6.068	794	806	824	rBV	176247	458206	33.78%	6.414%
9	6.860	925	936	963	rBV	332650	843715	62.19%	11.811%
10	8.720	1233	1241	1263	rBV	779391	1356618	100.00%	18.990%
11	10.116	1463	1470	1490	rBV	724448	1036240	76.38%	14.506%
12	11.140	1632	1638	1652	rBV	751048	950600	70.07%	13.307%
13	12.079	1786	1792	1801	rBV	950637	1151733	84.90%	16.122%


Sum of corrected areas: 7143674

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100418\
Data File : VX005032.D
Acq On : 04 Oct 2018 21:22
Operator : JC/MD
Sample : J5207-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-TW507-4347

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

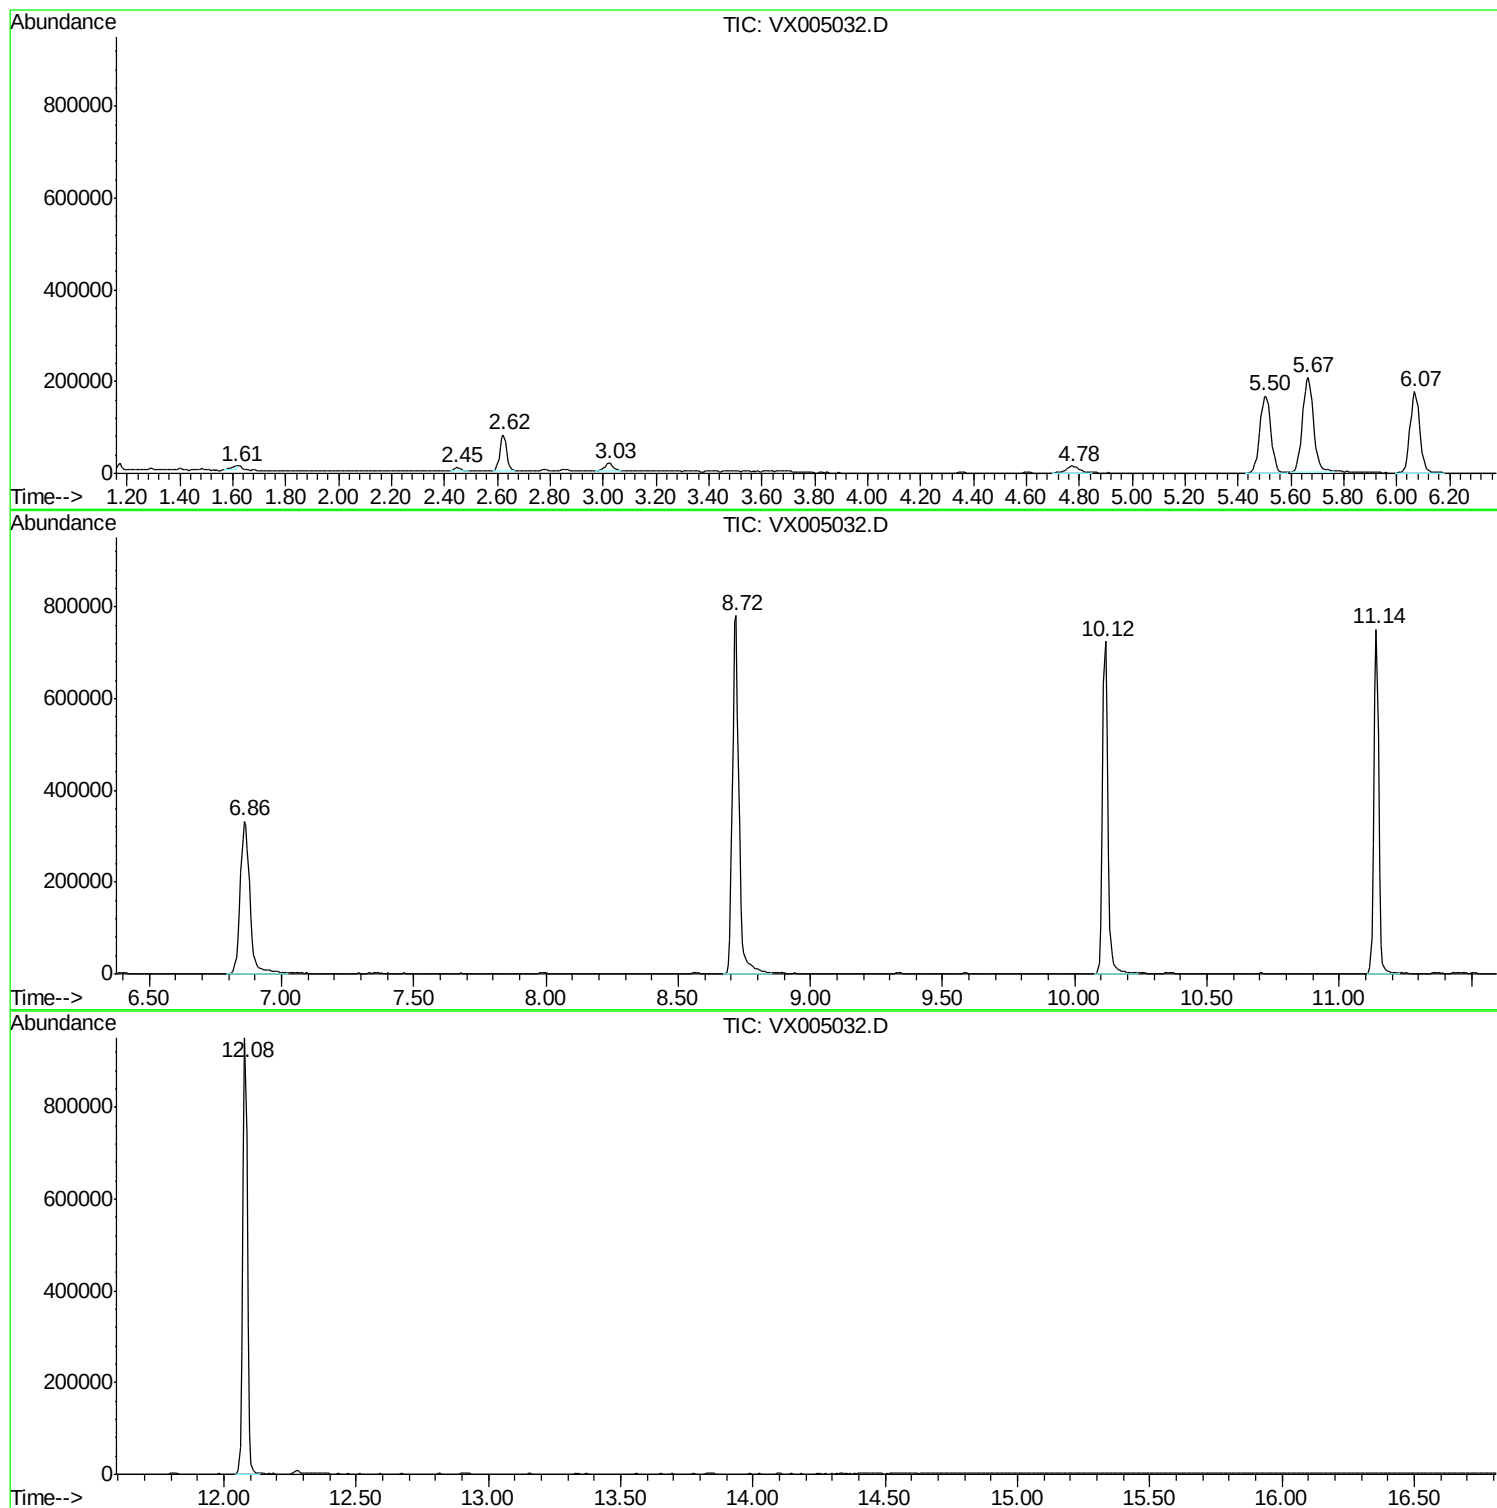

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100418\
Data File : VX005032.D
Acq On : 04 Oct 2018 21:22
Operator : JC/MD
Sample : J5207-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-TW507-4347










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.62	11.57 ug/l	140281	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		1-Butene, 4-methoxy	86	C5H10O	004696-30-4	4
4		2-Butanol	74	C4H10O	000078-92-2	4
5		Formamide	45	CH3NO	000075-12-7	4

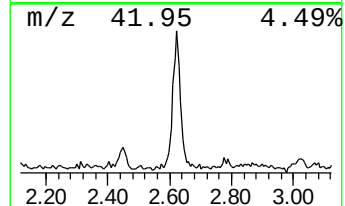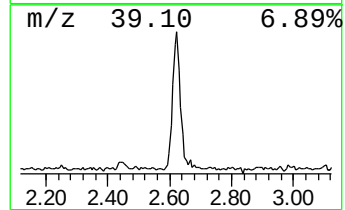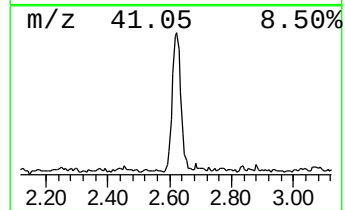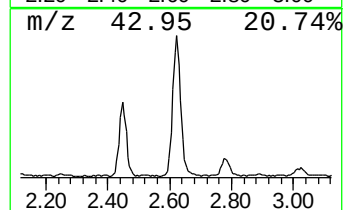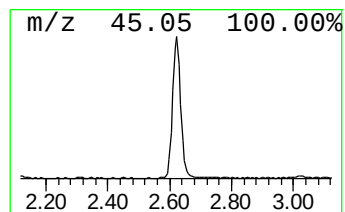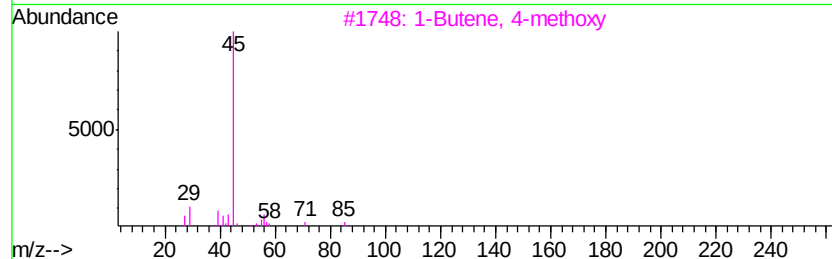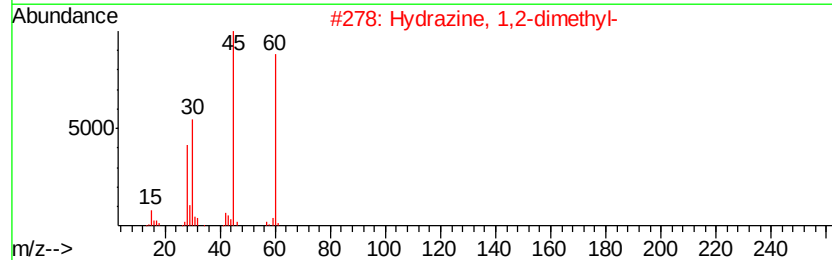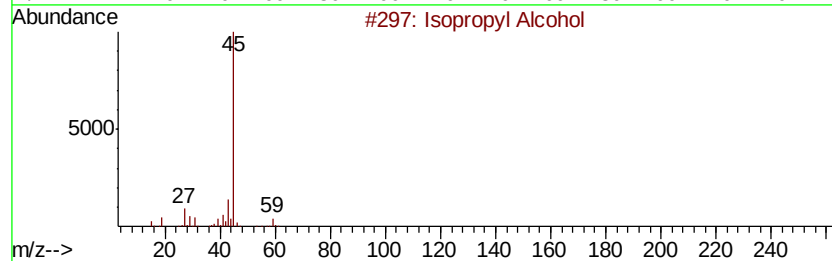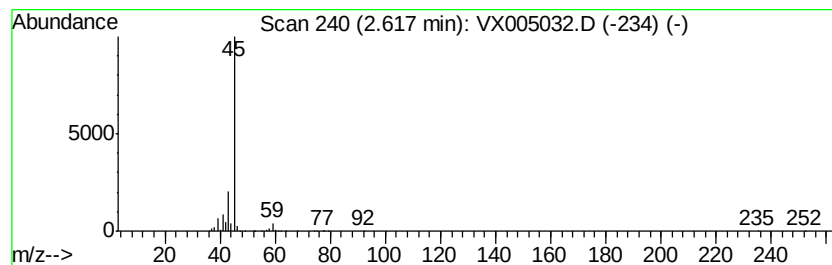

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100418\
Data File : VX005032.D
Acq On : 04 Oct 2018 21:22
Operator : JC/MD
Sample : J5207-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-TW507-4347

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.62	11.6	ug/l	140281	1	5.67	606004	50.0