


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100418\
 Data File : VX004967.D
 Acq On : 03 Oct 2018 14:14
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N100518W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Oct 05 11:11:26 2018

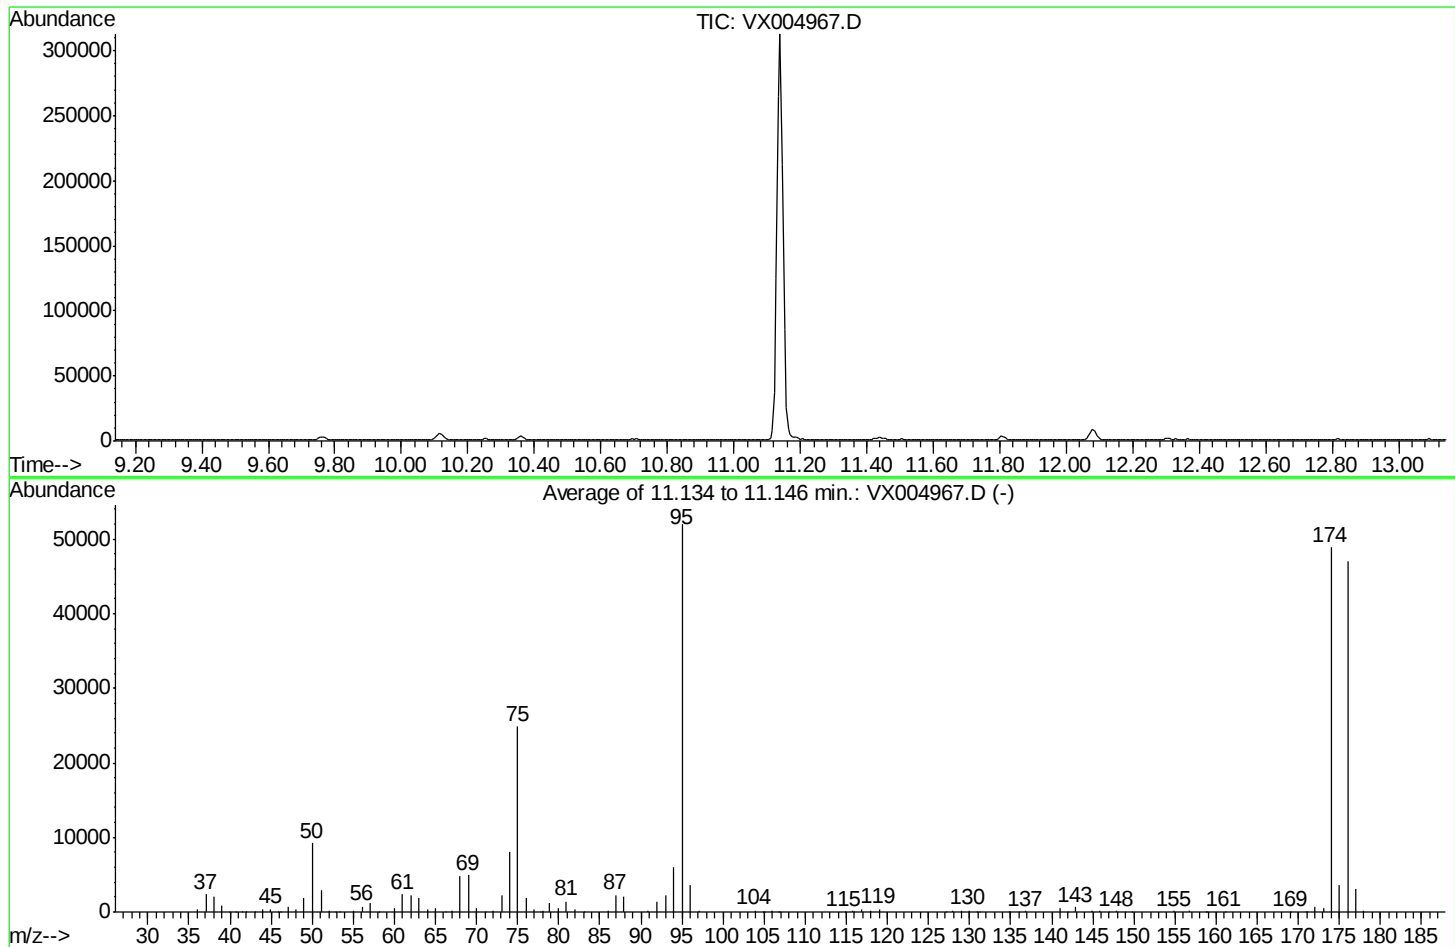

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	9226	PASS
75	95	30	60	47.7	24821	PASS
95	95	100	100	100.0	51984	PASS
96	95	5	9	7.0	3643	PASS
173	174	0.00	2	1.1	554	PASS
174	95	50	100	94.0	48842	PASS
175	174	5	9	7.5	3671	PASS
176	174	95	101	96.1	46960	PASS
177	176	5	9	6.6	3078	PASS