


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100418\
Data File : VX005017.D
Acq On : 04 Oct 2018 13:34
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N100518W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Oct 05 11:11:26 2018

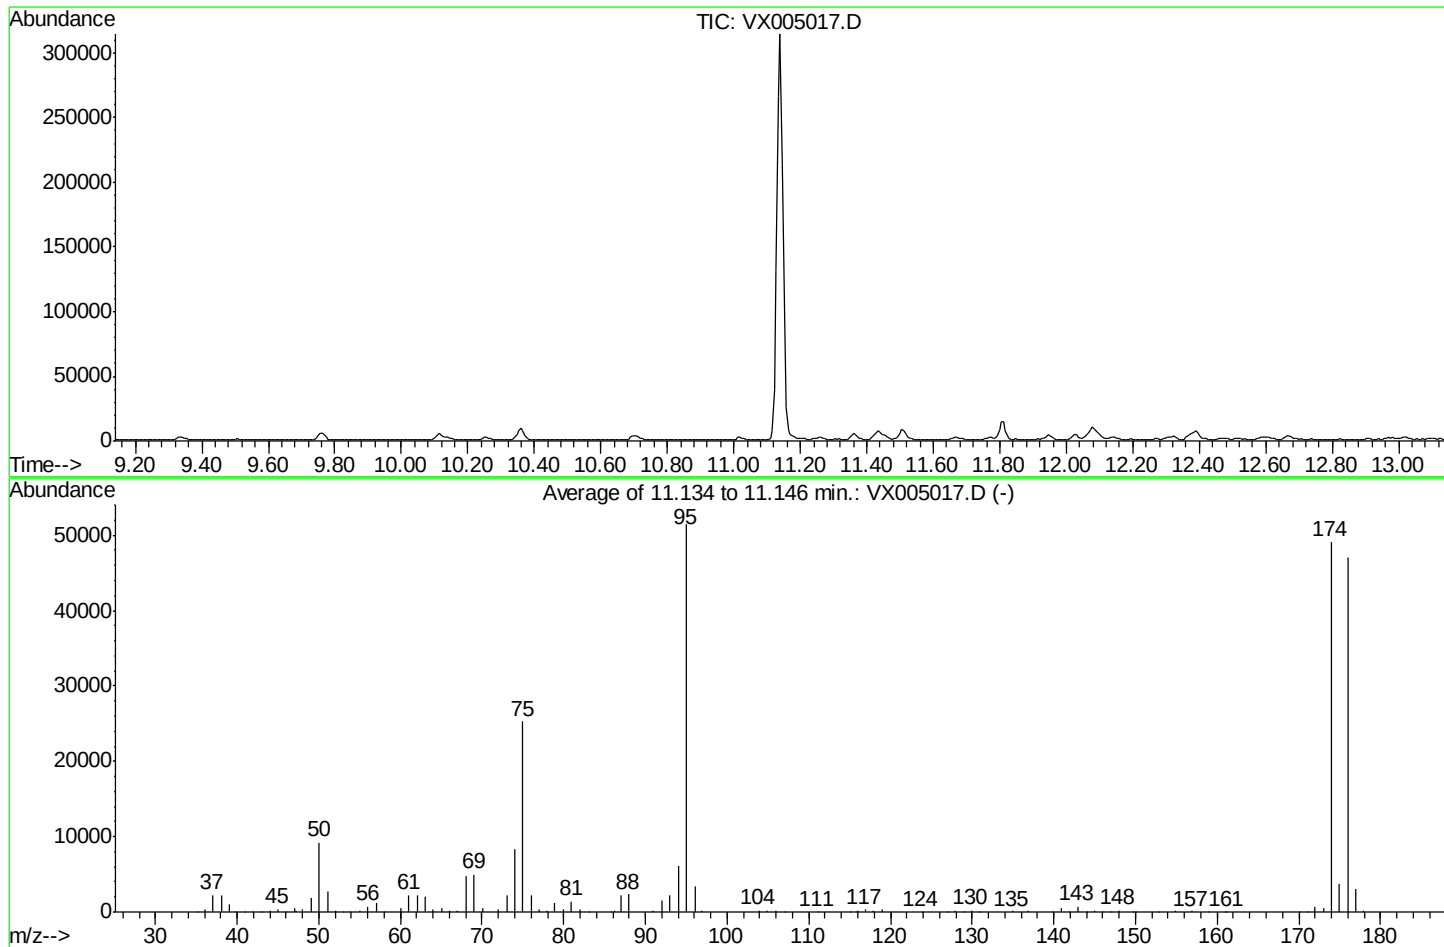

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9231	PASS
75	95	30	60	49.1	25274	PASS
95	95	100	100	100.0	51445	PASS
96	95	5	9	6.6	3377	PASS
173	174	0.00	2	1.1	548	PASS
174	95	50	100	95.5	49128	PASS
175	174	5	9	7.6	3747	PASS
176	174	95	101	95.8	47085	PASS
177	176	5	9	6.4	3029	PASS