


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100418\
 Data File : VX005042.D
 Acq On : 05 Oct 2018 02:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N100518W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Oct 05 11:11:26 2018

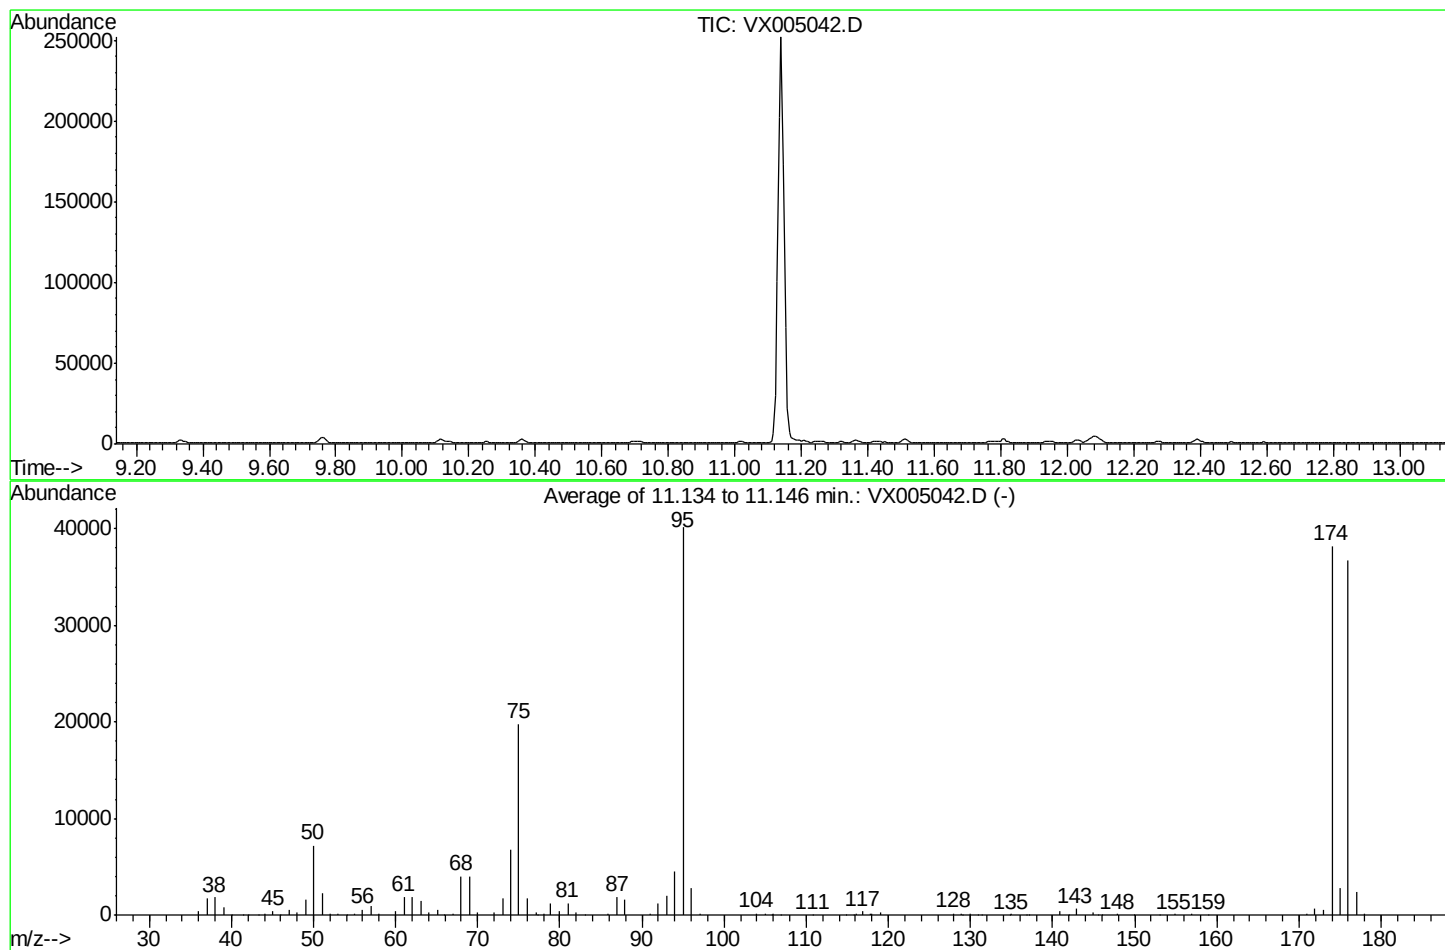

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	7229	PASS
75	95	30	60	49.3	19815	PASS
95	95	100	100	100.0	40157	PASS
96	95	5	9	6.9	2755	PASS
173	174	0.00	2	1.4	525	PASS
174	95	50	100	95.1	38200	PASS
175	174	5	9	7.5	2852	PASS
176	174	95	101	96.1	36722	PASS
177	176	5	9	6.7	2451	PASS