

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100419\
 Data File : VX012813.D
 Acq On : 04 Oct 2019 15:48
 Operator : JC/SP
 Sample : K5189-17
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ138I-20191001

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	419557	515583	53.31%	9.211%
2	1.265	58	62	69	rBV	33923	45197	4.67%	0.807%
3	2.436	249	254	263	rVB	7902	13563	1.40%	0.242%
4	2.594	271	280	291	rBV	71520	132886	13.74%	2.374%
5	5.490	742	755	767	rBV2	106398	303157	31.35%	5.416%
6	5.655	770	782	795	rVV	195002	544602	56.31%	9.730%
7	6.051	838	847	864	rBV2	124784	330820	34.21%	5.910%
8	6.849	969	978	993	rBV	307478	726247	75.10%	12.975%
9	8.709	1276	1283	1298	rBV	611246	967080	100.00%	17.278%
10	10.111	1507	1513	1530	rBV	584692	799344	82.66%	14.281%
11	11.135	1675	1681	1693	rBV	440039	566524	58.58%	10.121%
12	12.074	1830	1835	1845	rBV	529987	652268	67.45%	11.653%


Sum of corrected areas: 5597271

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100419\
Data File : VX012813.D
Acq On : 04 Oct 2019 15:48
Operator : JC/SP
Sample : K5189-17
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ138I-20191001

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

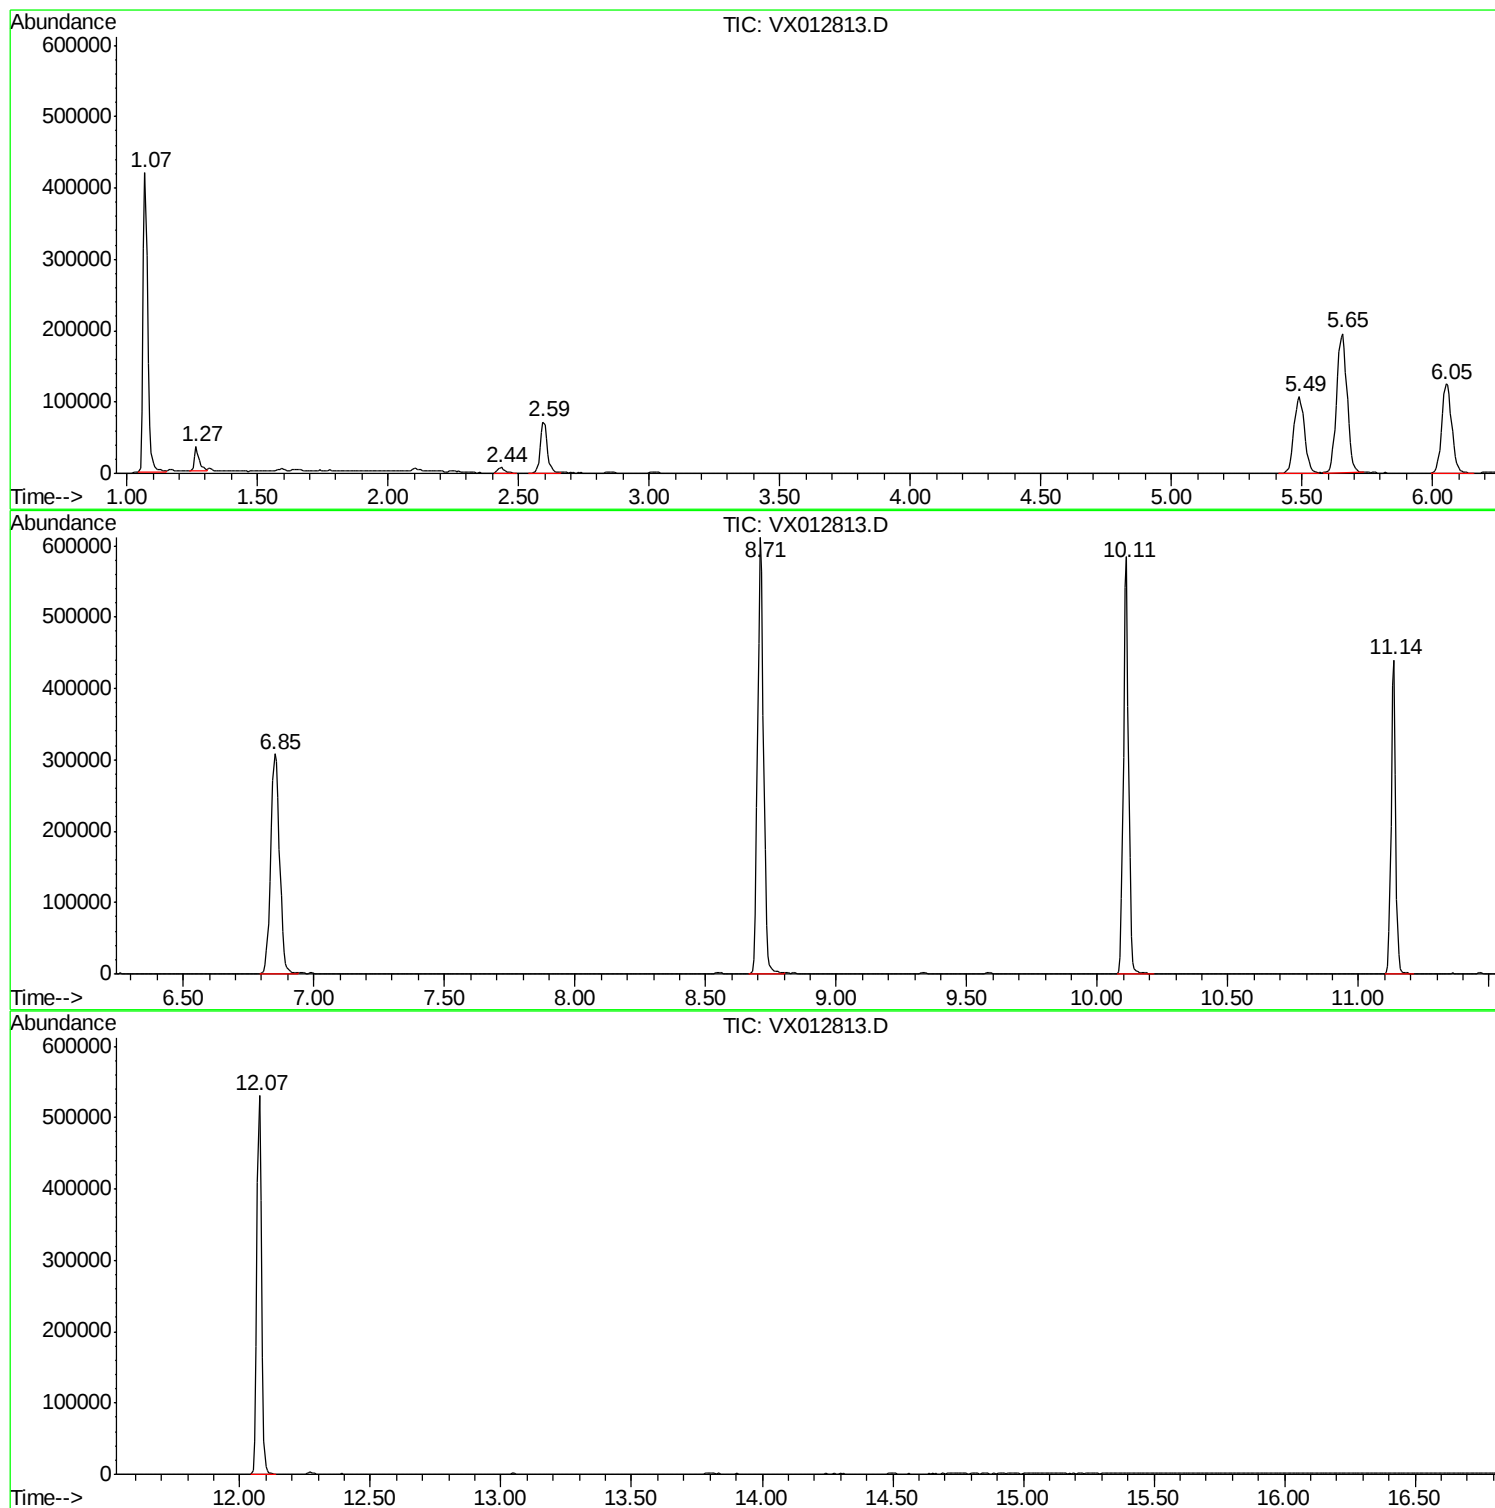

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100419\
Data File : VX012813.D
Acq On : 04 Oct 2019 15:48
Operator : JC/SP
Sample : K5189-17
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ138I-20191001










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	12.20 ug/l	132886	Pentafluorobenzene	5.65

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol	60	C3H8O	000067-63-0	83	
2	Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9	
3	Propanoic acid, 2-hydroxy-, meth...	104	C4H8O3	002155-30-8	4	
4	4-Penten-2-ol	86	C5H10O	000625-31-0	4	
5	Formamide	45	CH3NO	000075-12-7	4	

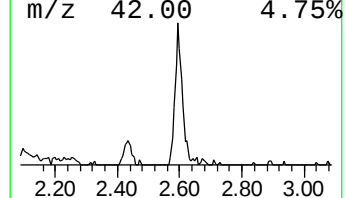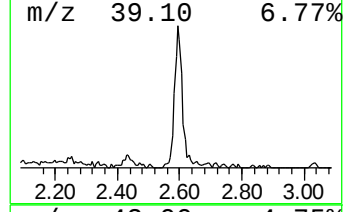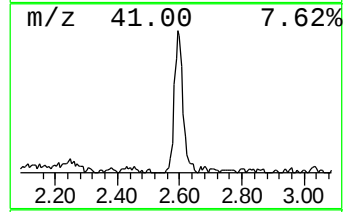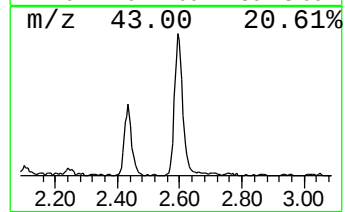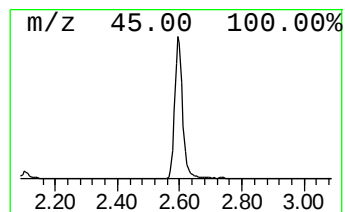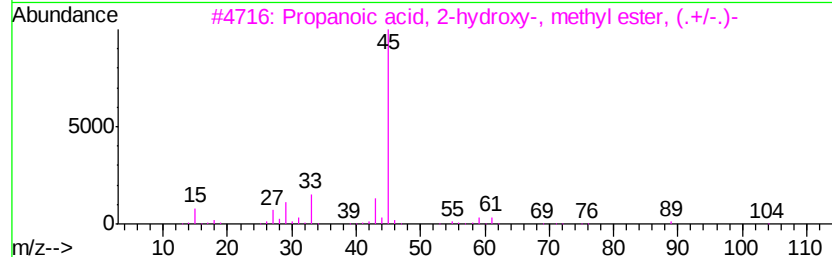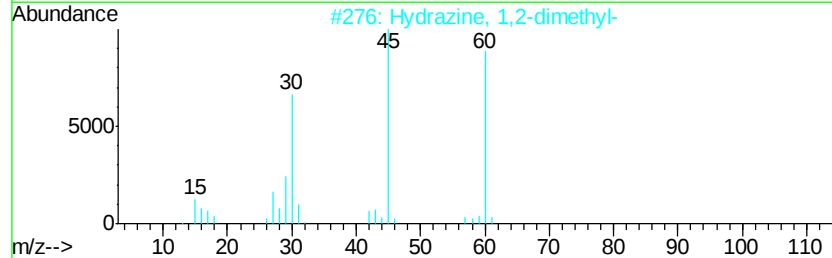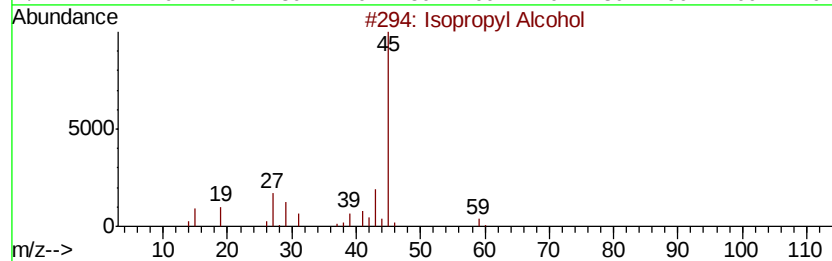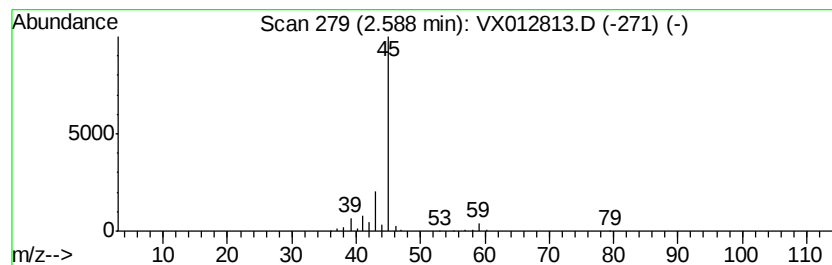

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100419\
Data File : VX012813.D
Acq On : 04 Oct 2019 15:48
Operator : JC/SP
Sample : K5189-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ138I-20191001

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	12.2	ug/l	132886	1	5.65	544602	50.0