


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100419\
 Data File : VX012801.D
 Acq On : 04 Oct 2019 09:58
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Title : SW846 8260
 Last Update : Mon Sep 23 12:27:01 2019

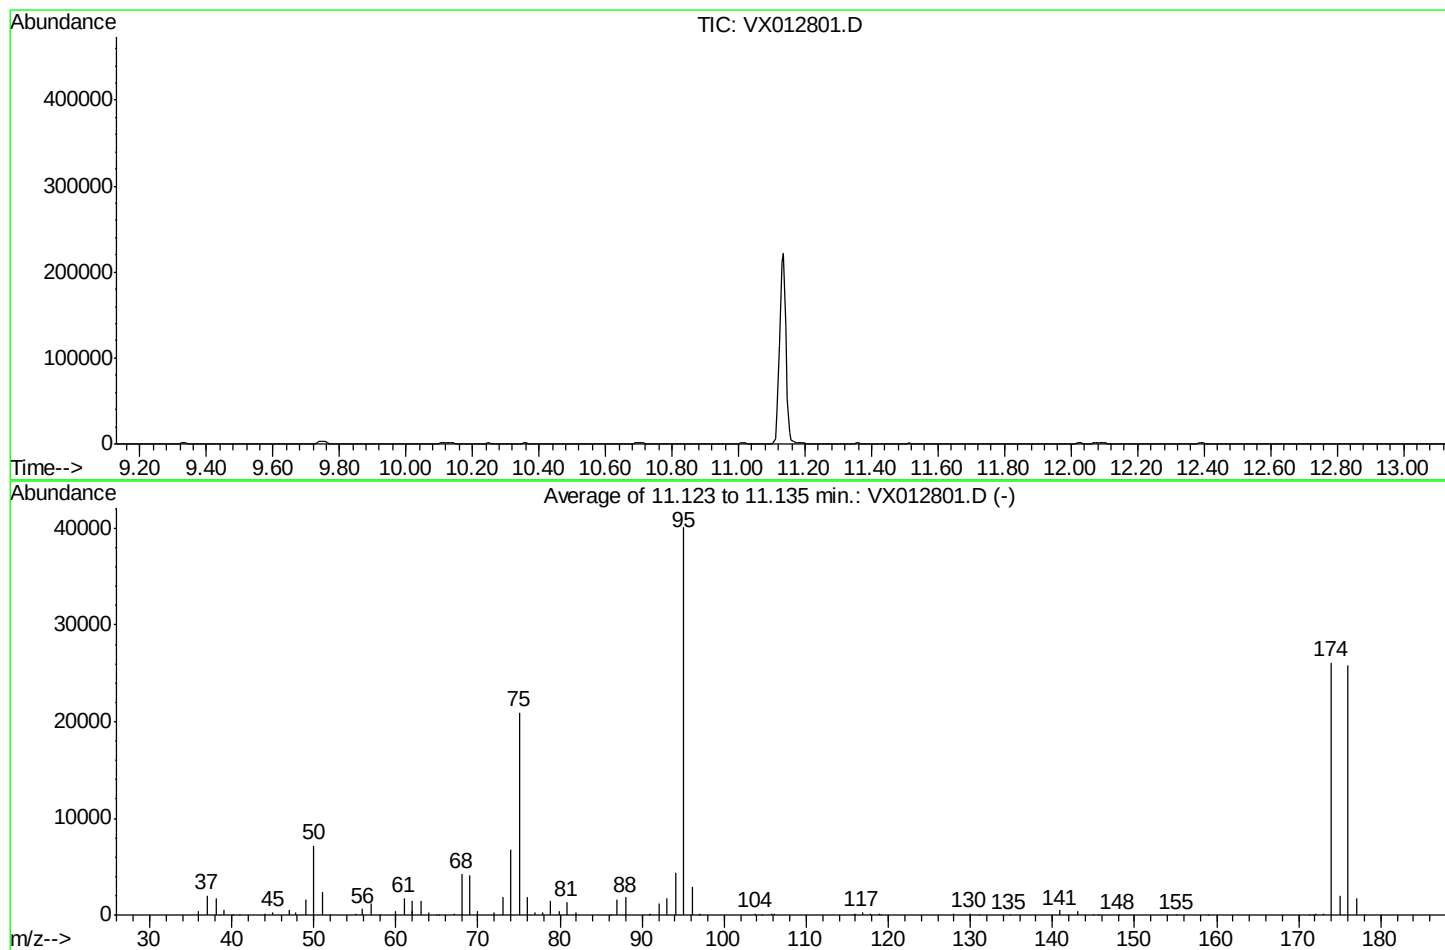

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	7178	PASS
75	95	30	60	52.3	20969	PASS
95	95	100	100	100.0	40098	PASS
96	95	5	9	7.4	2948	PASS
173	174	0.00	2	0.3	72	PASS
174	95	50	100	65.1	26114	PASS
175	174	5	9	7.6	1992	PASS
176	174	95	101	99.0	25851	PASS
177	176	5	9	6.5	1692	PASS