

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024522.D
 Acq On : 04 Oct 2021 15:58
 Operator : JC/MD
 Sample : M4063-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P287-DITCH

Quant Time: Oct 05 03:20:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 23 18:24:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	142688	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	234079	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	252358	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	116322	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	102746	51.09	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 102.18%	
35) Dibromofluoromethane	5.397	113	91820	59.05	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 118.10%	
50) Toluene-d8	8.653	98	333159	58.21	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 116.42%#	
62) 4-Bromofluorobenzene	11.085	95	125532	55.78	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 111.56%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024522.D
Acq On : 04 Oct 2021 15:58
Operator : JC/MD
Sample : M4063-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH

Quant Time: Oct 05 03:20:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 23 18:24:34 2021
Response via : Initial Calibration




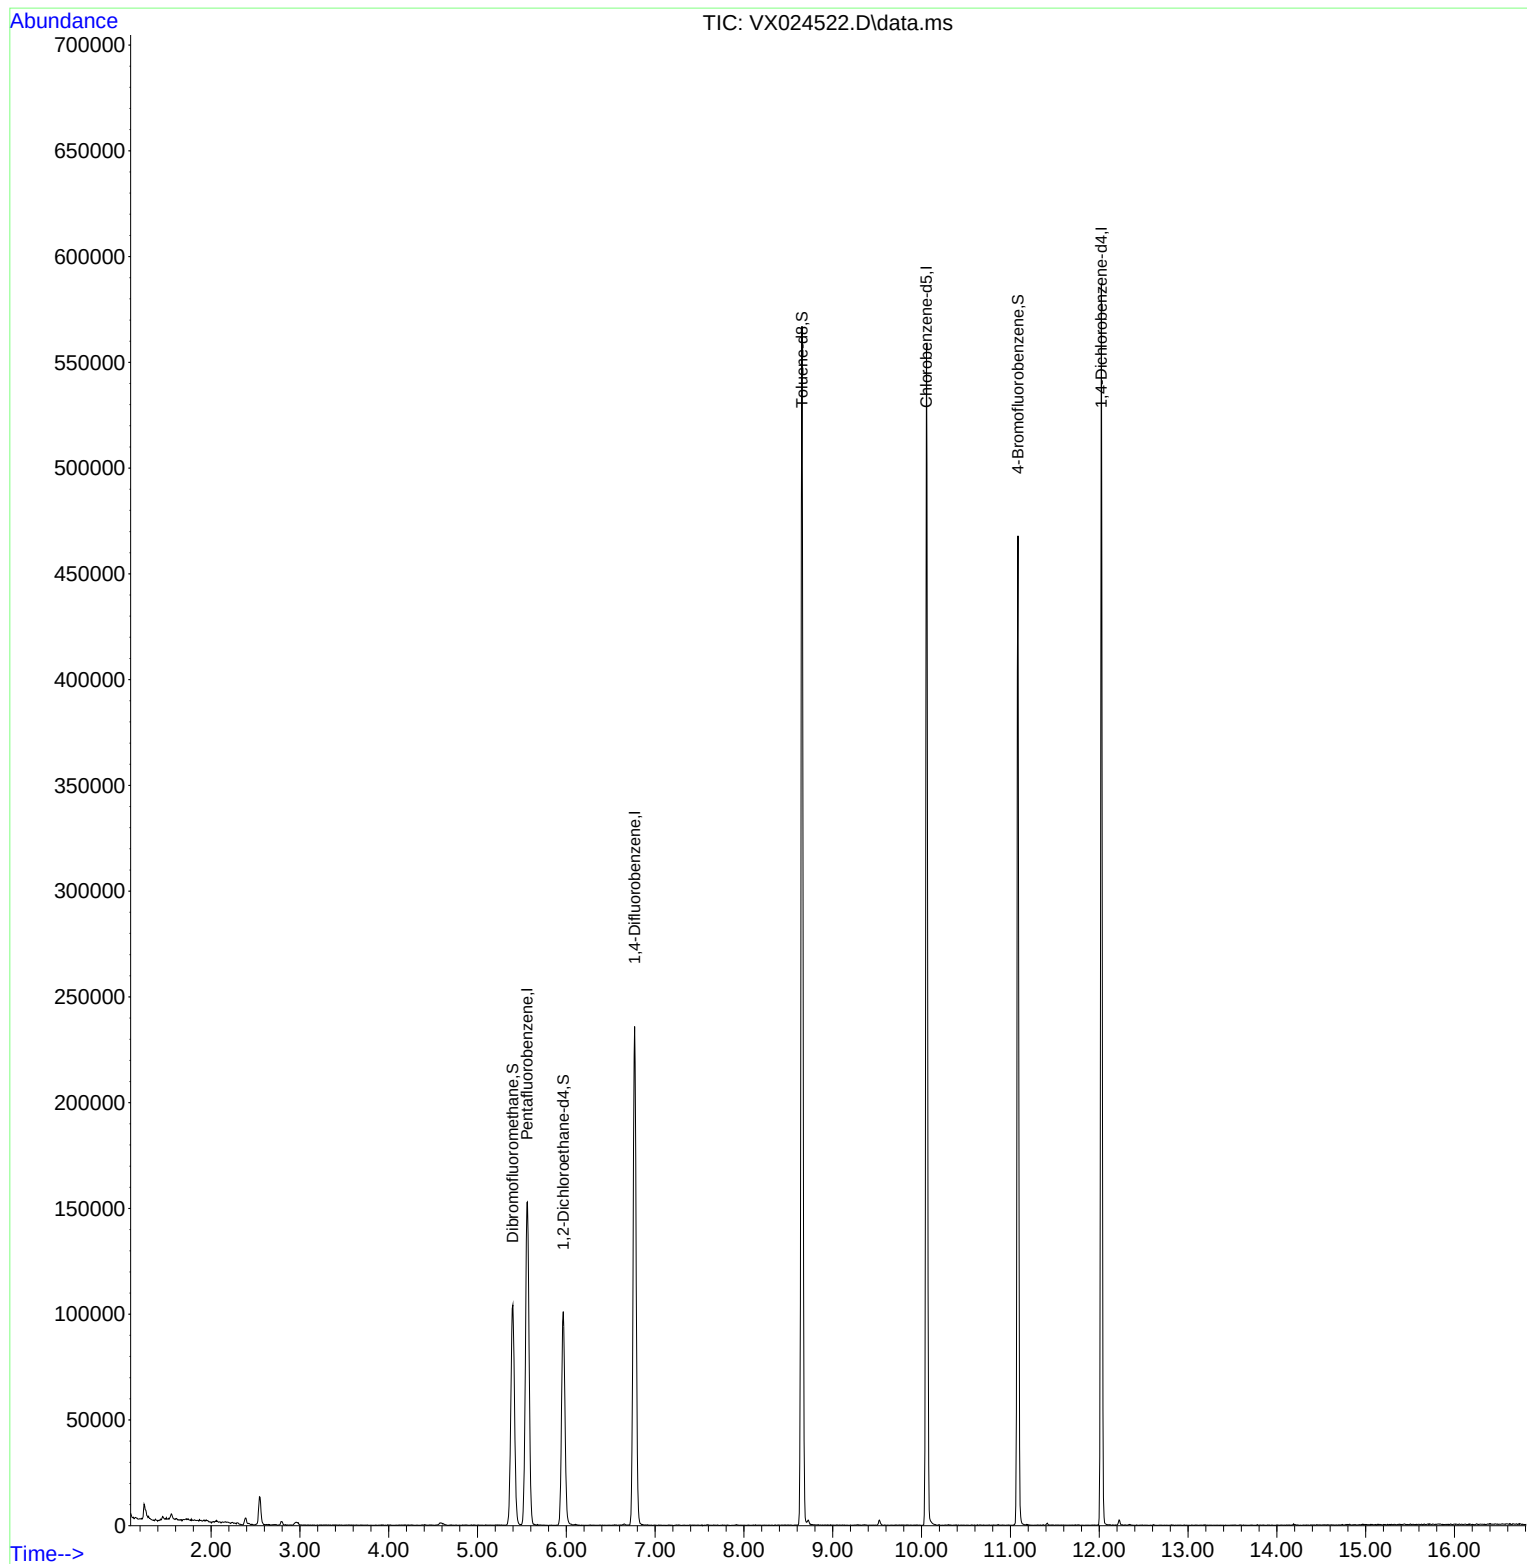


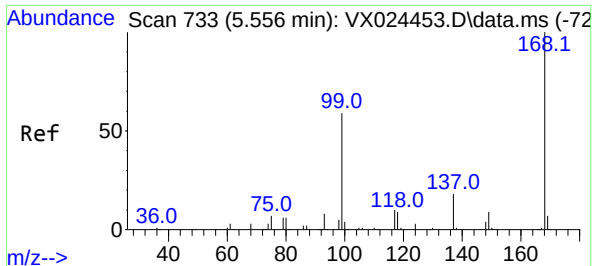

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58




Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH


Tgt Ion:168 Resp: 142688
Ion Ratio Lower Upper
168 100
99 61.7 45.8 68.6

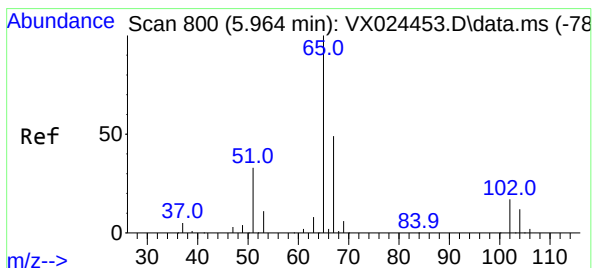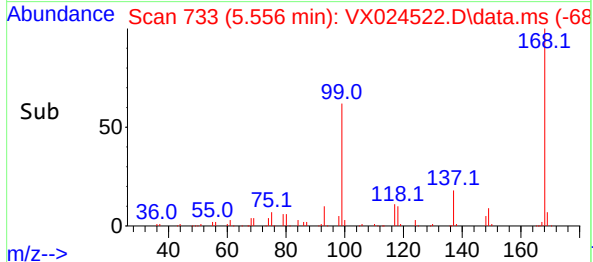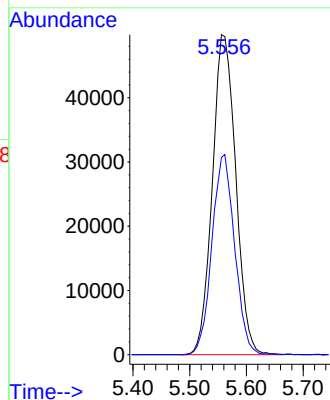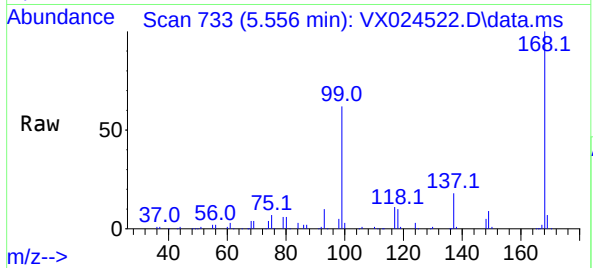

#33
1,2-Dichloroethane-d4
Concen: 51.09 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58

Tgt Ion: 65 Resp: 102746
Ion Ratio Lower Upper
65 100
67 49.8 0.0 105.4


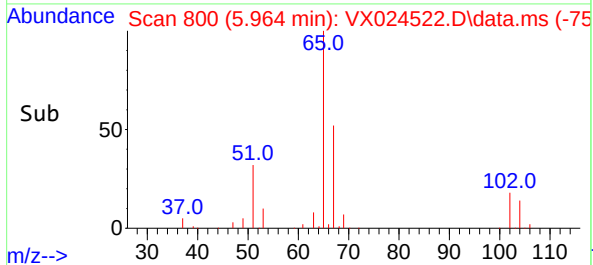
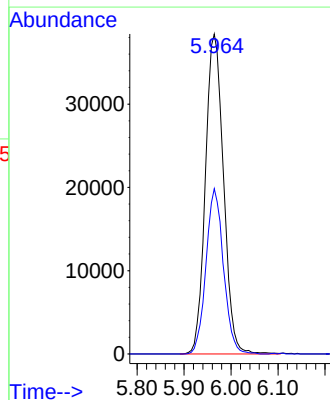
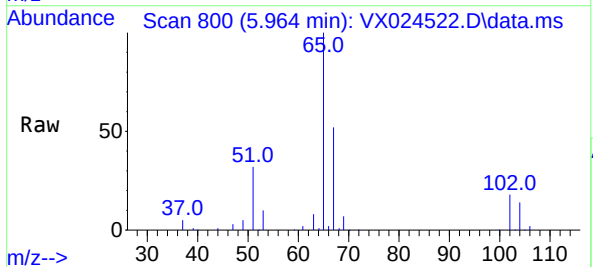


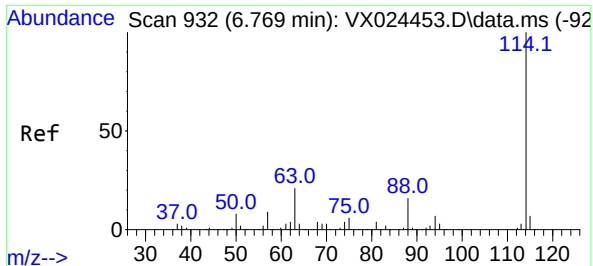

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58




Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH


Tgt Ion:114 Resp: 234079
Ion Ratio Lower Upper
114 100
63 20.8 0.0 40.8
88 16.7 0.0 32.8

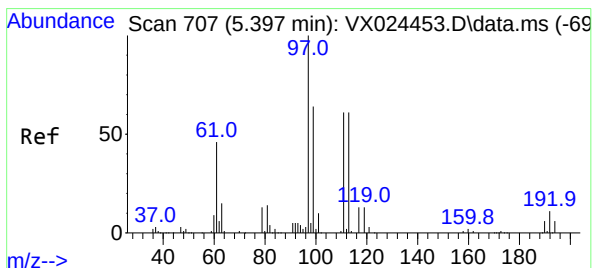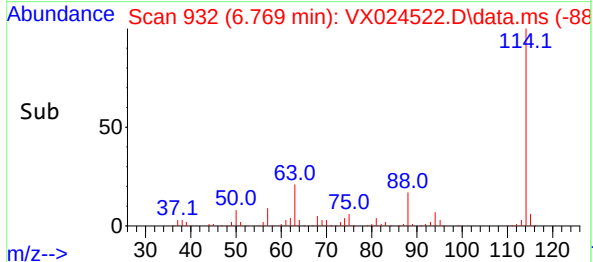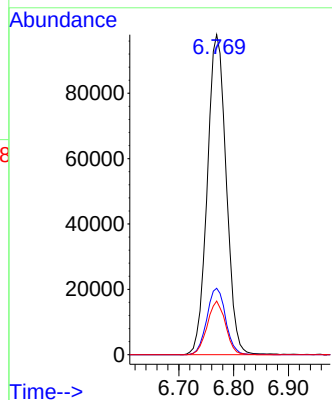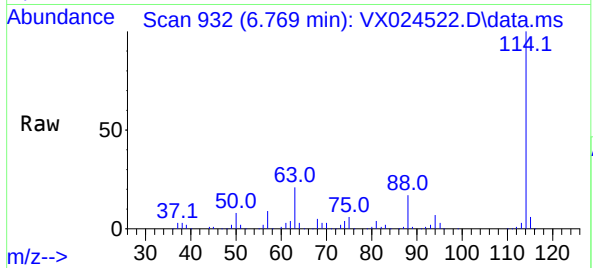

#35
Dibromofluoromethane
Concen: 59.05 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58

Tgt Ion:113 Resp: 91820
Ion Ratio Lower Upper
113 100
111 102.0 81.9 122.9
192 18.5 16.7 25.1


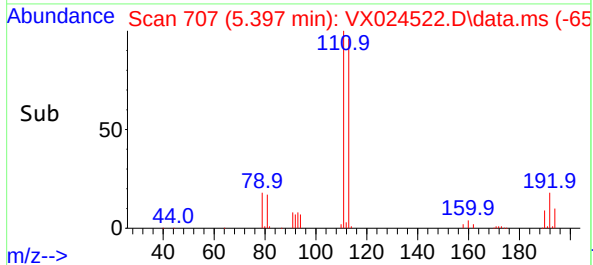
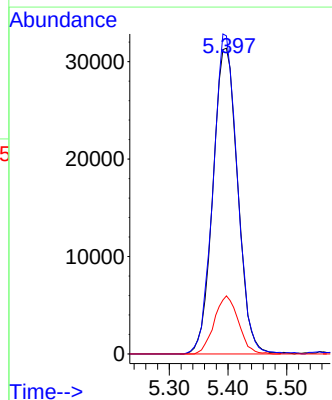
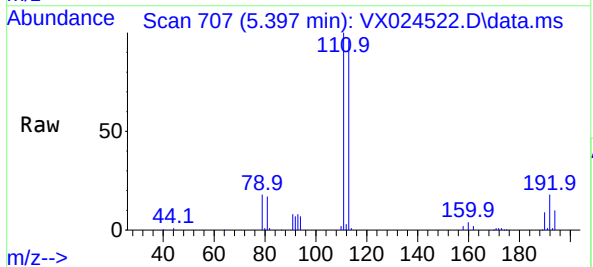


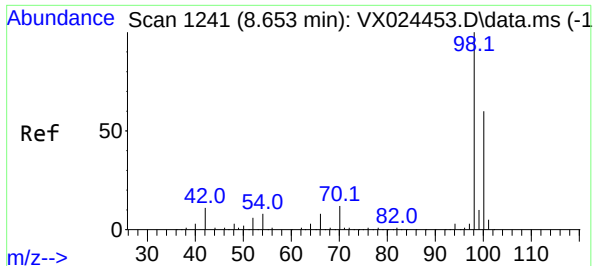

#50
Toluene-d8
Concen: 58.21 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58




Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH


Tgt Ion: 98 Resp: 333159
Ion Ratio Lower Upper
98 100
100 64.5 51.9 77.9

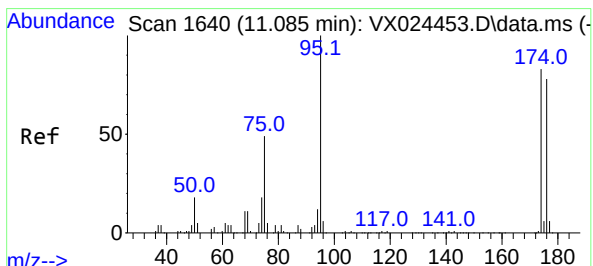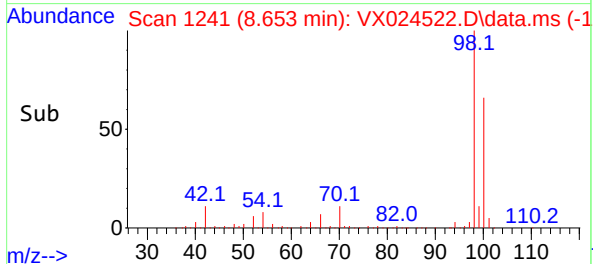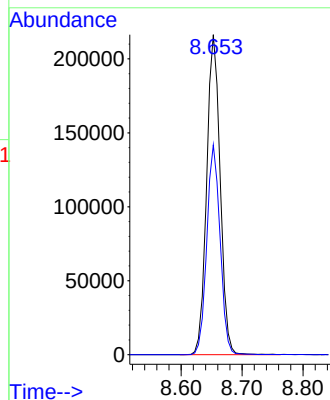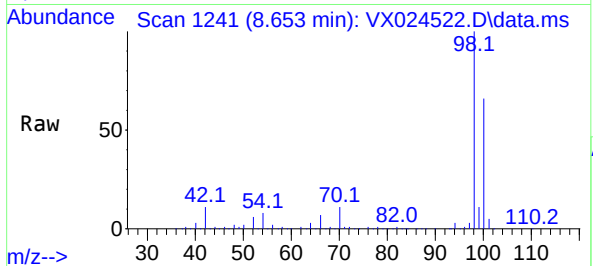

#62
4-Bromofluorobenzene
Concen: 55.78 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58

Tgt Ion: 95 Resp: 125532
Ion Ratio Lower Upper
95 100
174 80.7 0.0 154.6
176 77.6 0.0 155.8


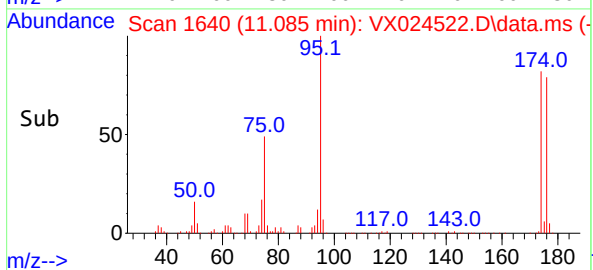
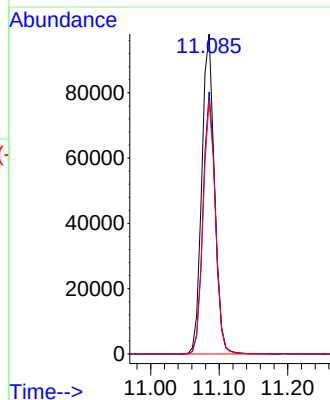
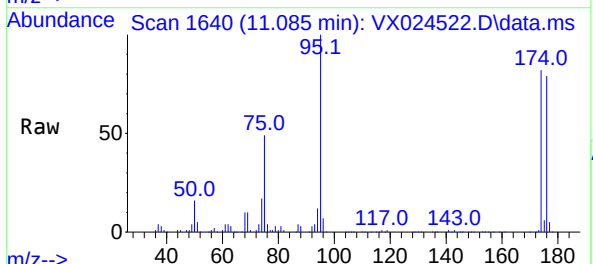


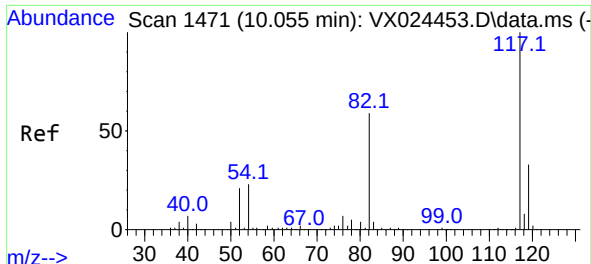

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58

Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH

Tgt Ion:117 Resp: 252358
Ion Ratio Lower Upper
117 100
82 58.7 47.4 71.2
119 31.7 26.6 39.8

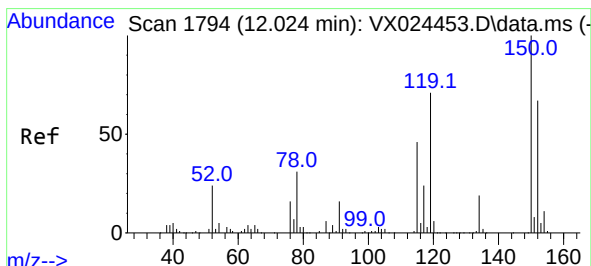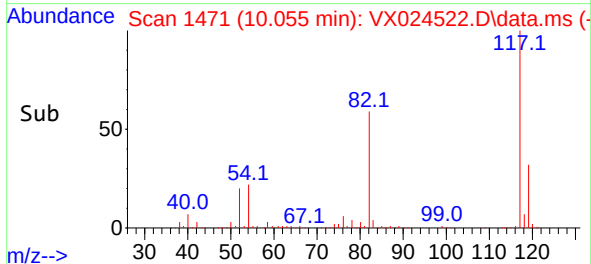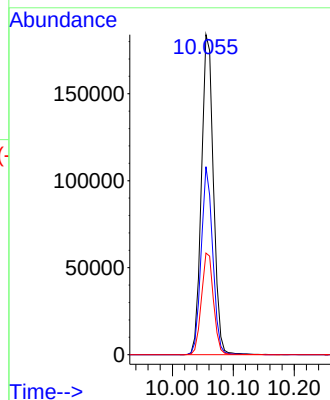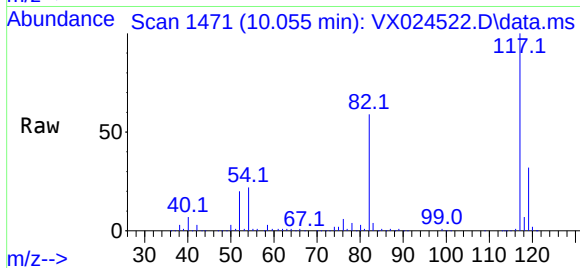

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024522.D
Acq: 04 Oct 2021 15:58

Tgt Ion:152 Resp: 116322
Ion Ratio Lower Upper
152 100
115 61.2 41.1 123.3
150 157.5 0.0 349.0

