

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024528.D
 Acq On : 04 Oct 2021 18:19
 Operator : JC/MD
 Sample : M4044-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Oct 05 03:21:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 23 18:24:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	153704	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	250425	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	225688	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	96721	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	110883	51.19	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 102.38%	
35) Dibromofluoromethane	5.397	113	89572	53.84	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 107.68%	
50) Toluene-d8	8.653	98	321603	52.52	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 105.04%	
62) 4-Bromofluorobenzene	11.085	95	121754	50.57	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 101.14%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024528.D
Acq On : 04 Oct 2021 18:19
Operator : JC/MD
Sample : M4044-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Oct 05 03:21:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 23 18:24:34 2021
Response via : Initial Calibration



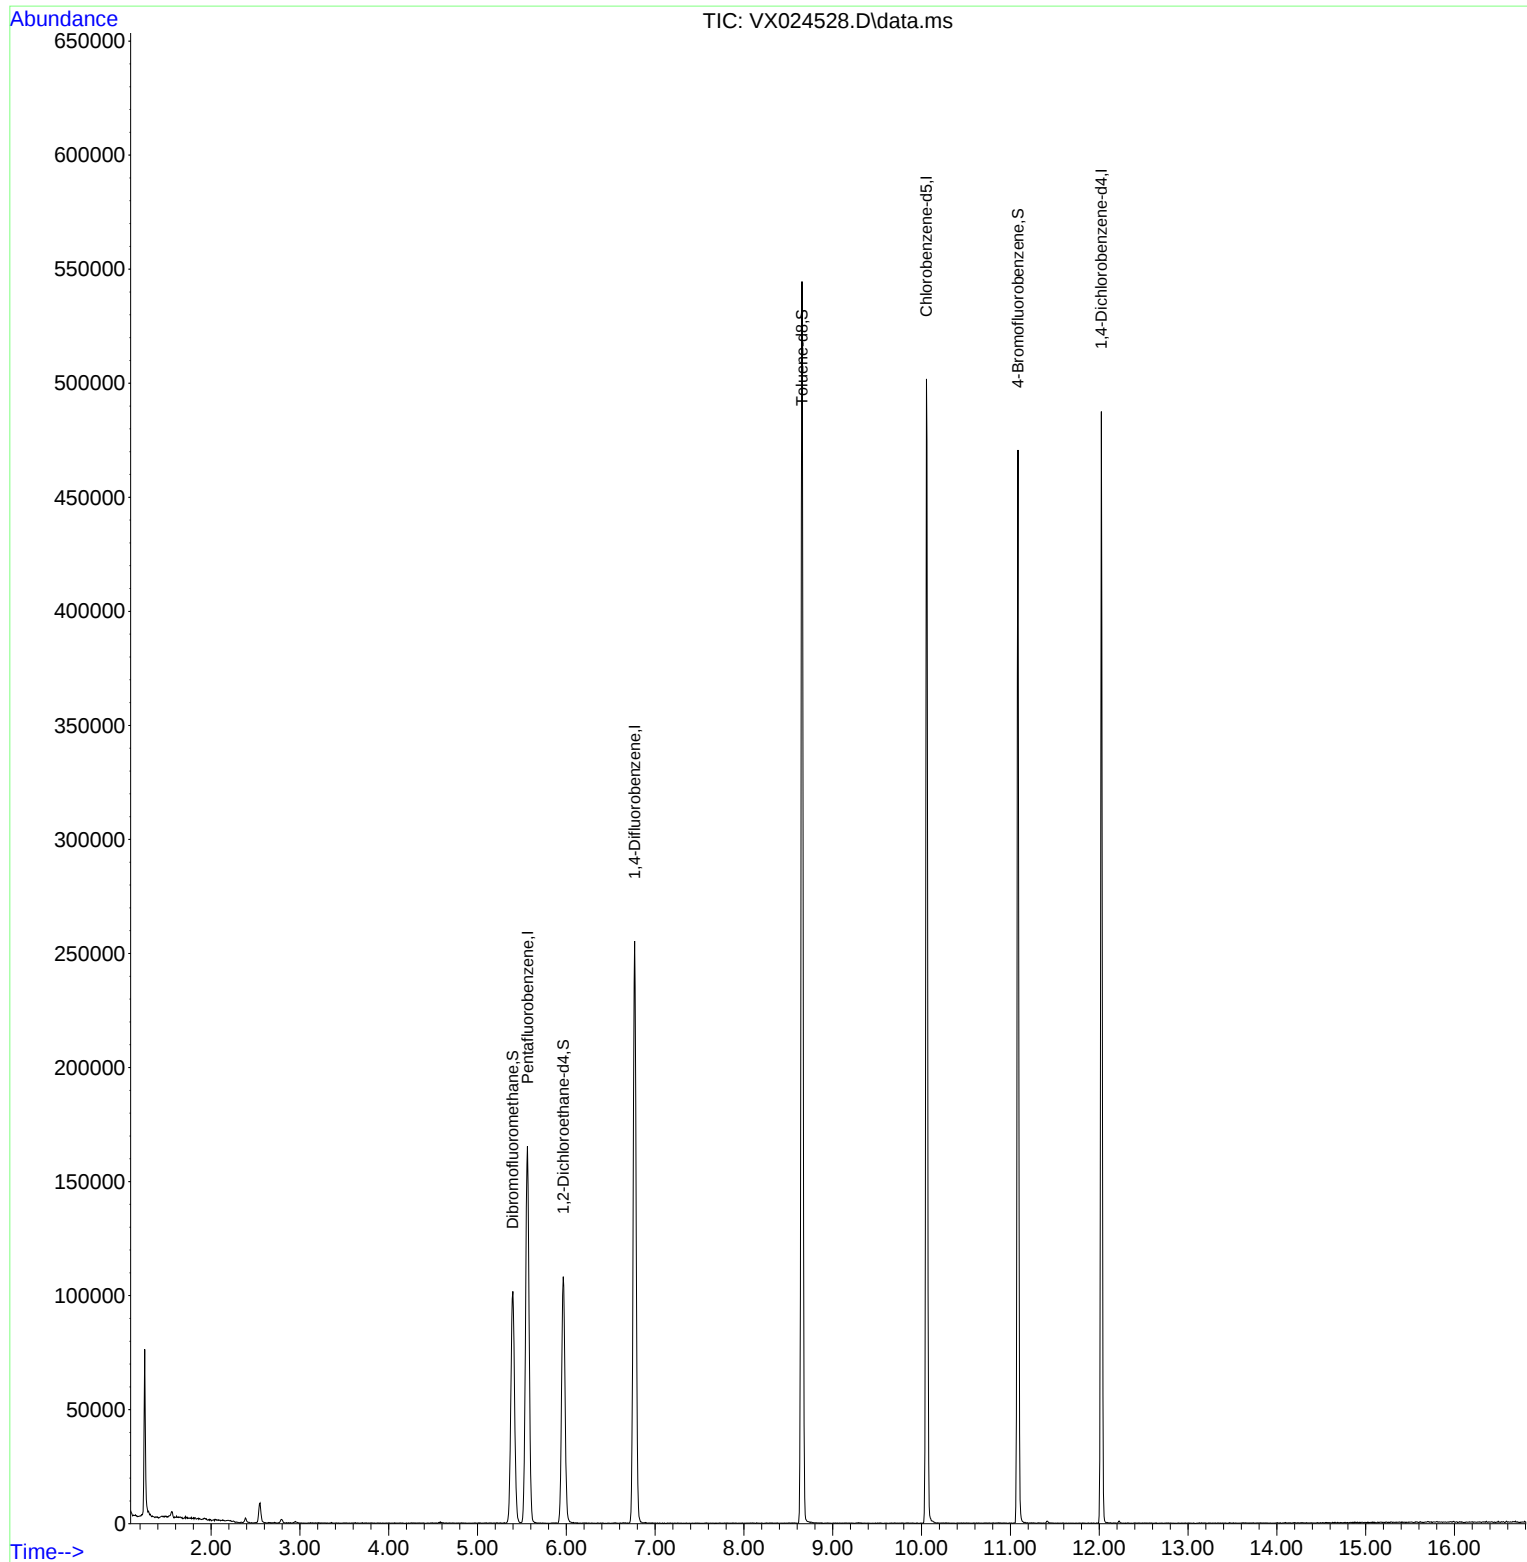


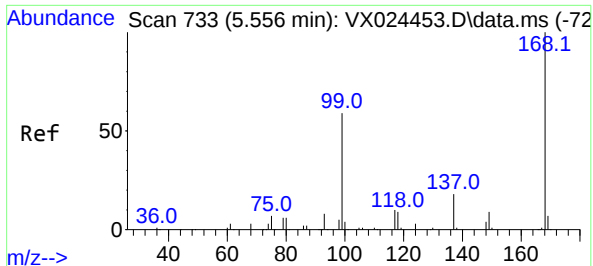

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.006 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 153704
Ion Ratio Lower Upper
168 100
99 60.3 45.8 68.6

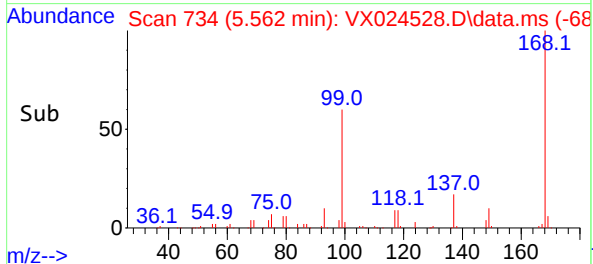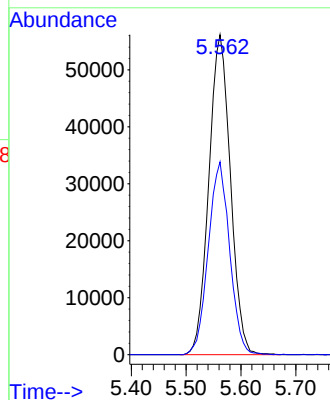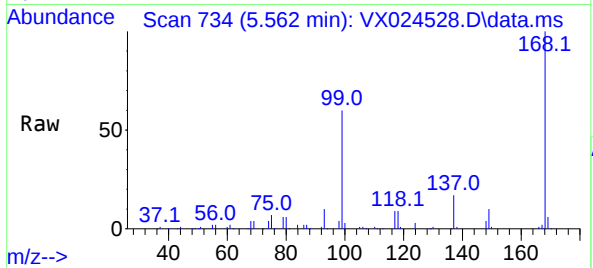

#33
1,2-Dichloroethane-d4
Concen: 51.19 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19

Tgt Ion: 65 Resp: 110883
Ion Ratio Lower Upper
65 100
67 50.9 0.0 105.4


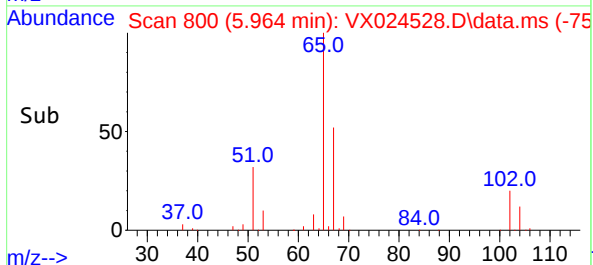
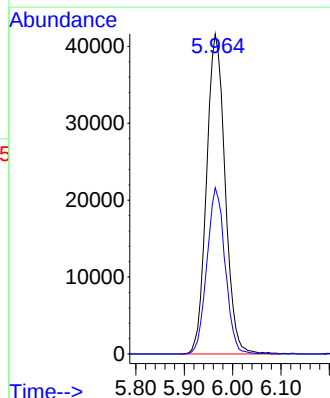
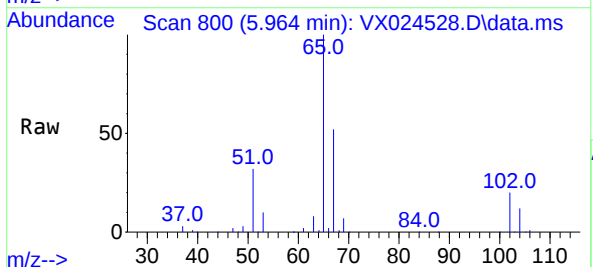


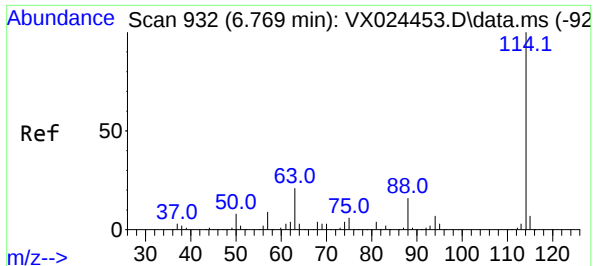

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 250425
Ion Ratio Lower Upper
114 100
63 19.8 0.0 40.8
88 15.7 0.0 32.8

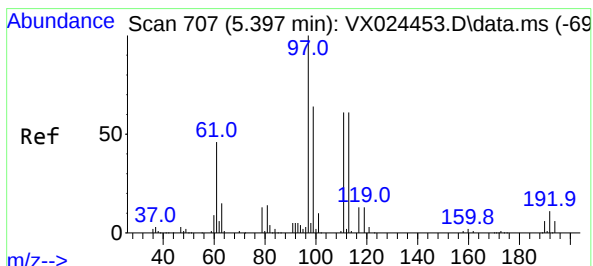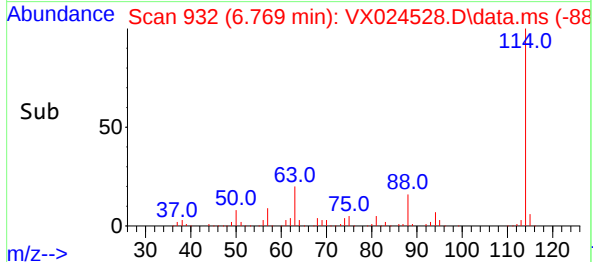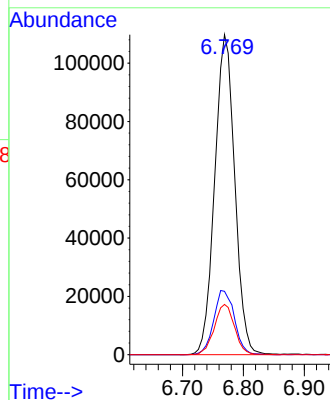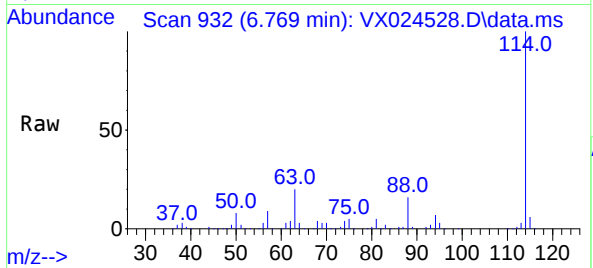

#35
Dibromofluoromethane
Concen: 53.84 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19

Tgt Ion:113 Resp: 89572
Ion Ratio Lower Upper
113 100
111 103.2 81.9 122.9
192 19.2 16.7 25.1


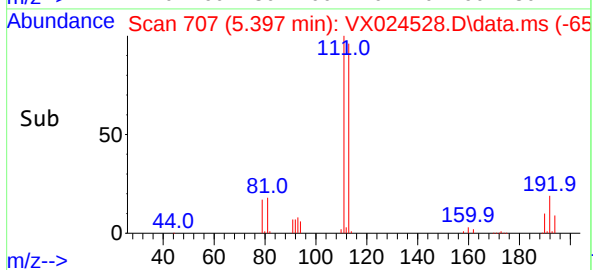
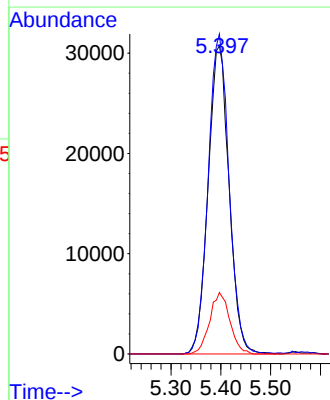
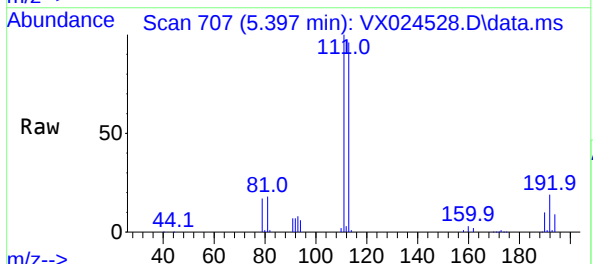


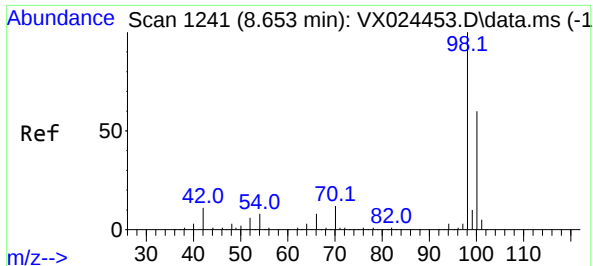

#50
Toluene-d8
Concen: 52.52 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 321603
Ion Ratio Lower Upper
98 100
100 64.1 51.9 77.9

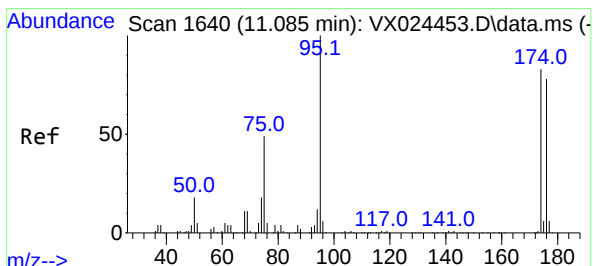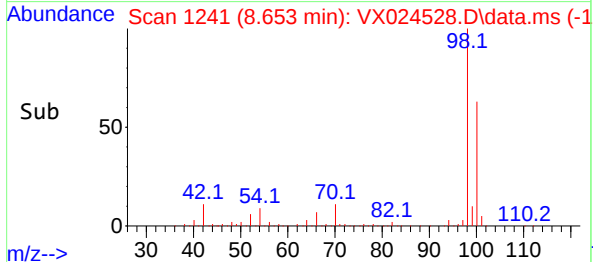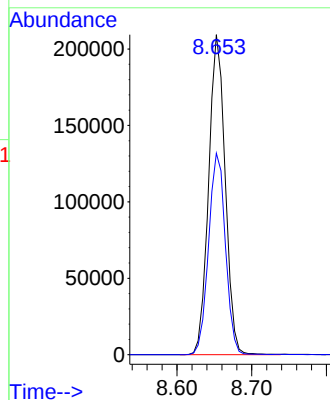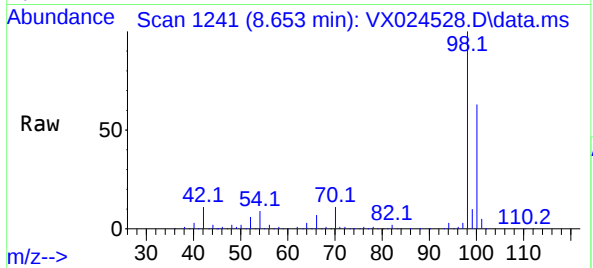

#62
4-Bromofluorobenzene
Concen: 50.57 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19

Tgt Ion: 95 Resp: 121754
Ion Ratio Lower Upper
95 100
174 79.3 0.0 154.6
176 76.4 0.0 155.8


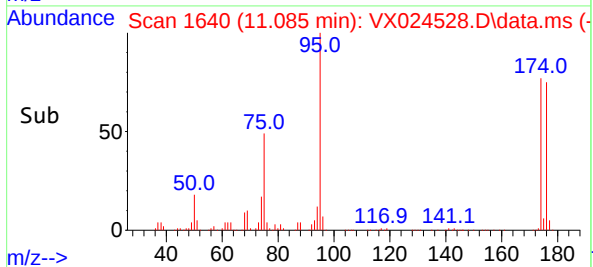
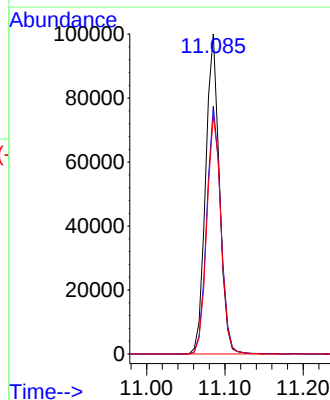
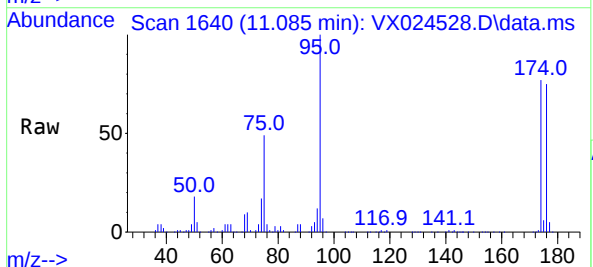


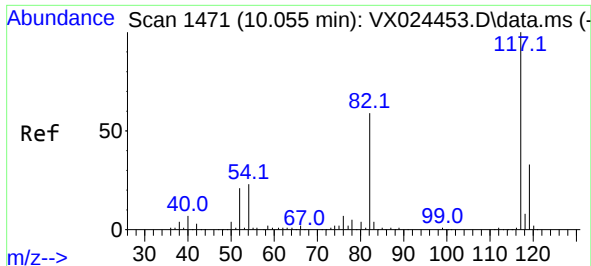

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 225688
Ion Ratio Lower Upper
117 100
82 57.3 47.4 71.2
119 32.2 26.6 39.8

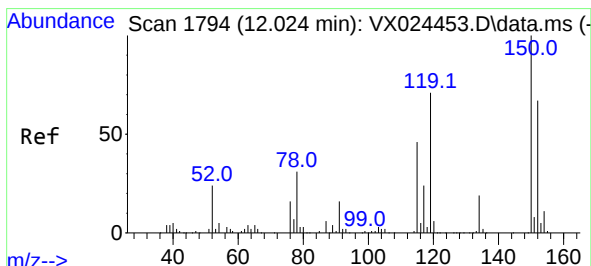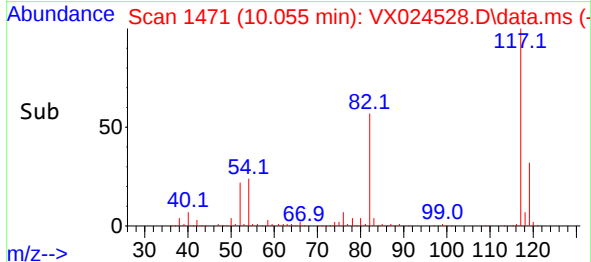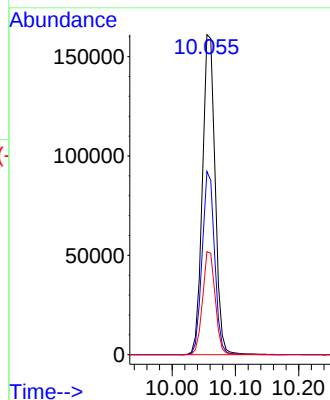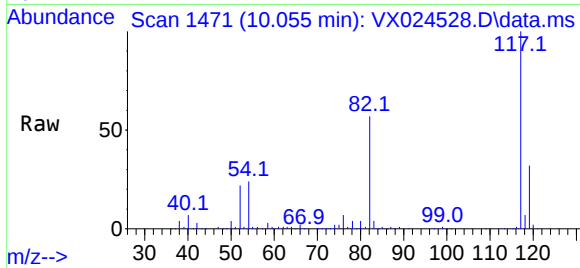

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX024528.D
Acq: 04 Oct 2021 18:19

Tgt Ion:152 Resp: 96721
Ion Ratio Lower Upper
152 100
115 61.0 41.1 123.3
150 157.1 0.0 349.0

