

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024516.D
 Acq On : 04 Oct 2021 13:37
 Operator : JC/MD
 Sample : M3911-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-CB-04-(0.5)RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.385	207	213	222	rBV	7159	12090	1.36%	0.217%
2	2.550	231	240	248	rVB2	9363	17271	1.94%	0.310%
3	4.592	566	575	585	rBV4	2999	9570	1.08%	0.172%
4	5.397	696	707	721	rBV2	97328	276636	31.14%	4.964%
5	5.562	721	734	747	rVV	155950	434294	48.88%	7.794%
6	5.964	789	800	808	rBV2	109349	289446	32.58%	5.194%
7	6.049	808	814	827	rVB2	18564	51763	5.83%	0.929%
8	6.769	922	932	943	rBV	270295	621317	69.93%	11.150%
9	8.653	1234	1241	1249	rBV	573699	888484	100.00%	15.944%
10	10.055	1466	1471	1486	rVB2	544696	864115	97.26%	15.507%
11	11.085	1634	1640	1653	rVB	469162	584802	65.82%	10.494%
12	12.024	1789	1794	1802	rVB	574504	726299	81.75%	13.034%
13	12.335	1840	1845	1850	rBV	19812	26358	2.97%	0.473%
14	13.780	2074	2082	2090	rBV	619963	761071	85.66%	13.658%
15	13.871	2093	2097	2105	rBV	6373	8967	1.01%	0.161%




Sum of corrected areas: 5572483

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024516.D
Acq On : 04 Oct 2021 13:37
Operator : JC/MD
Sample : M3911-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-04-(0.5)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

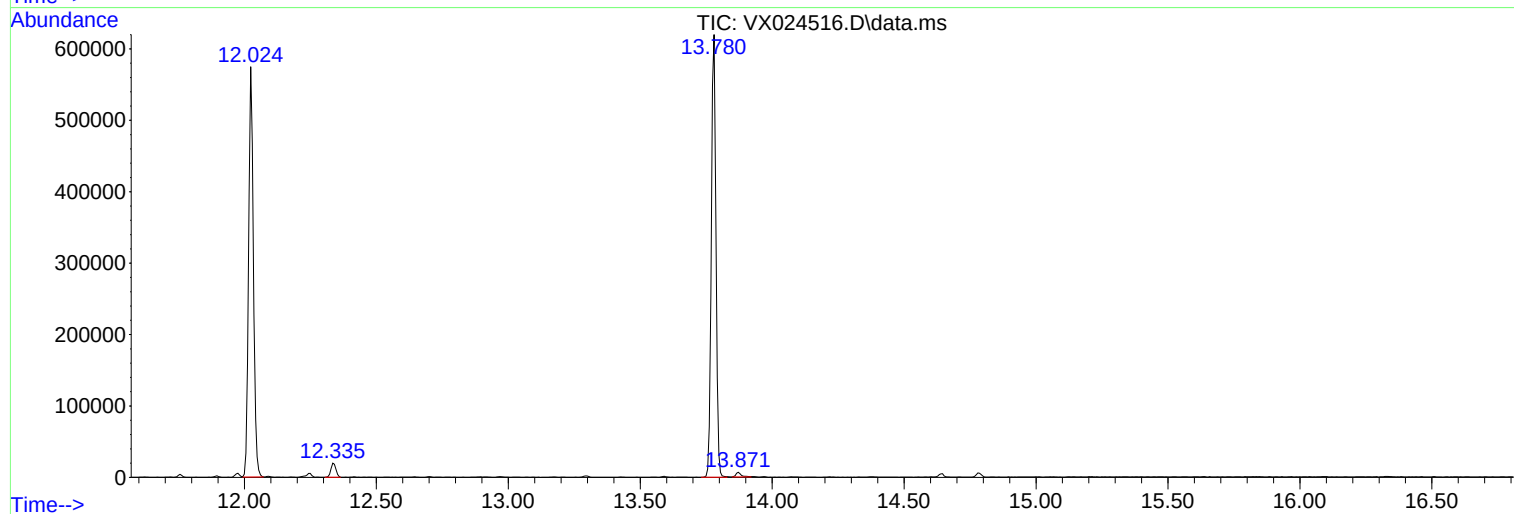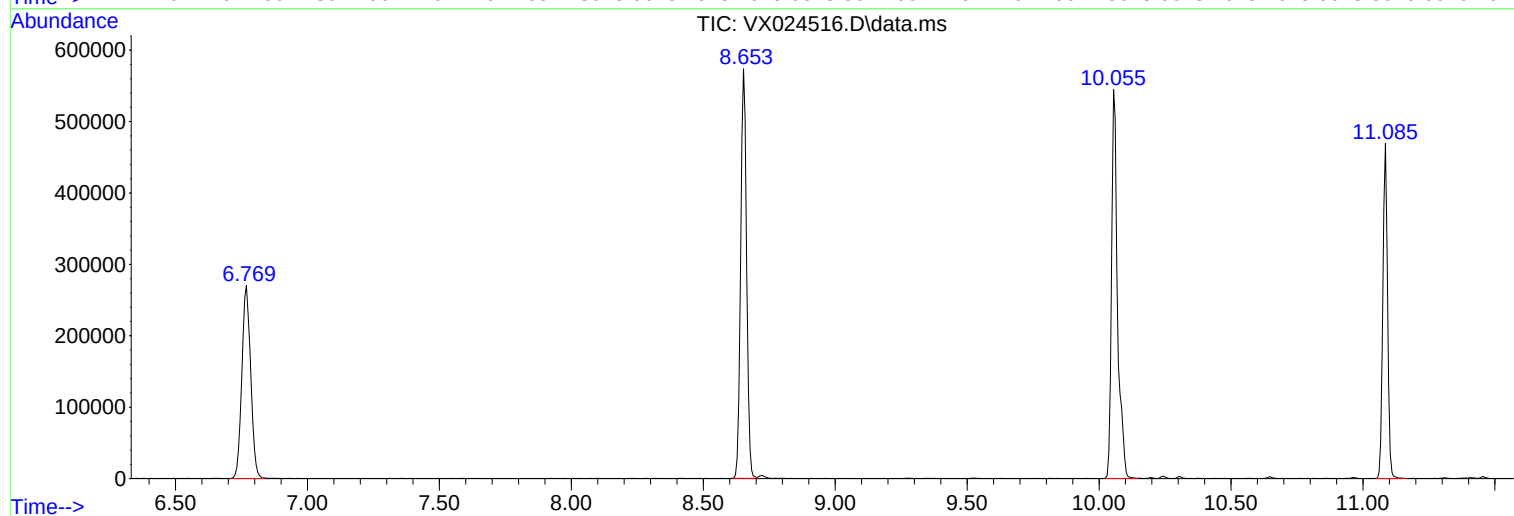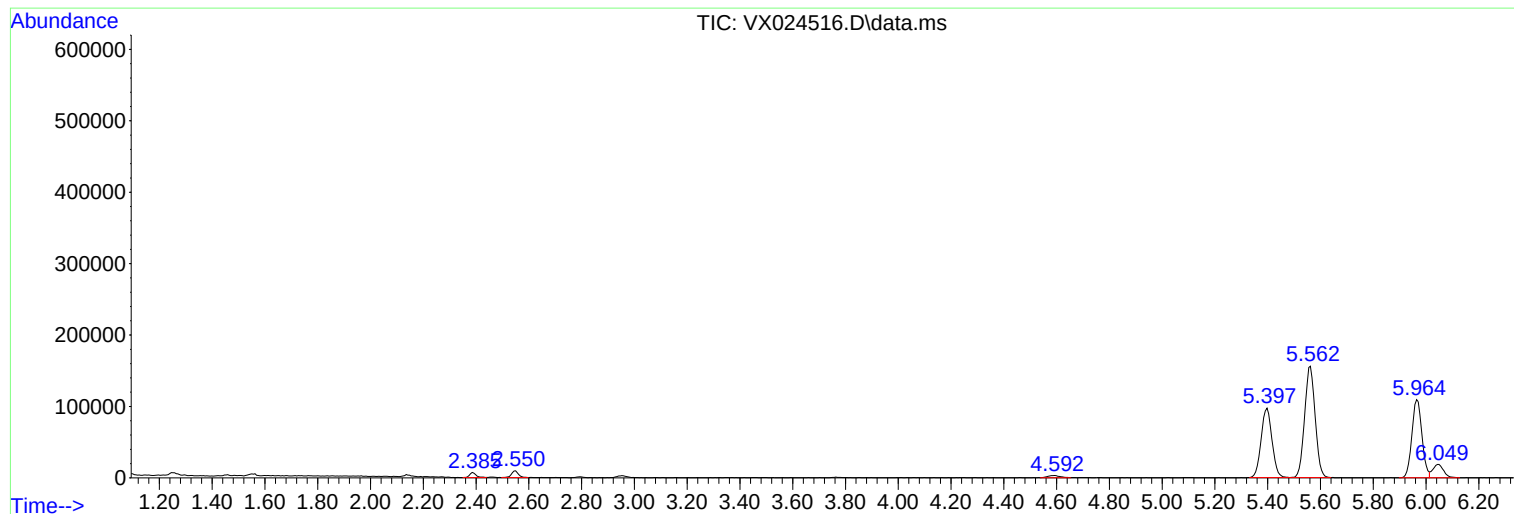

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024516.D
Acq On : 04 Oct 2021 13:37
Operator : JC/MD
Sample : M3911-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-04-(0.5)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024516.D
Acq On : 04 Oct 2021 13:37
Operator : JC/MD
Sample : M3911-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-CB-04-(0.5)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
