

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024519.D
 Acq On : 04 Oct 2021 14:48
 Operator : JC/MD
 Sample : M3911-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-RR-03-(SA)RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	41	rBV	6295	13858	1.72%	0.313%
2	2.544	230	239	246	rBV	8975	16573	2.05%	0.375%
3	5.397	695	707	720	rBV	102399	297586	36.87%	6.726%
4	5.562	722	734	751	rVB	162831	456721	56.59%	10.323%
5	5.964	789	800	810	rBV	105980	283517	35.13%	6.408%
6	6.044	810	813	822	rVB4	4670	10461	1.30%	0.236%
7	6.769	922	932	944	rBV	248158	584438	72.42%	13.210%
8	8.653	1234	1241	1250	rBV	520692	807020	100.00%	18.241%
9	10.055	1465	1471	1482	rBV	533984	726977	90.08%	16.432%
10	11.085	1634	1640	1653	rVB	440199	563146	69.78%	12.729%
11	12.024	1789	1794	1807	rBV	532556	654188	81.06%	14.786%
12	13.780	2076	2082	2087	rVB2	7455	9760	1.21%	0.221%




Sum of corrected areas: 4424245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024519.D
Acq On : 04 Oct 2021 14:48
Operator : JC/MD
Sample : M3911-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

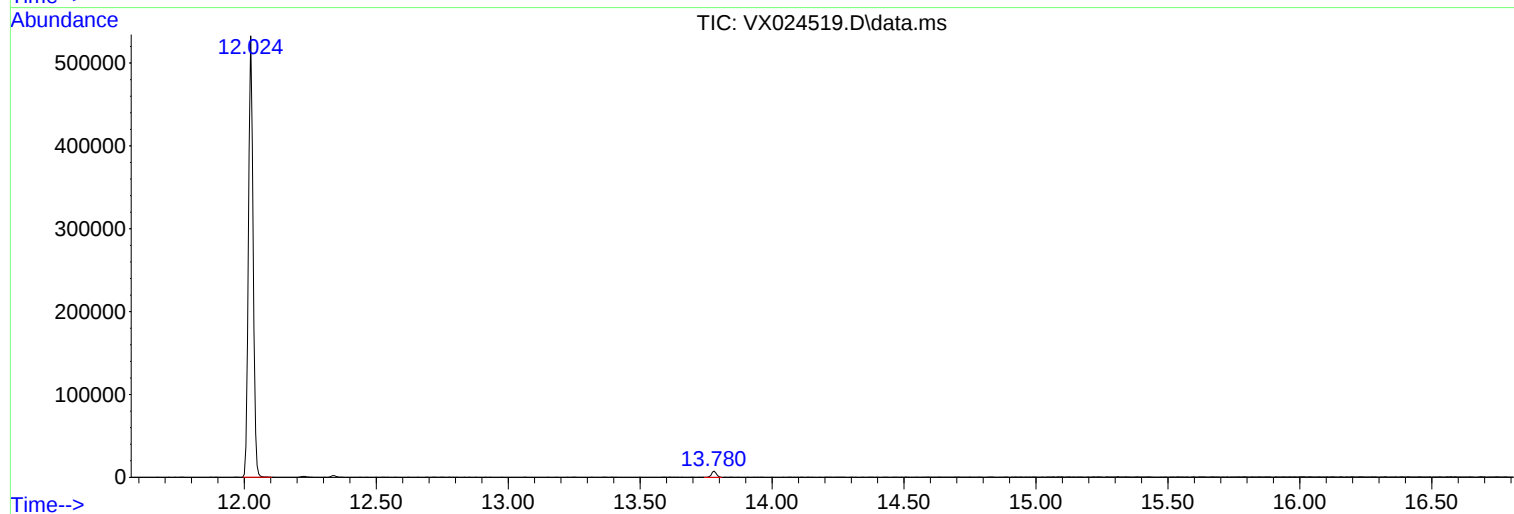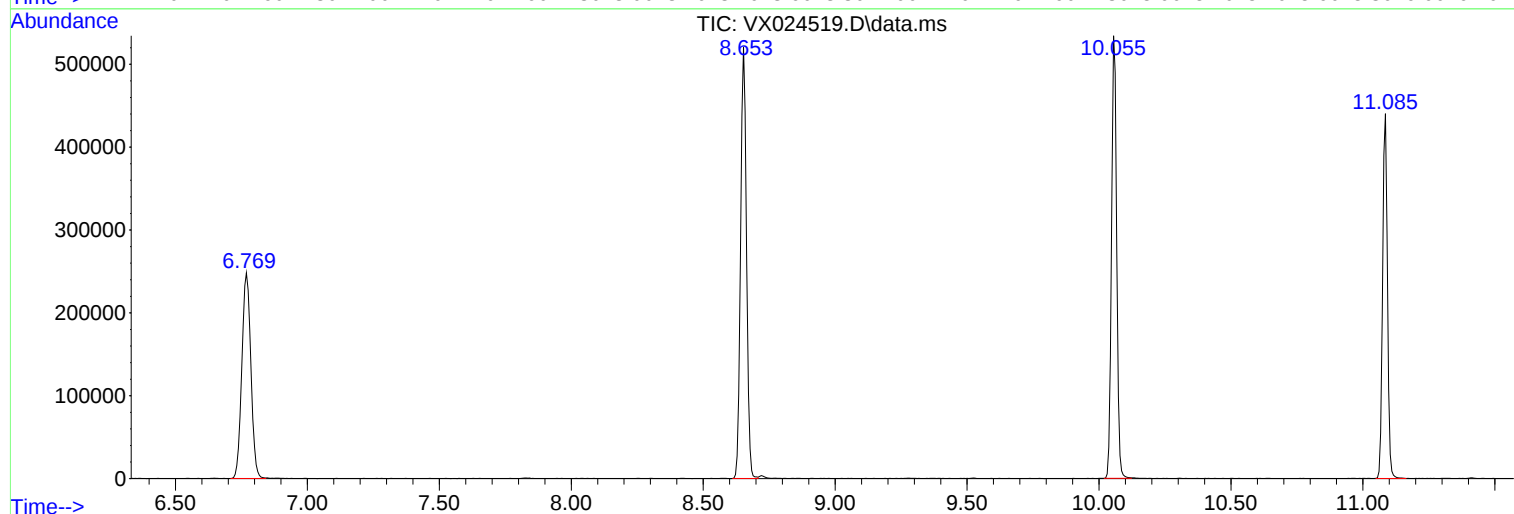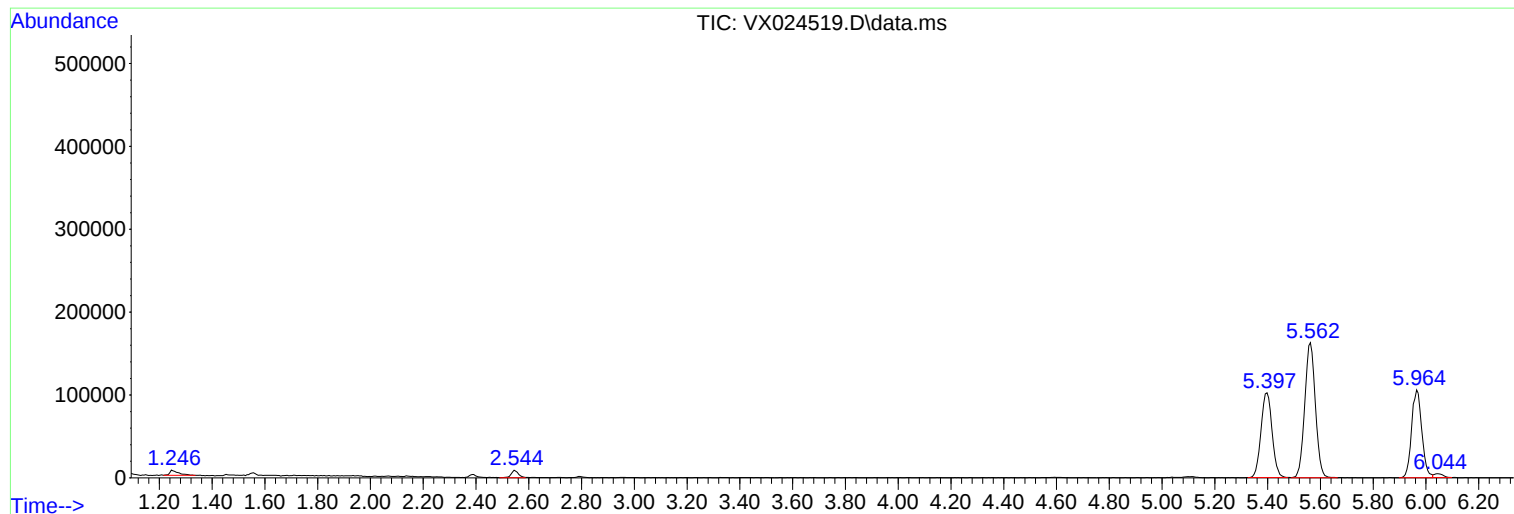

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024519.D
Acq On : 04 Oct 2021 14:48
Operator : JC/MD
Sample : M3911-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024519.D
Acq On : 04 Oct 2021 14:48
Operator : JC/MD
Sample : M3911-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
