

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024521.D
 Acq On : 04 Oct 2021 15:34
 Operator : JC/MD
 Sample : M3911-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANKRE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	34	rBV2	7540	12355	1.40%	0.267%
2	2.953	297	306	316	rVB	10738	25868	2.93%	0.560%
3	4.586	562	574	586	rBV2	7386	24725	2.80%	0.535%
4	5.397	694	707	722	rBV	105100	303682	34.44%	6.571%
5	5.562	722	734	747	rVB	167275	472954	53.64%	10.234%
6	5.964	788	800	817	rBV	112667	295330	33.49%	6.391%
7	6.769	920	932	949	rBV	248665	593906	67.36%	12.852%
8	8.653	1234	1241	1251	rBV	578705	881754	100.00%	19.080%
9	10.055	1465	1471	1493	rBV	514980	702334	79.65%	15.198%
10	11.085	1634	1640	1651	rBV	471024	601394	68.20%	13.014%
11	12.024	1789	1794	1802	rBV	572961	706945	80.17%	15.298%




Sum of corrected areas: 4621247

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024521.D
Acq On : 04 Oct 2021 15:34
Operator : JC/MD
Sample : M3911-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANKRE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

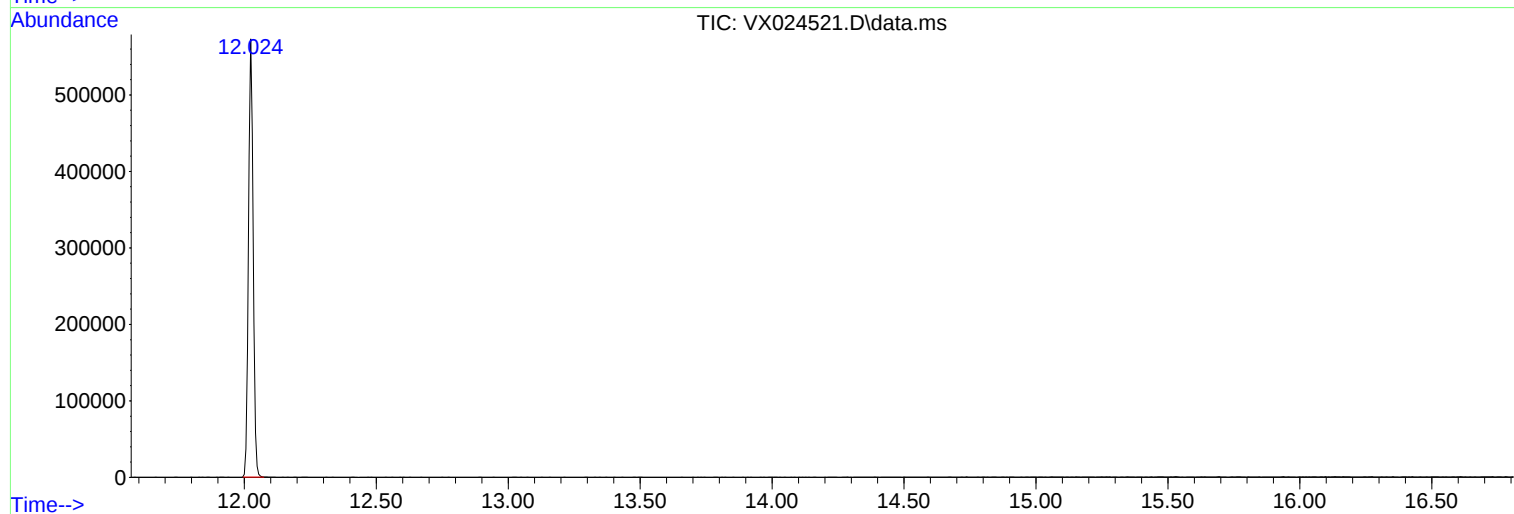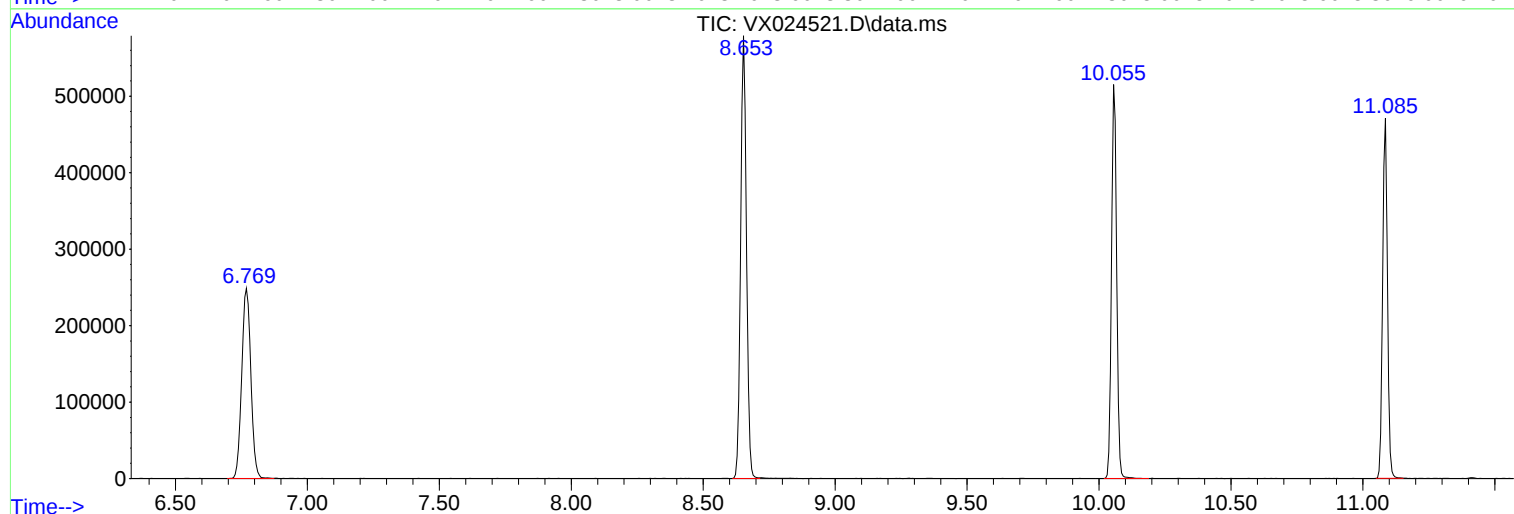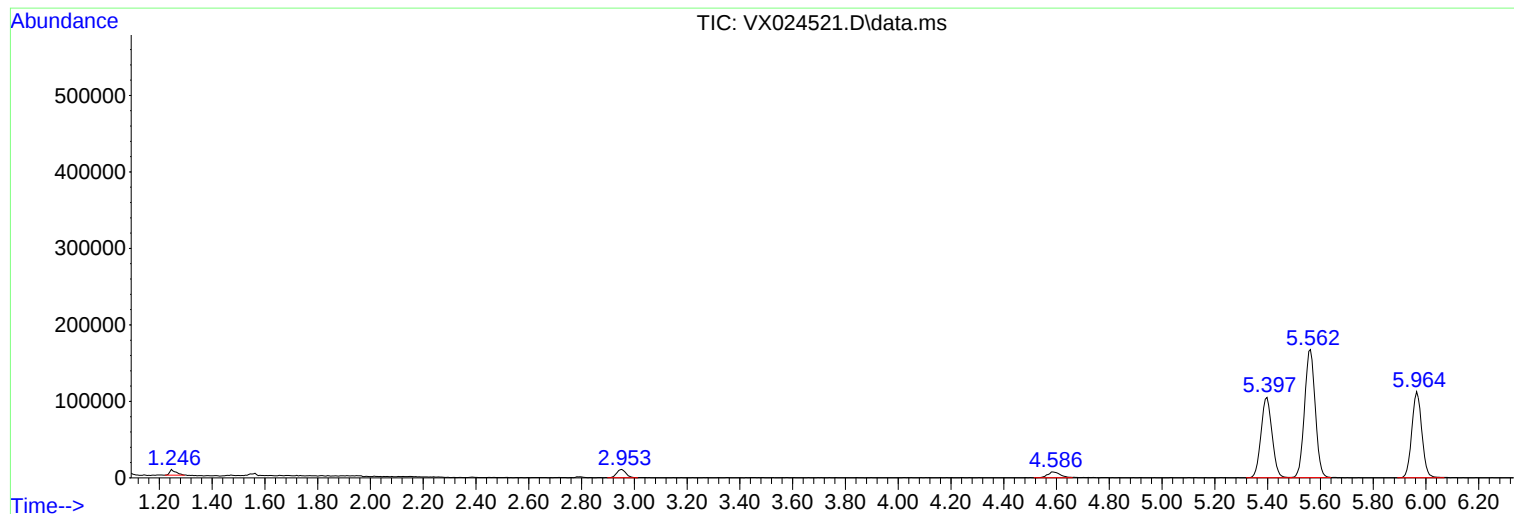

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024521.D
Acq On : 04 Oct 2021 15:34
Operator : JC/MD
Sample : M3911-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANKRE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024521.D
Acq On : 04 Oct 2021 15:34
Operator : JC/MD
Sample : M3911-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANKRE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------