

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024523.D
 Acq On : 04 Oct 2021 16:22
 Operator : JC/MD
 Sample : M4063-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-RR-03-(SA)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	34	rVB2	6835	11809	1.43%	0.285%
2	2.550	230	240	247	rBV	14093	26413	3.21%	0.637%
3	5.397	695	707	719	rBV	100128	287246	34.88%	6.932%
4	5.562	722	734	747	rVB	159382	446328	54.20%	10.771%
5	5.964	788	800	810	rBV2	106300	281427	34.17%	6.791%
6	6.769	922	932	947	rBV	257097	606088	73.59%	14.626%
7	8.653	1232	1241	1249	rBV	531281	823548	100.00%	19.874%
8	10.055	1465	1471	1489	rBV	512413	662106	80.40%	15.978%
9	11.085	1634	1640	1654	rBV	361459	460629	55.93%	11.116%
10	12.024	1789	1794	1805	rBV	427252	529158	64.25%	12.770%
11	13.780	2075	2082	2087	rBV	7231	9154	1.11%	0.221%




Sum of corrected areas: 4143906

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024523.D
Acq On : 04 Oct 2021 16:22
Operator : JC/MD
Sample : M4063-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

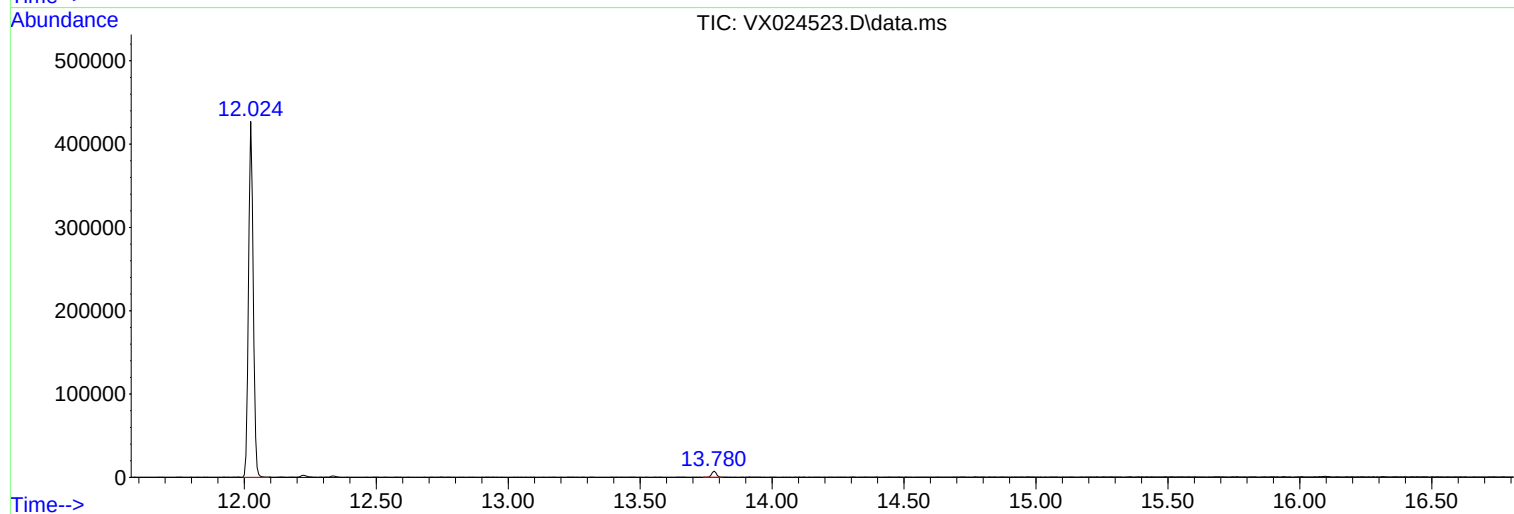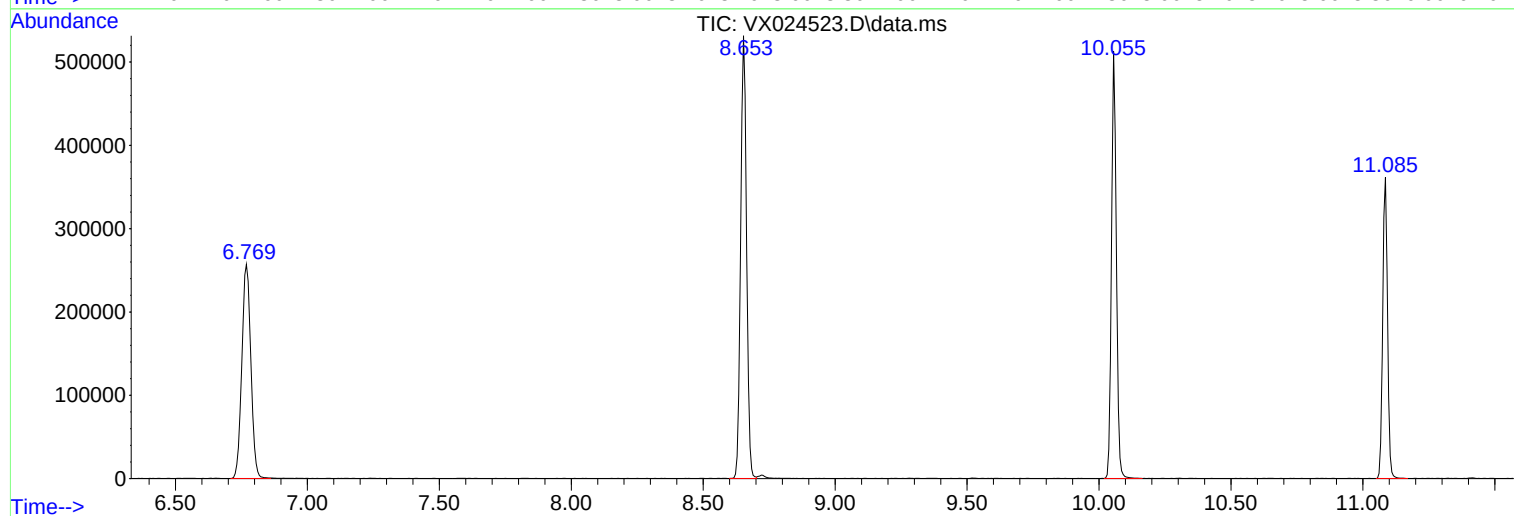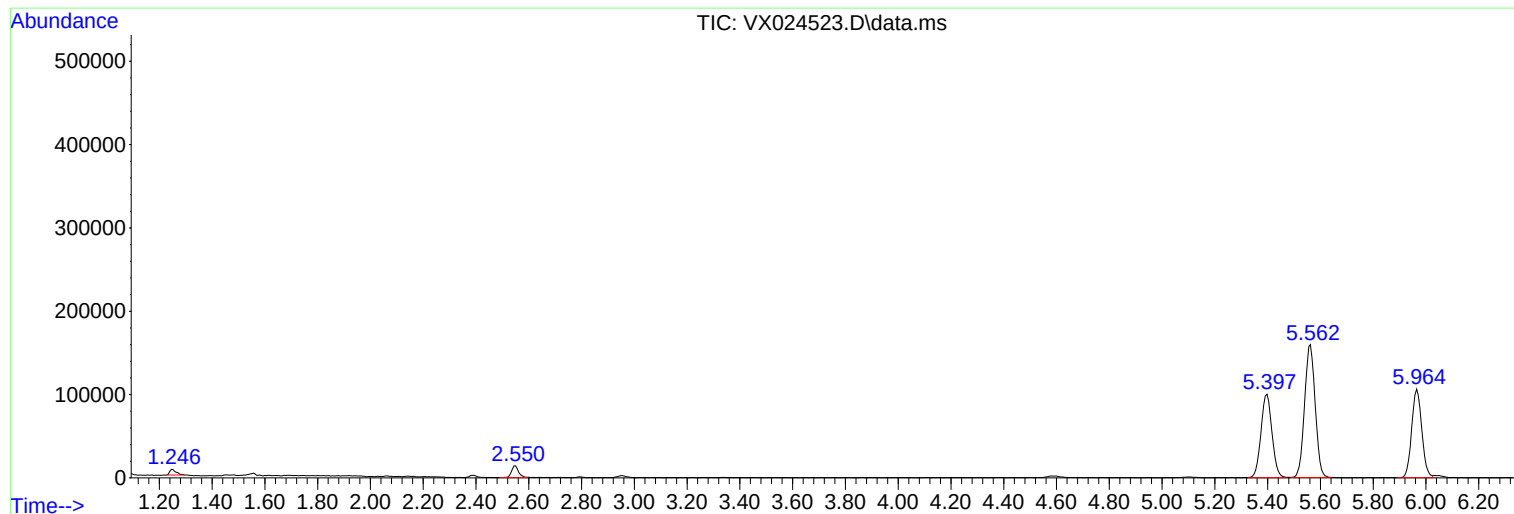

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024523.D
Acq On : 04 Oct 2021 16:22
Operator : JC/MD
Sample : M4063-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024523.D
Acq On : 04 Oct 2021 16:22
Operator : JC/MD
Sample : M4063-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
