

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024530.D
 Acq On : 04 Oct 2021 19:06
 Operator : JC/MD
 Sample : M4045-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-100121

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rBV2	76132	72938	8.83%	1.637%
2	2.544	231	239	246	rBV	7075	12453	1.51%	0.279%
3	5.397	695	707	722	rBV	103208	297155	35.99%	6.668%
4	5.562	722	734	749	rVB	159965	453041	54.86%	10.165%
5	5.964	789	800	820	rBV	108937	287668	34.84%	6.455%
6	6.769	920	932	947	rBV	263253	619337	75.00%	13.897%
7	8.653	1234	1241	1254	rBV	540569	825764	100.00%	18.529%
8	10.055	1466	1471	1485	rVB	560590	762003	92.28%	17.098%
9	11.085	1634	1640	1650	rBV	415279	518595	62.80%	11.636%
10	12.024	1789	1794	1803	rBV	504416	607732	73.60%	13.636%




Sum of corrected areas: 4456686

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024530.D
Acq On : 04 Oct 2021 19:06
Operator : JC/MD
Sample : M4045-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-100121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

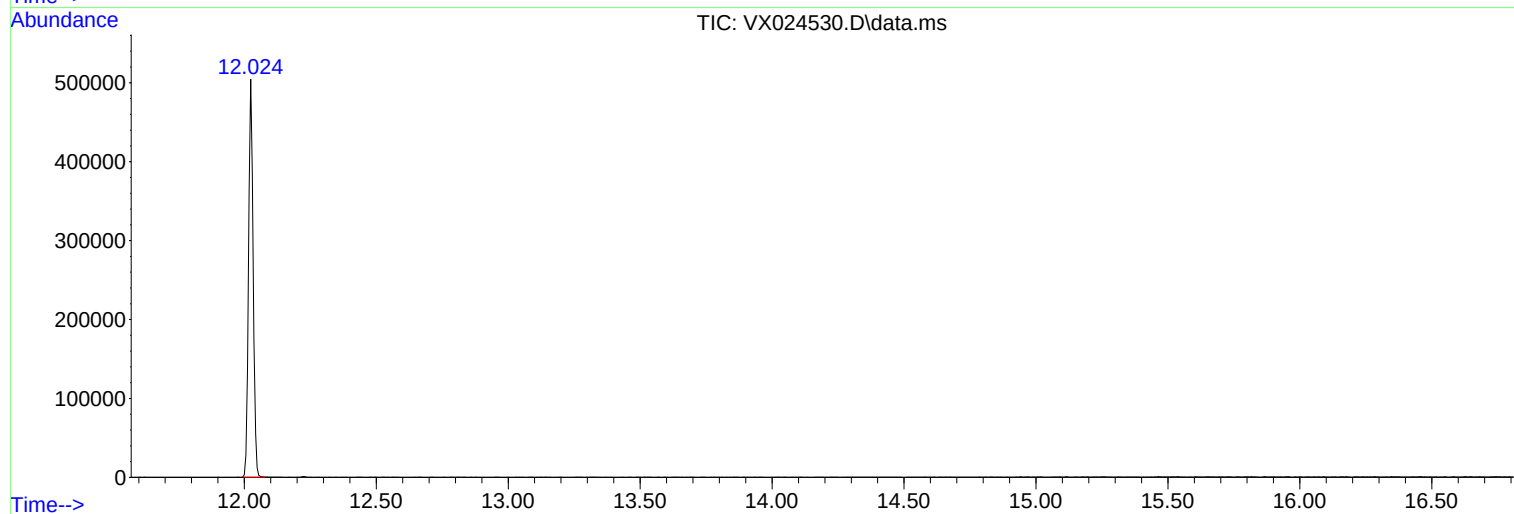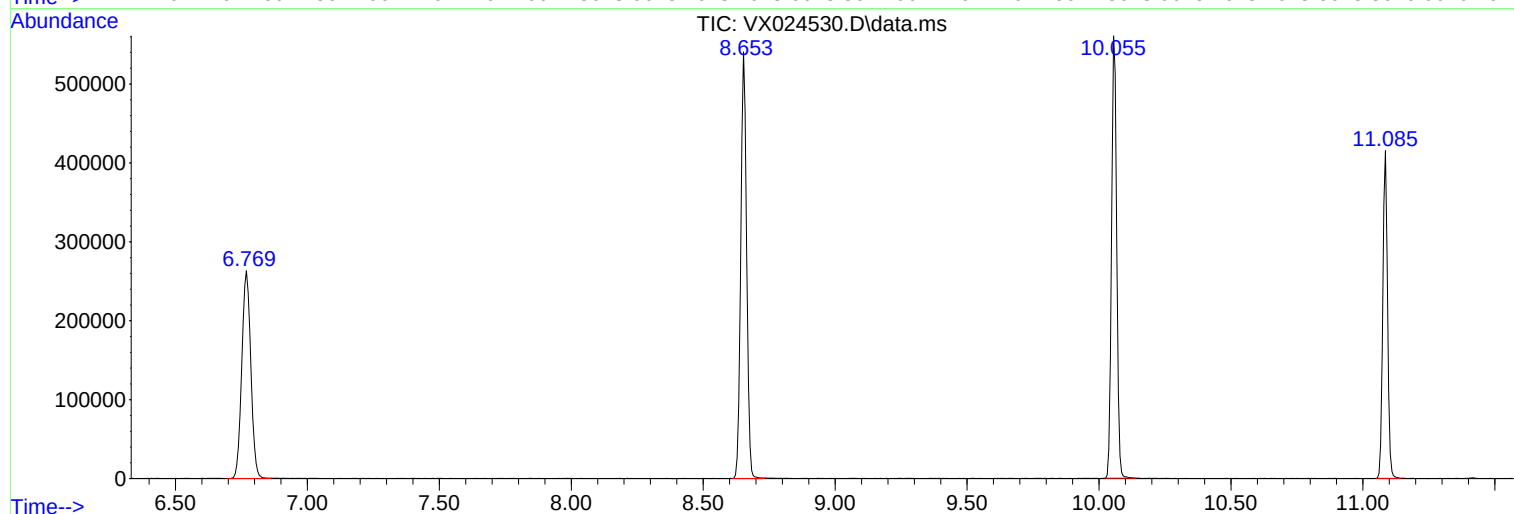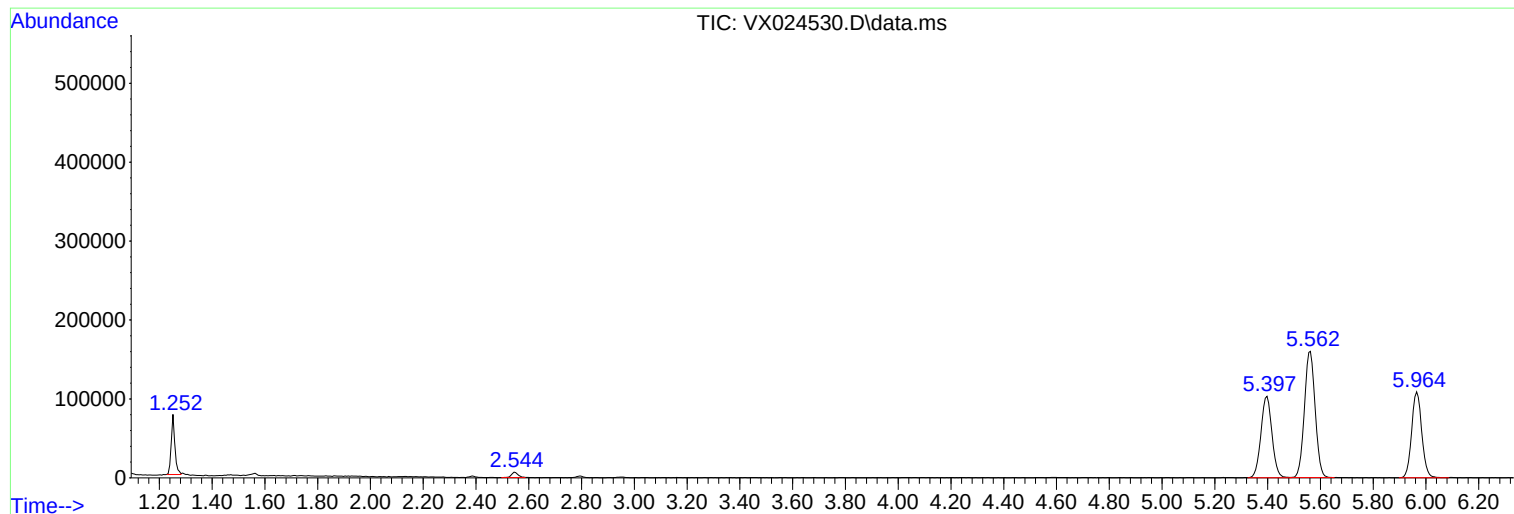

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024530.D
Acq On : 04 Oct 2021 19:06
Operator : JC/MD
Sample : M4045-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-100121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024530.D
Acq On : 04 Oct 2021 19:06
Operator : JC/MD
Sample : M4045-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-100121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
