

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
 Data File : VX024533.D
 Acq On : 04 Oct 2021 20:17
 Operator : JC/MD
 Sample : M3989-05 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-7

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	22	27	39	rBV2	45450	52619	6.63%	1.031%
2	2.971	299	309	317	rBV	40977	89271	11.25%	1.749%
3	3.123	322	334	347	rVV	250390	574367	72.41%	11.252%
4	3.770	433	440	451	rVB3	4098	10577	1.33%	0.207%
5	5.397	694	707	719	rBV2	106996	308426	38.88%	6.042%
6	5.562	722	734	751	rVB	174220	487466	61.45%	9.549%
7	5.964	788	800	815	rBV2	113844	297842	37.55%	5.835%
8	6.769	921	932	945	rBV	244046	573540	72.31%	11.235%
9	8.653	1234	1241	1249	rBV	517869	793209	100.00%	15.538%
10	10.055	1465	1471	1486	rVB	540863	715057	90.15%	14.008%
11	11.085	1634	1640	1651	rVB	426698	553229	69.75%	10.837%
12	12.024	1788	1794	1806	rVB	531814	649196	81.84%	12.717%




Sum of corrected areas: 5104799

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024533.D
Acq On : 04 Oct 2021 20:17
Operator : JC/MD
Sample : M3989-05 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

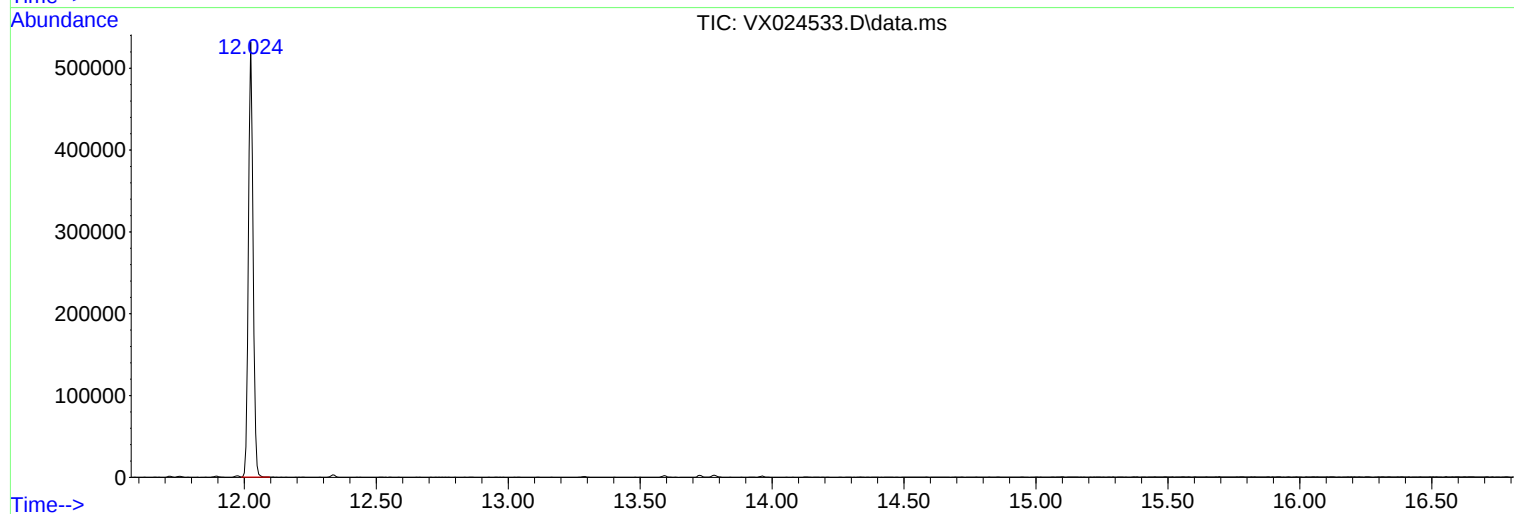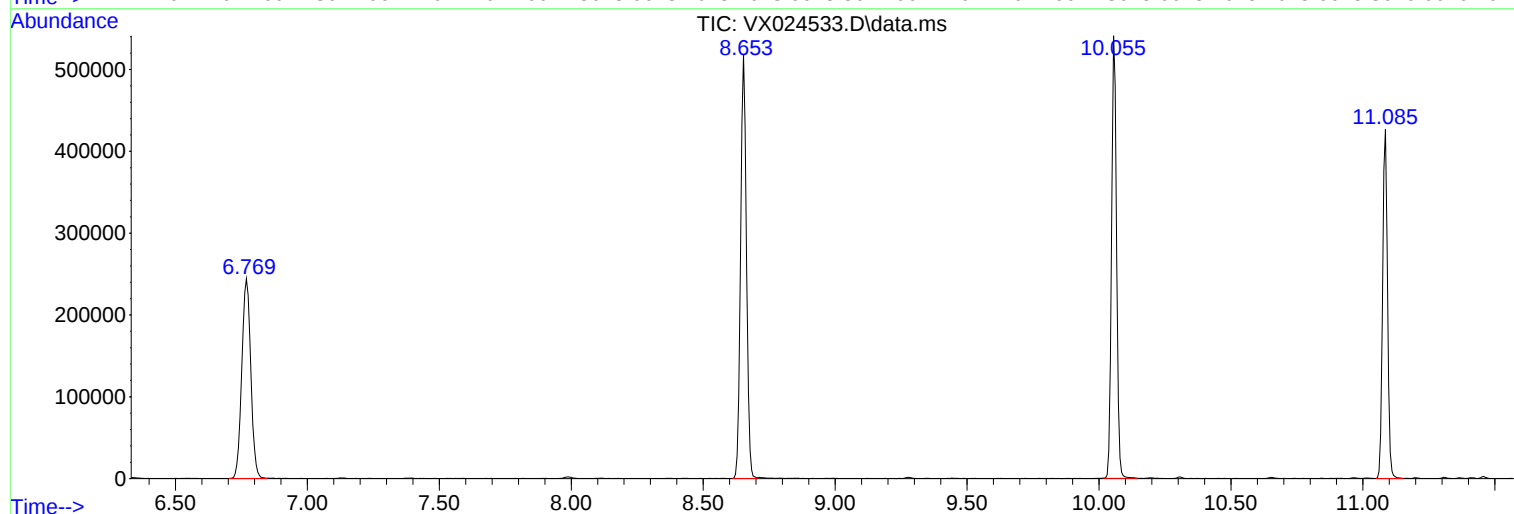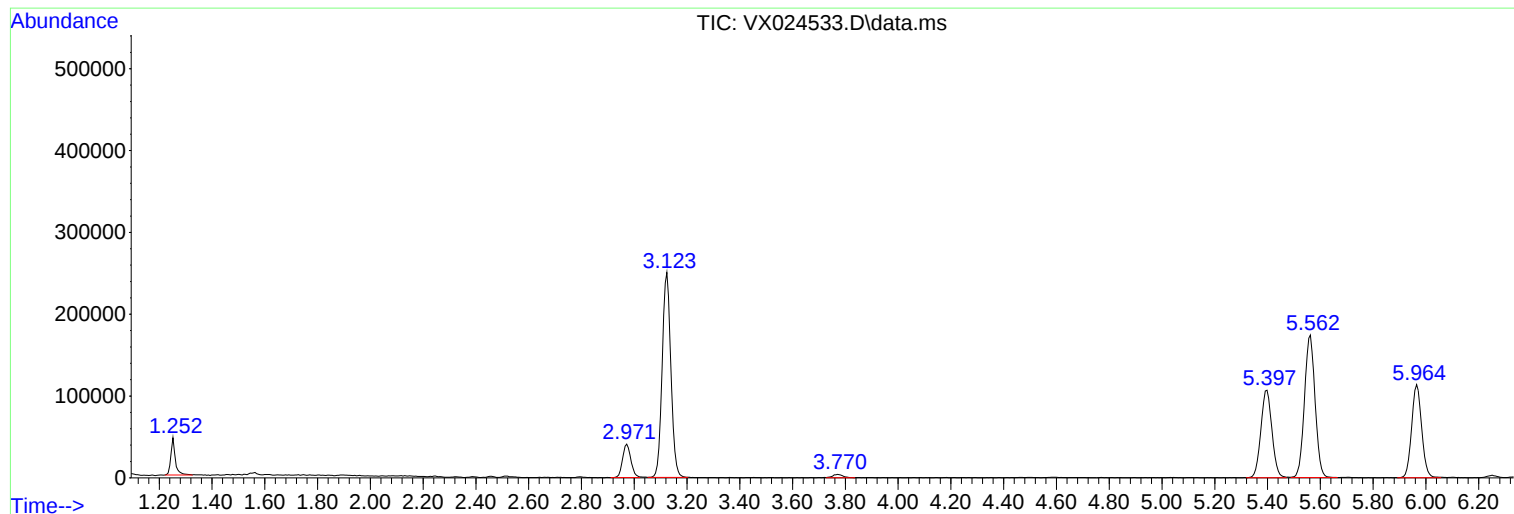

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024533.D
Acq On : 04 Oct 2021 20:17
Operator : JC/MD
Sample : M3989-05 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.252 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.252	5.40 ug/l	52619	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	37
2			Pentaborane(11)	66	B5H11	018433-84-6	9
3			Ethyl Chloride	64	C2H5Cl	000075-00-3	5
4			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	5
5			Methyl nitrite	61	CH3NO2	000624-91-9	5

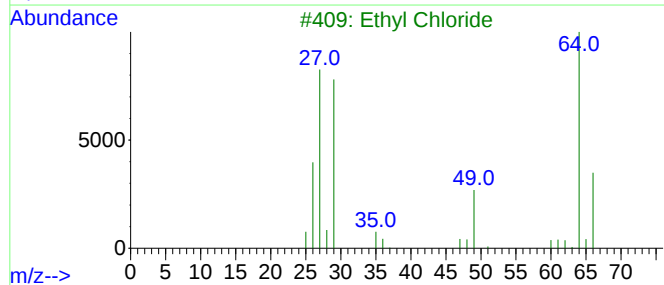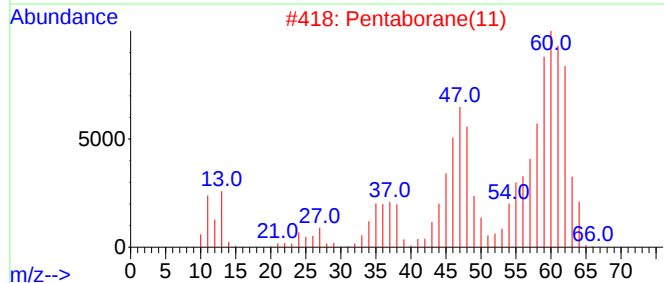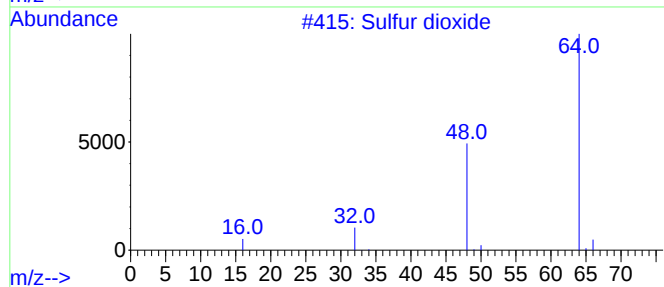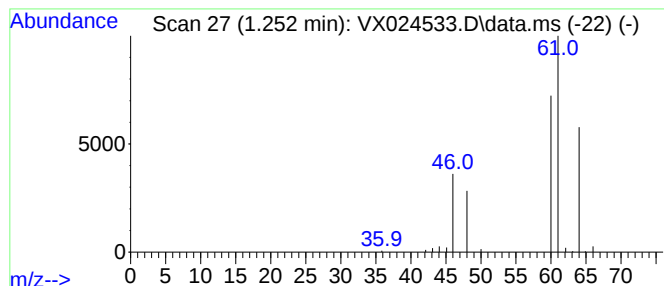

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100421\
Data File : VX024533.D
Acq On : 04 Oct 2021 20:17
Operator : JC/MD
Sample : M3989-05 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.252	1.252	5.4	ug/l	52619	1	5.562	487466	50.0