
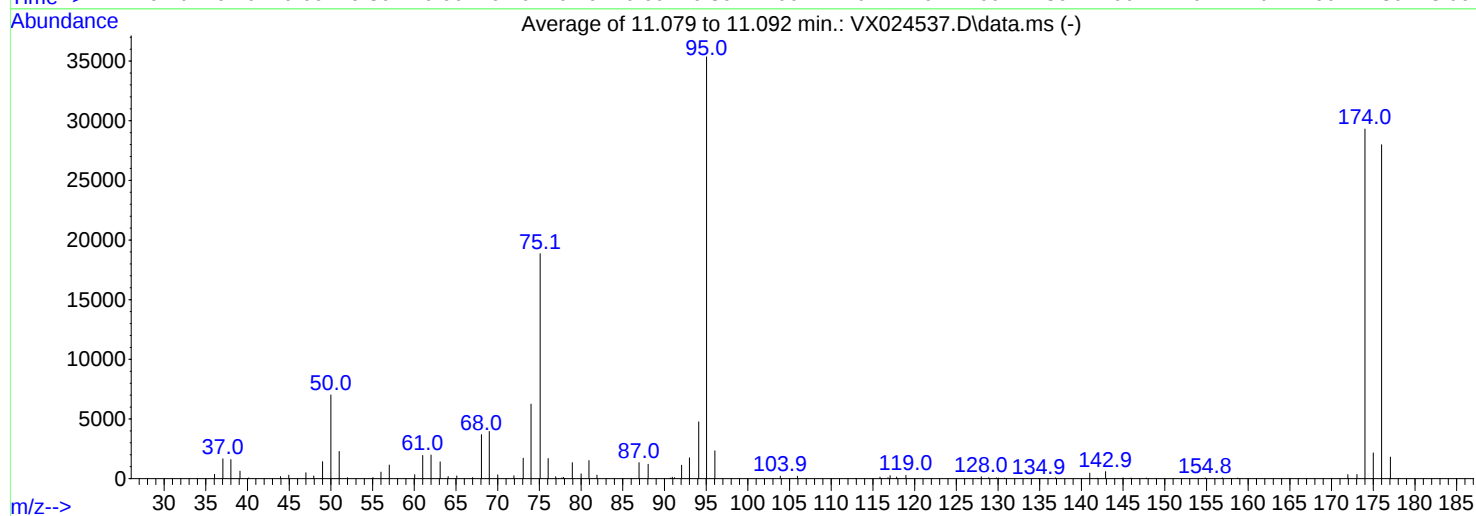


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100421\  
 Data File : VX024537.D  
 Acq On : 04 Oct 2021 22:14  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X092321W.M  
 Title : SW846 8260  
 Last Update : Thu Sep 23 18:24:34 2021

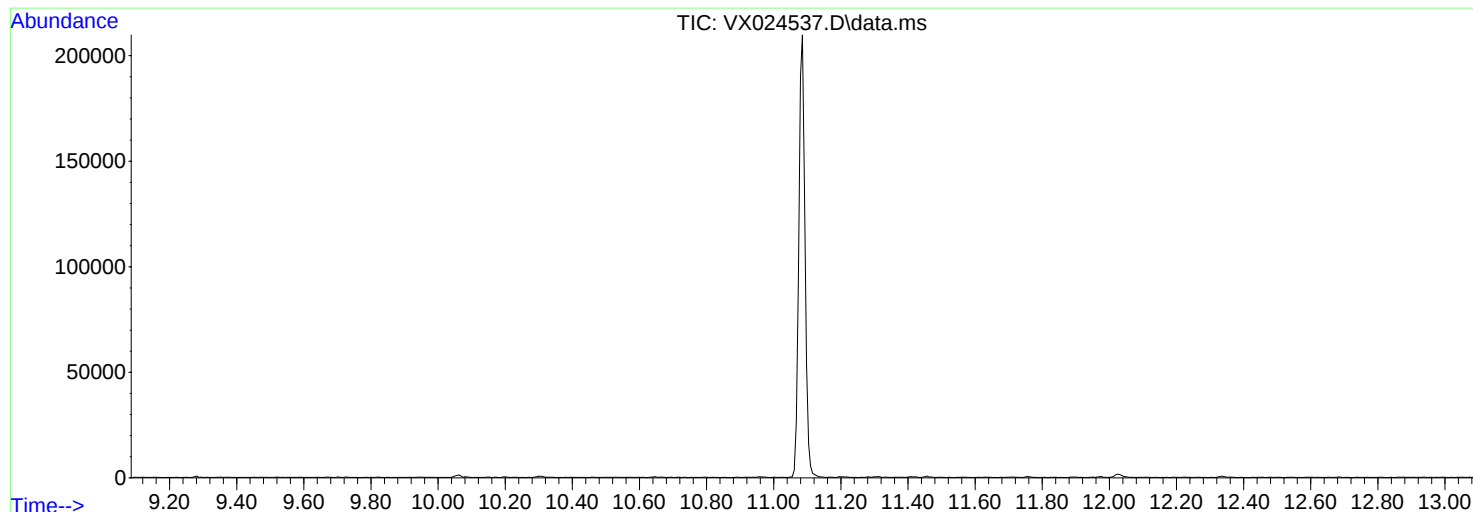

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.8         | 7017       | PASS                |
| 75             | 95              | 30              | 60              | 53.3         | 18853      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 35355      | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 2330       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 354        | PASS                |
| 174            | 95              | 50              | 100             | 82.9         | 29299      | PASS                |
| 175            | 174             | 5               | 9               | 7.4          | 2165       | PASS                |
| 176            | 174             | 95              | 101             | 95.5         | 27992      | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 1806       | PASS                |