
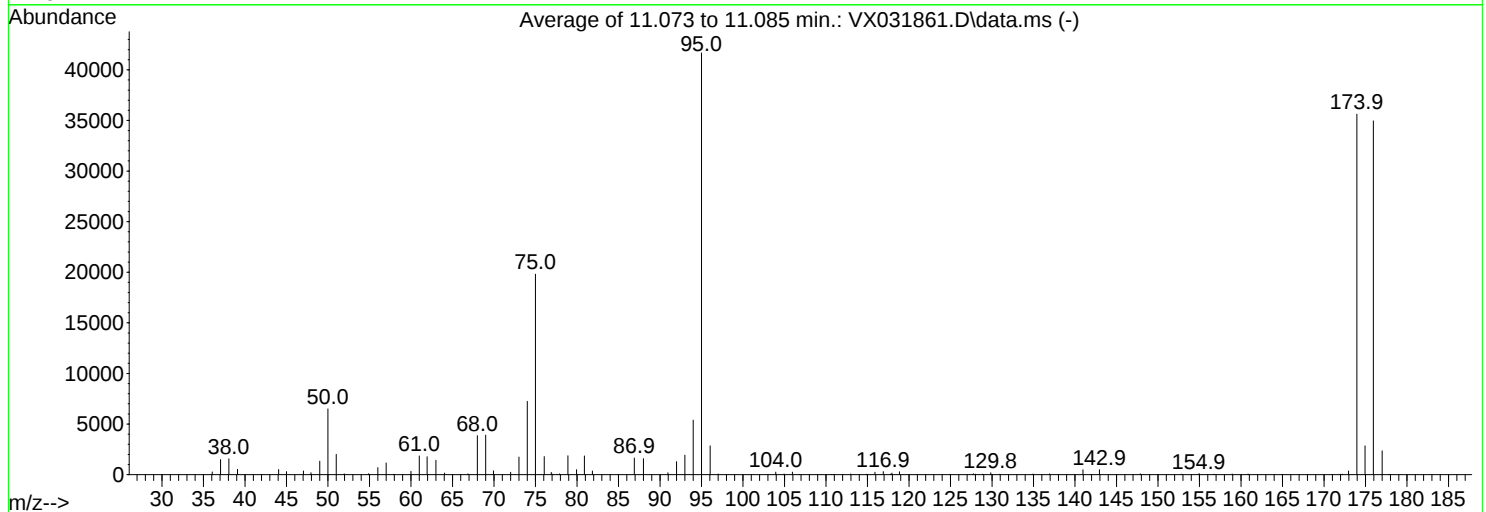


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100422\
Data File : VX031861.D
Acq On : 04 Oct 2022 08:22
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100322W.M
Title : SW846 8260
Last Update : Tue Oct 04 06:59:30 2022

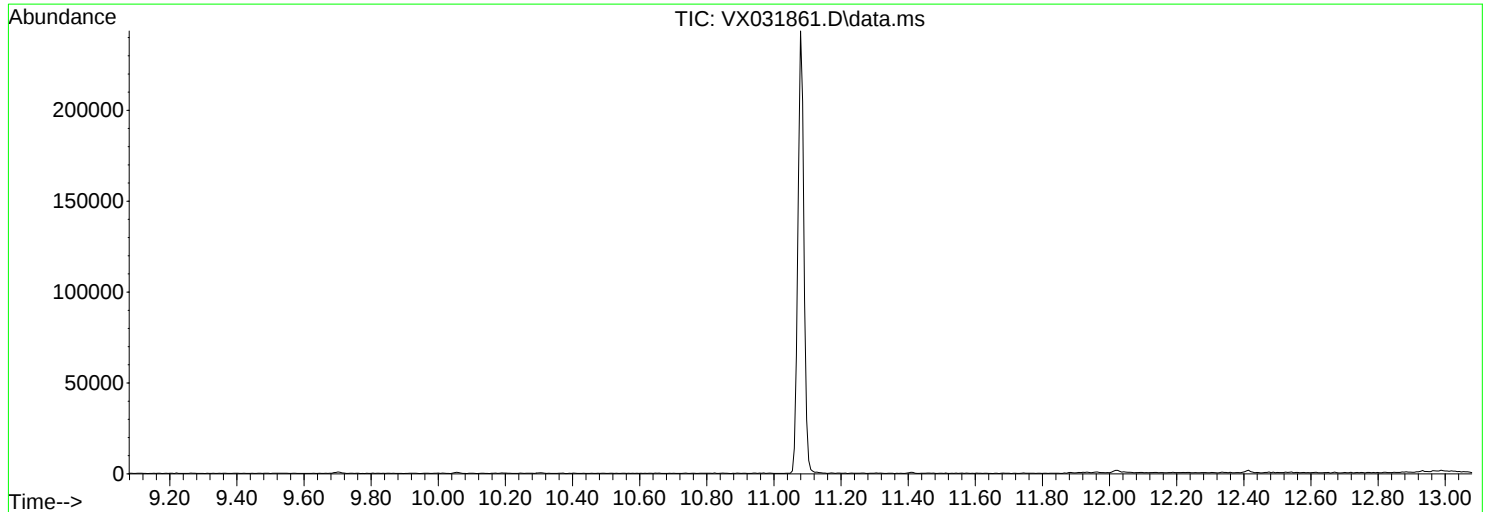

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	6499	PASS
75	95	30	60	47.5	19813	PASS
95	95	100	100	100.0	41683	PASS
96	95	5	9	6.8	2845	PASS
173	174	0.00	2	1.0	367	PASS
174	95	50	100	85.5	35624	PASS
175	174	5	9	8.0	2848	PASS
176	174	95	101	98.1	34960	PASS
177	176	5	9	6.7	2350	PASS