
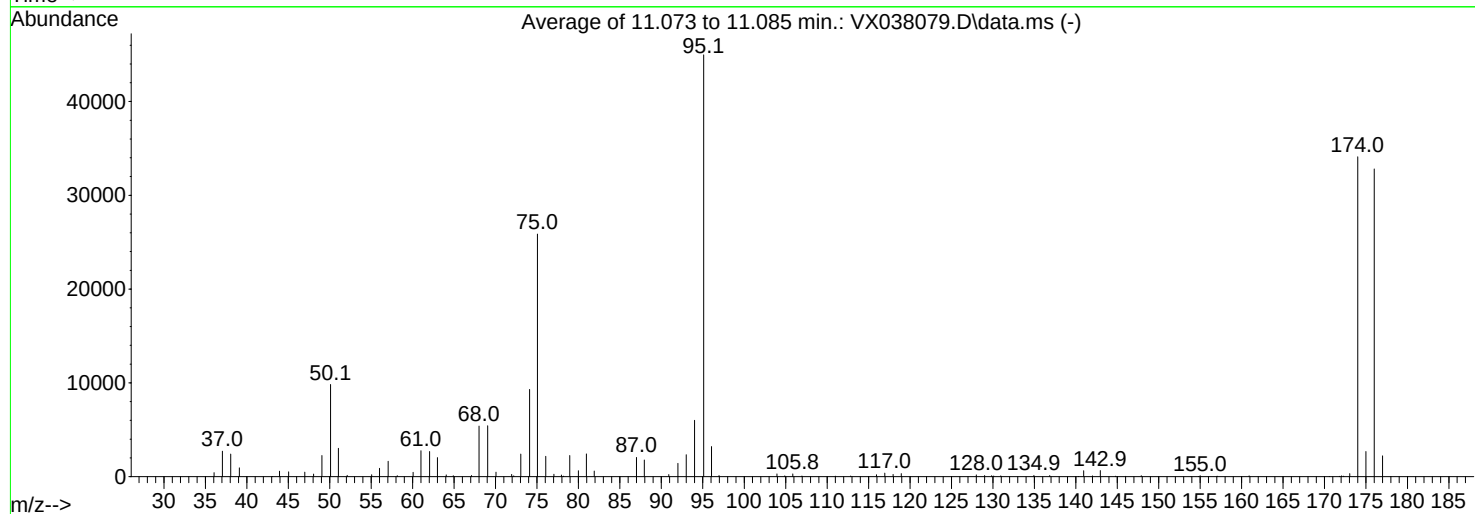


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100423\
Data File : VX038079.D
Acq On : 04 Oct 2023 21:48
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100323W.M
Title : SW846 8260
Last Update : Wed Oct 04 09:08:35 2023

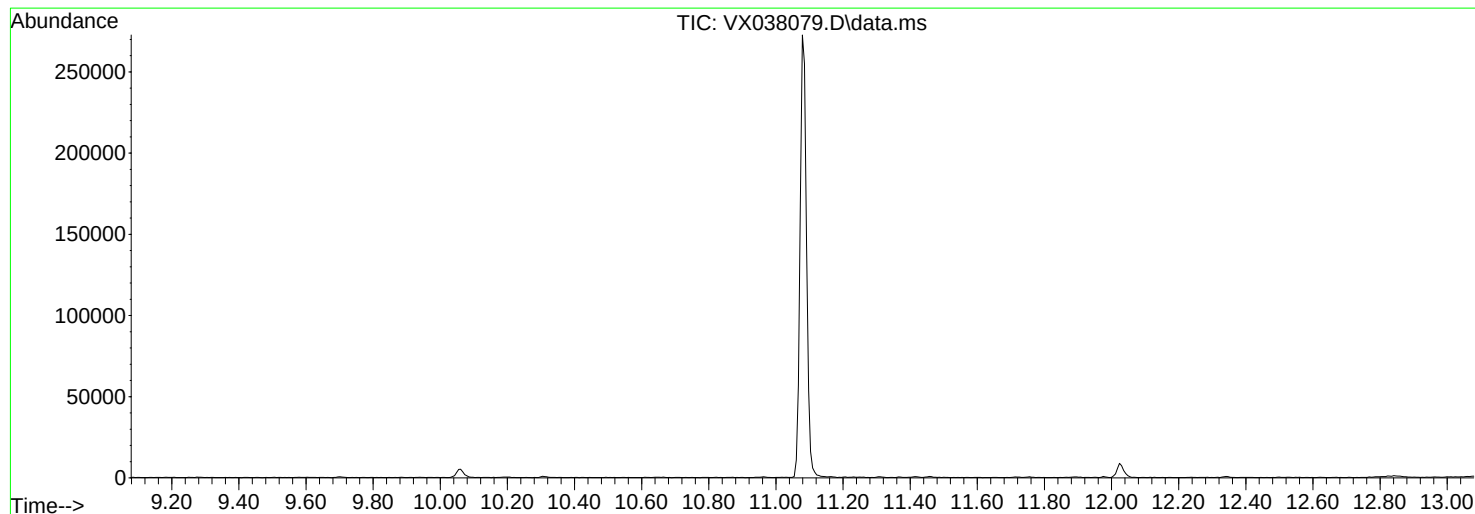

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	9836	PASS
75	95	30	60	57.5	25867	PASS
95	95	100	100	100.0	44976	PASS
96	95	5	9	7.1	3213	PASS
173	174	0.00	2	1.0	333	PASS
174	95	50	100	75.8	34112	PASS
175	174	5	9	7.9	2683	PASS
176	174	95	101	96.2	32816	PASS
177	176	5	9	6.8	2224	PASS