

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100424\
 Data File : VX043273.D
 Acq On : 04 Oct 2024 09:01
 Operator : JC/MD
 Sample : VX1004MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1004MBL01

Quant Time: Oct 04 23:23:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 16:50:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	80943	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	149302	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	130273	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	58428	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	68523	51.836	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	103.680%
35) Dibromofluoromethane	5.379	113	50297	48.849	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.700%
50) Toluene-d8	8.647	98	178891	50.135	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.260%
62) 4-Bromofluorobenzene	11.079	95	65005	50.146	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	100.300%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100424\
Data File : VX043273.D
Acq On : 04 Oct 2024 09:01
Operator : JC/MD
Sample : VX1004MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1004MBL01

Quant Time: Oct 04 23:23:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 16:50:57 2024
Response via : Initial Calibration




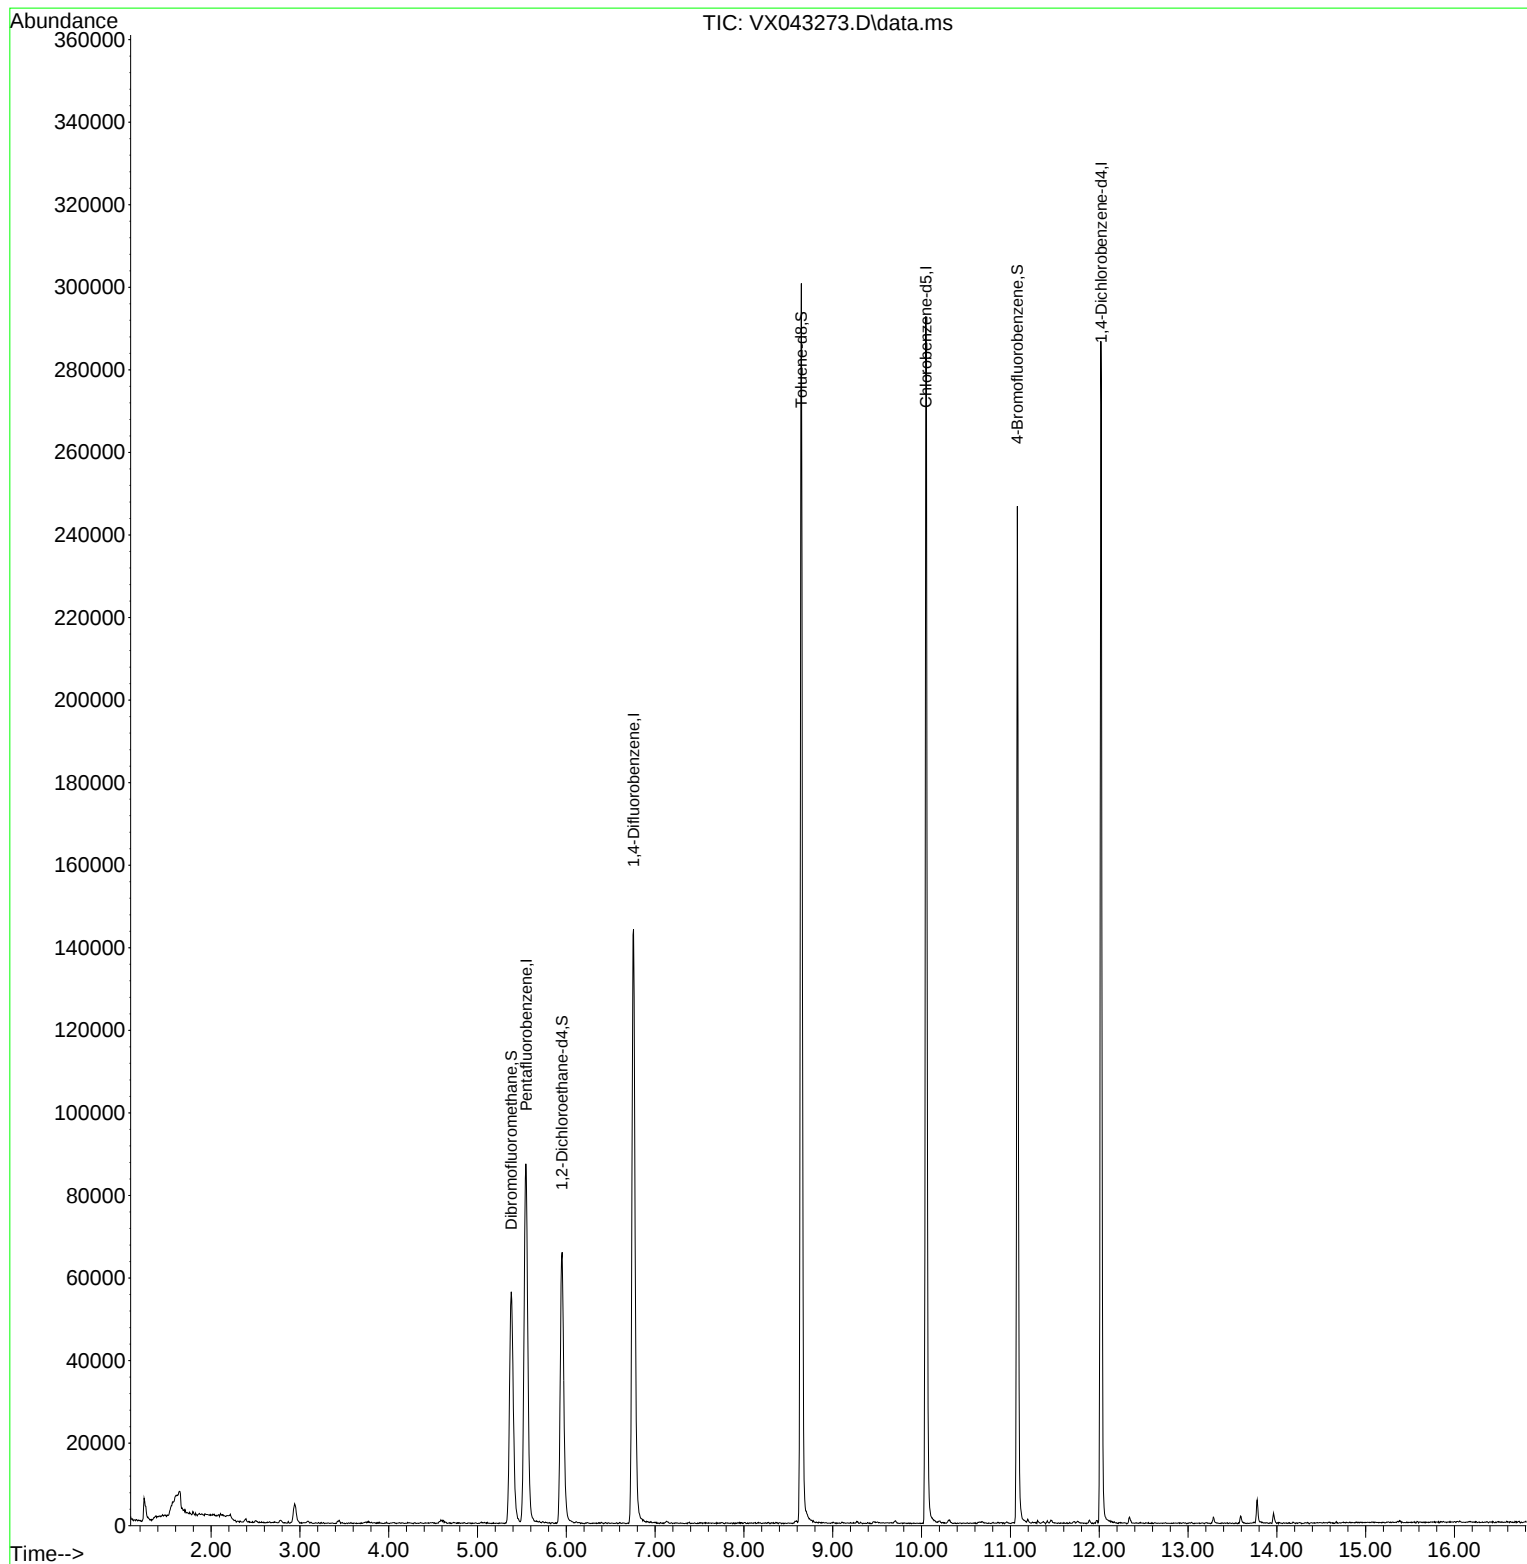




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01




Instrument :
MSVOA_X
ClientSampleId :
VX1004MBL01


Tgt Ion:168 Resp: 80943
Ion Ratio Lower Upper
168 100
99 59.4 49.7 74.5

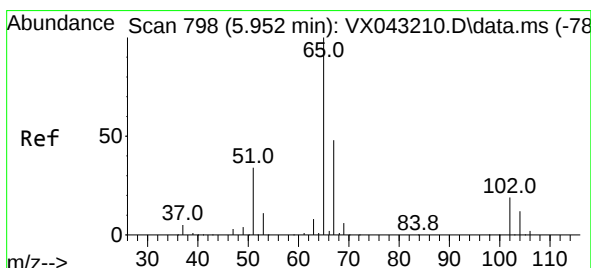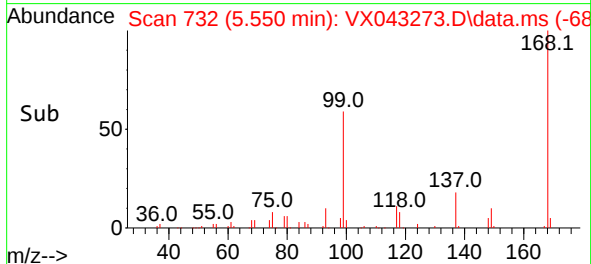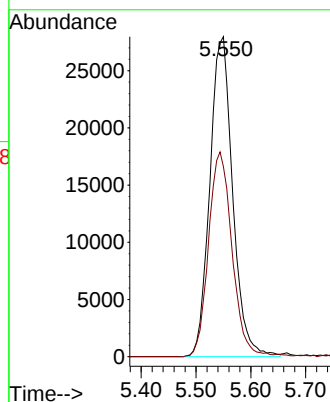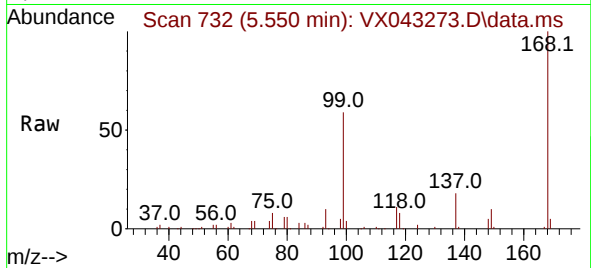

#33
1,2-Dichloroethane-d4
Concen: 51.836 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01

Tgt Ion: 65 Resp: 68523
Ion Ratio Lower Upper
65 100
67 48.7 0.0 99.0


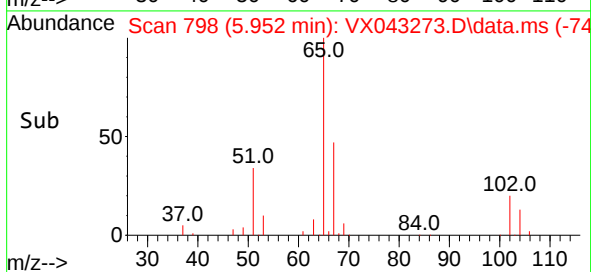
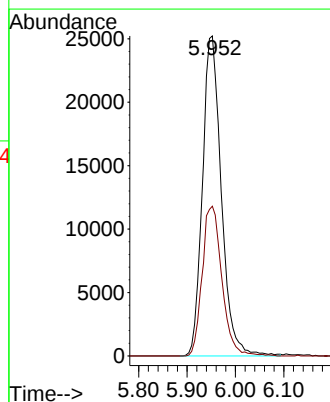
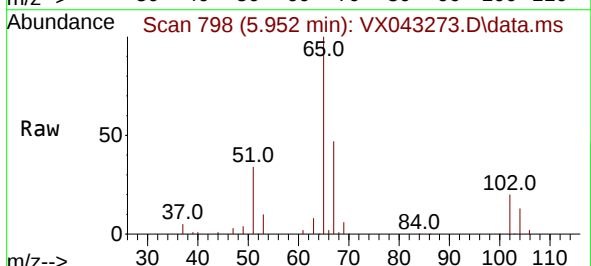


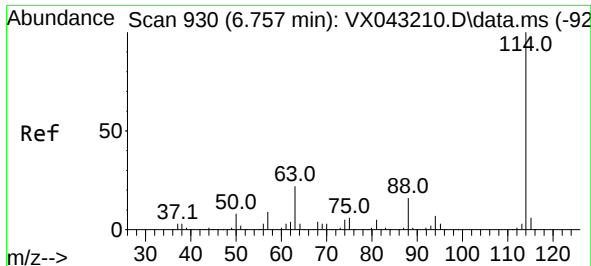

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01




Instrument :
MSVOA_X
ClientSampleId :
VX1004MBL01


Tgt Ion:114 Resp: 149302
Ion Ratio Lower Upper
114 100
63 21.4 0.0 43.0
88 16.9 0.0 33.0

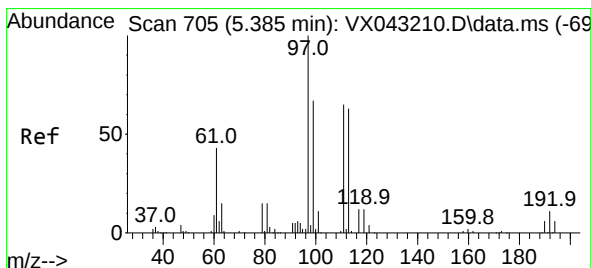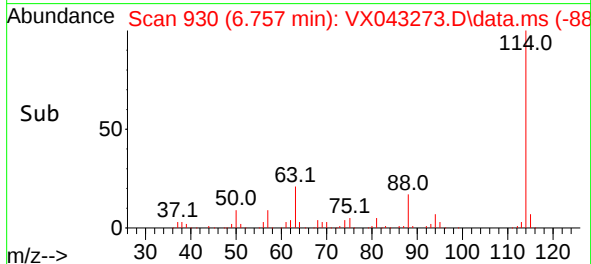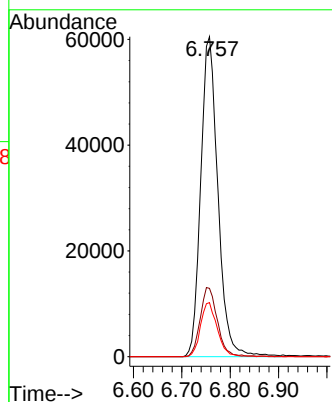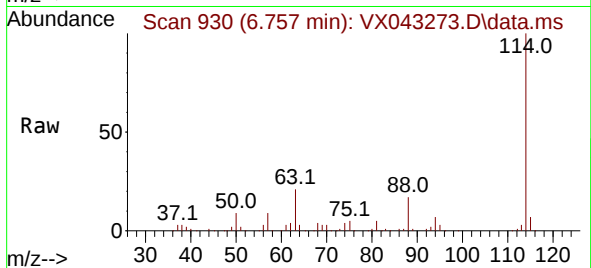

#35
Dibromofluoromethane
Concen: 48.849 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01

Tgt Ion:113 Resp: 50297
Ion Ratio Lower Upper
113 100
111 100.8 83.4 125.0
192 18.0 14.1 21.1


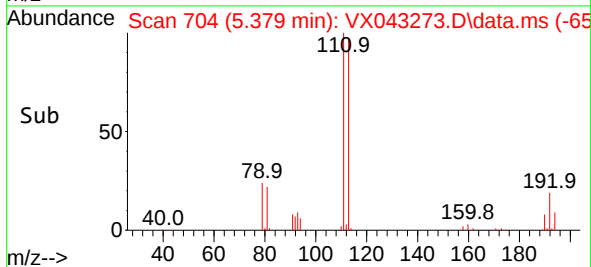
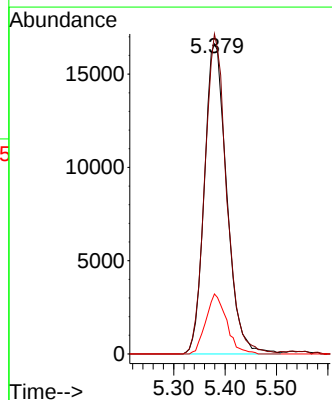
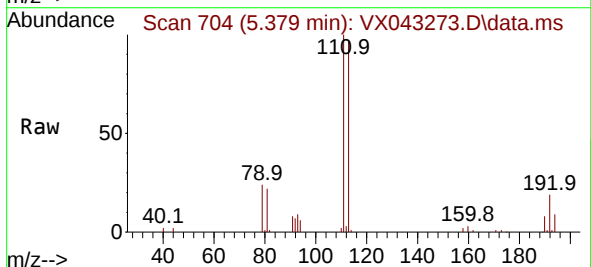


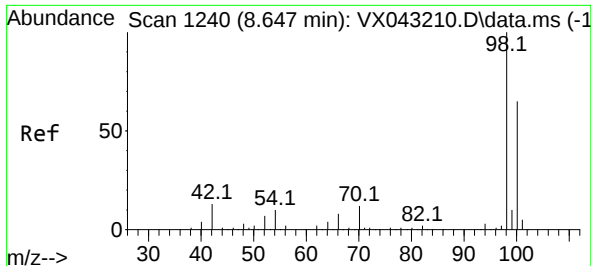

#50
Toluene-d8
Concen: 50.135 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01




Instrument :
MSVOA_X
ClientSampleId :
VX1004MBL01


Tgt Ion: 98 Resp: 178891
Ion Ratio Lower Upper
98 100
100 65.1 52.4 78.6

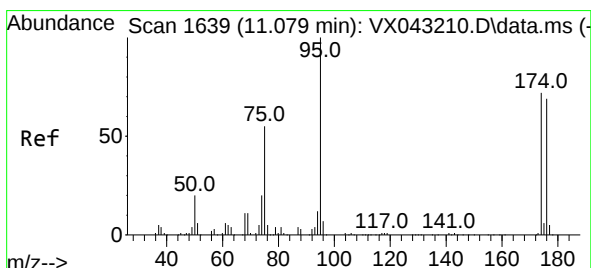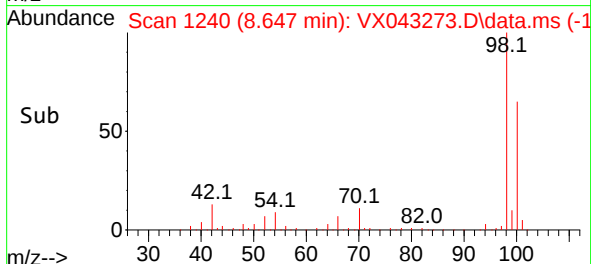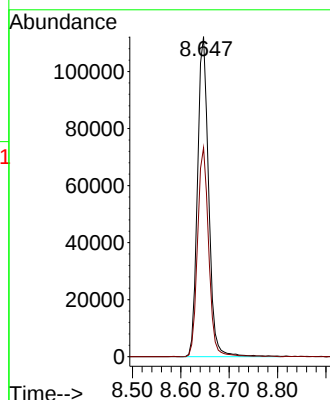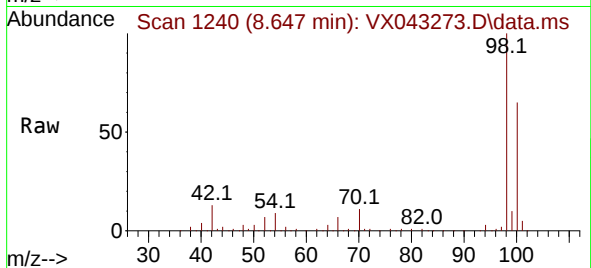

#62
4-Bromofluorobenzene
Concen: 50.146 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01

Tgt Ion: 95 Resp: 65005
Ion Ratio Lower Upper
95 100
174 72.6 0.0 145.0
176 70.3 0.0 143.0


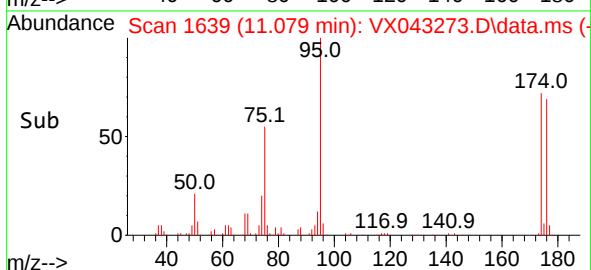
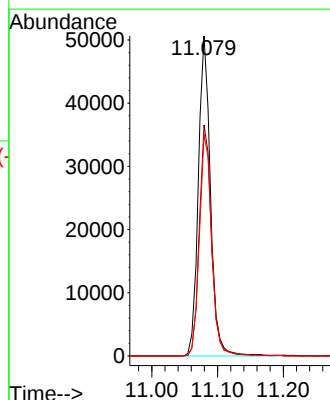
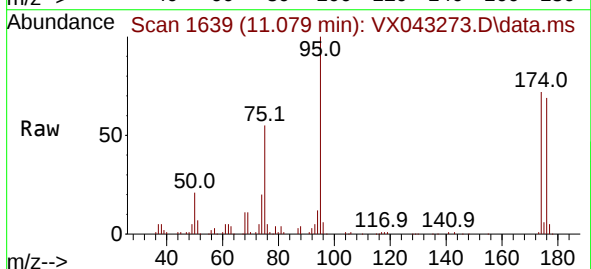


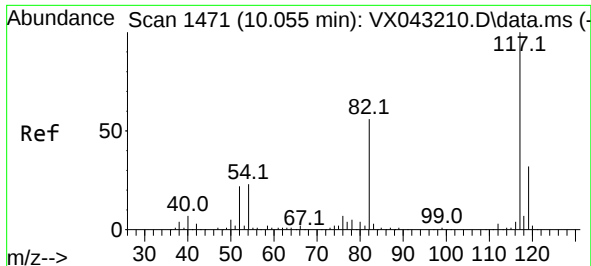

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01

Instrument :
MSVOA_X
ClientSampleId :
VX1004MBL01

Tgt Ion:117 Resp: 130273
Ion Ratio Lower Upper
117 100
82 58.5 45.0 67.6
119 31.3 25.3 37.9

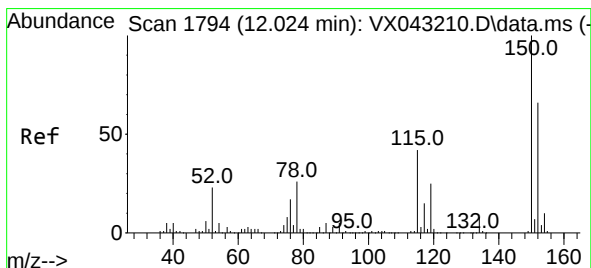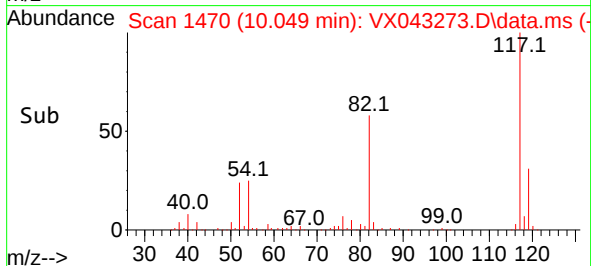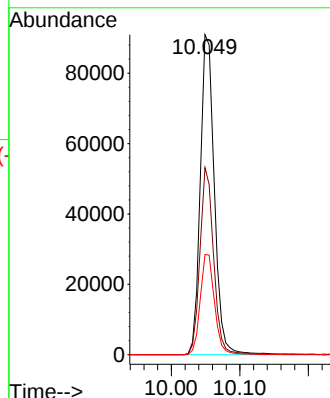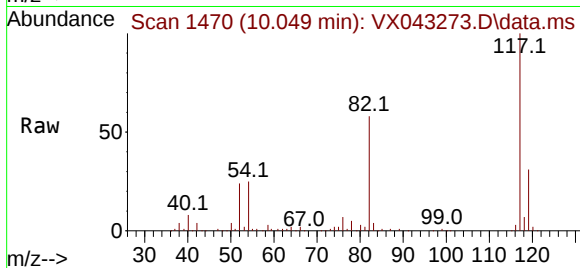

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX043273.D
Acq: 04 Oct 2024 09:01

Tgt Ion:152 Resp: 58428
Ion Ratio Lower Upper
152 100
115 63.7 44.1 132.3
150 159.8 0.0 347.4

