

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100424\
 Data File : VX043274.D
 Acq On : 04 Oct 2024 09:24
 Operator : JC/MD
 Sample : VX1004WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1004WBL01

Quant Time: Oct 04 23:24:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 16:50:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	77627	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	144088	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	122929	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	53080	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	66194	52.213	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	104.420%
35) Dibromofluoromethane	5.379	113	47988	48.293	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.580%
50) Toluene-d8	8.647	98	170850	49.614	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.220%
62) 4-Bromofluorobenzene	11.079	95	59917	47.894	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	95.780%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100424\
Data File : VX043274.D
Acq On : 04 Oct 2024 09:24
Operator : JC/MD
Sample : VX1004WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1004WBL01

Quant Time: Oct 04 23:24:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 16:50:57 2024
Response via : Initial Calibration




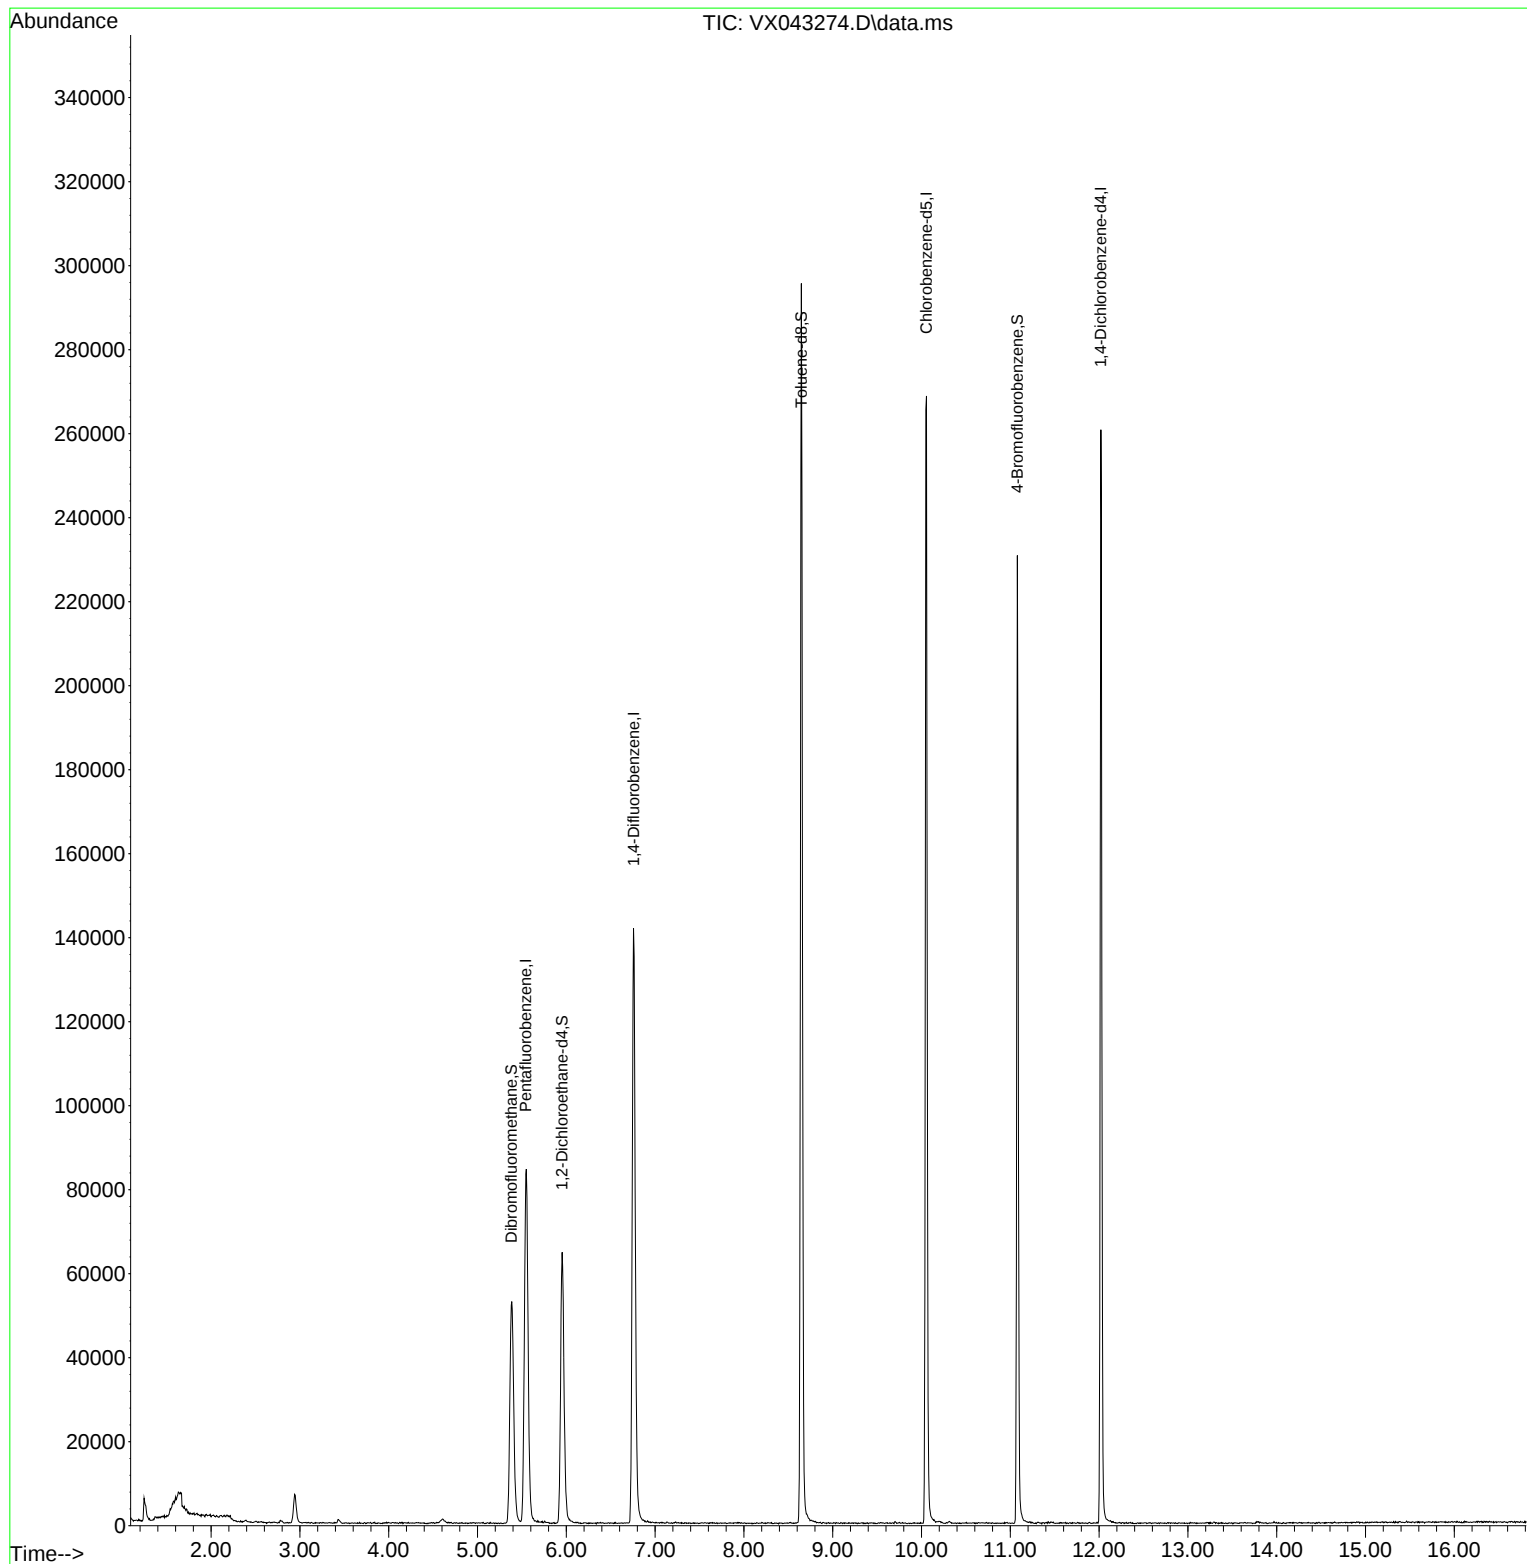




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX043274.D
Acq: 04 Oct 2024 09:24




Instrument :
MSVOA_X
ClientSampleId :
VX1004WBL01


Tgt Ion:168 Resp: 77627
Ion Ratio Lower Upper
168 100
99 64.3 49.7 74.5

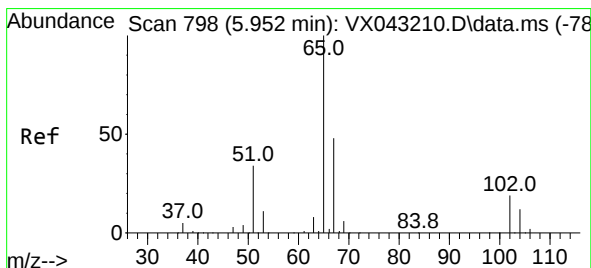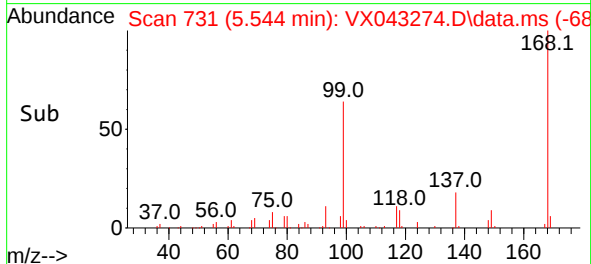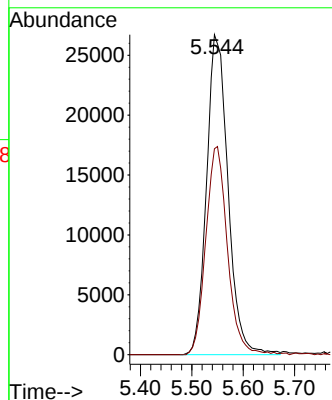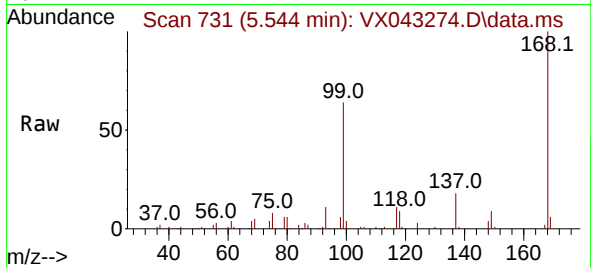

#33
1,2-Dichloroethane-d4
Concen: 52.213 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX043274.D
Acq: 04 Oct 2024 09:24

Tgt Ion: 65 Resp: 66194
Ion Ratio Lower Upper
65 100
67 49.9 0.0 99.0


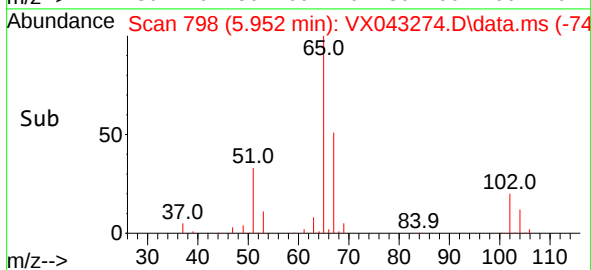
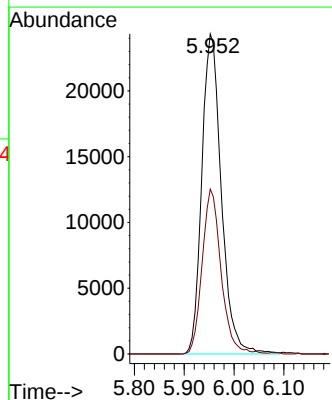
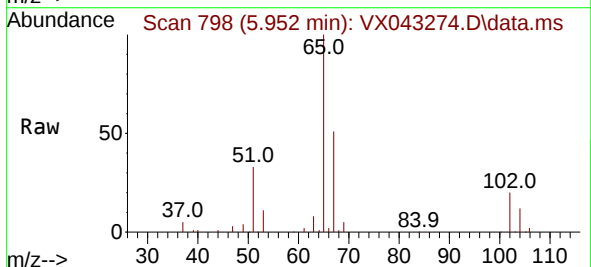


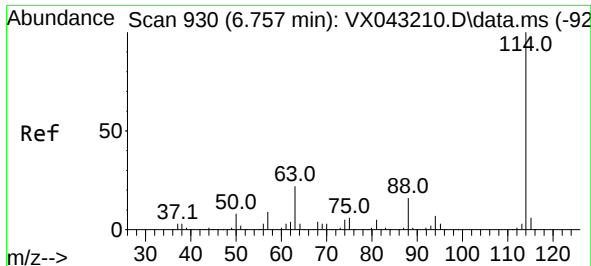

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX043274.D
Acq: 04 Oct 2024 09:24




Instrument :
MSVOA_X
ClientSampleId :
VX1004WBL01


Tgt Ion:114 Resp: 144088
Ion Ratio Lower Upper
114 100
63 21.2 0.0 43.0
88 16.8 0.0 33.0

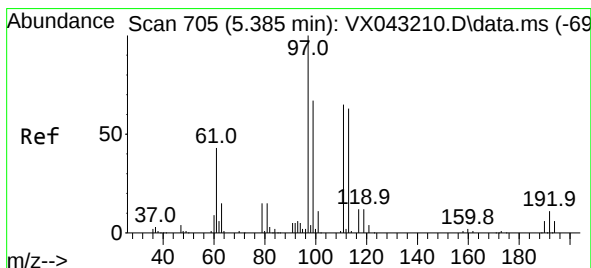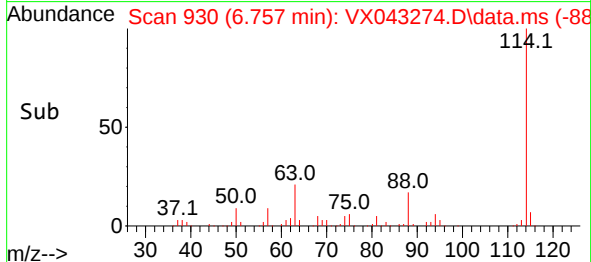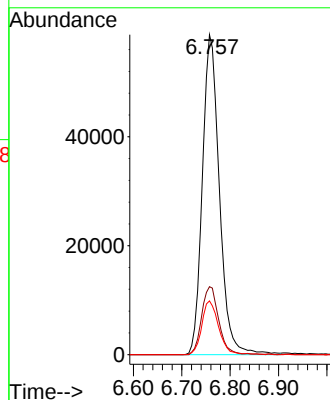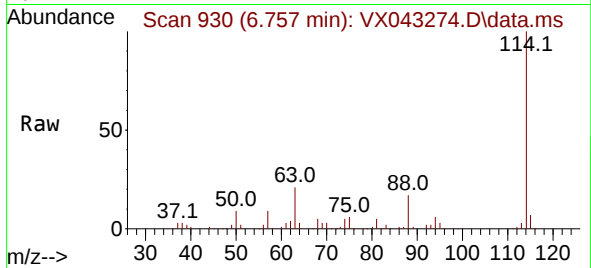

#35
Dibromofluoromethane
Concen: 48.293 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX043274.D
Acq: 04 Oct 2024 09:24

Tgt Ion:113 Resp: 47988
Ion Ratio Lower Upper
113 100
111 102.0 83.4 125.0
192 17.9 14.1 21.1


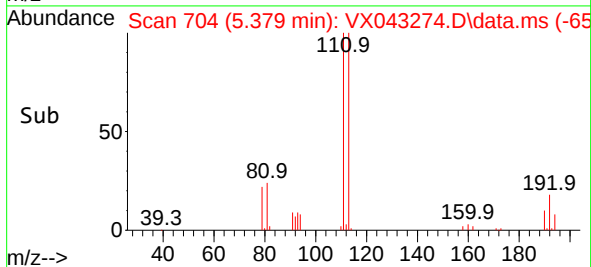
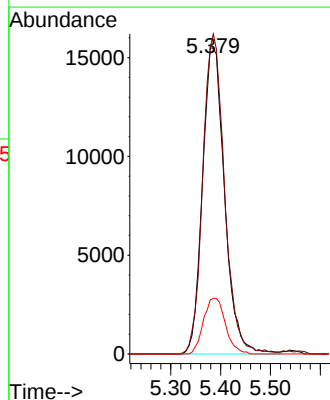
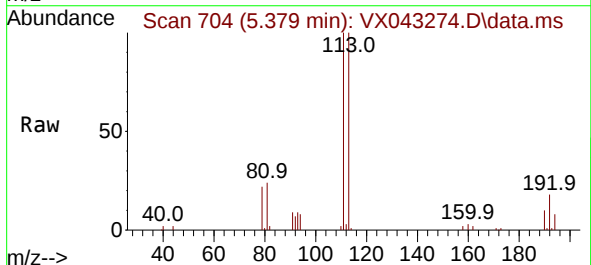


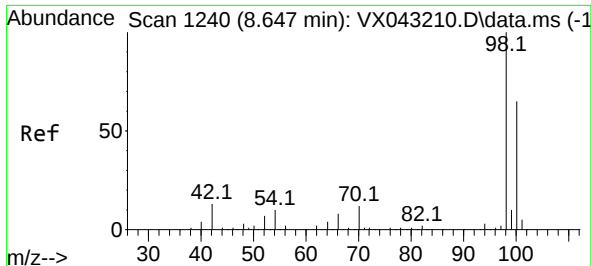

#50
Toluene-d8
Concen: 49.614 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX043274.D
Acq: 04 Oct 2024 09:24




Instrument :
MSVOA_X
ClientSampleId :
VX1004WBL01


Tgt Ion: 98 Resp: 170850
Ion Ratio Lower Upper
98 100
100 66.1 52.4 78.6

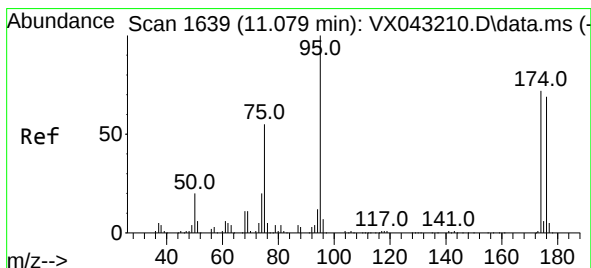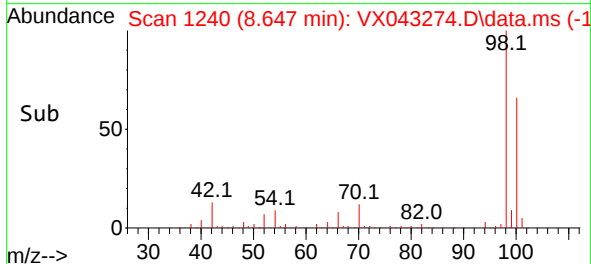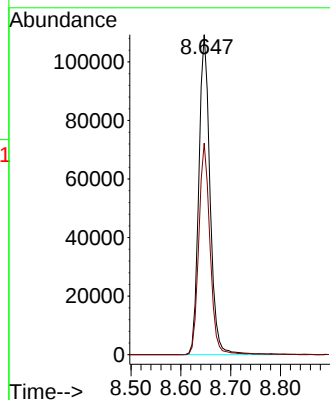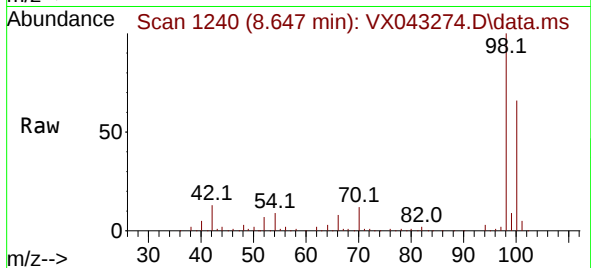

#62
4-Bromofluorobenzene
Concen: 47.894 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043274.D
Acq: 04 Oct 2024 09:24

Tgt Ion: 95 Resp: 59917
Ion Ratio Lower Upper
95 100
174 72.6 0.0 145.0
176 70.3 0.0 143.0

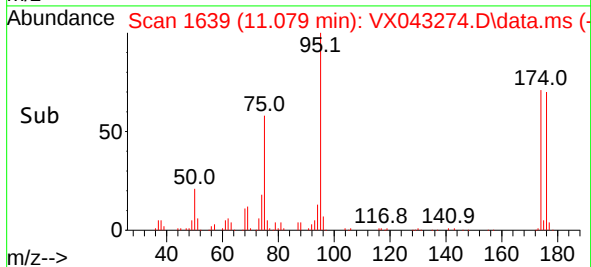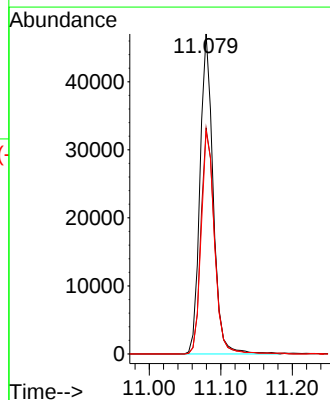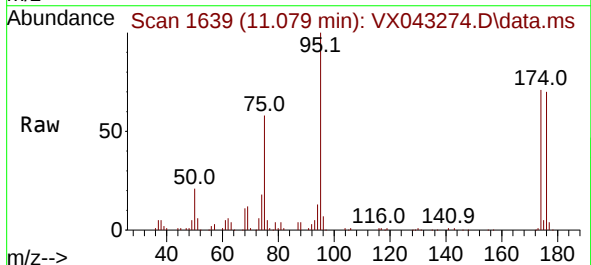

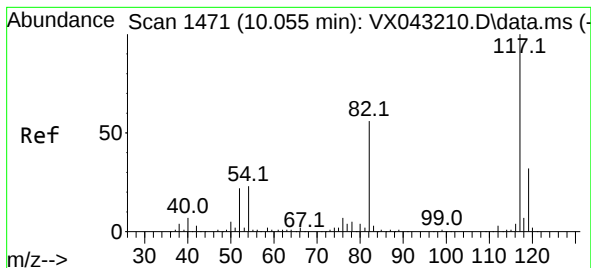

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX043274.D

Acq: 04 Oct 2024 09:24

Instrument :

MSVOA_X

ClientSampleId :

VX1004WBL01





Tgt Ion:117 Resp: 122929

Ion Ratio Lower Upper

117 100

82 56.3 45.0 67.6

119 32.0 25.3 37.9

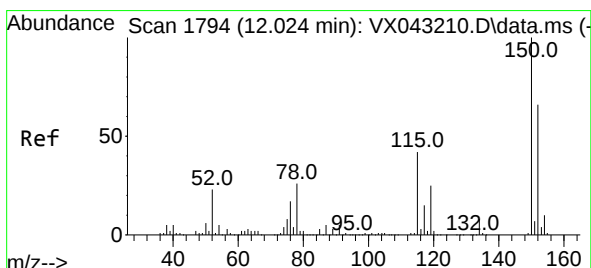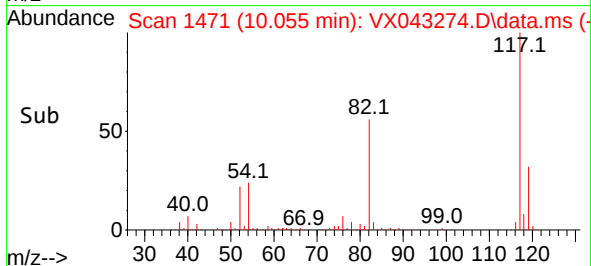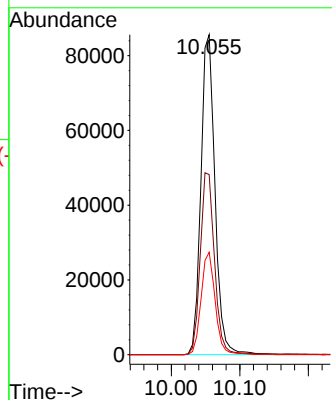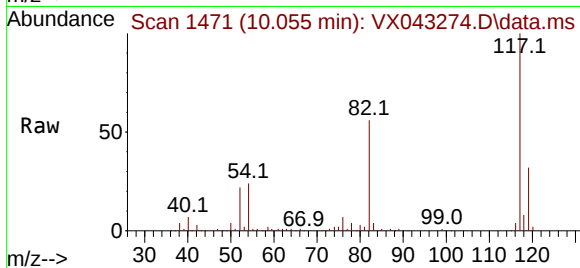

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX043274.D

Acq: 04 Oct 2024 09:24

Tgt Ion:152 Resp: 53080

Ion Ratio Lower Upper

152 100

115 61.8 44.1 132.3

150 155.5 0.0 347.4

