

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100518\
 Data File : VX005104.D
 Acq On : 06 Oct 2018 09:06
 Operator : JC/MD
 Sample : J5179-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 08 00:57:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 03 04:00:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	224746	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	322877	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	325387	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	181334	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	167588	52.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.40%	
35) Dibromofluoromethane	5.51	113	144017	52.63	ug/l	0.01
Spiked Amount	50.000		Recovery	=	105.26%	
50) Toluene-d8	8.71	98	470009	51.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.34%	
62) 4-Bromofluorobenzene	11.14	95	169562	51.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.48%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.65	94	550	0.266	ug/l #	57
6) Chloroethane	1.70	64	219	Below Cal	#	45
11) Tert butyl alcohol	3.02	59	2897	3.227	ug/l #	79
13) Acrolein	2.29	56	207	0.324	ug/l #	43
16) Acetone	2.45	43	41682	22.238	ug/l	97
18) Methyl Acetate	2.78	43	7626	1.606	ug/l	98
20) Methylene Chloride	2.86	84	35138	12.260	ug/l	93
25) 2-Butanone	4.70	43	9400	3.402	ug/l	100
29) Tetrahydrofuran	5.17	42	2652	1.544	ug/l #	85
30) Chloroform	5.21	83	1489	0.295	ug/l #	79
31) Cyclohexane	5.66	56	3884	0.951	ug/l #	1
36) 1,1-Dichloropropene	5.66	75	14001	3.750	ug/l #	47
38) Carbon Tetrachloride	5.67	117	19509	4.971	ug/l #	17
43) Isopropyl Acetate	6.46	43	167539	23.422	ug/l	96
48) Methyl methacrylate	7.88	41	12698	3.911	ug/l #	42
49) 1,4-Dioxane	7.90	88	20	0.248	ug/l #	1
51) 4-Methyl-2-Pentanone	8.65	43	1695	0.376	ug/l #	58
54) cis-1,3-Dichloropropene	8.62	75	927	0.232	ug/l #	54
56) Ethyl methacrylate	9.30	69	108	2.884	ug/l #	1
59) 2-Hexanone	9.50	43	1256	0.335	ug/l	81
70) Styrene	10.72	104	268	2.169	ug/l #	87
74) N-amyl acetate	10.92	43	260	1.788	ug/l #	25
76) 1,2,3-Trichloropropane	11.14	75	85147	20.950	ug/l #	35
80) 1,3,5-Trimethylbenzene	11.51	105	967	Below Cal		92
81) trans-1,4-Dichloro-2-buten	11.14	75	85147	56.854	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.81	105	1199	Below Cal		91
95) Naphthalene	13.83	128	17953	1.893	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100518\
Data File : VX005104.D
Acq On : 06 Oct 2018 09:06
Operator : JC/MD
Sample : J5179-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Oct 08 00:57:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 03 04:00:03 2018
Response via : Initial Calibration

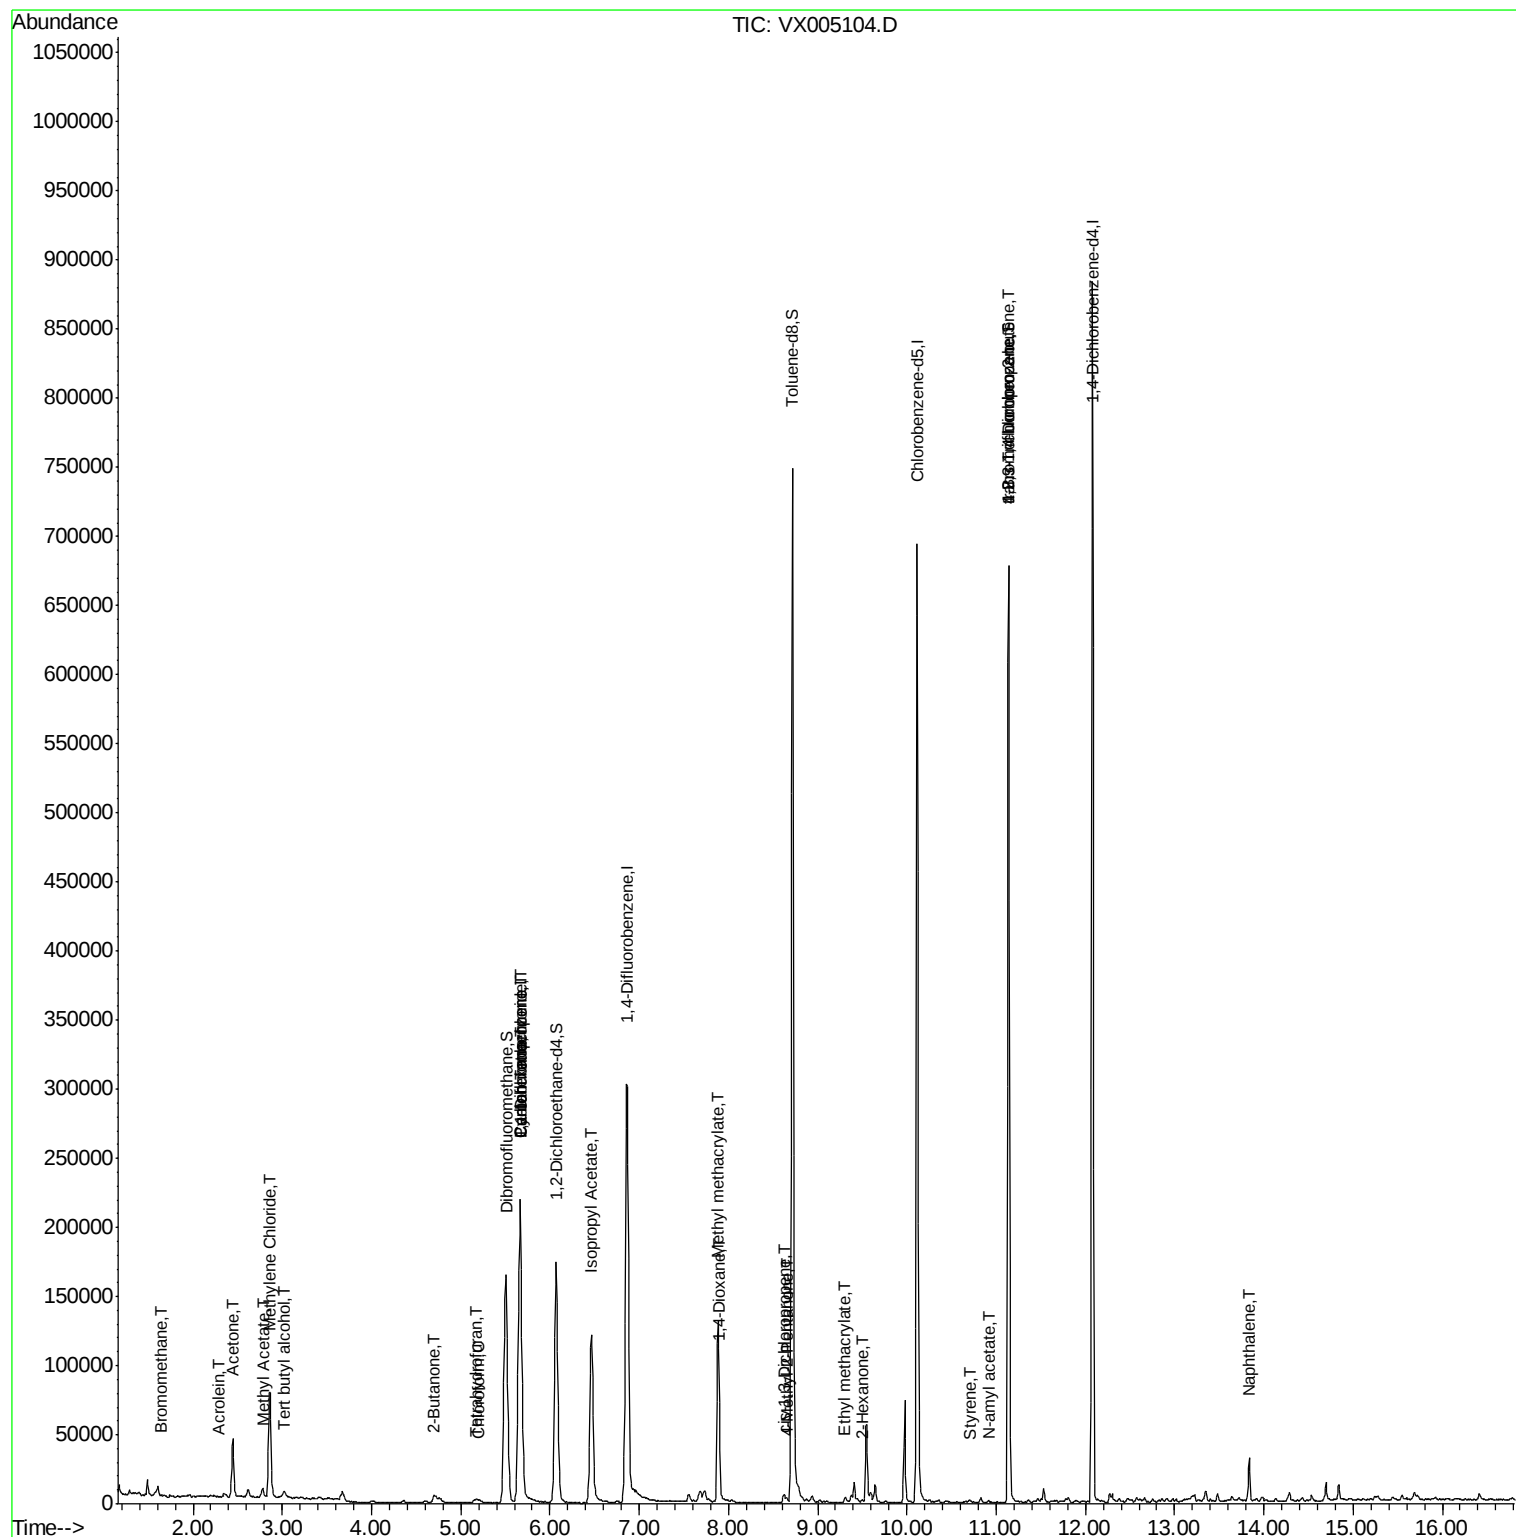



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:168 Resp: 224746

Ion Ratio Lower Upper

168 100

99 41.0 39.3 58.9

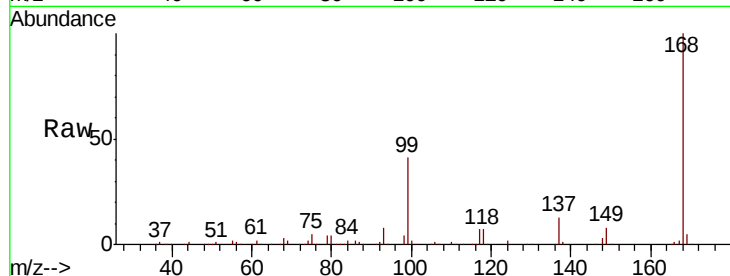

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

100000

80000

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80



#5

Bromomethane

Concen: 0.266 ug/l

RT: 1.65 min Scan# 81

Delta R.T. 0.01 min

Lab File: VX005104.D


Acq: 06 Oct 2018 09:06

Tgt Ion: 94 Resp: 550

Ion Ratio Lower Upper

94 100

96 56.4 79.5 119.3#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.65

250

200

150


100


50

0

Time-->

1.60 1.65 1.70



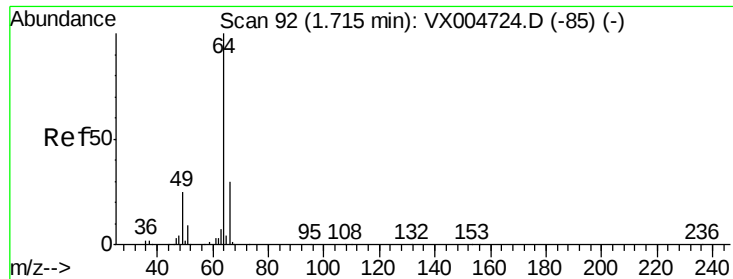

#6

Chloroethane

Concen: Below Cal

RT: 1.70 min Scan# 89

Delta R.T. -0.02 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06





Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 64 Resp: 219

Ion Ratio Lower Upper

64 100

66 0.0 23.8 35.6#

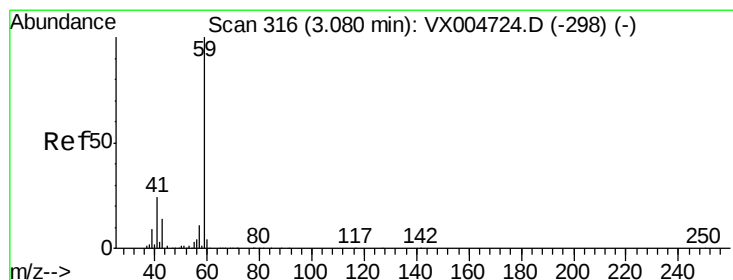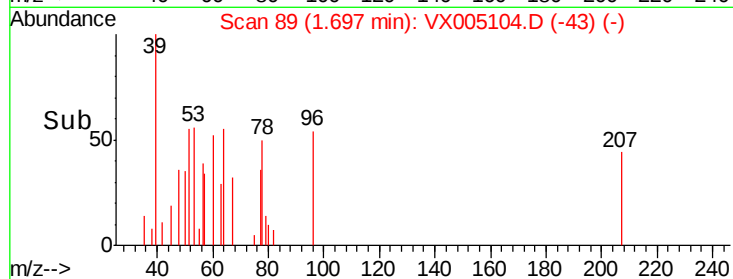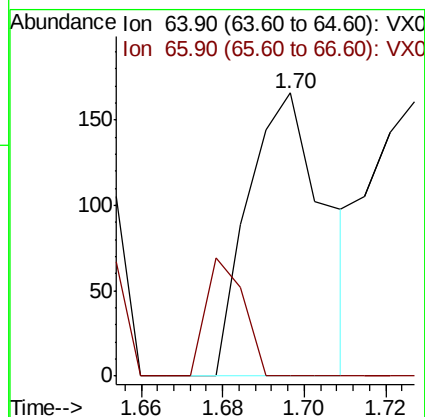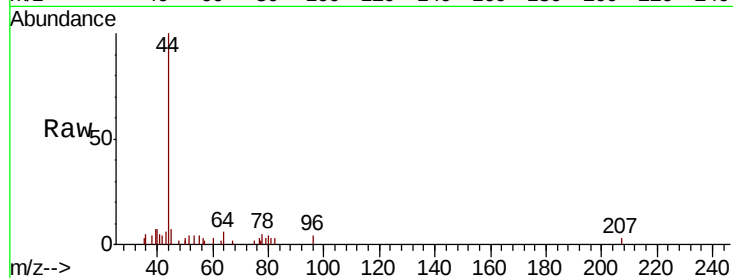

#11

Tert butyl alcohol

Concen: 3.227 ug/l

RT: 3.02 min Scan# 306

Delta R.T. -0.06 min

Lab File: VX005104.D




Acq: 06 Oct 2018 09:06


Tgt Ion: 59 Resp: 2897

Ion Ratio Lower Upper

59 100

57 2.7 8.6 12.8#

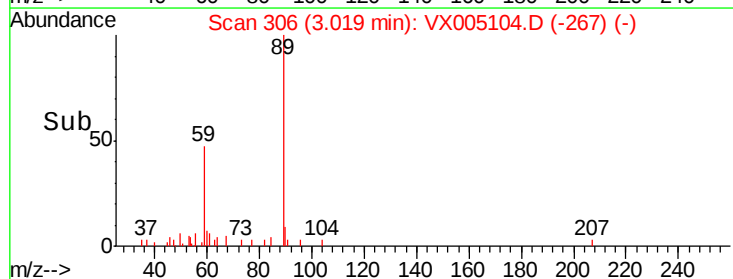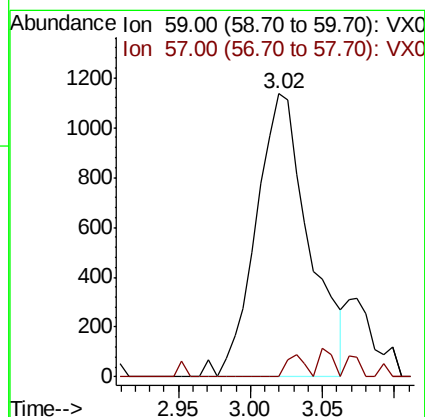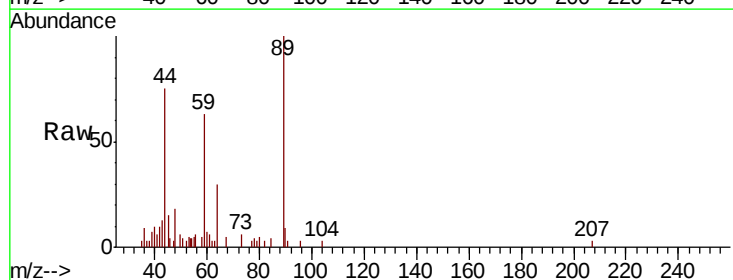

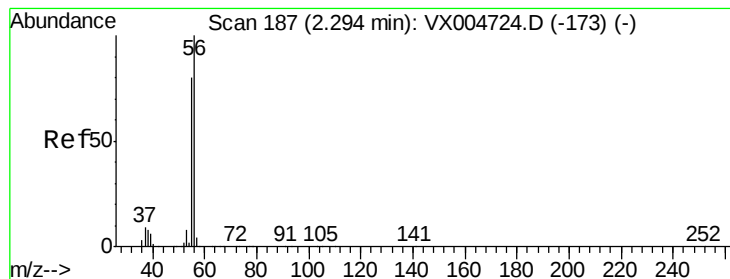

#13

Acrolein

Concen: 0.324 ug/l

RT: 2.29 min Scan# 187

Delta R.T. 0.00 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06


Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 56 Resp: 207

Ion Ratio Lower Upper




56 100

55 29.5 63.4 95.2#

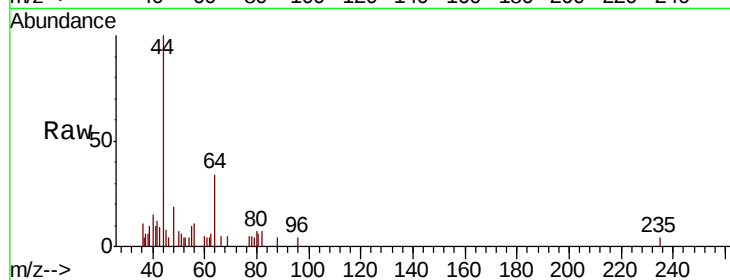

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

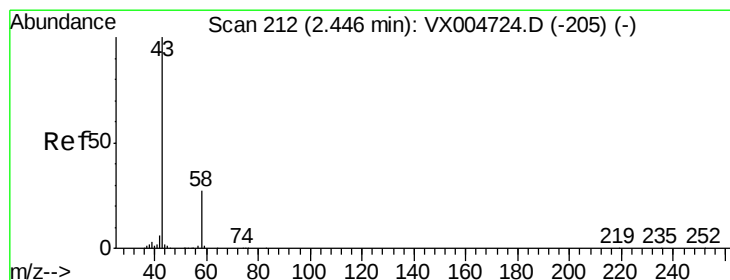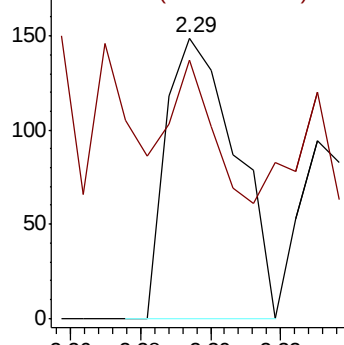

#16

Acetone

Concen: 22.238 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX005104.D


Acq: 06 Oct 2018 09:06

Tgt Ion: 43 Resp: 41682

Ion Ratio Lower Upper



43 100


58 28.7 21.8 32.6

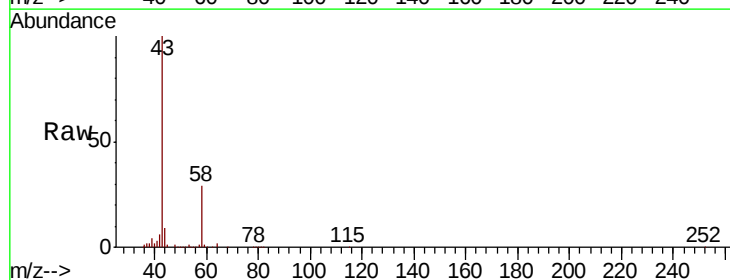

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



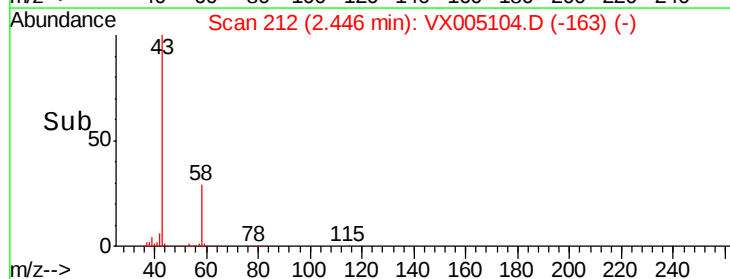
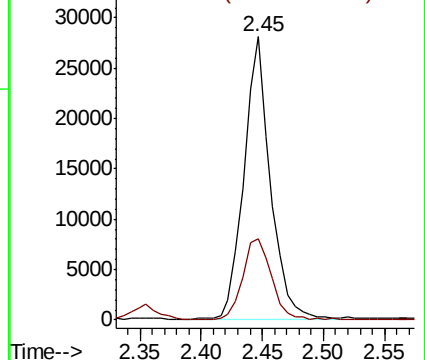




#18
Methvl Acetate
Concen: 1.606 ug/l
RT: 2.78 min Scan# 266
Delta R.T. -0.01 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 7626
Ion Ratio Lower Upper
43 100
74 23.1 17.8 26.8

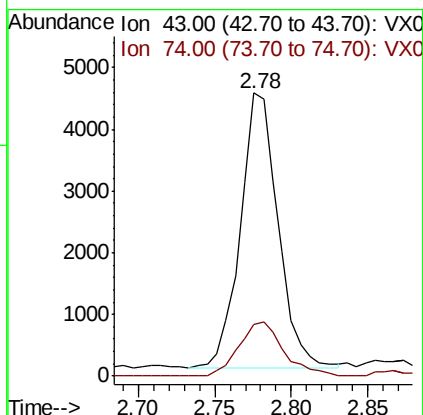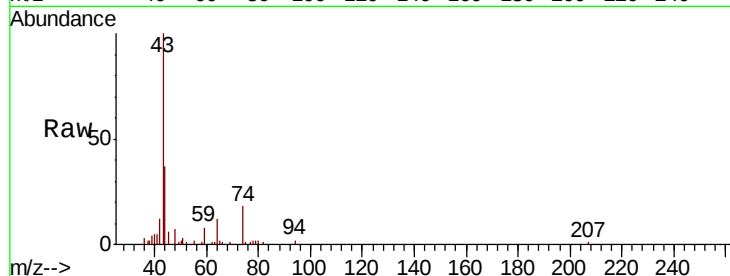

#20
Methylene Chloride
Concen: 12.260 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.01 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Tgt Ion: 84 Resp: 35138
Ion Ratio Lower Upper
84 100
49 110.4 92.3 138.5
51 34.2 31.8 47.6
86 53.4 48.5 72.7



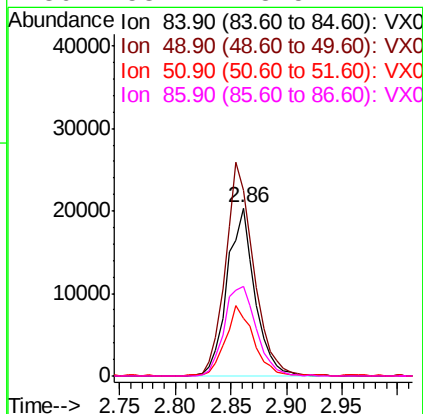



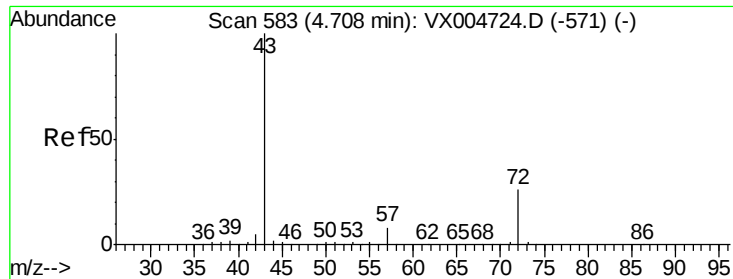

#25
 2-Butanone
 Concen: 3.402 ug/l
 RT: 4.70 min Scan# 582
 Delta R.T. -0.01 min
 Lab File: VX005104.D
 Acq: 06 Oct 2018 09:06




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 43 Resp: 9400
 Ion Ratio Lower Upper
 43 100
 72 25.9 20.8 31.2

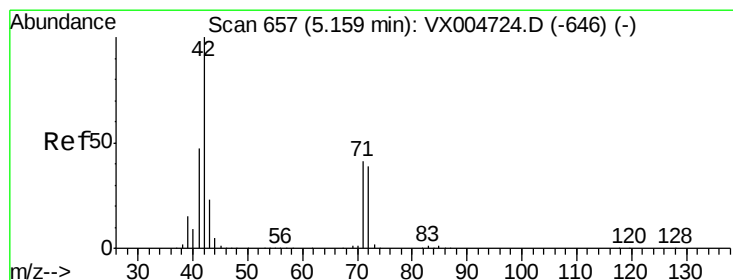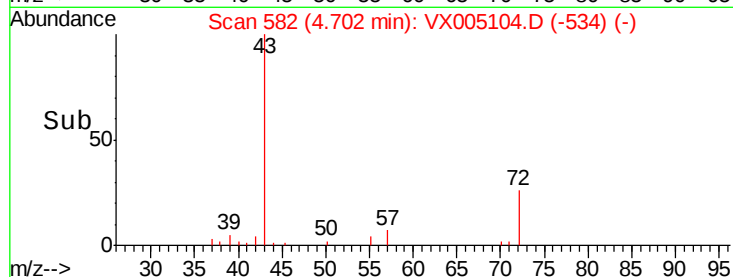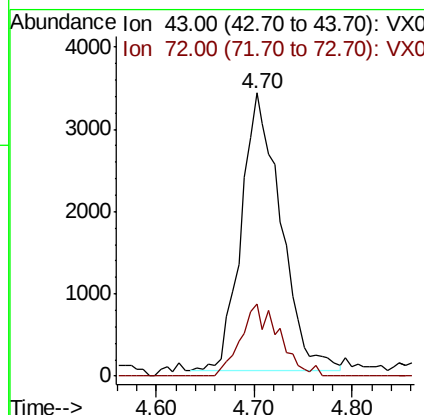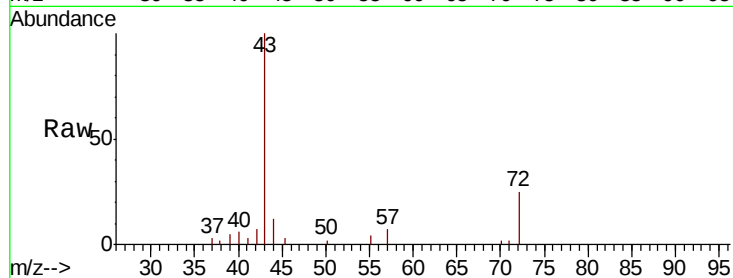

#29
 Tetrahydrofuran
 Concen: 1.544 ug/l
 RT: 5.17 min Scan# 658
 Delta R.T. 0.01 min
 Lab File: VX005104.D
 Acq: 06 Oct 2018 09:06

Tgt Ion: 42 Resp: 2652
 Ion Ratio Lower Upper
 42 100
 72 40.8 33.7 50.5
 71 22.6 32.2 48.4#


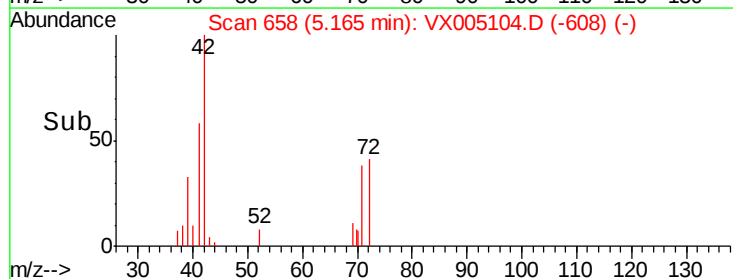
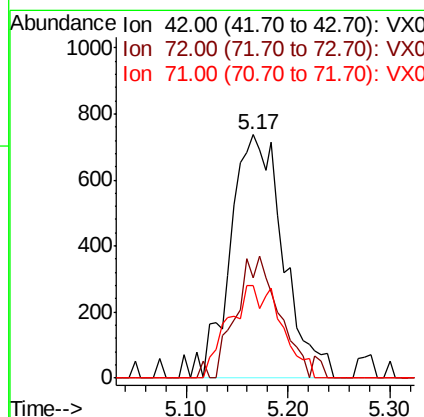
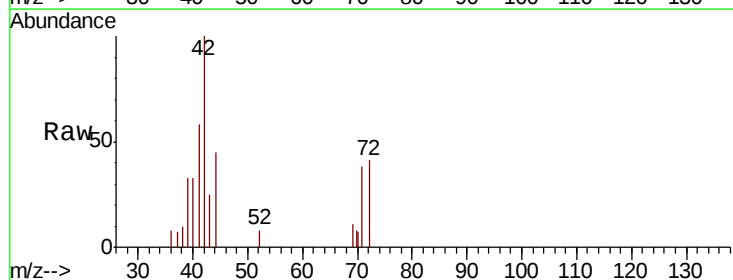




#30
Chloroform
Concen: 0.295 ug/l
RT: 5.21 min Scan# 665
Delta R.T. -0.01 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 83 Resp: 1489
Ion Ratio Lower Upper
83 100
85 49.0 52.4 78.6#

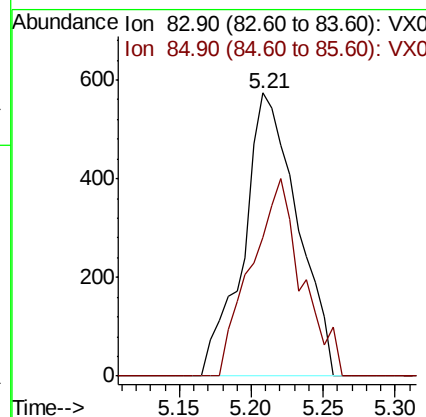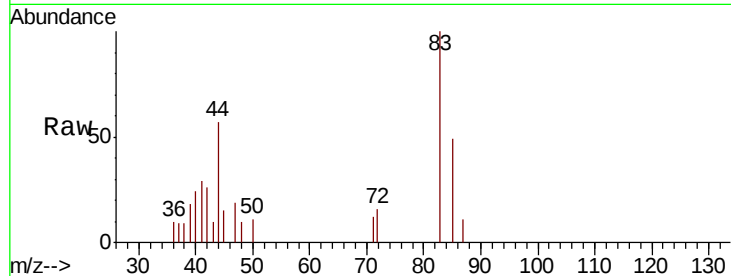

#31
Cyclohexane
Concen: 0.951 ug/l
RT: 5.66 min Scan# 739
Delta R.T. 0.09 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Tgt Ion: 56 Resp: 3884
Ion Ratio Lower Upper
56 100
69 185.9 25.9 38.9#
84 135.5 71.9 107.9#

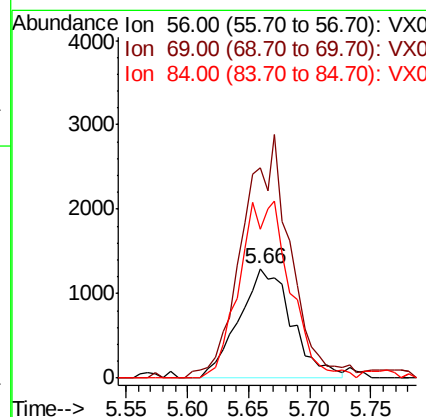

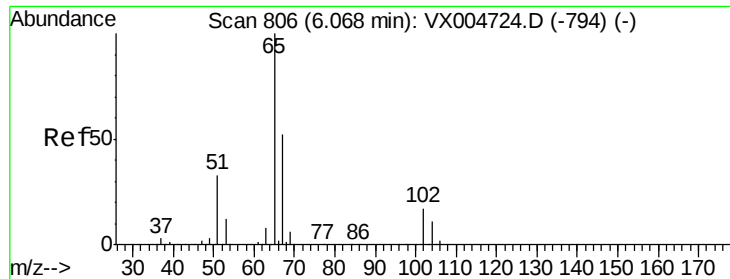

#33

1,2-Dichloroethane-d4

Concen: 52.200 ug/l

RT: 6.07 min Scan# 807

Delta R.T. 0.01 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 65 Resp: 167588

Ion Ratio Lower Upper




65 100

67 51.8 0.0 107.4

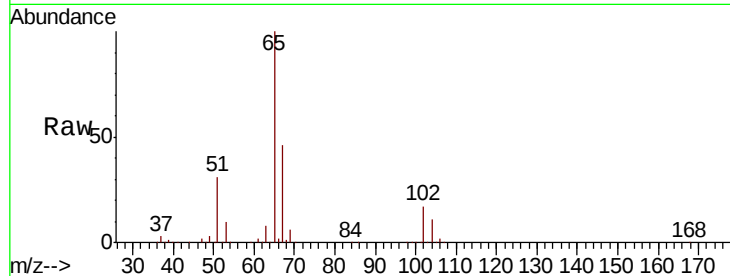

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

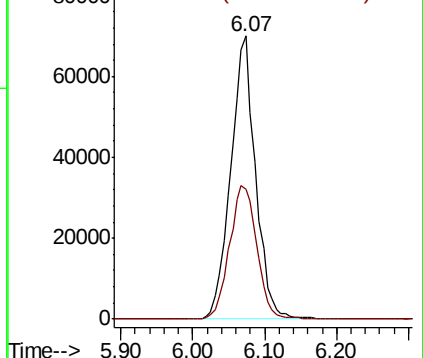

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.87 min Scan# 937

Delta R.T. 0.01 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06


Tgt Ion: 114 Resp: 322877

Ion Ratio Lower Upper

114 100

63 22.2 0.0 39.8



88 15.4 0.0 27.0




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

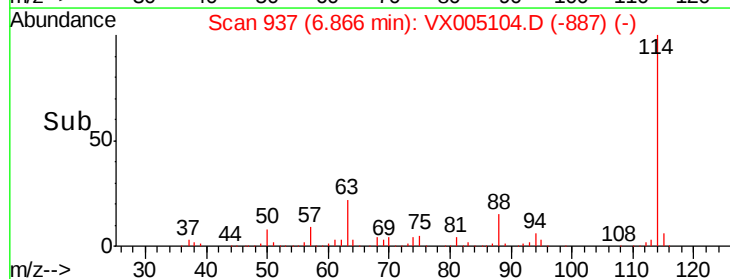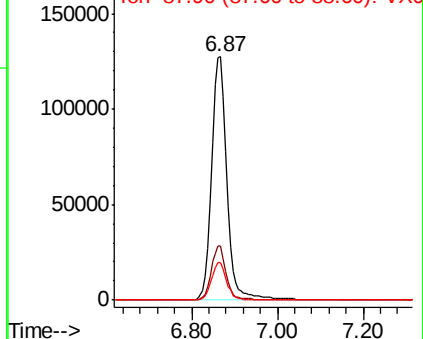



#35

Dibromofluoromethane

Concen: 52.630 ug/l

RT: 5.51 min Scan# 715

Delta R.T. 0.01 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:113 Resp: 144017

Ion Ratio Lower Upper

113 100

111 100.9 77.0 115.4




192 24.4 17.0 25.6



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

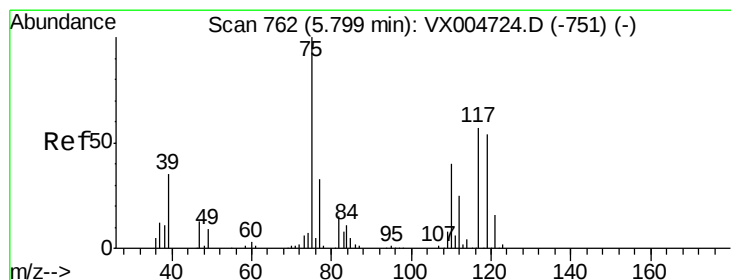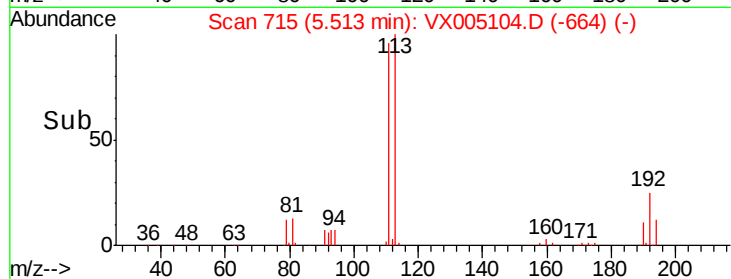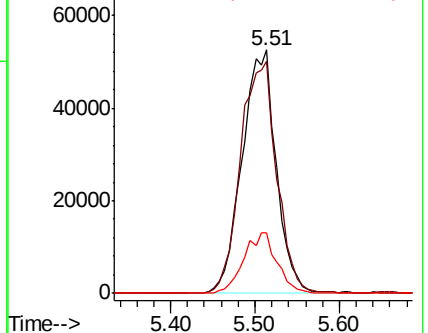

#36

1,1-Dichloropropene

Concen: 3.750 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06


Tgt Ion: 75 Resp: 14001

Ion Ratio Lower Upper

75 100

110 10.2 20.0 59.9#



77 0.0 27.1 40.7#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

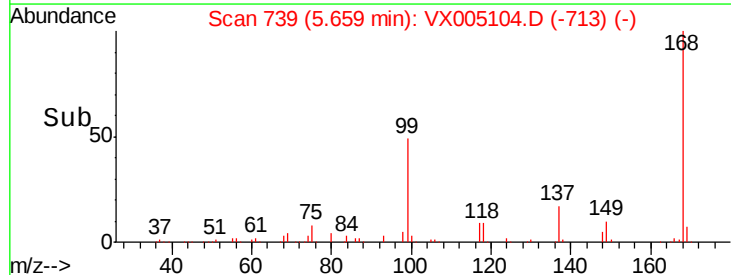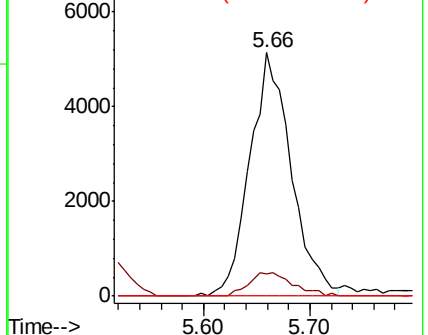

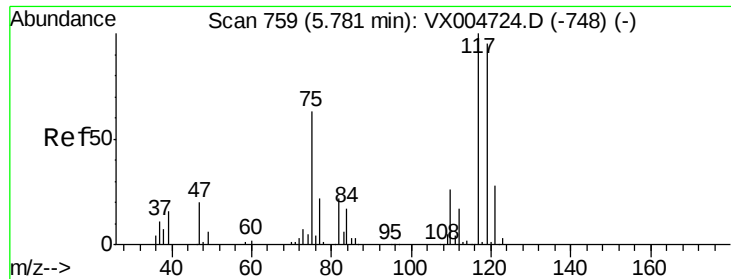

#38

Carbon Tetrachloride

Concen: 4.971 ug/l

RT: 5.67 min Scan# 741

Delta R.T. -0.11 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:117 Resp: 19509

Ion Ratio Lower Upper

117 100

119 5.7 75.2 112.8#




121 0.0 22.5 33.7#

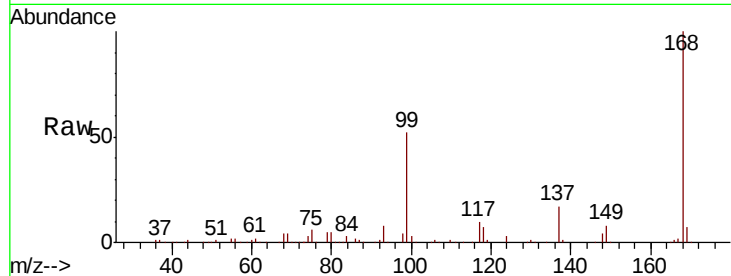

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

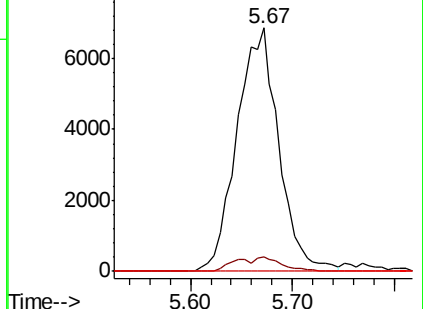

#43

Isopropyl Acetate

Concen: 23.422 ug/l

RT: 6.46 min Scan# 871

Delta R.T. 0.00 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06


Tgt Ion: 43 Resp: 167539

Ion Ratio Lower Upper

43 100

61 19.9 14.2 21.4



87 12.6 9.3 13.9




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

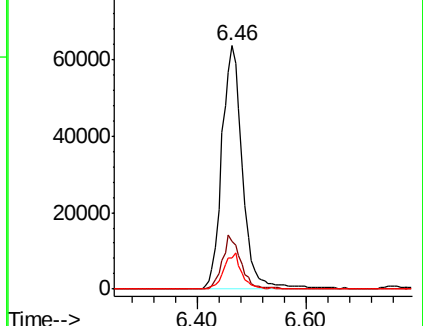







#48
Methyl methacrylate
Concen: 3.911 ug/l
RT: 7.88 min Scan# 1104
Delta R.T. 0.10 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Instrument :
MSVOA_X
ClientSampled :

Tot Ion: 41 Resp: 12698
Ion Ratio Lower Upper
41 100
69 0.1 63.8 95.6#
39 55.8 40.7 61.1




Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0


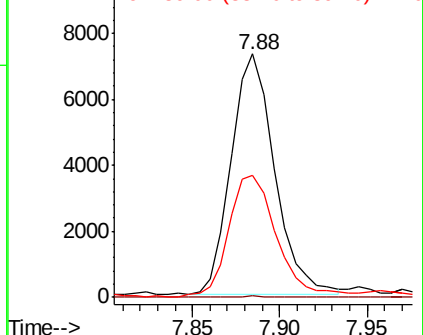



#49
1,4-Dioxane
Concen: 0.248 ug/l
RT: 7.90 min Scan# 1107
Delta R.T. 0.15 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Tgt Ion: 88 Resp: 20
Ion Ratio Lower Upper
88 100
43 611970.0 25.1 37.7#
58 6485.0 56.2 84.2#



Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0

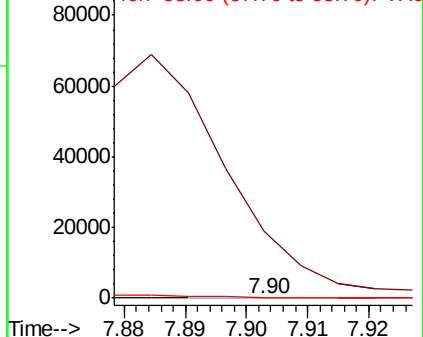

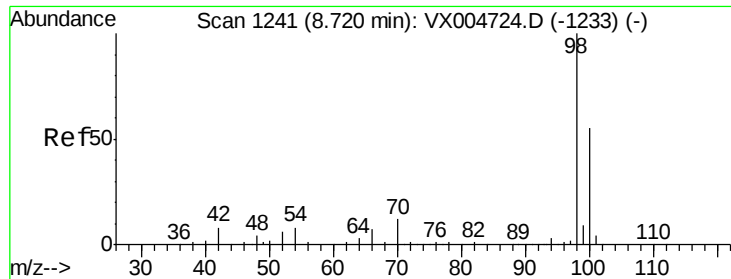

#50

Toluene-d8

Concen: 51.665 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.01 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 98 Resp: 470009

Ion Ratio Lower Upper

98 100

100 63.0 51.9 77.9



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

8.71



300000

200000

100000

0

Time-->

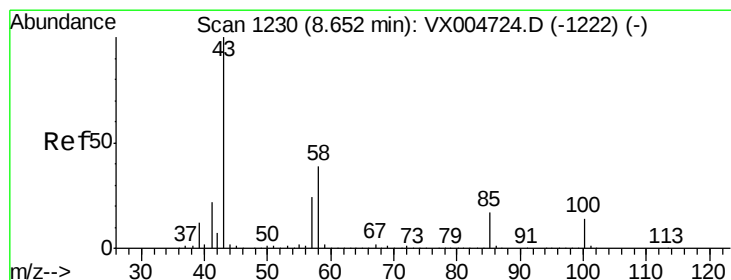

#51

4-Methyl-2-Pentanone

Concen: 0.376 ug/l

RT: 8.65 min Scan# 1230

Delta R.T. 0.00 min

Lab File: VX005104.D


Acq: 06 Oct 2018 09:06

Tgt Ion: 43 Resp: 1695

Ion Ratio Lower Upper

43 100

58 63.2 30.5 45.7#

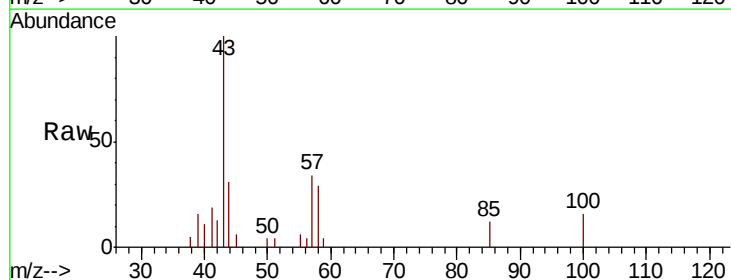

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

8.65


1500


1000

500

0

Time-->

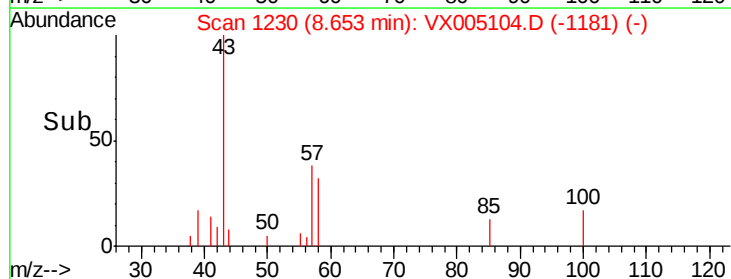







#54

cis-1,3-Dichloropropene
Concen: 0.232 ug/l
RT: 8.62 min Scan# 1224
Delta R.T. 0.18 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Instrument :
MSVOA_X
ClientSampleId :




Tot Ion: 75 Resp: 927
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#
39 21.6 38.3 57.5#

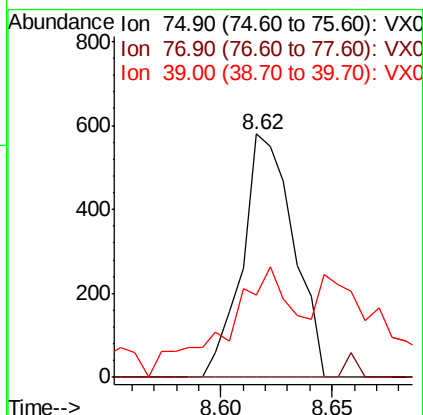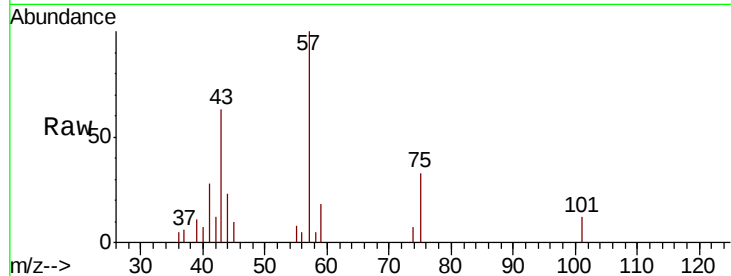


#56

Ethyl methacrylate
Concen: 2.884 ug/l
RT: 9.30 min Scan# 1336
Delta R.T. 0.12 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Tgt Ion: 69 Resp: 108
Ion Ratio Lower Upper
69 100
41 849.1 56.9 85.3#
39 442.6 28.4 42.6#



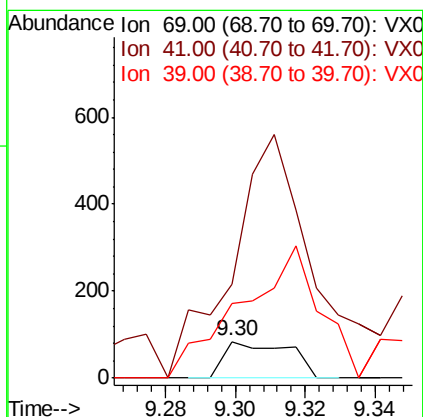
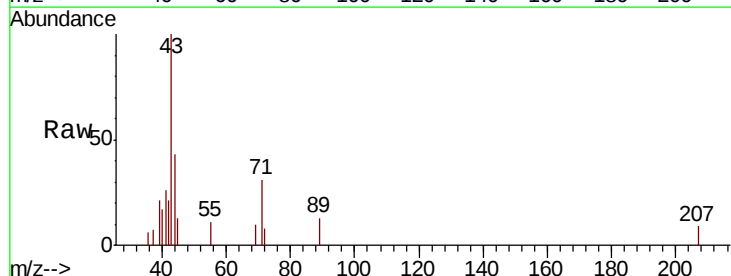




#59
2-Hexanone
Concen: 0.335 ug/l
RT: 9.50 min Scan# 1369
Delta R.T. 0.00 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 43 Resp: 1256
Ion Ratio Lower Upper
43 100
58 43.2 28.4 85.3

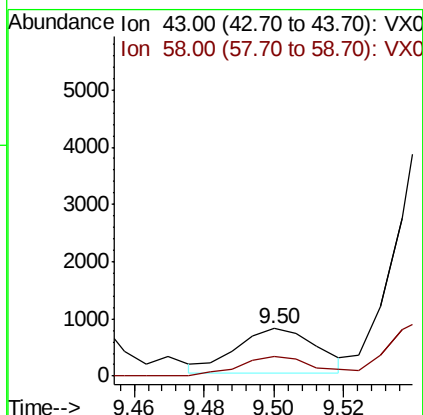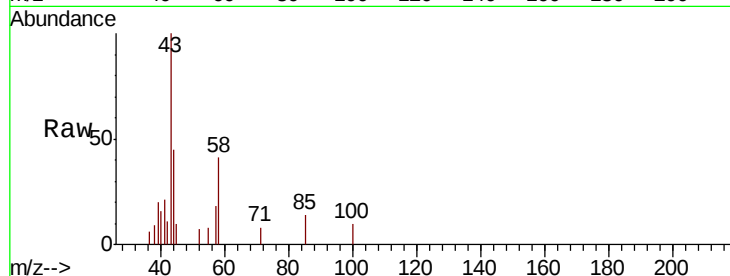

#62
4-Bromofluorobenzene
Concen: 51.738 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. 0.00 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Tgt Ion: 95 Resp: 169562
Ion Ratio Lower Upper
95 100
174 93.8 0.0 185.0
176 90.0 0.0 180.2

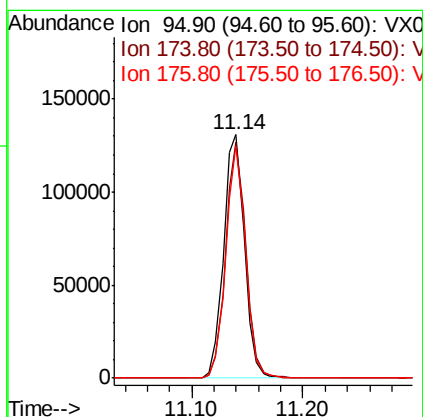


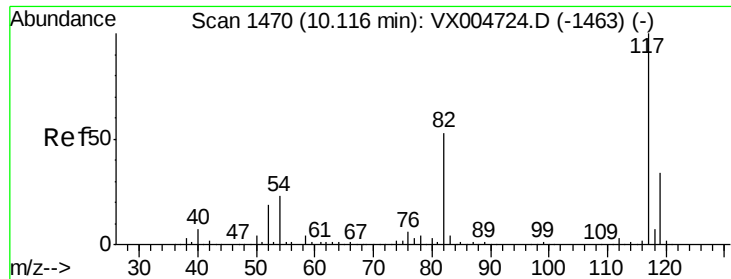




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.00 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:117 Resp: 325387
Ion Ratio Lower Upper
117 100
82 54.1 42.2 63.4
119 32.6 27.4 41.0

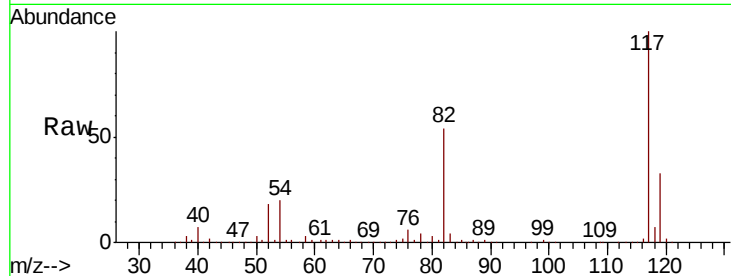


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

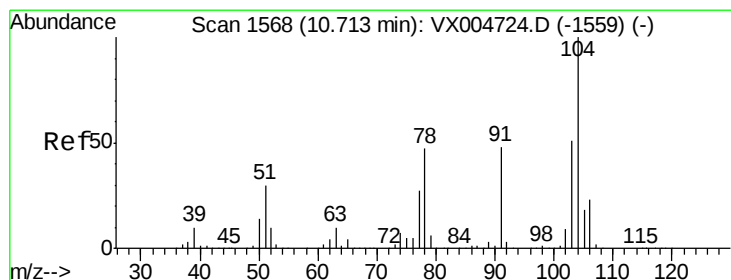
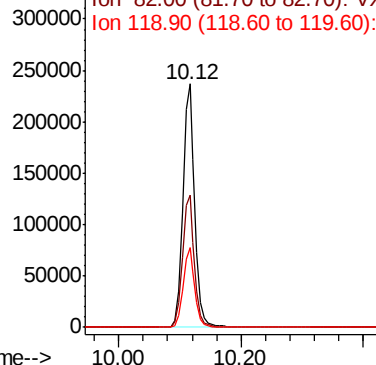



#70
Styrene
Concen: 2.169 ug/l
RT: 10.72 min Scan# 1569
Delta R.T. 0.01 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Tgt Ion:104 Resp: 268
Ion Ratio Lower Upper
104 100
78 56.3 40.0 60.0
103 67.2 44.3 66.5#



Abundance Ion 104.00 (103.70 to 104.70): V
Ion 78.00 (77.70 to 78.70): VX0
Ion 103.00 (102.70 to 103.70): V

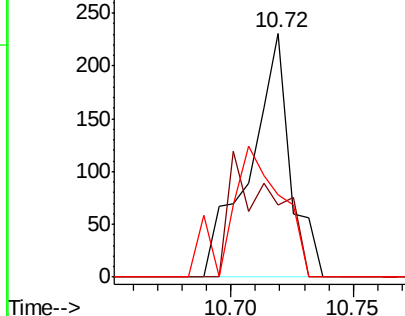



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:152 Resp: 181334

Ion Ratio Lower Upper

152 100

115 55.5 40.2 120.6




150 156.5 0.0 351.0



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

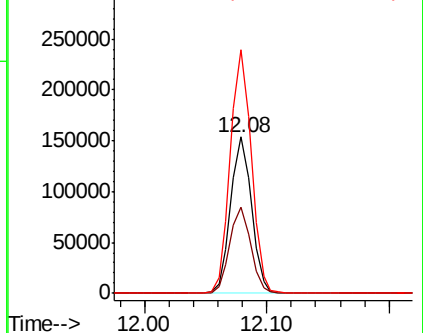

#74

N-ethyl acetate

Concen: 1.788 ug/l

RT: 10.92 min Scan# 1602

Delta R.T. 0.02 min

Lab File: VX005104.D

Acq: 06 Oct 2018 09:06

Tgt Ion: 43 Resp: 260


Ion Ratio Lower Upper

43 100

70 80.0 32.6 48.8#

55 86.9 21.6 32.4#

61 0.0 19.1 28.7#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0




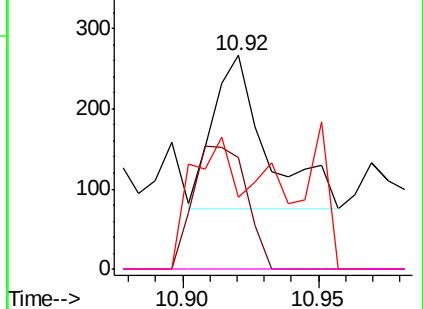


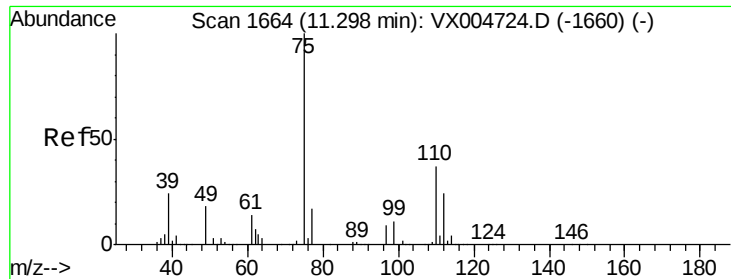

#76
 1,2,3-Trichloropropane
 Concen: 20.950 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. -0.16 min
 Lab File: VX005104.D
 Acq: 06 Oct 2018 09:06




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 75 Resp: 85147
 Ion Ratio Lower Upper
 75 100
 77 1.2 21.4 64.3#

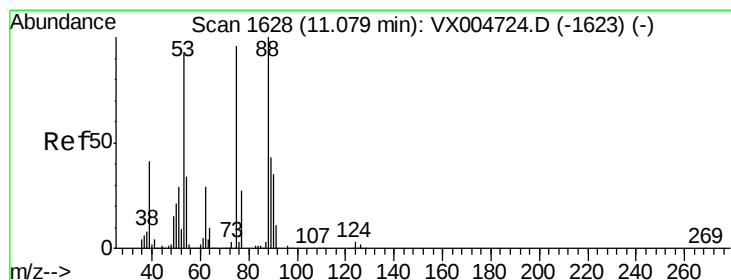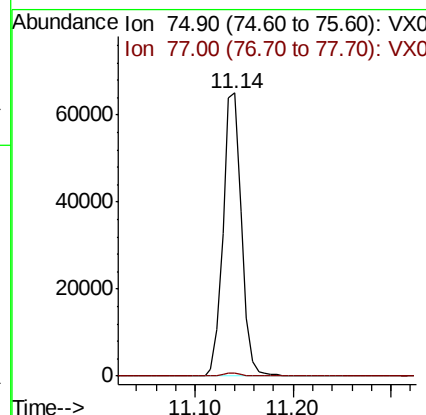

#81
 trans-1,4-Dichloro-2-butene
 Concen: 56.854 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. 0.06 min
 Lab File: VX005104.D
 Acq: 06 Oct 2018 09:06

Tgt Ion: 75 Resp: 85147
 Ion Ratio Lower Upper
 75 100
 53 0.3 80.2 120.4#
 89 0.0 37.1 55.7#

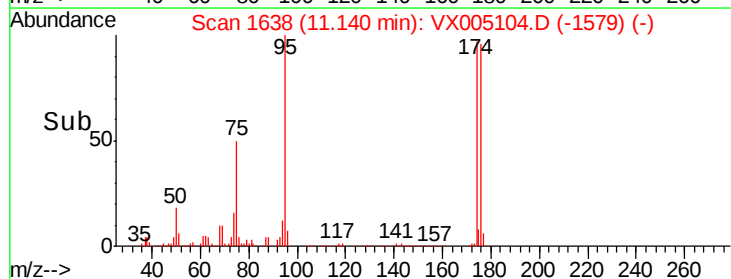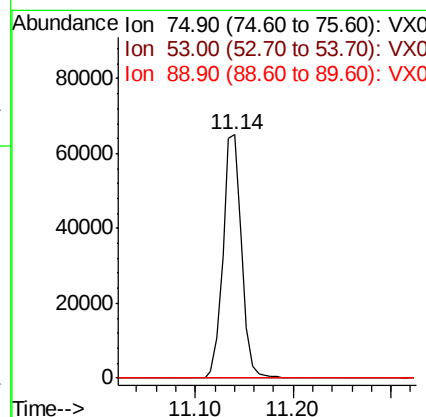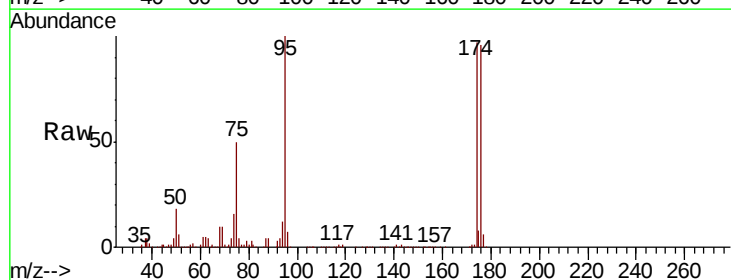


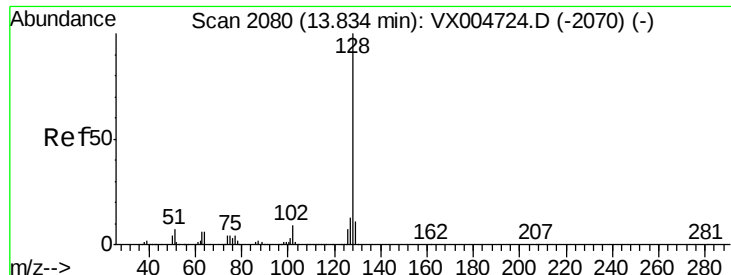

#95
Naphthalene
Concen: 1.893 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. 0.00 min
Lab File: VX005104.D
Acq: 06 Oct 2018 09:06

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.4	10.4	15.6
129	10.7	8.7	13.1



Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

