

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100518\
 Data File : VX005106.D
 Acq On : 06 Oct 2018 09:59
 Operator : JC/MD
 Sample : J5238-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Oct 08 00:58:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 03 04:00:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	221243	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	329262	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	321508	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	189864	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	163495	51.73	ug/l	0.00
Spiked Amount			Recovery	=	103.46%	
35) Dibromofluoromethane	5.51	113	152149	54.52	ug/l	0.00
Spiked Amount			Recovery	=	109.04%	
50) Toluene-d8	8.72	98	469310	50.59	ug/l	0.00
Spiked Amount			Recovery	=	101.18%	
62) 4-Bromofluorobenzene	11.14	95	171727	51.38	ug/l	0.00
Spiked Amount			Recovery	=	102.76%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.65	94	453	0.223	ug/l #	78
6) Chloroethane	1.71	64	46	Below Cal	#	45
11) Tert butyl alcohol	3.03	59	3216	3.639	ug/l #	73
16) Acetone	2.45	43	74509	40.381	ug/l #	89
18) Methyl Acetate	2.78	43	9873	2.112	ug/l	99
20) Methylene Chloride	2.85	84	6858	1.746	ug/l	91
25) 2-Butanone	4.70	43	7241	2.662	ug/l	96
29) Tetrahydrofuran	5.17	42	2270	1.343	ug/l	91
30) Chloroform	5.21	83	8296	1.671	ug/l	84
36) 1,1-Dichloropropene	5.66	75	15003	3.941	ug/l #	45
37) Ethyl Acetate	4.70	43	7241	1.433	ug/l #	70
38) Carbon Tetrachloride	5.67	117	19878	4.967	ug/l #	18
43) Isopropyl Acetate	6.46	43	101505	13.915	ug/l	97
47) Bromodichloromethane	7.90	83	1619	0.471	ug/l	100
48) Methyl methacrylate	7.69	41	1511	0.456	ug/l #	21
51) 4-Methyl-2-Pentanone	8.65	43	930	0.202	ug/l #	47
56) Ethyl methacrylate	9.38	69	86	2.879	ug/l #	1
69) o-Xylene	10.70	106	2805	0.597	ug/l	97
70) Styrene	10.69	104	336	2.177	ug/l #	1
74) N-amyl acetate	10.87	43	107	1.764	ug/l #	53
76) 1,2,3-Trichloropropane	11.14	75	85797	20.161	ug/l #	35
80) 1,3,5-Trimethylbenzene	11.51	105	8909	0.617	ug/l	98
81) trans-1,4-Dichloro-2-buten	11.14	75	85797	54.789	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.81	105	10891	0.768	ug/l	98
90) Hexachloroethane	12.61	117	506	0.279	ug/l #	1
95) Naphthalene	13.83	128	8928	1.277	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100518\
Data File : VX005106.D
Acq On : 06 Oct 2018 09:59
Operator : JC/MD
Sample : J5238-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Oct 08 00:58:06 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 03 04:00:03 2018
Response via : Initial Calibration

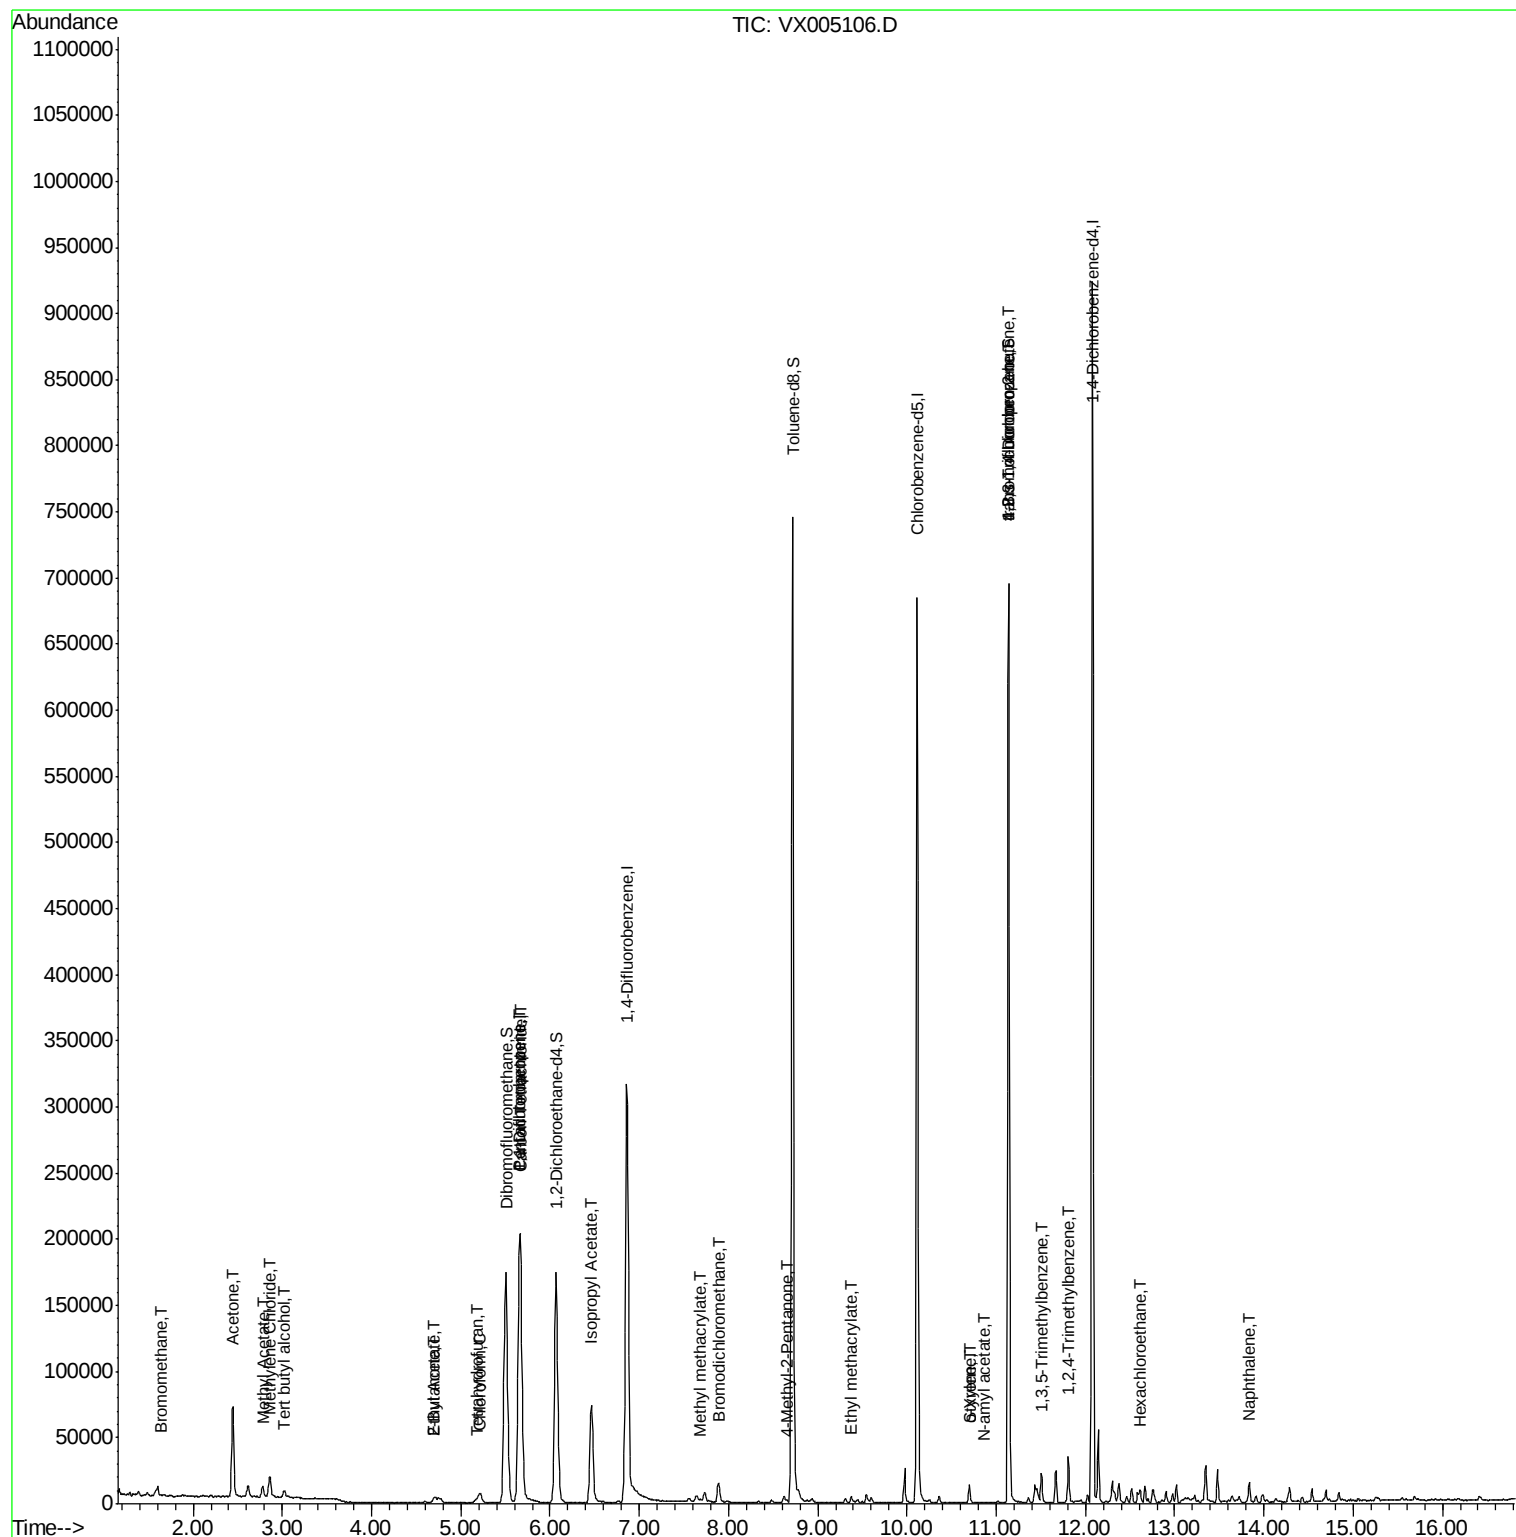



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:168 Resp: 221243

Ion Ratio Lower Upper

168 100

99 50.2 39.3 58.9

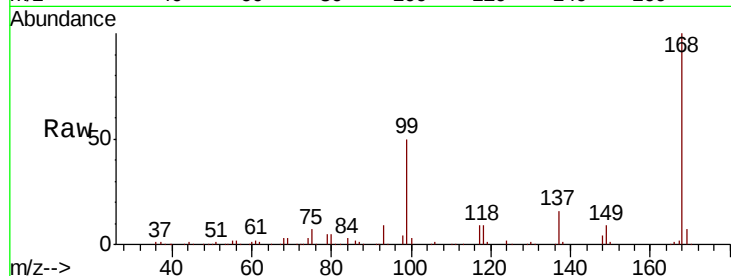

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#5

Bromomethane

Concen: 0.223 ug/l

RT: 1.65 min Scan# 81

Delta R.T. 0.01 min

Lab File: VX005106.D


Acq: 06 Oct 2018 09:59

Tgt Ion: 94 Resp: 453

Ion Ratio Lower Upper

94 100

96 77.2 79.5 119.3#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.65

200


150


100

50

0

Time--> 1.60 1.65 1.70



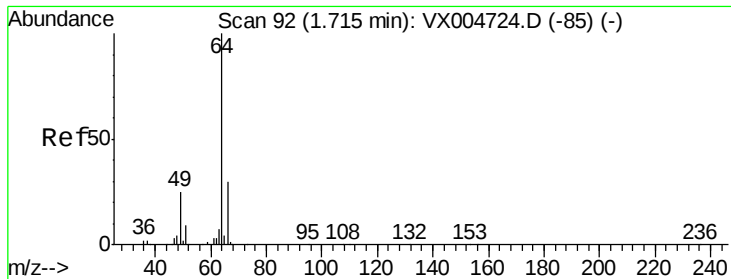

#6

Chloroethane

Concen: Below Cal

RT: 1.71 min Scan# 92

Delta R.T. -0.00 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 64 Resp: 46

Ion Ratio Lower Upper

64 100

66 0.0 23.8 35.6#

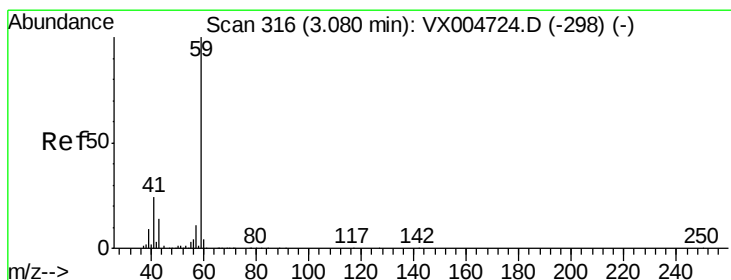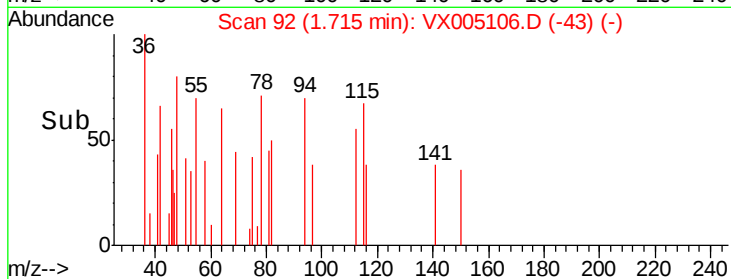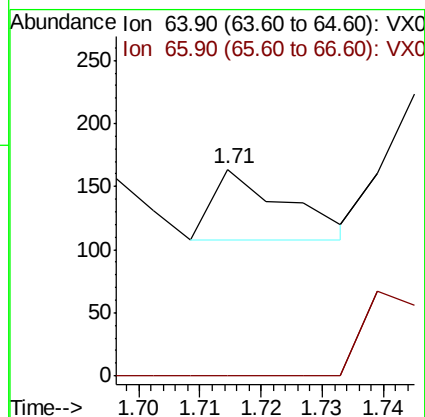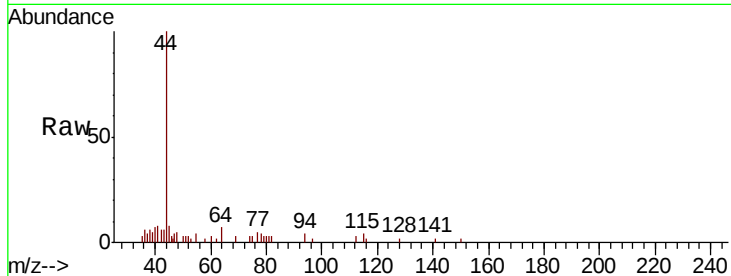

#11

Tert butyl alcohol

Concen: 3.639 ug/l

RT: 3.03 min Scan# 307

Delta R.T. -0.05 min

Lab File: VX005106.D




Acq: 06 Oct 2018 09:59


Tgt Ion: 59 Resp: 3216

Ion Ratio Lower Upper

59 100

57 0.6 8.6 12.8#



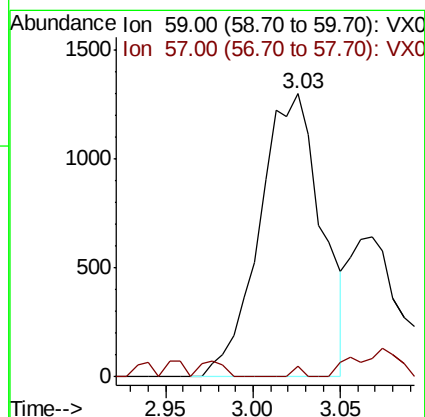





#16
Acetone
Concen: 40.381 ug/l
RT: 2.45 min Scan# 212
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 74509
Ion Ratio Lower Upper
43 100
58 32.7 21.8 32.6#

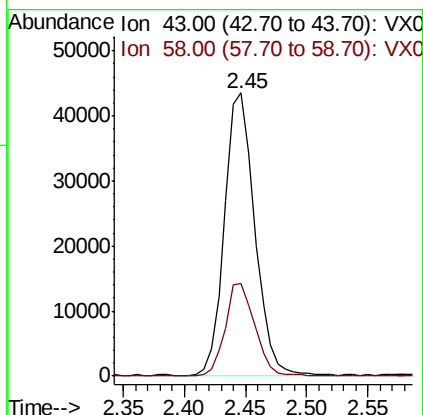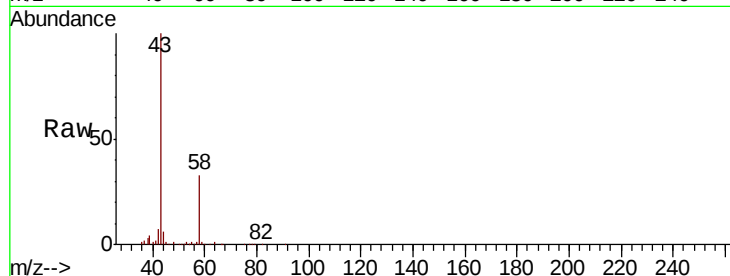

#18
Methyl Acetate
Concen: 2.112 ug/l
RT: 2.78 min Scan# 267
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion: 43 Resp: 9873
Ion Ratio Lower Upper
43 100
74 21.9 17.8 26.8


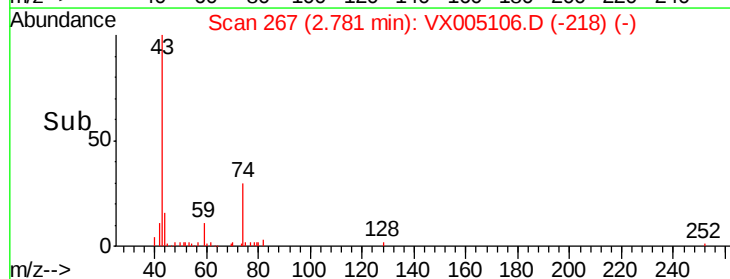
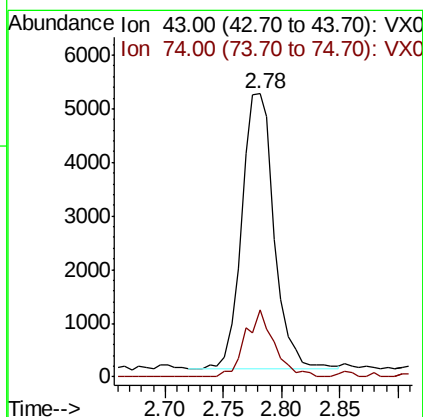





#20
Methvlene Chloride
Concen: 1.746 ug/l
RT: 2.85 min Scan# 279
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:	84	Resp:	6858
Ion	Ratio	Lower	Upper
84	100		
49	131.2	92.3	138.5
51	41.7	31.8	47.6
86	62.5	48.5	72.7

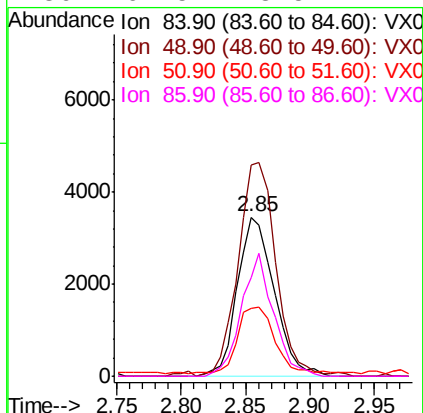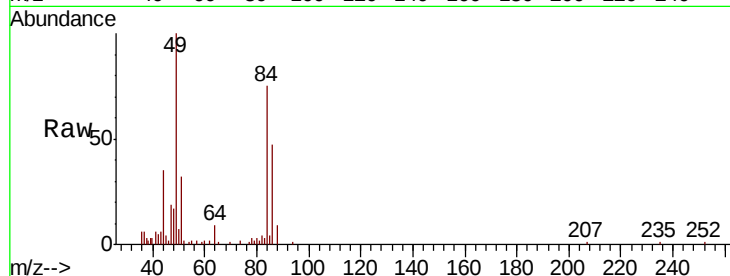

#25
2-Butanone
Concen: 2.662 ug/l
RT: 4.70 min Scan# 582
Delta R.T. -0.01 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion:	43	Resp:	7241
Ion	Ratio	Lower	Upper
43	100		
72	24.2	20.8	31.2

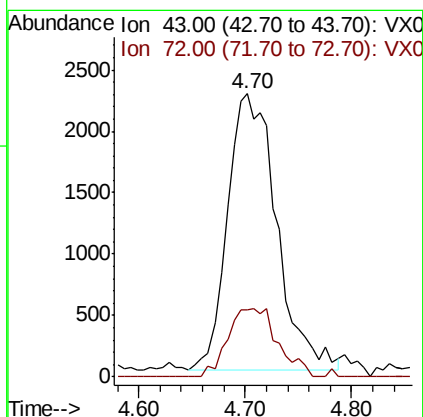

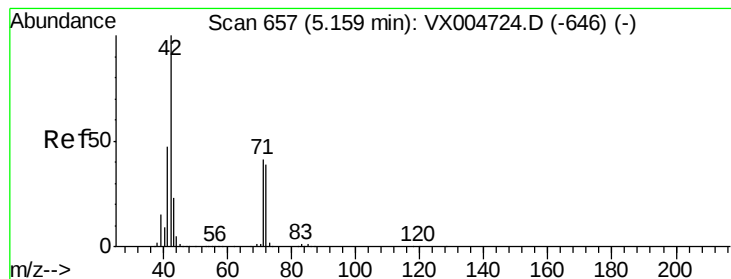

#29

Tetrahydrofuran

Concen: 1.343 ug/l

RT: 5.17 min Scan# 659

Delta R.T. 0.01 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 42 Resp: 2270

Ion Ratio Lower Upper




42 100

72 45.6 33.7 50.5

71 32.9 32.2 48.4



Abundance Ion 42.00 (41.70 to 42.70): VX0
Ion 72.00 (71.70 to 72.70): VX0
Ion 71.00 (70.70 to 71.70): VX0

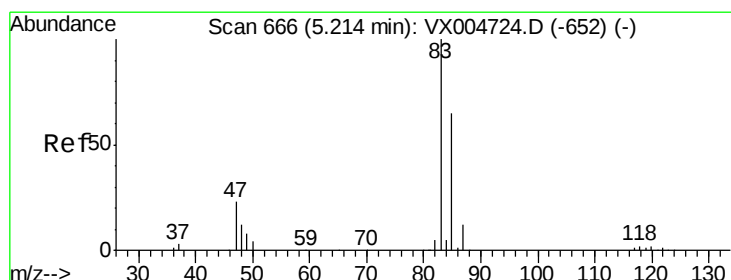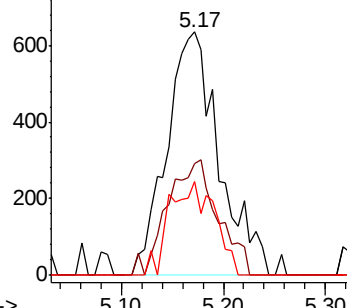

#30

Chloroform

Concen: 1.671 ug/l

RT: 5.21 min Scan# 666

Delta R.T. -0.00 min

Lab File: VX005106.D


Acq: 06 Oct 2018 09:59

Tgt Ion: 83 Resp: 8296



Ion Ratio Lower Upper


83 100

85 53.1 52.4 78.6

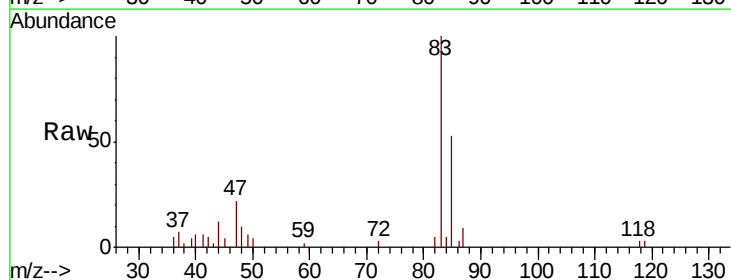

Abundance Ion 82.90 (82.60 to 83.60): VX0
Ion 84.90 (84.60 to 85.60): VX0

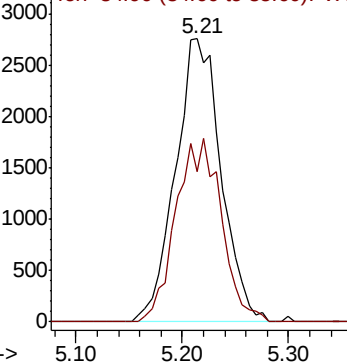

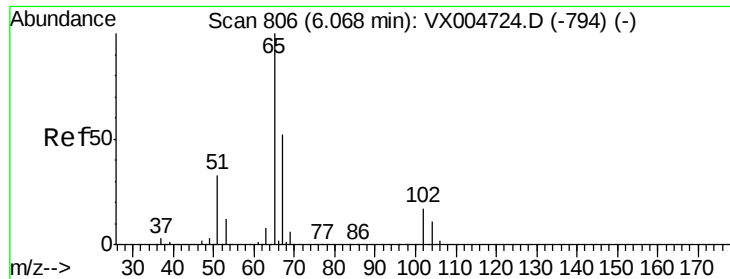

#33

1,2-Dichloroethane-d4

Concen: 51.731 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 65 Resp: 163495

Ion Ratio Lower Upper




65 100

67 55.8 0.0 107.4

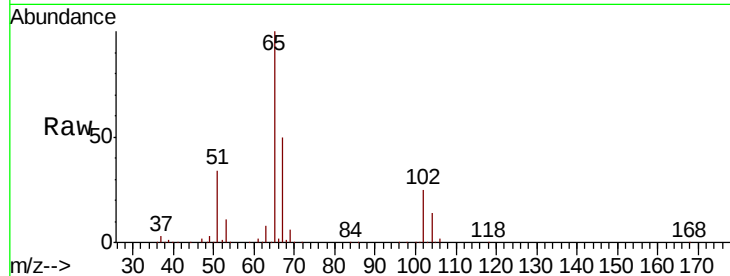

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

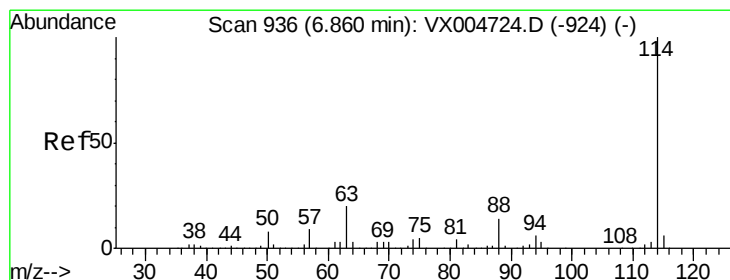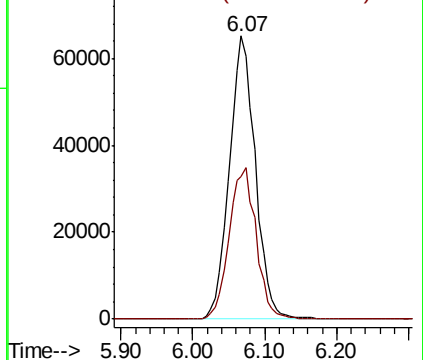

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59


Tgt Ion: 114 Resp: 329262

Ion Ratio Lower Upper

114 100

63 22.2 0.0 39.8



88 15.3 0.0 27.0




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

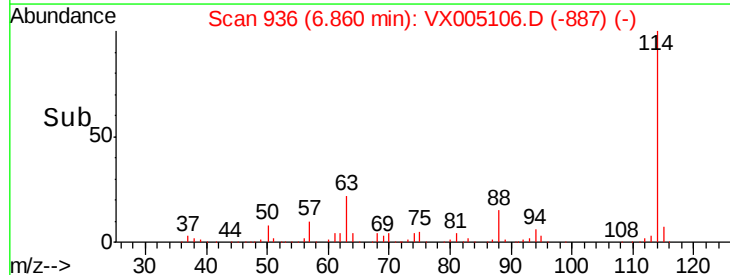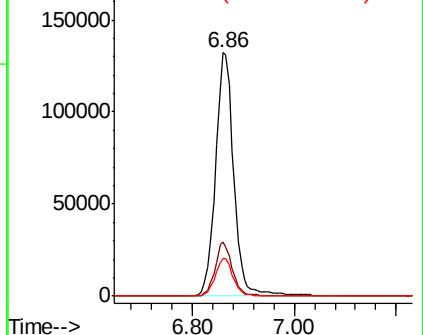



#35

Dibromofluoromethane

Concen: 54.523 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:113 Resp: 152149

Ion Ratio Lower Upper

113 100

111 96.0 77.0 115.4




192 22.2 17.0 25.6



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

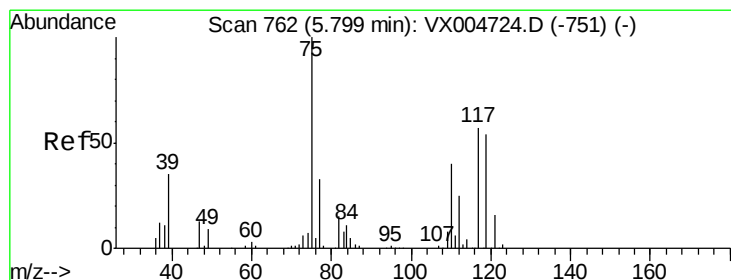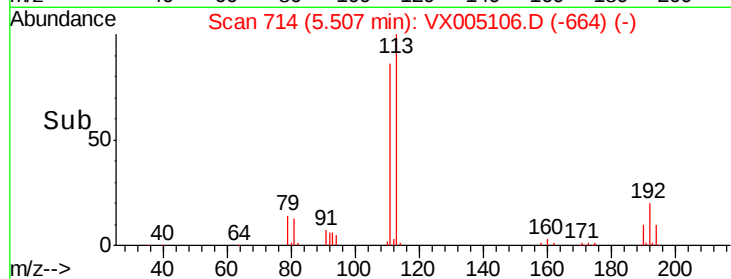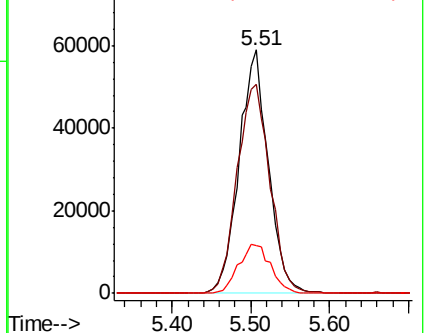

#36

1,1-Dichloropropene

Concen: 3.941 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59


Tgt Ion: 75 Resp: 15003

Ion Ratio Lower Upper

75 100

110 8.1 20.0 59.9#



77 0.0 27.1 40.7#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

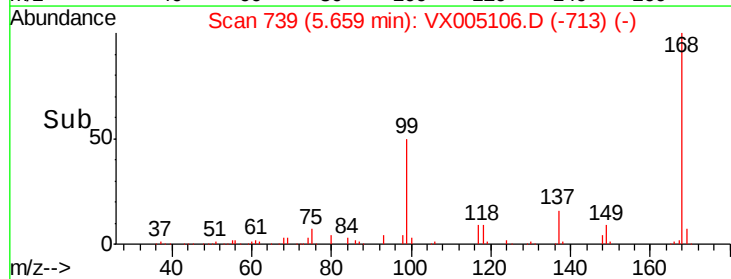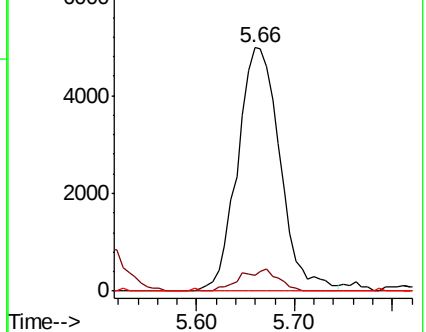



#37

Ethyl Acetate

Concen: 1.433 ug/l

RT: 4.70 min Scan# 582

Delta R.T. -0.16 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 7241

Ion Ratio Lower Upper




43 100

61 0.7 10.4 15.6#

70 0.0 8.7 13.1#

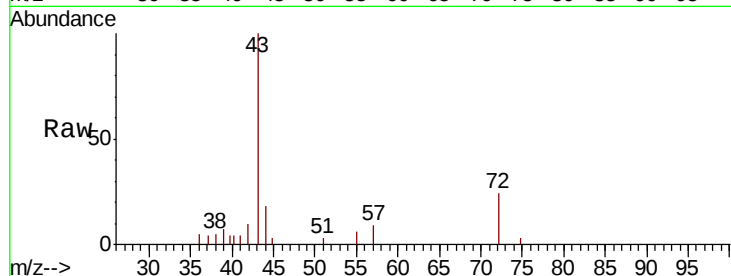

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 60.90 (60.60 to 61.60): VX0
Ion 70.00 (69.70 to 70.70): VX0

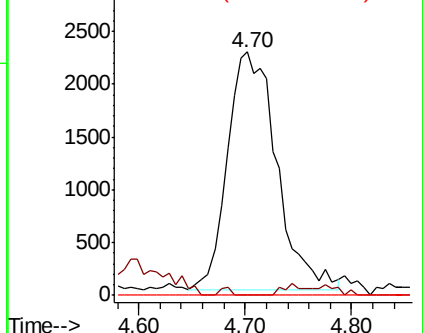

#38

Carbon Tetrachloride

Concen: 4.967 ug/l

RT: 5.67 min Scan# 741

Delta R.T. -0.11 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59


Tgt Ion: 117 Resp: 19878

Ion Ratio Lower Upper



117 100


119 7.1 75.2 112.8#

121 0.0 22.5 33.7#



Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

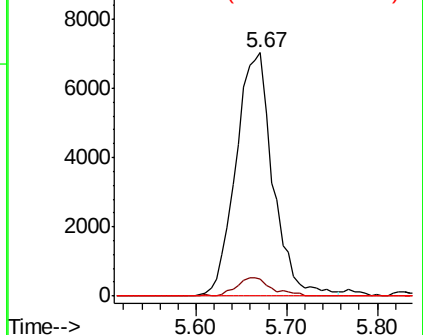







#43
Isopropyl Acetate
Concen: 13.915 ug/l
RT: 6.46 min Scan# 871
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
43	100		
61	19.7	14.2	21.4
87	12.1	9.3	13.9

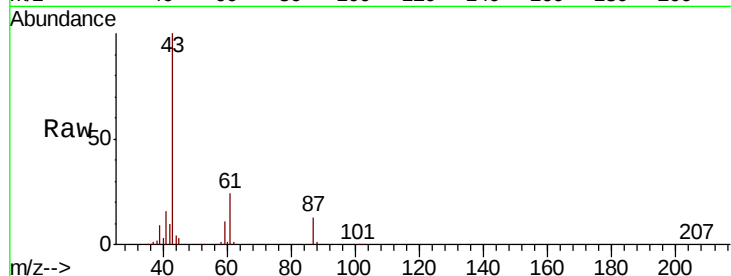


Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0


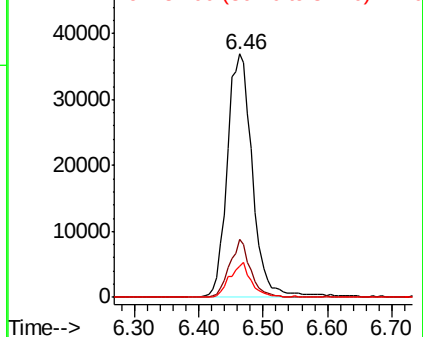



#47
Bromodichloromethane
Concen: 0.471 ug/l
RT: 7.90 min Scan# 1106
Delta R.T. -0.01 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion	Ratio	Lower	Upper
83	100		
85	64.1	51.2	76.8
127	9.7	7.0	10.6



Abundance Ion 82.90 (82.60 to 83.60): VX0
Ion 84.90 (84.60 to 85.60): VX0
Ion 126.80 (126.50 to 127.50): V




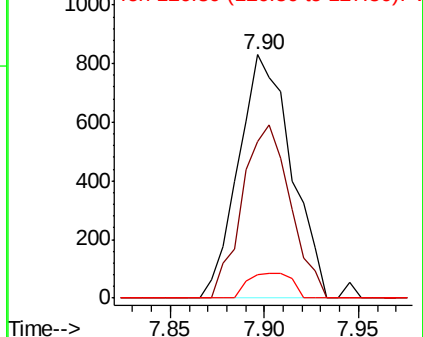




#48
Methyl methacrylate
Concen: 0.456 ug/l
RT: 7.69 min Scan# 1072
Delta R.T. -0.09 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 41 Resp: 1511
Ion Ratio Lower Upper
41 100
69 0.0 63.8 95.6#
39 8.1 40.7 61.1#

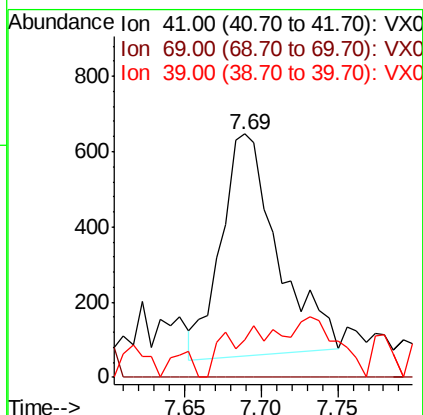

#50
Toluene-d8
Concen: 50.588 ug/l
RT: 8.72 min Scan# 1241
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion: 98 Resp: 469310
Ion Ratio Lower Upper
98 100
100 63.8 51.9 77.9

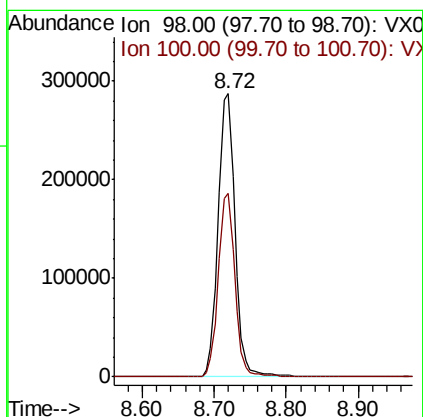



#51

4-Methyl-2-Pentanone

Concen: 0.202 ug/l

RT: 8.65 min Scan# 1230

Delta R.T. -0.00 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59


Instrument :
MSVOA_X
ClientSampled :

Tot Ion: 43 Resp: 930




Ion Ratio Lower Upper

43 100

58 69.9 30.5 45.7#



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0

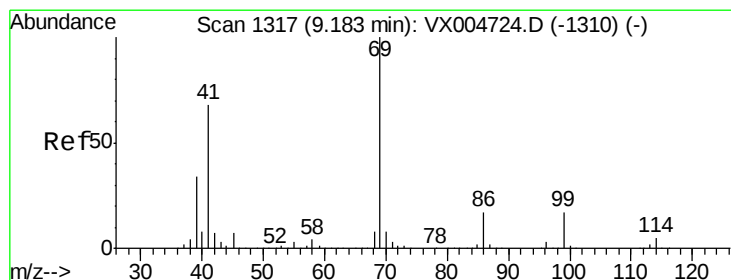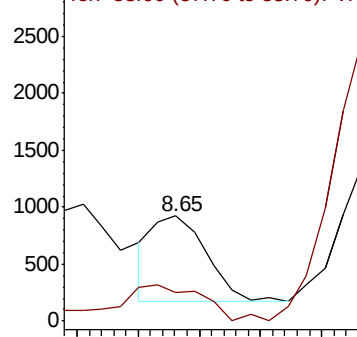

#56

Ethyl methacrylate

Concen: 2.879 ug/l

RT: 9.38 min Scan# 1349

Delta R.T. 0.19 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59


Tgt Ion: 69 Resp: 86

Ion Ratio Lower Upper



69 100


41 704.7 56.9 85.3#

39 597.7 28.4 42.6#



Abundance Ion 69.00 (68.70 to 69.70): VX0
Ion 41.00 (40.70 to 41.70): VX0
Ion 39.00 (38.70 to 39.70): VX0

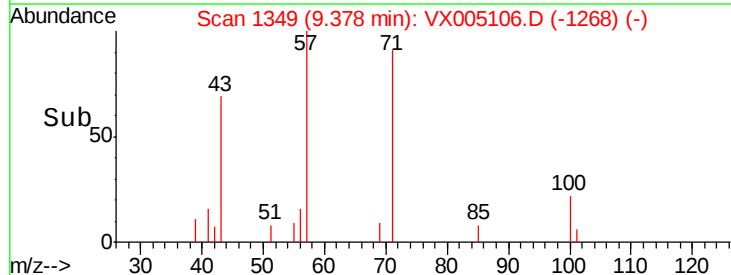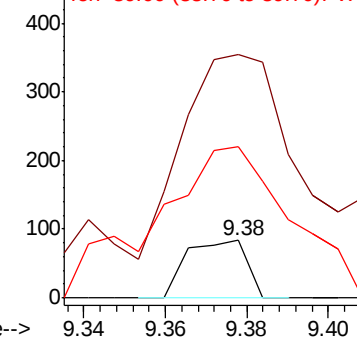







#62
4-Bromofluorobenzene
Concen: 51.382 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 95 Resp: 171727
Ion Ratio Lower Upper
95 100
174 94.3 0.0 185.0
176 89.9 0.0 180.2

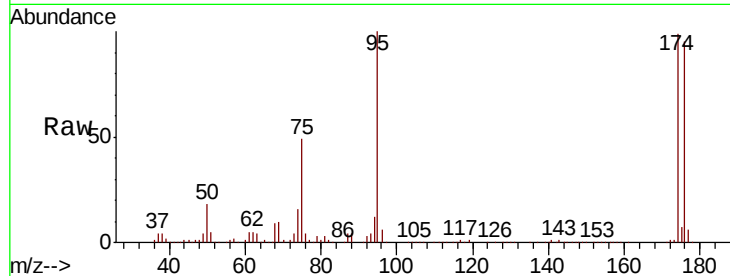


Abundance Ion 94.90 (94.60 to 95.60): VX0
Ion 173.80 (173.50 to 174.50): V
Ion 175.80 (175.50 to 176.50): V


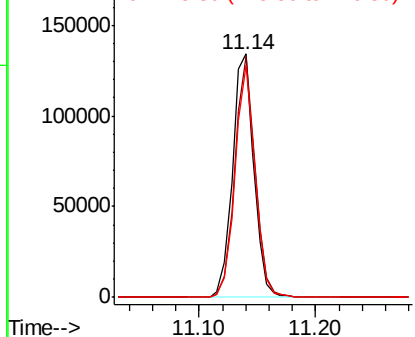



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion: 117 Resp: 321508
Ion Ratio Lower Upper
117 100
82 55.4 42.2 63.4
119 32.2 27.4 41.0

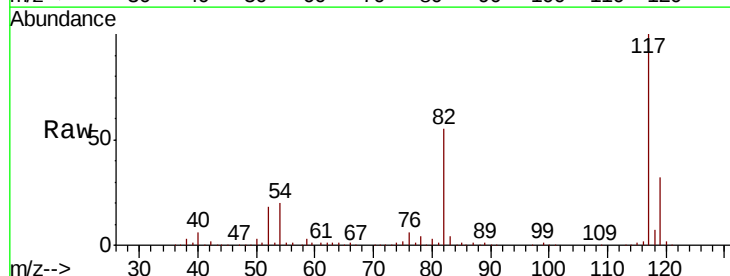

Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V




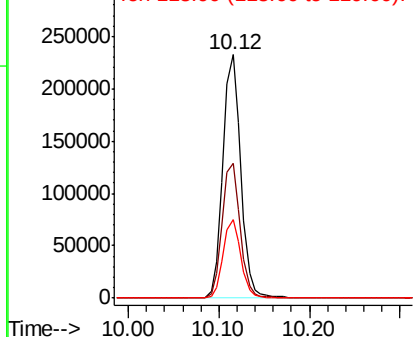




#69
o-Xylene
Concen: 0.597 ug/l
RT: 10.70 min Scan# 1566
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59




Instrument :
MSVOA_X
ClientSampled :


Tot Ion:106 Resp: 2805
Ion Ratio Lower Upper
106 100
91 221.5 108.3 324.8

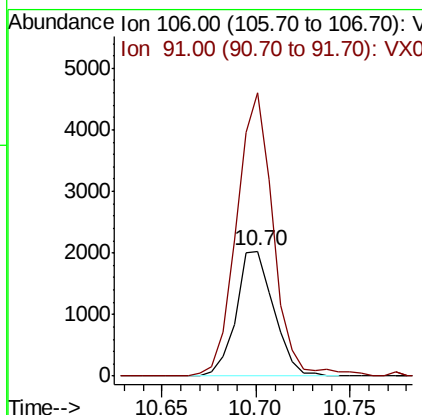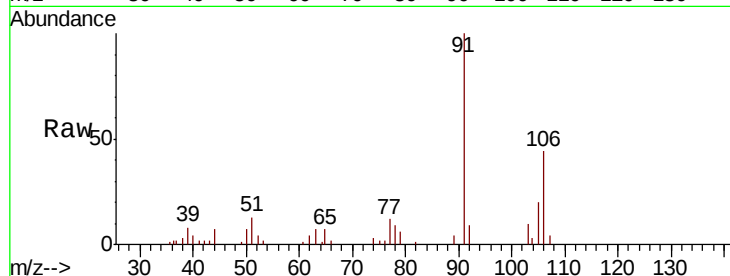

#70
Styrene
Concen: 2.177 ug/l
RT: 10.69 min Scan# 1565
Delta R.T. -0.02 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion:104 Resp: 336
Ion Ratio Lower Upper
104 100
78 174.4 40.0 60.0#
103 166.4 44.3 66.5#

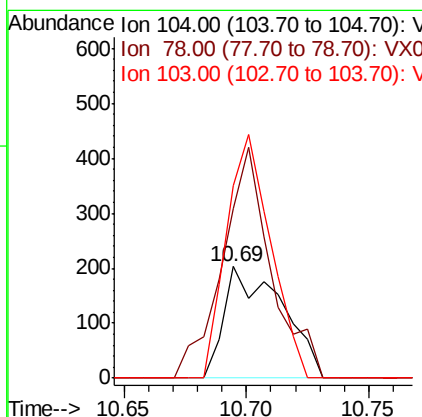




#72




1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:152 Resp: 189864
Ion Ratio Lower Upper
152 100
115 55.1 40.2 120.6
150 155.0 0.0 351.0




Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

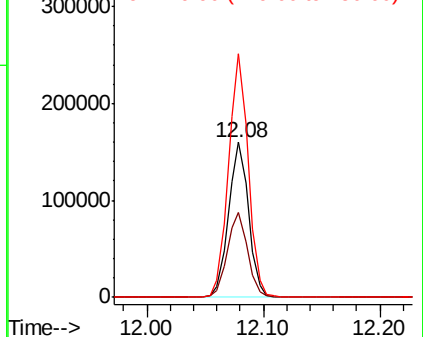



#74


N-ethyl acetate
Concen: 1.764 ug/l
RT: 10.87 min Scan# 1594
Delta R.T. -0.03 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion: 43 Resp: 107
Ion Ratio Lower Upper
43 100
70 0.0 32.6 48.8#
55 17.8 21.6 32.4#
61 0.0 19.1 28.7#



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 70.00 (69.70 to 70.70): VX0
Ion 55.00 (54.70 to 55.70): VX0
Ion 61.00 (60.70 to 61.70): VX0

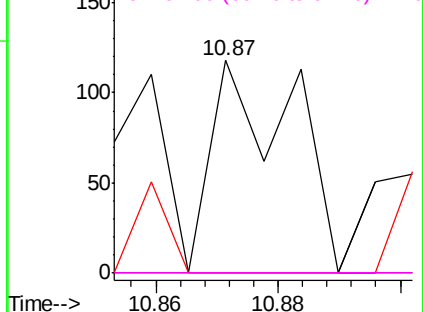



#76

1,2,3-Trichloropropane

Concen: 20.161 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. -0.16 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 75 Resp: 85797

Ion Ratio Lower Upper

75 100

77 1.3 21.4 64.3#

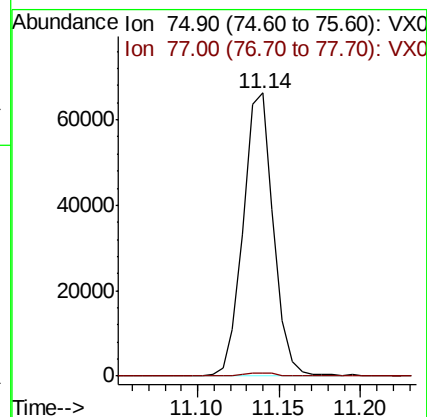

#80

1,3,5-Trimethylbenzene

Concen: 0.617 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. -0.00 min

Lab File: VX005106.D




Acq: 06 Oct 2018 09:59


Tgt Ion: 105 Resp: 8909

Ion Ratio Lower Upper

105 100

120 49.8 24.3 72.8



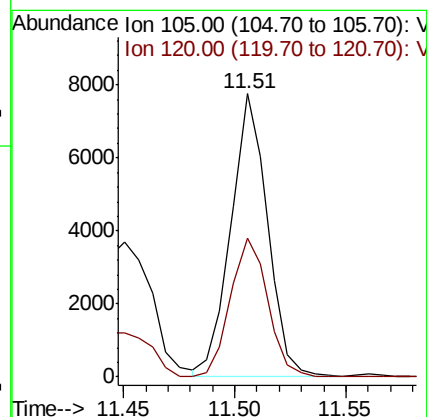





#81
trans-1,4-Dichloro-2-butene
Concen: 54.789 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. 0.06 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 75 Resp: 85797
Ion Ratio Lower Upper
75 100
53 0.3 80.2 120.4#
89 0.0 37.1 55.7#

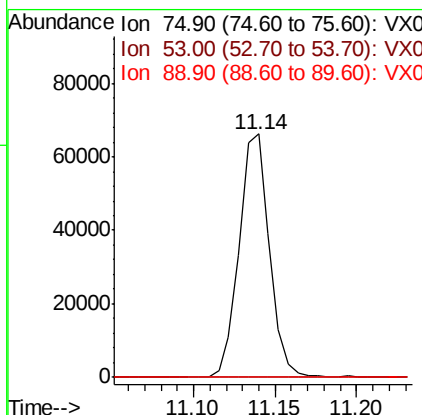

#84
1,2,4-Trimethylbenzene
Concen: 0.768 ug/l
RT: 11.81 min Scan# 1748
Delta R.T. -0.00 min
Lab File: VX005106.D
Acq: 06 Oct 2018 09:59

Tgt Ion: 105 Resp: 10891
Ion Ratio Lower Upper
105 100
120 43.9 22.8 68.3

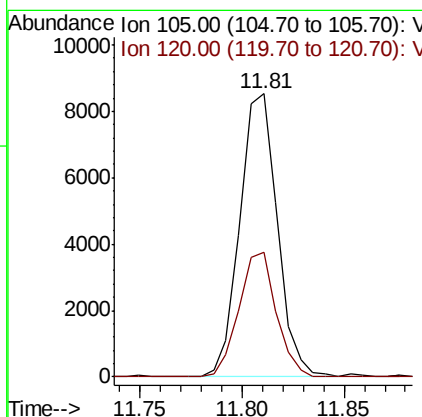



#90

Hexachloroethane

Concen: 0.279 ug/l

RT: 12.61 min Scan# 1879

Delta R.T. 0.01 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59

Instrument :

MSVOA_X


ClientSampled :

Tot Ion:117 Resp: 506

Ion Ratio Lower Upper




117 100

201 0.0 48.4 145.0#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

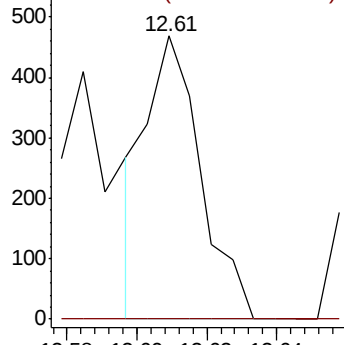

#95

Naphthalene

Concen: 1.277 ug/l

RT: 13.83 min Scan# 2080

Delta R.T. -0.00 min

Lab File: VX005106.D

Acq: 06 Oct 2018 09:59


Tgt Ion:128 Resp: 8928

Ion Ratio Lower Upper

128 100

127 14.2 10.4 15.6

129 11.6 8.7 13.1



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

