

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100518\
 Data File : VX005070.D
 Acq On : 05 Oct 2018 17:05
 Operator : JC/MD
 Sample : VX1005WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1005WBL01

Quant Time: Oct 05 18:27:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 03 04:00:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	187485	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	300594	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	291375	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	165510	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	144434	53.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.86%	
35) Dibromofluoromethane	5.50	113	122571	48.11	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.22%	
50) Toluene-d8	8.71	98	431454	50.94	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.88%	
62) 4-Bromofluorobenzene	11.14	95	156009	51.13	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.26%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100518\
Data File : VX005070.D
Acq On : 05 Oct 2018 17:05
Operator : JC/MD
Sample : VX1005WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1005WBL01

Quant Time: Oct 05 18:27:36 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 03 04:00:03 2018
Response via : Initial Calibration

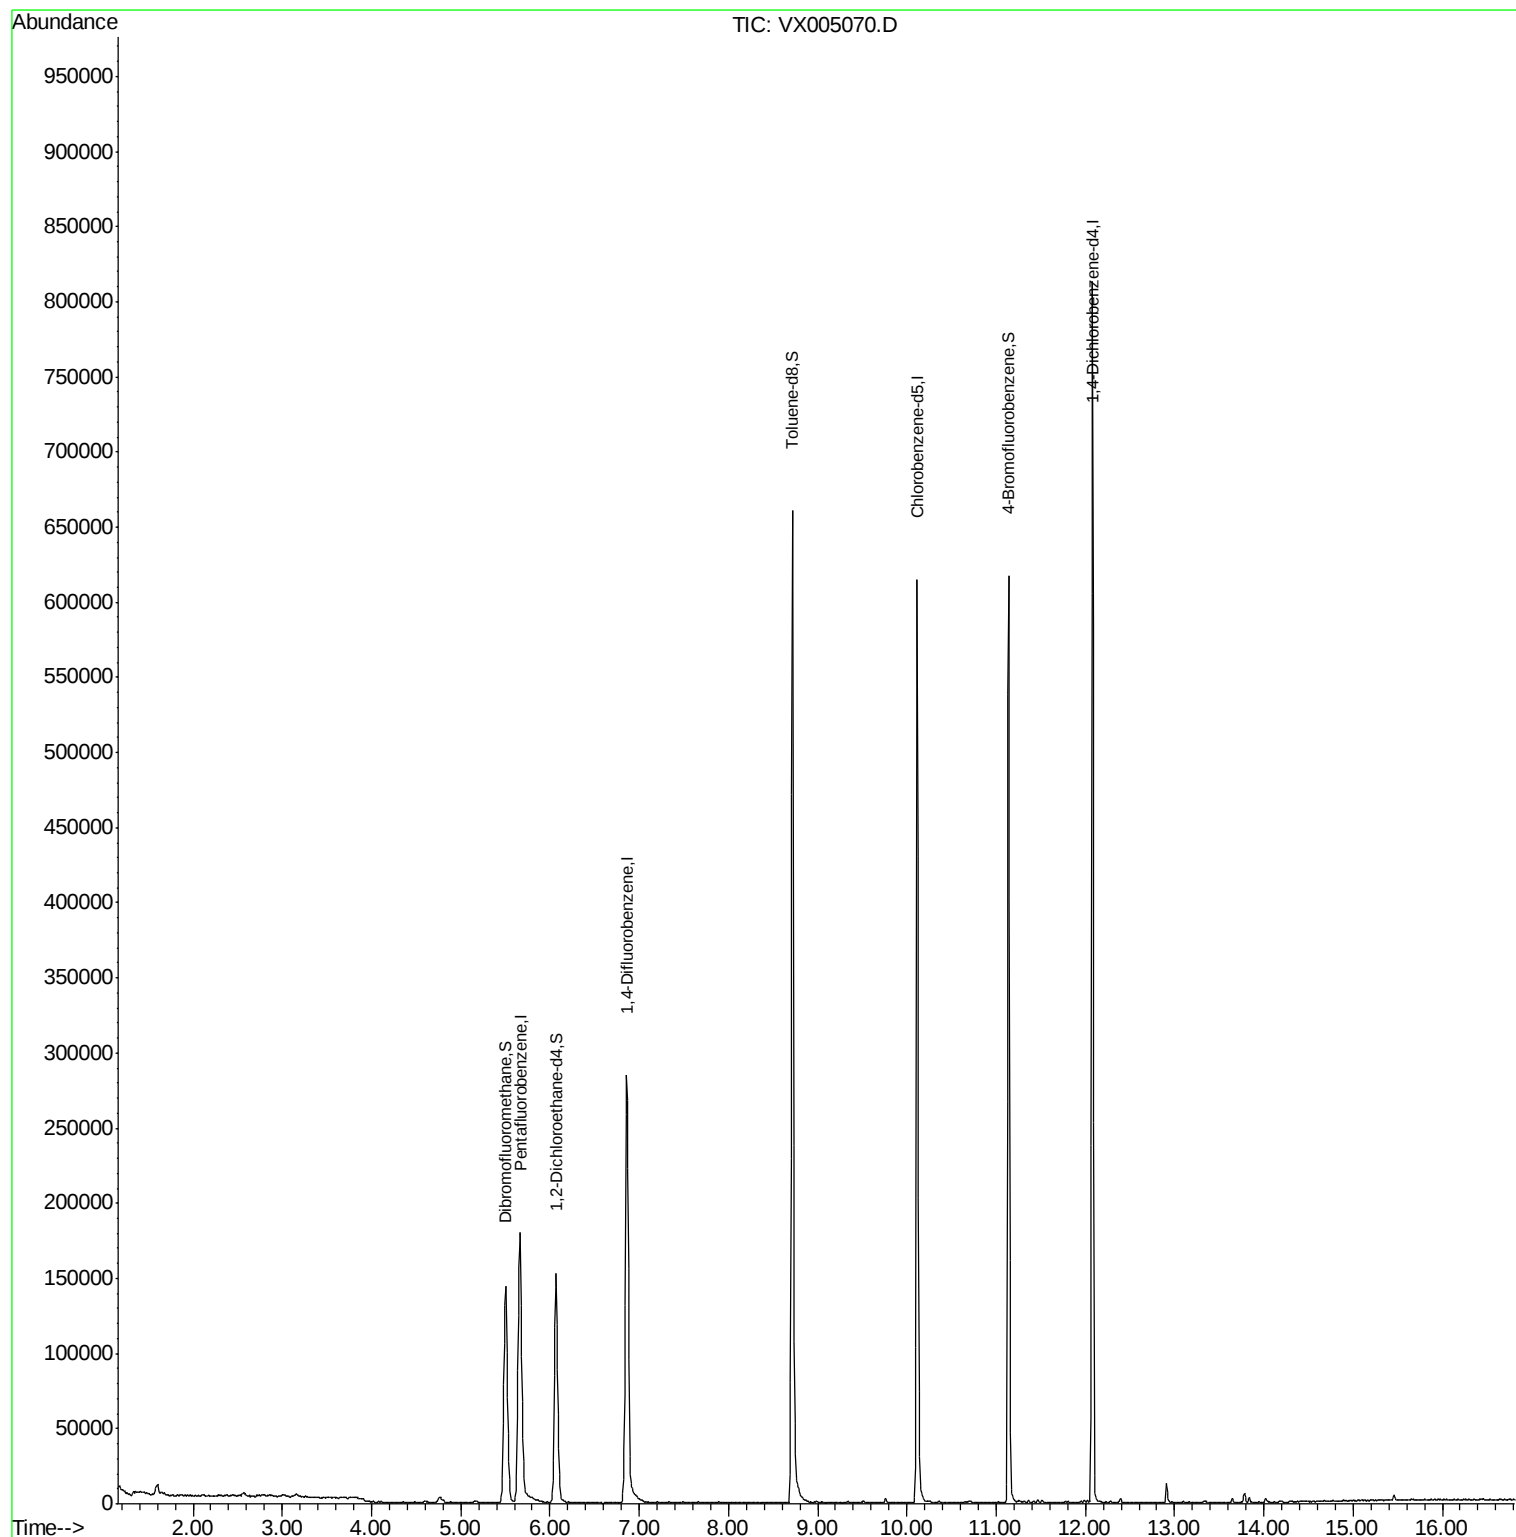



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX005070.D

Acq: 05 Oct 2018 17:05

Instrument :

MSVOA_X

ClientSampleId :


VX1005WBL01

Tot Ion:168 Resp: 187485

Ion Ratio Lower Upper




168 100

99 50.4 39.3 58.9

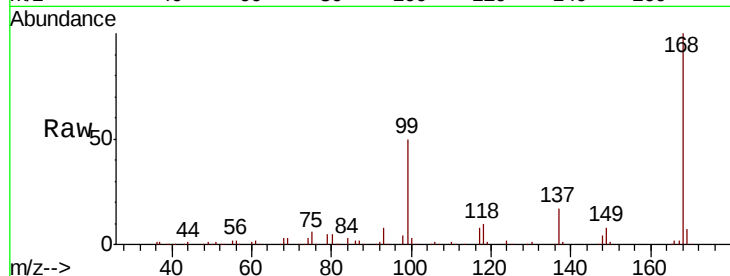

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

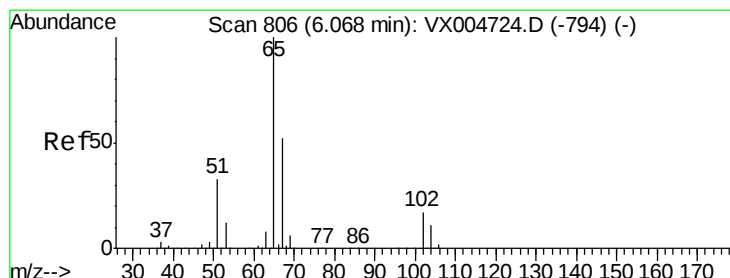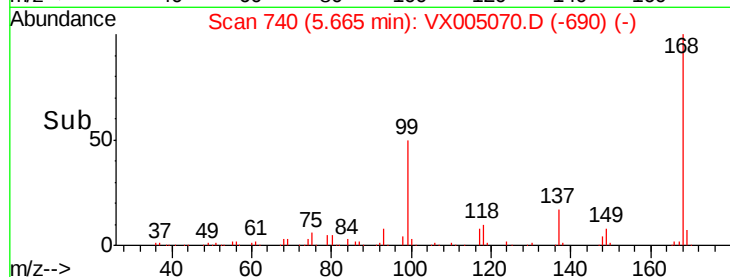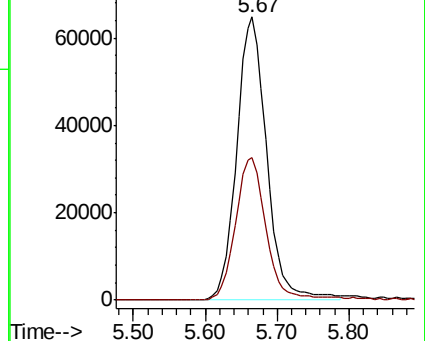

#33

1,2-Dichloroethane-d4

Concen: 53.929 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX005070.D


Acq: 05 Oct 2018 17:05

Tgt Ion: 65 Resp: 144434

Ion Ratio Lower Upper



65 100

67 54.2 0.0 107.4

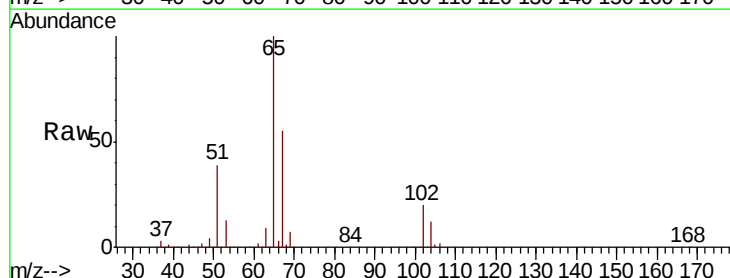

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

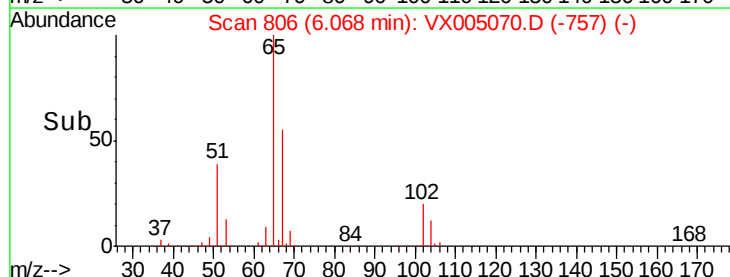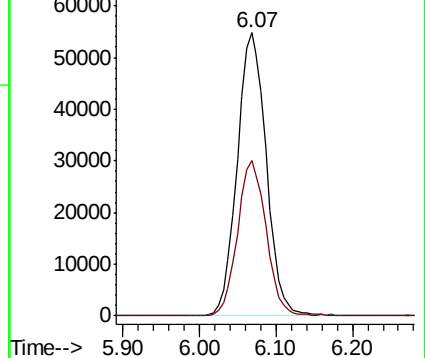







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX005070.D
 Acq: 05 Oct 2018 17:05

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1005WBL01

Tot Ion:114 Resp: 300594
 Ion Ratio Lower Upper
 114 100
 63 21.3 0.0 39.8
 88 15.1 0.0 27.0

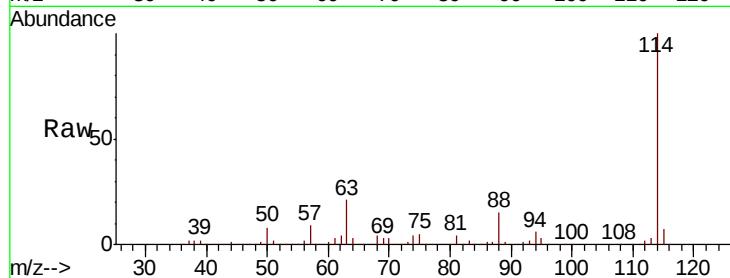


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

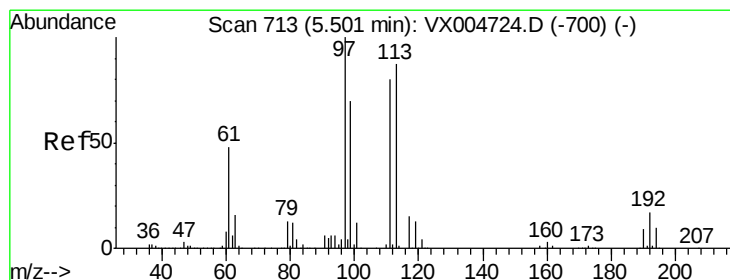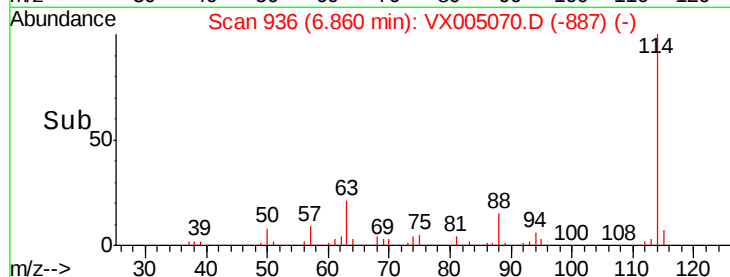
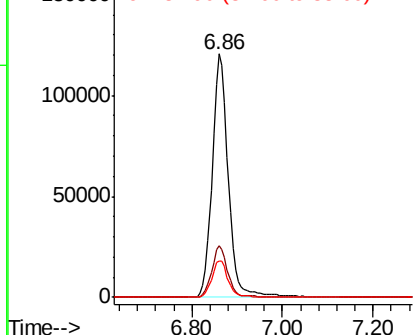



#35
 Dibromofluoromethane
 Concen: 48.113 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.00 min
 Lab File: VX005070.D
 Acq: 05 Oct 2018 17:05

Tgt Ion:113 Resp: 122571
 Ion Ratio Lower Upper
 113 100
 111 102.0 77.0 115.4
 192 23.4 17.0 25.6

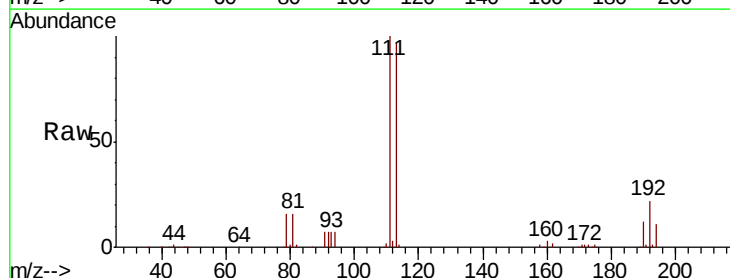

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

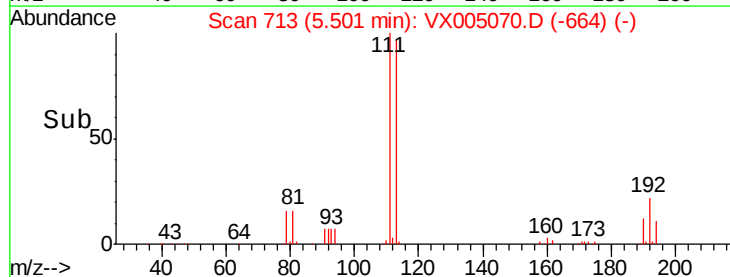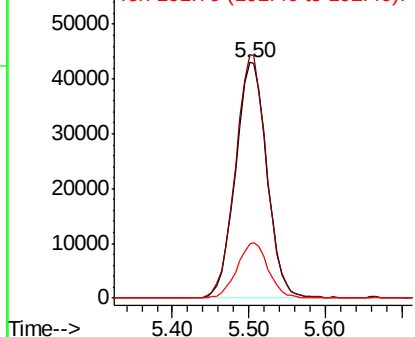

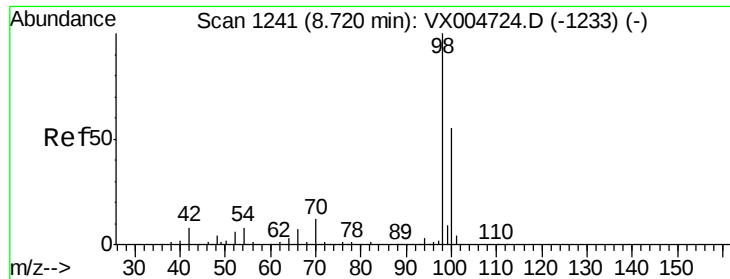

#50

Toluene-d8

Concen: 50.943 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.01 min

Lab File: VX005070.D

Acq: 05 Oct 2018 17:05

Instrument :

MSVOA_X

ClientSampleId :


VX1005WBL01

Tot Ion: 98 Resp: 431454

Ion Ratio Lower Upper

98 100

100 63.4 51.9 77.9

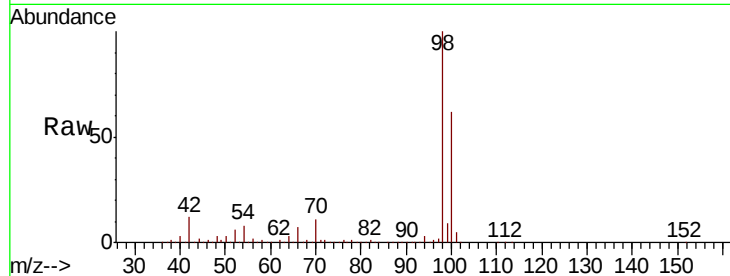

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

8.71

250000

200000



150000

100000

50000

0

Time-->

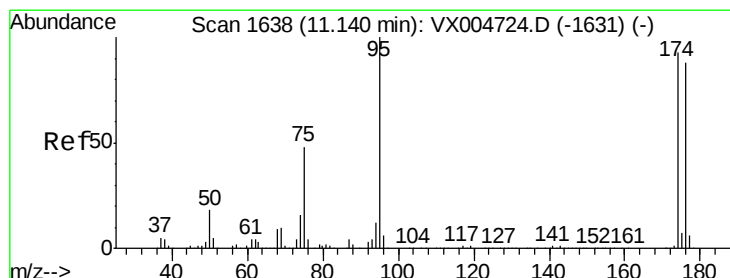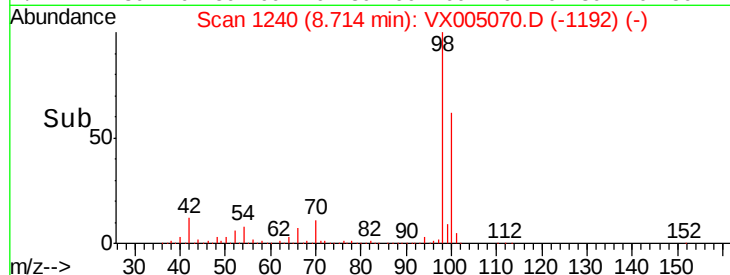

#62

4-Bromofluorobenzene

Concen: 51.131 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. 0.00 min

Lab File: VX005070.D

Acq: 05 Oct 2018 17:05


Tgt Ion: 95 Resp: 156009

Ion Ratio Lower Upper

95 100

174 92.1 0.0 185.0

176 87.8 0.0 180.2

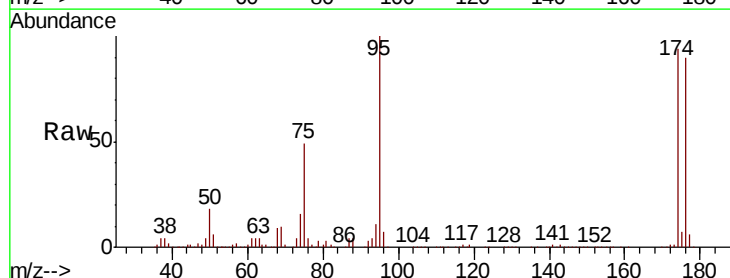

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.14


150000


100000

50000

0

Time-->




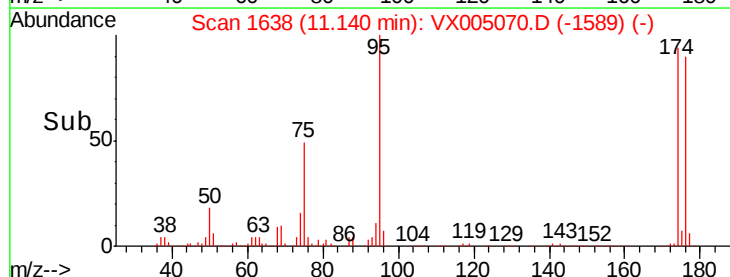


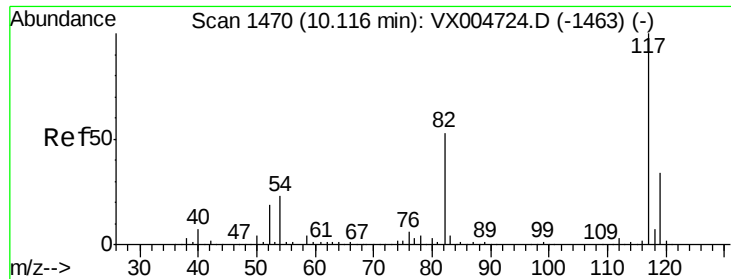

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.00 min
Lab File: VX005070.D
Acq: 05 Oct 2018 17:05

Instrument :
MSVOA_X
ClientSampleId :
VX1005WBL01

Tot Ion:117 Resp: 291375
Ion Ratio Lower Upper
117 100
82 54.9 42.2 63.4
119 32.3 27.4 41.0

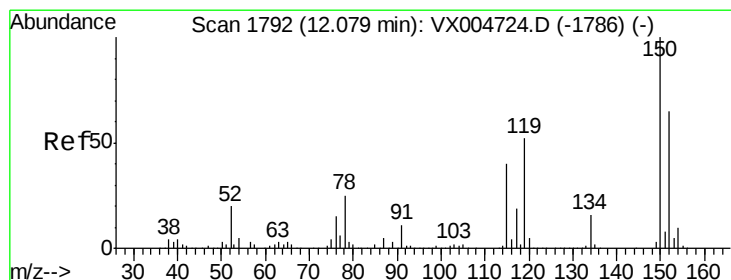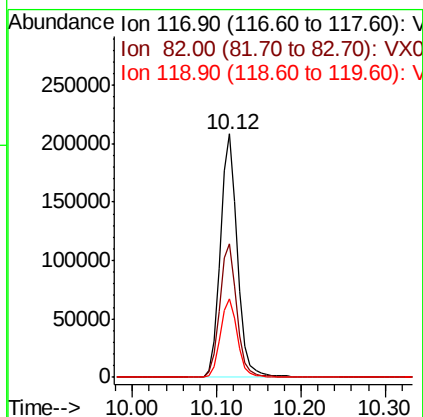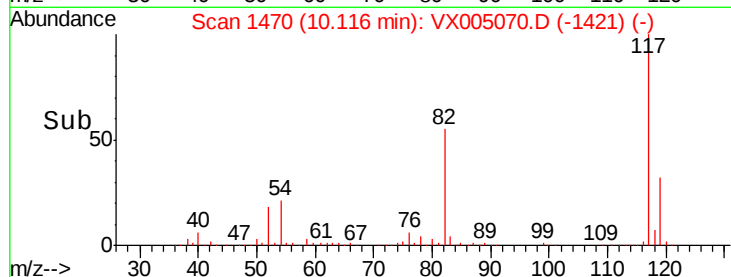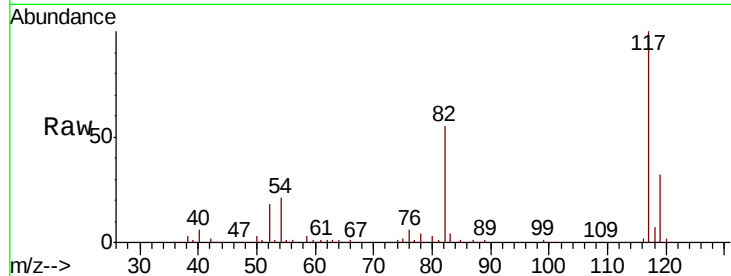

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX005070.D
Acq: 05 Oct 2018 17:05

Tgt Ion:152 Resp: 165510
Ion Ratio Lower Upper
152 100
115 54.8 40.2 120.6
150 156.5 0.0 351.0

