


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100518\
Data File : VX005068.D
Acq On : 05 Oct 2018 14:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Title : SW846 8260
Last Update : Fri Oct 05 02:22:33 2018

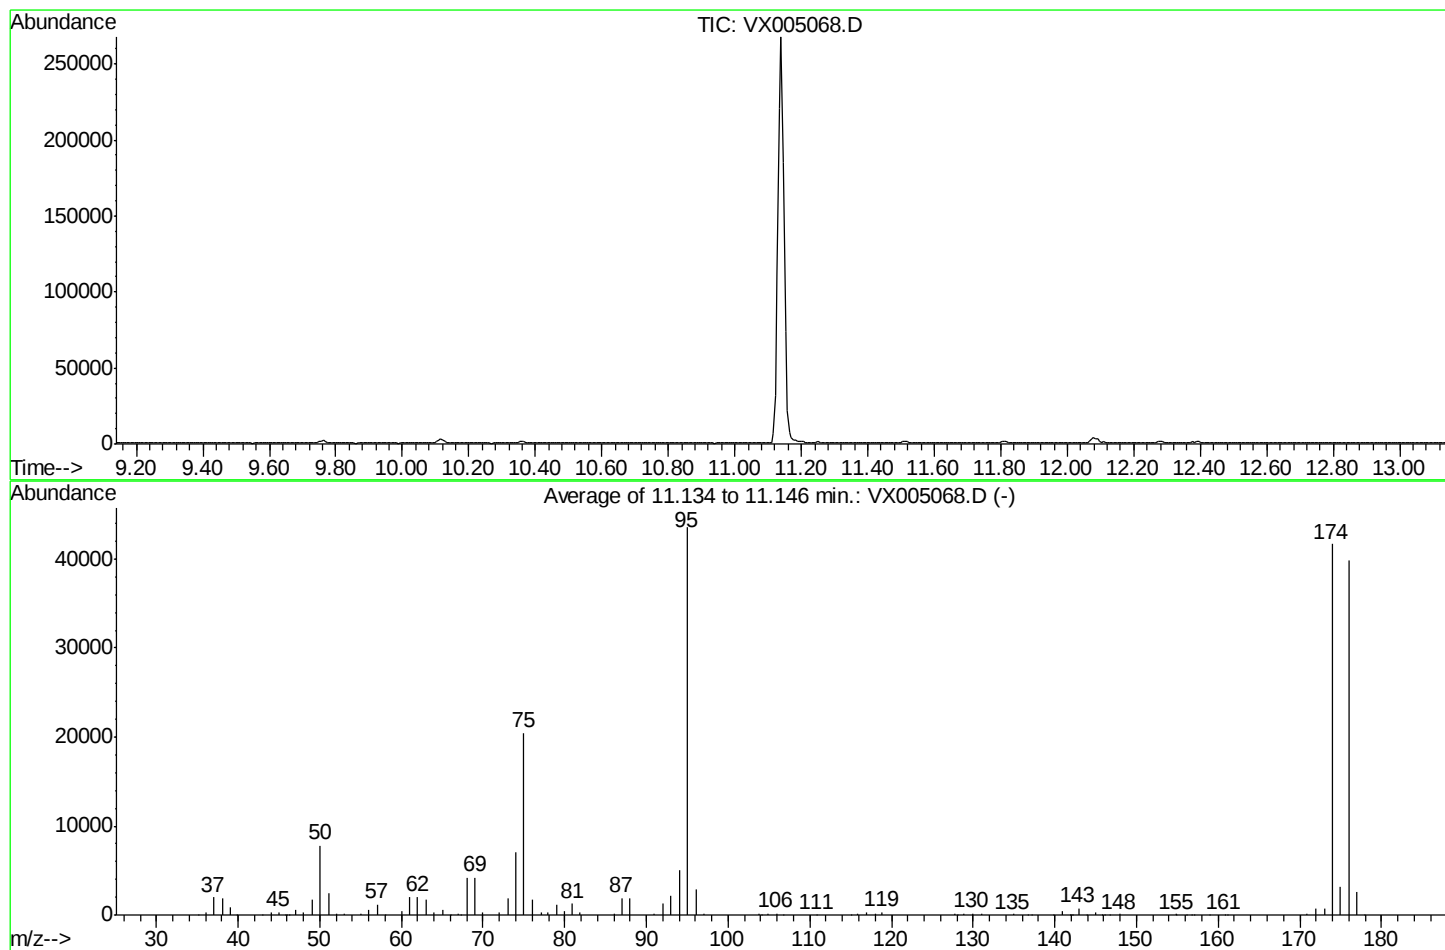

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	7814	PASS
75	95	30	60	47.0	20495	PASS
95	95	100	100	100.0	43570	PASS
96	95	5	9	6.5	2812	PASS
173	174	0.00	2	1.7	691	PASS
174	95	50	100	95.7	41714	PASS
175	174	5	9	7.5	3136	PASS
176	174	95	101	95.4	39789	PASS
177	176	5	9	6.4	2536	PASS