


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100518\
Data File : VX005091.D
Acq On : 06 Oct 2018 02:52
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N100418W.M
Title : SW846 8260
Last Update : Fri Oct 05 02:22:33 2018

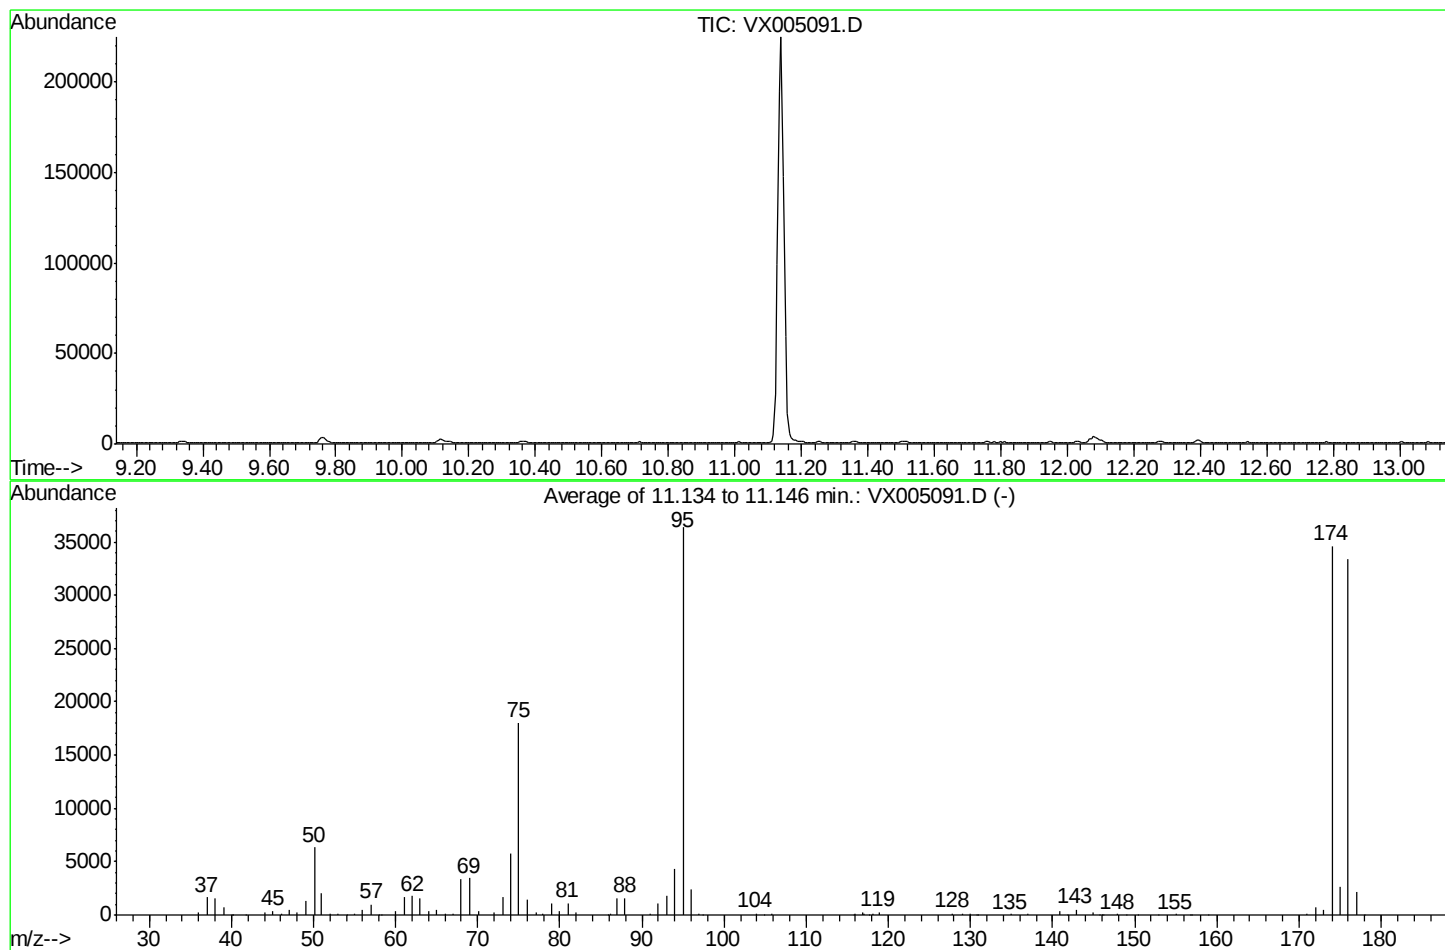

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6358	PASS
75	95	30	60	49.6	18042	PASS
95	95	100	100	100.0	36368	PASS
96	95	5	9	6.6	2406	PASS
173	174	0.00	2	1.5	503	PASS
174	95	50	100	95.1	34584	PASS
175	174	5	9	7.8	2681	PASS
176	174	95	101	96.5	33368	PASS
177	176	5	9	6.6	2193	PASS