
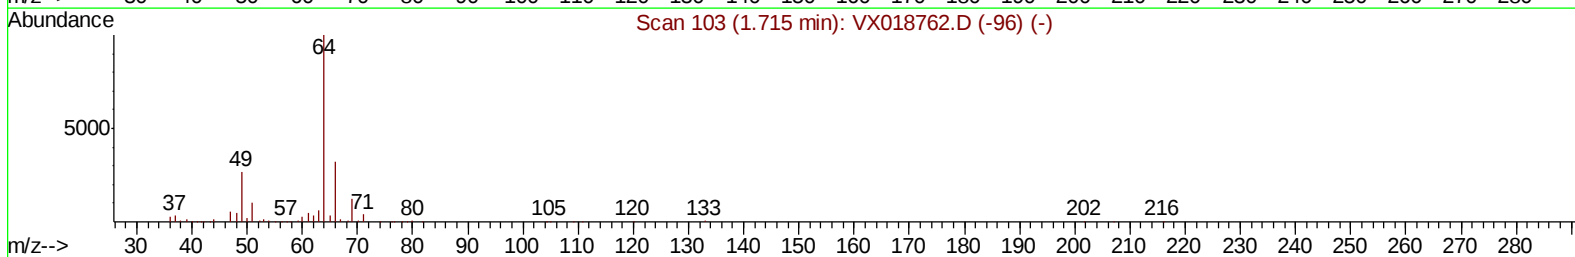
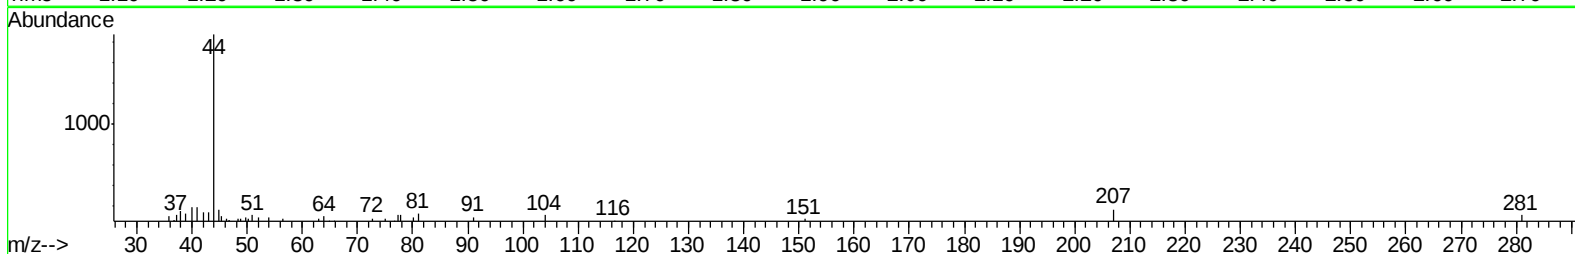


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100520\
Data File : VX018772.D
Acq On : 05 Oct 2020 17:54
Operator : JC/SP
Sample : L4239-03DL 100X
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Oct 06 03:07:54 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 06 02:55:01 2020
Response via : Initial Calibration

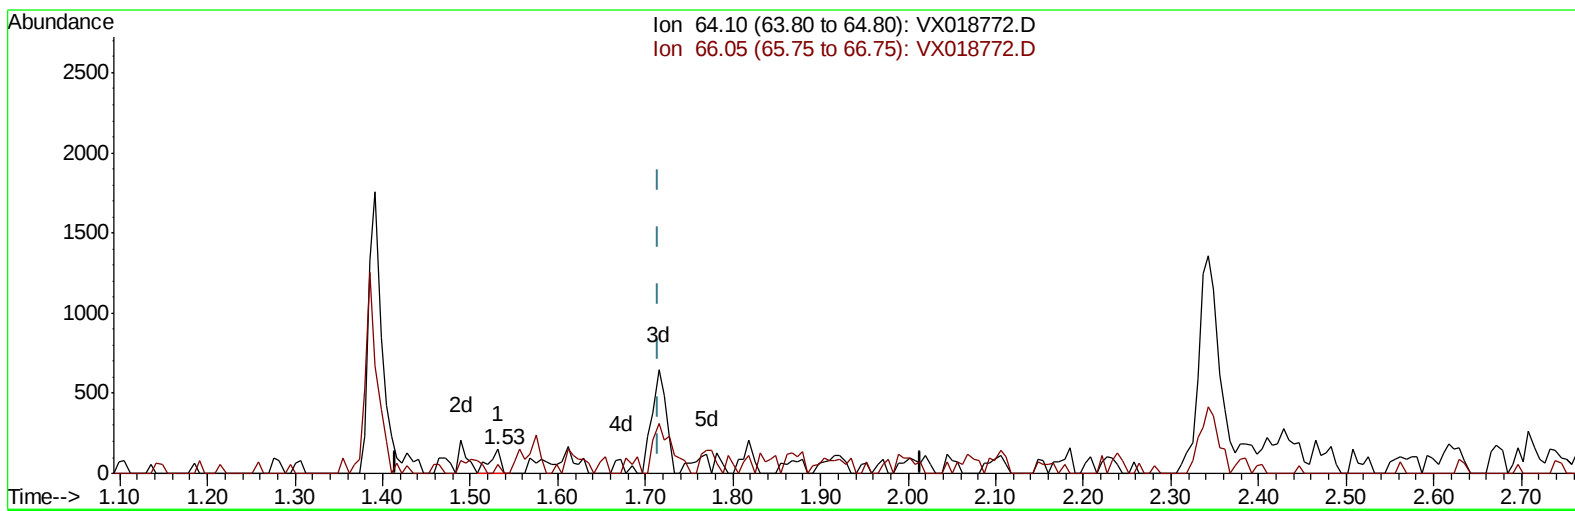

TIC: VX018772.D

(8) Chloroethane (T)

1.532min (-0.183) 0.03ug/L

response 136

Ion	Exp%	Act%
64.10	100	100
66.05	30.70	35.57
0.00	0.00	0.00
0.00	0.00	0.00